

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025626.D
 Acq On : 08 Dec 2021 17:56
 Operator : JC/MD
 Sample : VX1208MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	58818	57905	14.15%	1.773%
2	1.666	91	95	106	rVB	42642	57503	14.05%	1.761%
3	2.307	194	200	211	rBV	85846	140976	34.45%	4.317%
4	2.471	225	227	229	rBV	392	451	0.11%	0.014%
5	2.788	275	279	286	rVB2	4977	9124	2.23%	0.279%
6	2.947	301	305	311	rVB2	1715	3269	0.80%	0.100%
7	3.099	328	330	332	rBV	395	321	0.08%	0.010%
8	3.398	376	379	380	rBV2	433	447	0.11%	0.014%
9	3.922	464	465	468	rBV2	337	302	0.07%	0.009%
10	4.056	485	487	490	rBV	341	301	0.07%	0.009%
11	4.142	499	501	505	rBV	286	327	0.08%	0.010%
12	4.453	543	552	565	rBV	34927	99902	24.41%	3.059%
13	4.782	604	606	609	rVB2	317	289	0.07%	0.009%
14	5.062	640	652	665	rBV	55018	167031	40.82%	5.115%
15	5.440	711	714	716	rBV2	230	301	0.07%	0.009%
16	5.526	724	728	729	rBV	389	477	0.12%	0.015%
17	5.641	745	747	750	rVB	212	241	0.06%	0.007%
18	5.690	750	755	758	rBV2	314	611	0.15%	0.019%
19	5.971	790	801	822	rBV2	137468	409230	100.00%	12.532%
20	6.428	871	876	879	rVV	220	449	0.11%	0.014%
21	6.629	906	909	911	rBV	283	284	0.07%	0.009%
22	6.763	921	931	945	rVB	111690	263741	64.45%	8.077%
23	6.995	968	969	972	rVB	336	311	0.08%	0.010%
24	7.025	972	974	976	rBV	283	315	0.08%	0.010%
25	7.074	980	982	983	rBV	357	251	0.06%	0.008%
26	7.111	983	988	997	rVV5	1911	4793	1.17%	0.147%
27	7.220	1003	1006	1008	rBV2	246	279	0.07%	0.009%
28	7.312	1012	1021	1031	rBV	86217	186508	45.58%	5.712%
29	7.537	1054	1058	1059	rBV2	214	231	0.06%	0.007%
30	7.806	1099	1102	1106	rVV2	389	653	0.16%	0.020%
31	7.860	1110	1111	1114	rBV	334	381	0.09%	0.012%
32	7.928	1117	1122	1124	rBV3	366	566	0.14%	0.017%
33	8.098	1146	1150	1151	rBV	294	275	0.07%	0.008%
34	8.117	1151	1153	1158	rVB	296	351	0.09%	0.011%
35	8.281	1176	1180	1181	rBV2	207	306	0.07%	0.009%
36	8.324	1181	1187	1195	rBV	55982	90515	22.12%	2.772%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025626.D
 Acq On : 08 Dec 2021 17:56
 Operator : JC/MD
 Sample : VX1208MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.421	1201	1203	1206	rBV	347	365	0.09%	0.011%
38	8.470	1208	1211	1215	rVB3	252	375	0.09%	0.011%
39	8.537	1218	1222	1223	rBV2	230	275	0.07%	0.008%
40	8.653	1234	1241	1248	rBV	209536	335396	81.96%	10.271%
41	8.720	1249	1252	1258	rVV3	2906	4828	1.18%	0.148%
42	8.952	1284	1290	1298	rBV	40609	58103	14.20%	1.779%
43	9.037	1301	1304	1306	rBV	334	353	0.09%	0.011%
44	9.385	1355	1361	1375	rBV	153447	217325	53.11%	6.655%
45	9.866	1437	1440	1442	rBV2	331	454	0.11%	0.014%
46	9.921	1447	1449	1453	rBV	382	659	0.16%	0.020%
47	10.055	1465	1471	1482	rBV	233663	311890	76.21%	9.551%
48	10.195	1491	1494	1495	rBV	491	407	0.10%	0.012%
49	10.238	1499	1501	1503	rBV	292	233	0.06%	0.007%
50	10.451	1534	1536	1538	rBV	357	241	0.06%	0.007%
51	10.561	1553	1554	1557	rVB	408	299	0.07%	0.009%
52	10.592	1557	1559	1560	rBV	433	314	0.08%	0.010%
53	10.653	1565	1569	1572	rBV3	561	755	0.18%	0.023%
54	10.714	1577	1579	1583	rVV	287	431	0.11%	0.013%
55	10.768	1583	1588	1590	rVB2	347	520	0.13%	0.016%
56	10.933	1613	1615	1617	rBV	291	306	0.07%	0.009%
57	11.061	1633	1636	1637	rVB2	363	265	0.06%	0.008%
58	11.122	1643	1646	1651	rVB2	1234	1698	0.41%	0.052%
59	11.195	1652	1658	1665	rBV	163129	208473	50.94%	6.384%
60	11.409	1692	1693	1697	rVB	336	255	0.06%	0.008%
61	11.457	1699	1701	1704	rVV	380	395	0.10%	0.012%
62	11.579	1719	1721	1723	rVB	382	253	0.06%	0.008%
63	11.610	1723	1726	1727	rBV	385	398	0.10%	0.012%
64	11.750	1743	1749	1753	rBV3	1473	2246	0.55%	0.069%
65	11.823	1759	1761	1764	rBV	323	521	0.13%	0.016%
66	11.939	1776	1780	1782	rVB2	729	875	0.21%	0.027%
67	11.976	1782	1786	1789	rBV4	663	892	0.22%	0.027%
68	12.024	1789	1794	1804	rVB	241729	300827	73.51%	9.213%
69	12.134	1809	1812	1813	rBV2	573	705	0.17%	0.022%
70	12.201	1820	1823	1824	rBV	287	239	0.06%	0.007%
71	12.323	1837	1843	1850	rVB	235353	301667	73.72%	9.238%
72	12.427	1858	1860	1862	rBV2	323	284	0.07%	0.009%
73	12.585	1883	1886	1890	rBV	268	445	0.11%	0.014%
74	12.658	1896	1898	1900	rBV	309	234	0.06%	0.007%
75	12.756	1912	1914	1920	rBV2	361	680	0.17%	0.021%
76	12.914	1938	1940	1942	rBV	205	259	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025626.D
 Acq On : 08 Dec 2021 17:56
 Operator : JC/MD
 Sample : VX1208MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.975	1948	1950	1952	rBV	378	270	0.07%	0.008%
78	13.061	1960	1964	1965	rBV2	344	376	0.09%	0.012%
79	13.122	1970	1974	1977	rBV3	749	909	0.22%	0.028%
80	13.262	1993	1997	1999	rBV2	241	321	0.08%	0.010%
81	13.299	2002	2003	2007	rBV2	248	337	0.08%	0.010%
82	13.506	2035	2037	2040	rBV	242	285	0.07%	0.009%
83	13.591	2049	2051	2055	rVB	753	868	0.21%	0.027%
84	13.780	2080	2082	2086	rVB2	820	830	0.20%	0.025%
85	13.963	2110	2112	2118	rVB3	555	820	0.20%	0.025%
86	14.128	2136	2139	2142	rBV2	753	1164	0.28%	0.036%
87	14.323	2169	2171	2173	rVB	339	238	0.06%	0.007%
88	14.426	2185	2188	2189	rBV2	240	293	0.07%	0.009%
89	14.603	2214	2217	2219	rVB3	394	338	0.08%	0.010%
90	14.621	2219	2220	2222	rBV	358	281	0.07%	0.009%
91	14.743	2238	2240	2242	rBV2	252	272	0.07%	0.008%
92	14.817	2250	2252	2254	rBV2	330	431	0.11%	0.013%
93	14.878	2260	2262	2265	rBV	303	373	0.09%	0.011%
94	14.975	2276	2278	2280	rBV	318	319	0.08%	0.010%
95	15.066	2291	2293	2295	rBV2	300	318	0.08%	0.010%
96	15.950	2435	2438	2440	rBV	387	428	0.10%	0.013%
97	16.182	2474	2476	2477	rBV	421	278	0.07%	0.009%
98	16.432	2513	2517	2519	rBV	344	486	0.12%	0.015%
99	16.530	2532	2533	2537	rVB	359	345	0.08%	0.011%
100	16.597	2542	2544	2547	rVB2	429	418	0.10%	0.013%




Sum of corrected areas: 3265355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025626.D
Acq On : 08 Dec 2021 17:56
Operator : JC/MD
Sample : VX1208MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

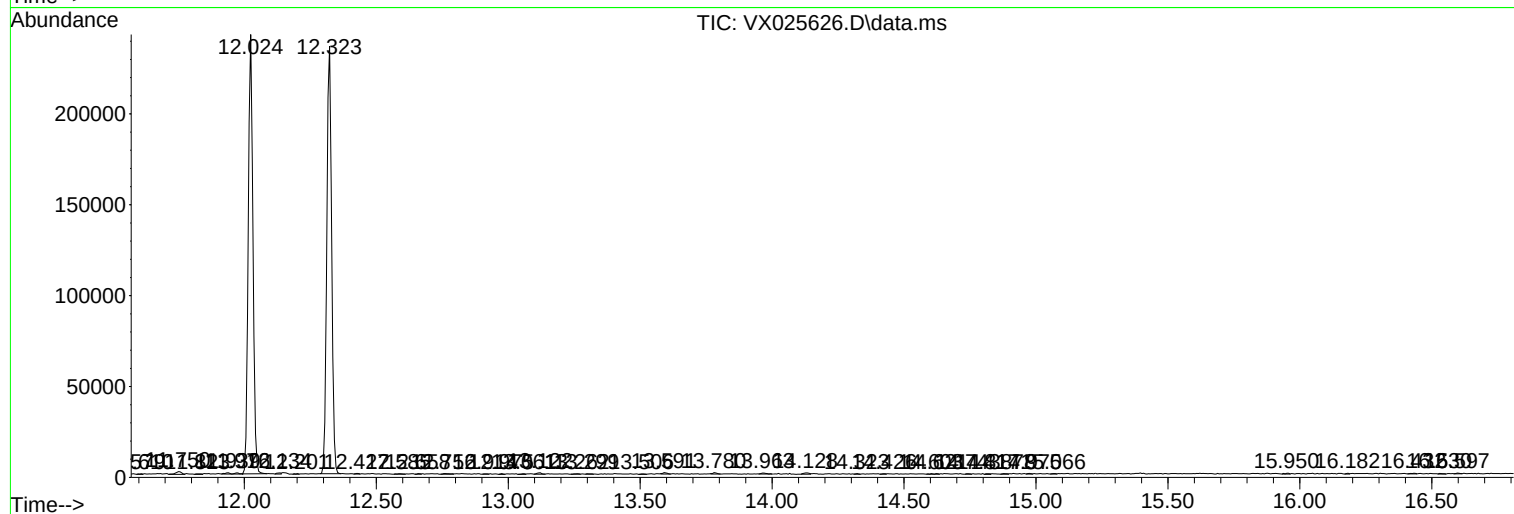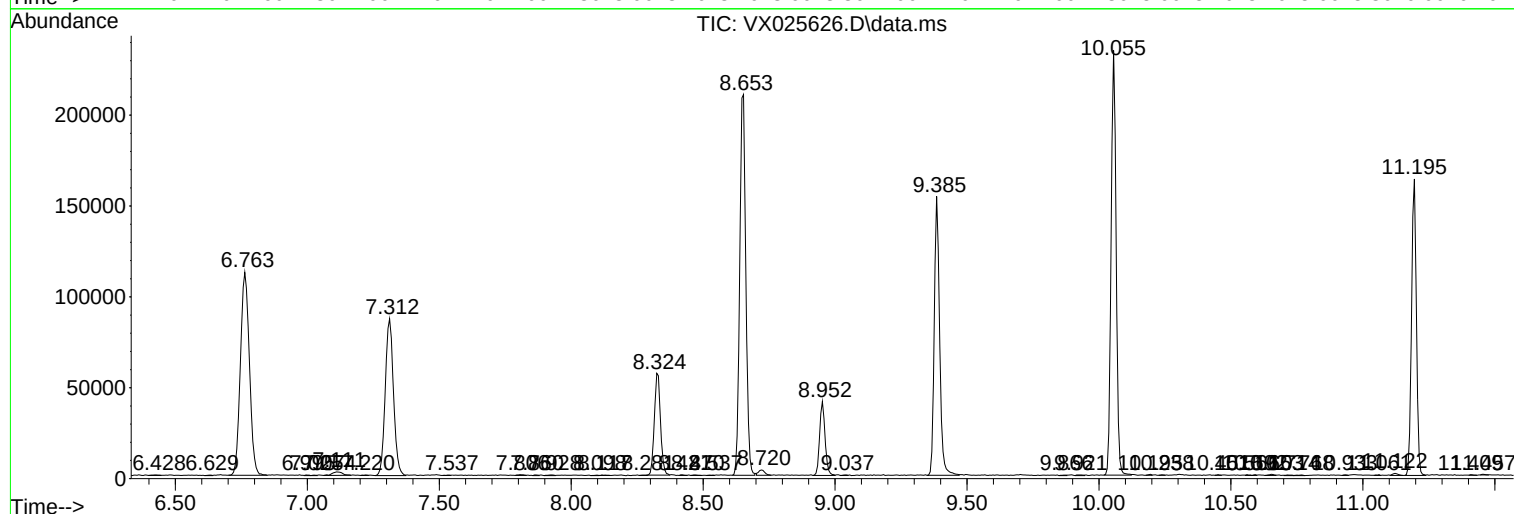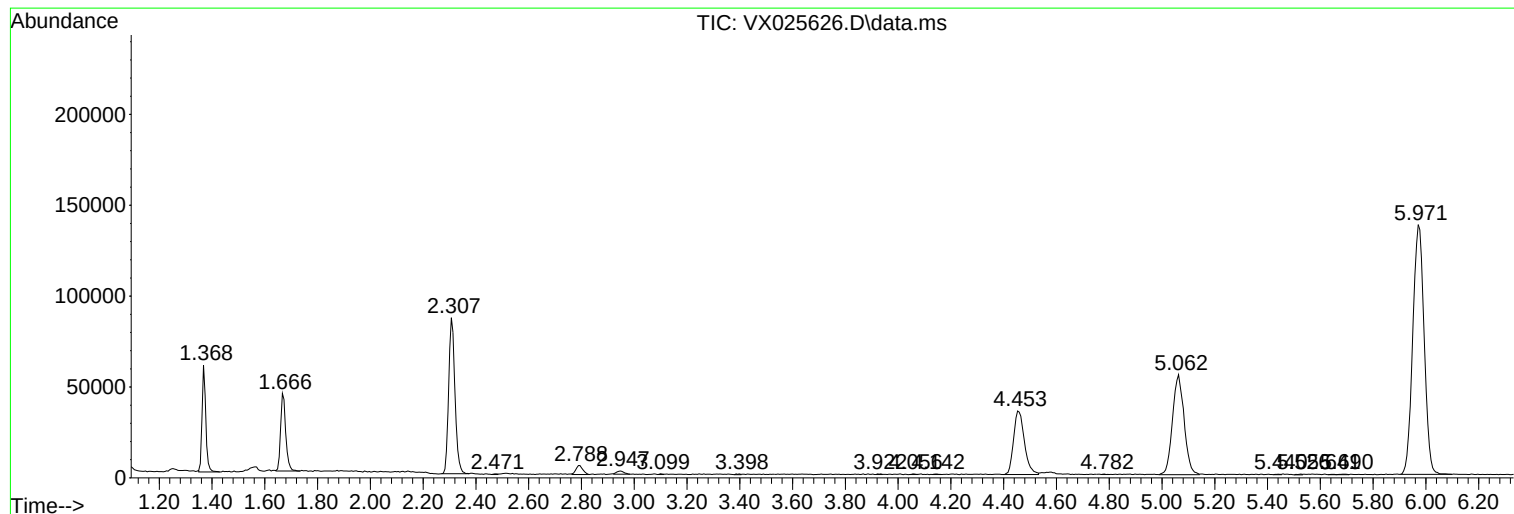

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025626.D
Acq On : 08 Dec 2021 17:56
Operator : JC/MD
Sample : VX1208MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025626.D
Acq On : 08 Dec 2021 17:56
Operator : JC/MD
Sample : VX1208MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc