

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025643.D
 Acq On : 09 Dec 2021 00:32
 Operator : JC/MD
 Sample : M4975-08
 Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV2	3928	7056	0.15%	0.063%
2	1.368	43	46	54	rVB	56889	64217	1.33%	0.572%
3	1.648	88	92	99	rBV	34045	39714	0.82%	0.354%
4	2.282	190	196	207	rBV2	121485	246340	5.09%	2.193%
5	2.947	297	305	316	rBV2	6996	20527	0.42%	0.183%
6	3.489	393	394	398	rVB2	442	330	0.01%	0.003%
7	3.605	403	413	431	rVV	350707	857844	17.71%	7.637%
8	3.800	444	445	448	rBV2	246	229	0.00%	0.002%
9	4.282	522	524	527	rBV	369	338	0.01%	0.003%
10	4.349	532	535	538	rBV	466	572	0.01%	0.005%
11	4.495	549	559	587	rBV2	22889	108507	2.24%	0.966%
12	5.068	641	653	674	rVB	56585	192335	3.97%	1.712%
13	5.245	681	682	684	rBV	444	397	0.01%	0.004%
14	5.385	694	705	718	rVB4	14183	44950	0.93%	0.400%
15	5.532	727	729	731	rBV2	393	306	0.01%	0.003%
16	5.751	763	765	766	rBV	366	241	0.00%	0.002%
17	5.879	784	786	788	rBB	369	206	0.00%	0.002%
18	5.971	788	801	818	rBV2	165634	485414	10.02%	4.321%
19	6.153	830	831	835	rVB2	382	266	0.01%	0.002%
20	6.288	852	853	856	rBV	227	198	0.00%	0.002%
21	6.367	860	866	880	rVB7	1970	6573	0.14%	0.059%
22	6.769	920	932	948	rBV	125037	334759	6.91%	2.980%
23	6.964	962	964	967	rVB3	322	286	0.01%	0.003%
24	7.129	979	991	1013	rBV	2137037	4842540	100.00%	43.111%
25	7.312	1014	1021	1038	rVB	90722	220292	4.55%	1.961%
26	7.440	1040	1042	1046	rVB2	314	362	0.01%	0.003%
27	7.489	1048	1050	1051	rBV2	290	217	0.00%	0.002%
28	7.623	1070	1072	1073	rBV	412	229	0.00%	0.002%
29	7.909	1116	1119	1122	rBV	304	459	0.01%	0.004%
30	7.952	1122	1126	1127	rBV2	297	459	0.01%	0.004%
31	8.330	1182	1188	1201	rBV	55047	103266	2.13%	0.919%
32	8.482	1211	1213	1216	rBV	437	504	0.01%	0.004%
33	8.653	1234	1241	1247	rBV	234090	392916	8.11%	3.498%
34	8.720	1247	1252	1269	rVB	102518	169227	3.49%	1.507%
35	8.958	1285	1291	1301	rBV	36998	65938	1.36%	0.587%
36	9.116	1316	1317	1320	rVB	410	243	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025643.D
 Acq On : 09 Dec 2021 00:32
 Operator : JC/MD
 Sample : M4975-08
 Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	9.141	1320	1321	1323	rBV	488	397	0.01%	0.004%
38	9.196	1328	1330	1331	rVB	460	251	0.01%	0.002%
39	9.214	1331	1333	1336	rBV	603	730	0.02%	0.006%
40	9.275	1336	1343	1354	rBV	935416	1404256	29.00%	12.501%
41	9.403	1357	1364	1375	rVV	127966	216325	4.47%	1.926%
42	9.714	1411	1415	1425	rVB3	1143	2322	0.05%	0.021%
43	9.823	1431	1433	1434	rVB	371	206	0.00%	0.002%
44	9.909	1444	1447	1448	rBV3	398	357	0.01%	0.003%
45	9.952	1453	1454	1455	rVV	470	241	0.00%	0.002%
46	9.994	1459	1461	1463	rVV	514	444	0.01%	0.004%
47	10.061	1466	1472	1485	rVB	255607	389649	8.05%	3.469%
48	10.305	1508	1512	1518	rVB2	2033	2898	0.06%	0.026%
49	10.561	1551	1554	1556	rBV	300	337	0.01%	0.003%
50	10.647	1565	1568	1571	rVB2	855	1094	0.02%	0.010%
51	10.701	1575	1577	1578	rBV	368	302	0.01%	0.003%
52	10.854	1600	1602	1605	rVB	282	226	0.00%	0.002%
53	10.915	1608	1612	1615	rBV2	377	549	0.01%	0.005%
54	10.994	1622	1625	1628	rBV2	482	573	0.01%	0.005%
55	11.098	1638	1642	1649	rVB5	3051	5215	0.11%	0.046%
56	11.153	1649	1651	1653	rVB2	264	198	0.00%	0.002%
57	11.201	1653	1659	1665	rBV	169429	228225	4.71%	2.032%
58	11.372	1685	1687	1690	rBV3	336	396	0.01%	0.004%
59	11.457	1699	1701	1702	rBV	273	280	0.01%	0.002%
60	11.476	1702	1704	1705	rVV2	469	330	0.01%	0.003%
61	11.543	1712	1715	1716	rBV2	303	314	0.01%	0.003%
62	11.659	1733	1734	1736	rBV	222	215	0.00%	0.002%
63	11.756	1741	1750	1754	rVB3	1506	2890	0.06%	0.026%
64	11.805	1754	1758	1762	rBV2	457	790	0.02%	0.007%
65	11.835	1762	1763	1764	rBV	374	211	0.00%	0.002%
66	11.933	1777	1779	1785	rBV2	972	1152	0.02%	0.010%
67	12.024	1789	1794	1800	rBV	312178	390787	8.07%	3.479%
68	12.152	1813	1815	1818	rVB2	1072	990	0.02%	0.009%
69	12.323	1838	1843	1851	rVB	286304	360263	7.44%	3.207%
70	12.421	1856	1859	1864	rVB3	981	1392	0.03%	0.012%
71	12.561	1880	1882	1886	rBV2	280	282	0.01%	0.003%
72	12.731	1908	1910	1911	rBV	371	287	0.01%	0.003%
73	12.945	1943	1945	1947	rBV	294	233	0.00%	0.002%
74	13.042	1960	1961	1962	rBV	359	209	0.00%	0.002%
75	13.134	1974	1976	1977	rVB	373	204	0.00%	0.002%
76	13.177	1982	1983	1986	rVB2	438	357	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025643.D
 Acq On : 09 Dec 2021 00:32
 Operator : JC/MD
 Sample : M4975-08
 Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	13.262	1995	1997	2000	rBV4	405	353	0.01%	0.003%
78	13.353	2009	2012	2014	rBV2	235	247	0.01%	0.002%
79	13.469	2029	2031	2033	rVB	266	227	0.00%	0.002%
80	13.573	2046	2048	2053	rBV2	389	725	0.01%	0.006%
81	13.609	2053	2054	2057	rVV2	267	243	0.01%	0.002%
82	13.774	2079	2081	2083	rVB2	382	288	0.01%	0.003%
83	13.987	2114	2116	2118	rBV2	393	443	0.01%	0.004%
84	14.030	2121	2123	2124	rBV	234	231	0.00%	0.002%
85	14.128	2137	2139	2143	rVB2	561	694	0.01%	0.006%
86	14.189	2143	2149	2150	rBV2	381	746	0.02%	0.007%
87	14.463	2193	2194	2197	rBV2	272	356	0.01%	0.003%
88	14.640	2221	2223	2224	rBV	376	274	0.01%	0.002%
89	14.695	2230	2232	2233	rBV	286	292	0.01%	0.003%
90	14.756	2240	2242	2245	rVB2	348	239	0.00%	0.002%
91	14.896	2263	2265	2267	rBV	335	281	0.01%	0.003%
92	14.938	2269	2272	2274	rBV	349	426	0.01%	0.004%
93	15.804	2413	2414	2417	rBV2	249	217	0.00%	0.002%
94	16.225	2481	2483	2484	rVB2	417	236	0.00%	0.002%
95	16.310	2495	2497	2500	rBV	212	237	0.00%	0.002%
96	16.450	2518	2520	2522	rBV2	310	287	0.01%	0.003%
97	16.536	2532	2534	2536	rBV2	406	324	0.01%	0.003%
98	16.670	2554	2556	2558	rBV	377	240	0.00%	0.002%
99	16.737	2566	2567	2570	rBV2	339	333	0.01%	0.003%
100	16.767	2570	2572	2574	rBV2	355	243	0.01%	0.002%




Sum of corrected areas: 11232816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025643.D
Acq On : 09 Dec 2021 00:32
Operator : JC/MD
Sample : M4975-08
Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

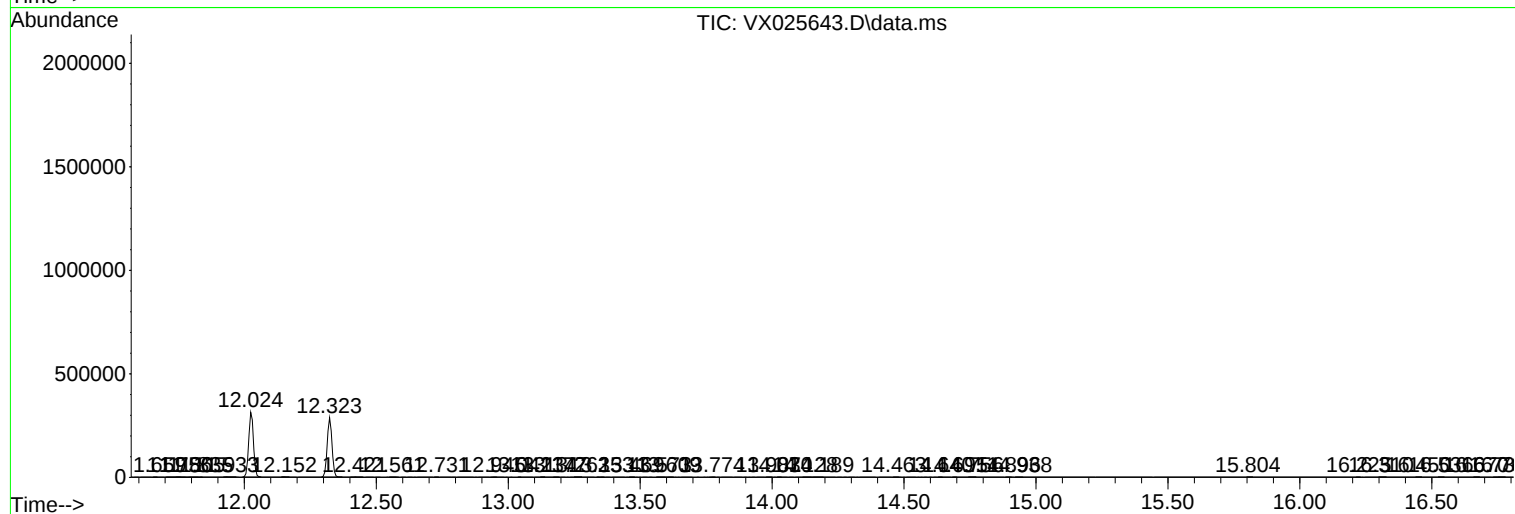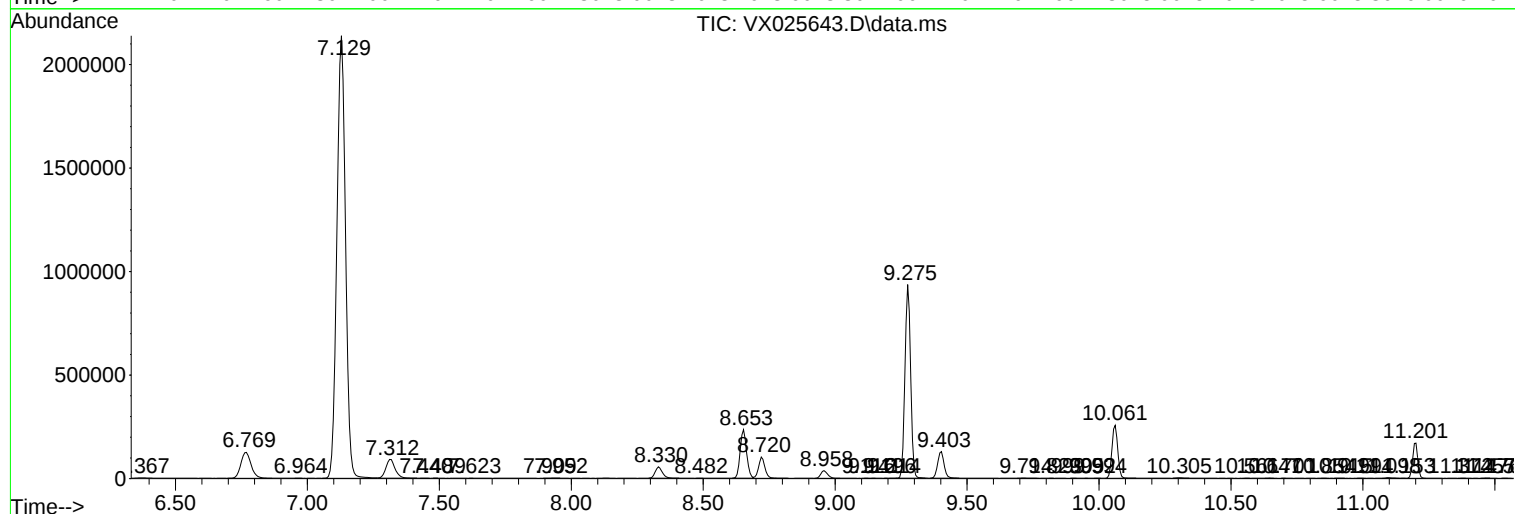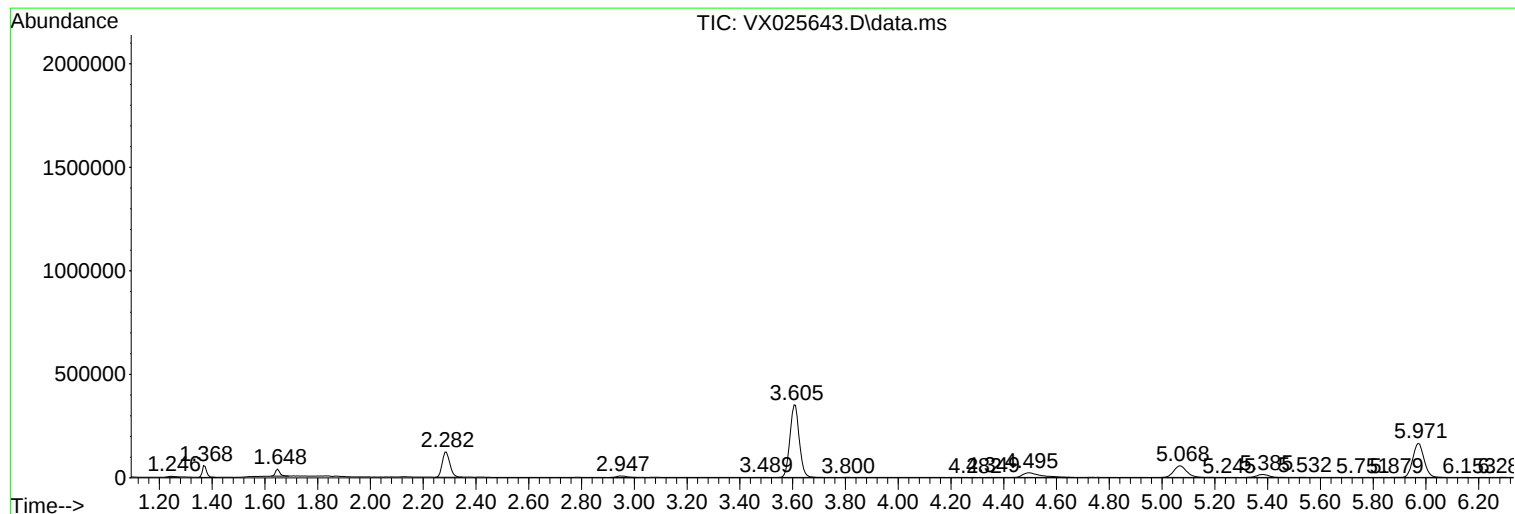

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025643.D
Acq On : 09 Dec 2021 00:32
Operator : JC/MD
Sample : M4975-08
Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025643.D
Acq On : 09 Dec 2021 00:32
Operator : JC/MD
Sample : M4975-08
Misc : 6.39g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc