

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025647.D
 Acq On : 09 Dec 2021 02:05
 Operator : JC/MD
 Sample : M4975-12
 Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV2	3948	6991	1.41%	0.178%
2	1.374	43	47	56	rVB	53585	62225	12.52%	1.583%
3	1.648	88	92	99	rBV	34436	42043	8.46%	1.069%
4	2.282	190	196	206	rBV	98628	162258	32.64%	4.127%
5	2.568	241	243	246	rBV	427	345	0.07%	0.009%
6	2.946	297	305	314	rBV2	6329	17093	3.44%	0.435%
7	3.135	335	336	339	rBV	305	283	0.06%	0.007%
8	3.160	339	340	341	rVB	541	198	0.04%	0.005%
9	3.276	357	359	360	rBV	357	201	0.04%	0.005%
10	3.440	385	386	389	rBV	303	285	0.06%	0.007%
11	3.715	429	431	434	rVB	364	273	0.05%	0.007%
12	3.745	434	436	438	rBV	318	270	0.05%	0.007%
13	3.800	444	445	447	rVB	568	231	0.05%	0.006%
14	4.099	491	494	496	rBV2	475	491	0.10%	0.012%
15	4.117	496	497	499	rBV	382	245	0.05%	0.006%
16	4.257	519	520	521	rBV	365	167	0.03%	0.004%
17	4.495	549	559	586	rBV	21604	99243	19.96%	2.524%
18	5.068	642	653	672	rVB	58226	194984	39.22%	4.960%
19	5.196	672	674	675	rBV	307	256	0.05%	0.007%
20	5.330	694	696	698	rBV	501	306	0.06%	0.008%
21	5.385	704	705	708	rBV2	239	188	0.04%	0.005%
22	5.428	711	712	714	rBV2	459	405	0.08%	0.010%
23	5.470	717	719	720	rBV2	333	209	0.04%	0.005%
24	5.745	762	764	767	rBV2	277	354	0.07%	0.009%
25	5.818	774	776	779	rBV2	273	318	0.06%	0.008%
26	5.842	779	780	783	rVV	335	312	0.06%	0.008%
27	5.970	790	801	818	rVV2	171894	497168	100.00%	12.647%
28	6.214	839	841	844	rVB	296	279	0.06%	0.007%
29	6.367	860	866	868	rBV5	2091	4457	0.90%	0.113%
30	6.488	885	886	889	rVB	344	199	0.04%	0.005%
31	6.763	922	931	945	rBV	131022	335140	67.41%	8.525%
32	6.873	947	949	951	rBV	250	225	0.05%	0.006%
33	7.123	984	990	999	rVB6	2360	6708	1.35%	0.171%
34	7.312	1013	1021	1037	rVB	95634	221656	44.58%	5.638%
35	7.415	1037	1038	1040	rVV	539	297	0.06%	0.008%
36	7.433	1040	1041	1042	rVV	335	194	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025647.D
 Acq On : 09 Dec 2021 02:05
 Operator : JC/MD
 Sample : M4975-12
 Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.476	1046	1048	1051	rVV	447	585	0.12%	0.015%
38	7.525	1054	1056	1058	rVV2	367	362	0.07%	0.009%
39	7.568	1062	1063	1065	rVB2	327	178	0.04%	0.005%
40	7.592	1065	1067	1069	rBV	299	307	0.06%	0.008%
41	7.641	1073	1075	1077	rBV	276	225	0.05%	0.006%
42	7.726	1087	1089	1090	rBV2	285	177	0.04%	0.005%
43	7.818	1103	1104	1107	rBV2	338	386	0.08%	0.010%
44	8.067	1143	1145	1147	rVB	280	223	0.04%	0.006%
45	8.330	1182	1188	1197	rBV	54893	100636	20.24%	2.560%
46	8.580	1227	1229	1230	rBV	256	221	0.04%	0.006%
47	8.653	1234	1241	1249	rVV	248040	408529	82.17%	10.392%
48	8.720	1249	1252	1257	rVB	2896	4492	0.90%	0.114%
49	8.958	1285	1291	1300	rBV	37933	63283	12.73%	1.610%
50	9.128	1314	1319	1321	rVB	326	543	0.11%	0.014%
51	9.153	1321	1323	1324	rVB	479	292	0.06%	0.007%
52	9.177	1324	1327	1329	rBV2	522	670	0.13%	0.017%
53	9.220	1332	1334	1337	rBV	315	374	0.08%	0.010%
54	9.275	1337	1343	1352	rVB	56832	83256	16.75%	2.118%
55	9.336	1352	1353	1354	rBV	249	174	0.03%	0.004%
56	9.403	1357	1364	1377	rBV	128411	218030	43.85%	5.546%
57	9.622	1399	1400	1403	rBV	324	345	0.07%	0.009%
58	9.707	1412	1414	1415	rBV	692	579	0.12%	0.015%
59	9.848	1436	1437	1440	rBV	202	162	0.03%	0.004%
60	10.061	1466	1472	1482	rVB	263082	390344	78.51%	9.929%
61	10.305	1508	1512	1513	rBV2	374	405	0.08%	0.010%
62	10.390	1525	1526	1529	rBV	291	214	0.04%	0.005%
63	10.439	1531	1534	1535	rBV2	368	453	0.09%	0.012%
64	10.500	1543	1544	1547	rBV	283	213	0.04%	0.005%
65	10.695	1575	1576	1578	rVB	408	232	0.05%	0.006%
66	10.872	1603	1605	1606	rBV	360	272	0.05%	0.007%
67	11.067	1635	1637	1641	rBV	275	300	0.06%	0.008%
68	11.122	1643	1646	1650	rVV2	1280	1480	0.30%	0.038%
69	11.195	1653	1658	1667	rVV	178553	232926	46.85%	5.925%
70	11.451	1699	1700	1703	rBV	346	365	0.07%	0.009%
71	11.750	1746	1749	1753	rBV4	1072	1321	0.27%	0.034%
72	11.878	1769	1770	1772	rVB	384	163	0.03%	0.004%
73	11.908	1773	1775	1777	rVV	395	264	0.05%	0.007%
74	11.939	1777	1780	1783	rVB3	567	642	0.13%	0.016%
75	12.024	1789	1794	1802	rBV	316554	388203	78.08%	9.875%
76	12.225	1825	1827	1829	rBV	342	203	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025647.D
 Acq On : 09 Dec 2021 02:05
 Operator : JC/MD
 Sample : M4975-12
 Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.323	1838	1843	1851	rVB	293642	365339	73.48%	9.293%
78	12.457	1863	1865	1868	rBV2	257	260	0.05%	0.007%
79	12.646	1894	1896	1899	rBV	317	272	0.05%	0.007%
80	12.725	1906	1909	1910	rBV2	507	552	0.11%	0.014%
81	12.756	1913	1914	1915	rVV	475	227	0.05%	0.006%
82	12.792	1919	1920	1922	rBV	349	249	0.05%	0.006%
83	12.890	1934	1936	1938	rBV	280	229	0.05%	0.006%
84	12.908	1938	1939	1941	rVB	354	231	0.05%	0.006%
85	12.987	1949	1952	1957	rBV2	315	542	0.11%	0.014%
86	13.060	1962	1964	1965	rBV2	314	219	0.04%	0.006%
87	13.091	1967	1969	1970	rBV2	276	179	0.04%	0.005%
88	13.140	1975	1977	1980	rVB	350	380	0.08%	0.010%
89	13.188	1983	1985	1987	rBV	269	229	0.05%	0.006%
90	13.347	2008	2011	2013	rBV	244	297	0.06%	0.008%
91	13.451	2026	2028	2029	rBV	455	277	0.06%	0.007%
92	13.646	2058	2060	2064	rVB	495	698	0.14%	0.018%
93	13.676	2064	2065	2067	rBV	221	230	0.05%	0.006%
94	14.341	2172	2174	2175	rBV	419	342	0.07%	0.009%
95	15.103	2298	2299	2301	rBV	396	241	0.05%	0.006%
96	15.615	2380	2383	2386	rBV2	433	491	0.10%	0.012%
97	15.682	2392	2394	2395	rBV	417	278	0.06%	0.007%
98	16.286	2492	2493	2496	rVB	534	297	0.06%	0.008%
99	16.462	2520	2522	2523	rBV	358	217	0.04%	0.006%
100	16.670	2554	2556	2558	rBV2	427	424	0.09%	0.011%




Sum of corrected areas: 3931226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025647.D
Acq On : 09 Dec 2021 02:05
Operator : JC/MD
Sample : M4975-12
Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

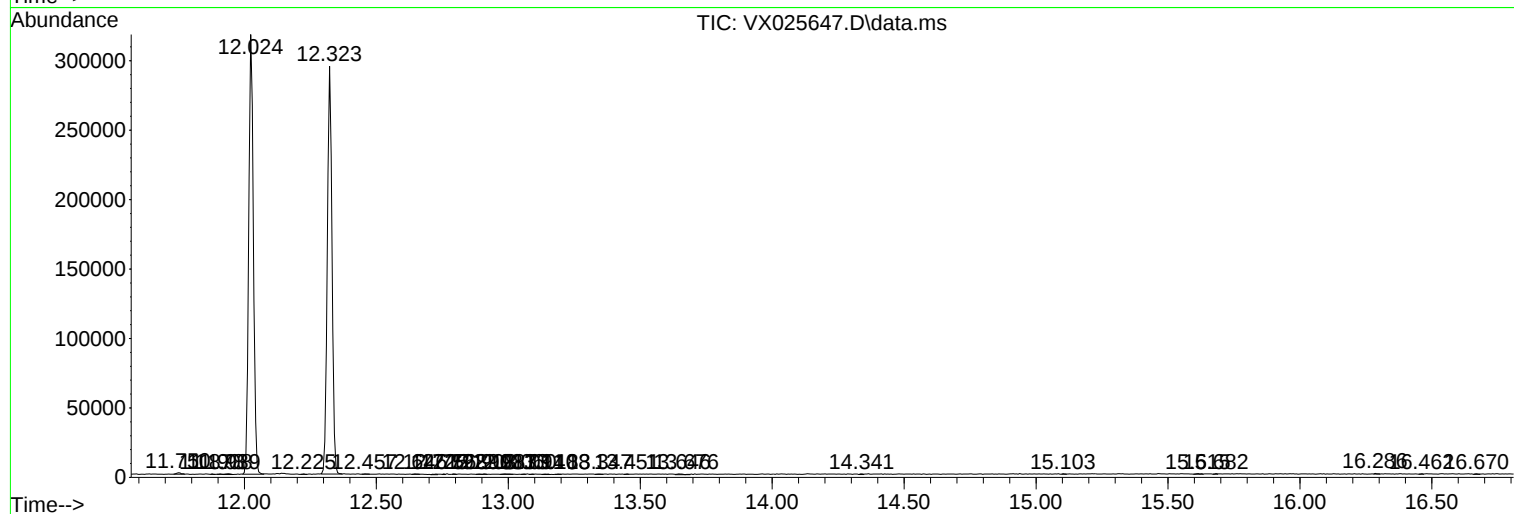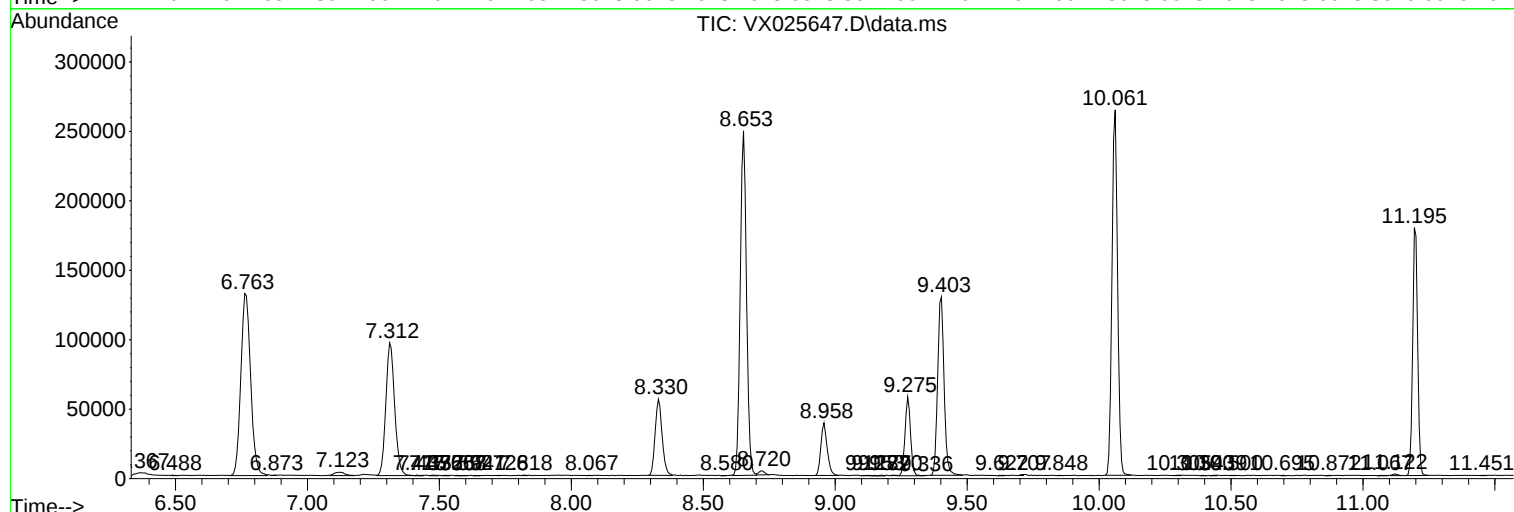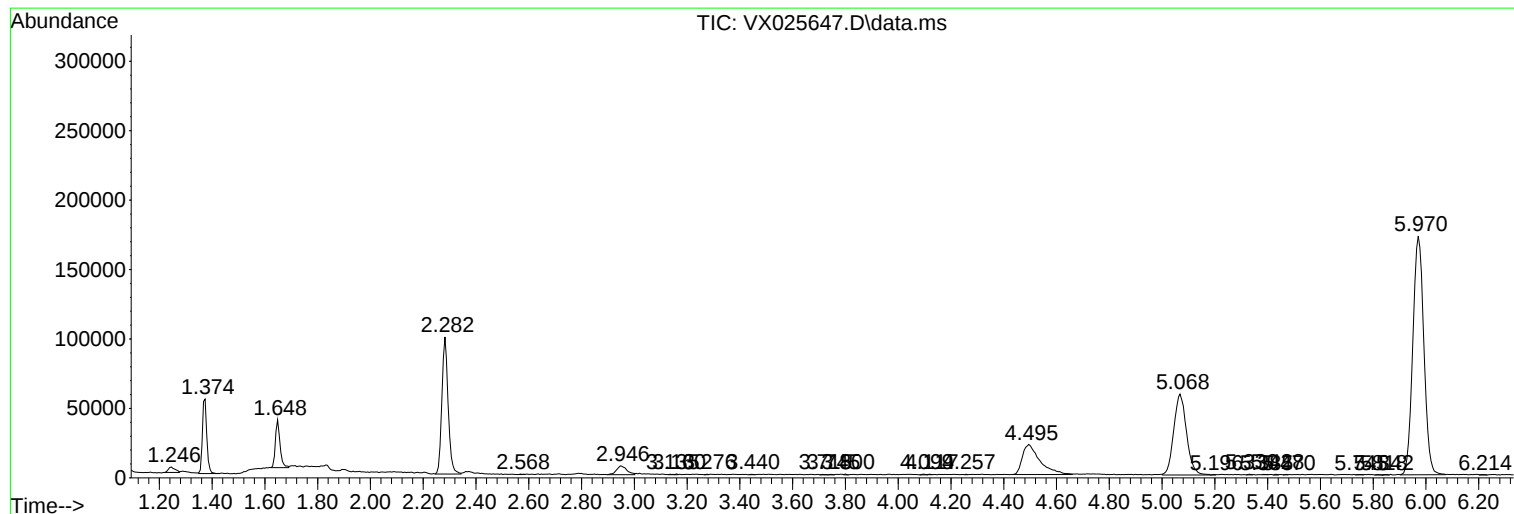

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025647.D
Acq On : 09 Dec 2021 02:05
Operator : JC/MD
Sample : M4975-12
Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025647.D
Acq On : 09 Dec 2021 02:05
Operator : JC/MD
Sample : M4975-12
Misc : 5.53g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc