

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
 Data File : VX033324.D
 Acq On : 08 Dec 2022 15:28
 Operator : JC/MD
 Sample : N5906-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB120522

Quant Time: Dec 09 00:48:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 07 12:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	146632	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	232083	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203976	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	92134	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	45835	48.725	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.440%
35) Dibromofluoromethane	5.391	113	49041	46.980	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.960%
50) Toluene-d8	8.647	98	105588	48.353	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.700%
62) 4-Bromofluorobenzene	11.079	95	80294	48.089	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.180%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
Data File : VX033324.D
Acq On : 08 Dec 2022 15:28
Operator : JC/MD
Sample : N5906-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB120522

Quant Time: Dec 09 00:48:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 07 12:43:54 2022
Response via : Initial Calibration




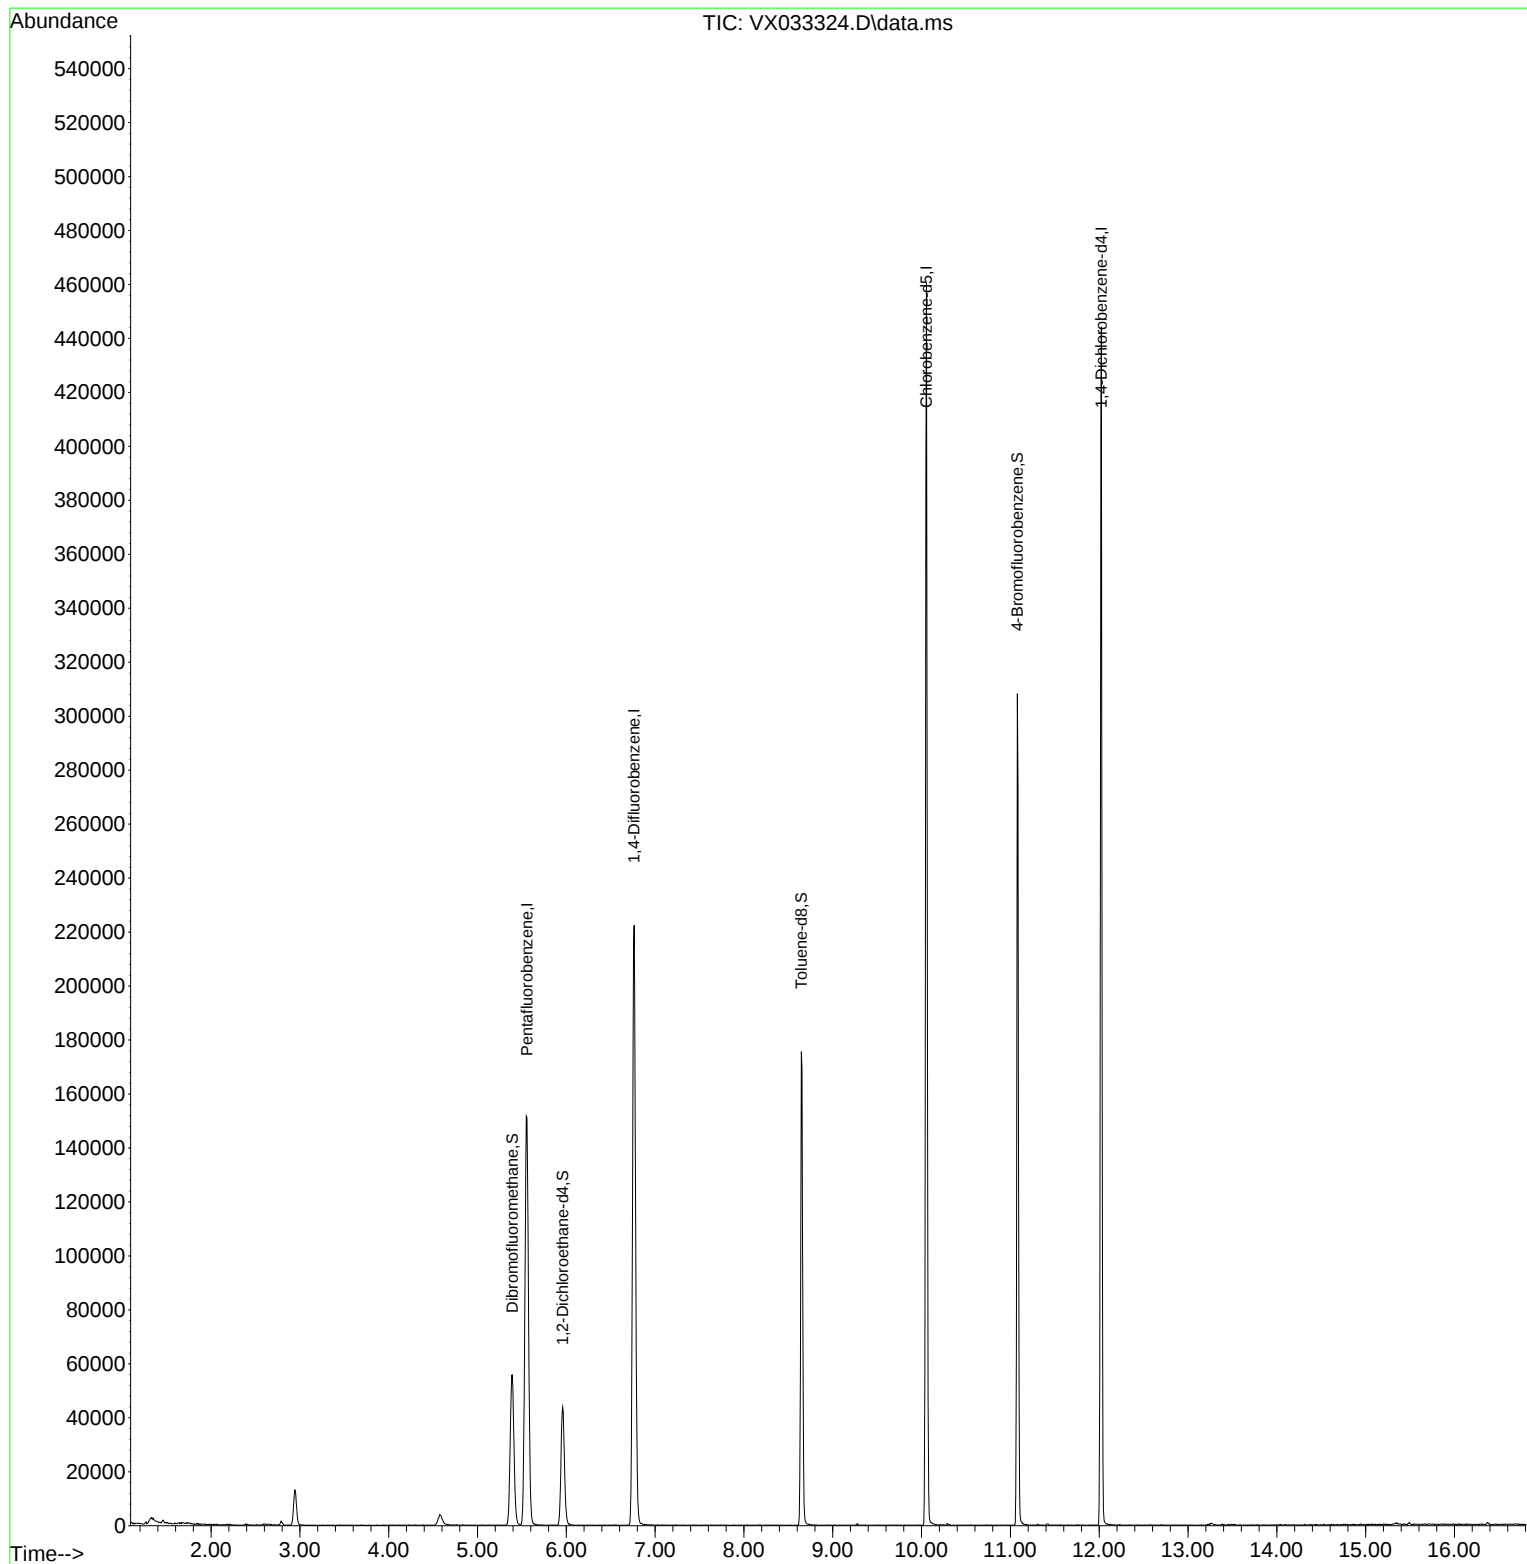




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28




Instrument :
MSVOA_X
ClientSampleId :
FB120522


Tgt Ion:168 Resp: 146632
Ion Ratio Lower Upper
168 100
99 56.7 46.1 69.1

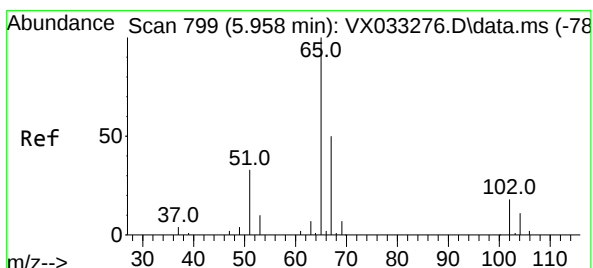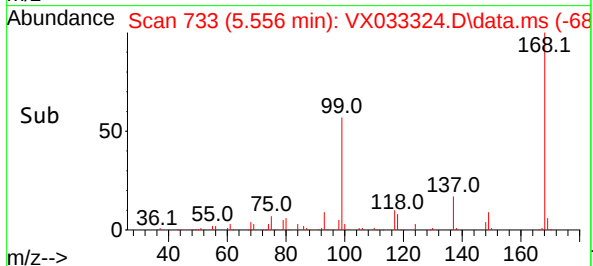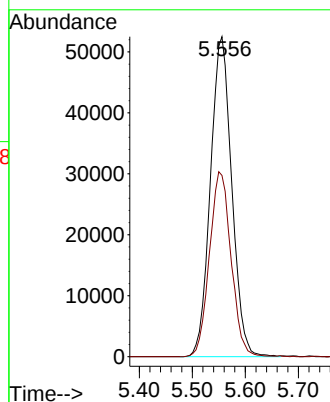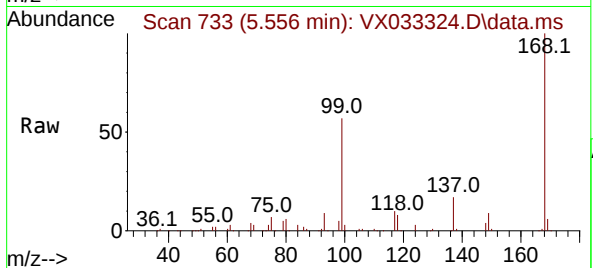

#33
1,2-Dichloroethane-d4
Concen: 48.725 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28

Tgt Ion: 65 Resp: 45835
Ion Ratio Lower Upper
65 100
67 51.4 0.0 101.8


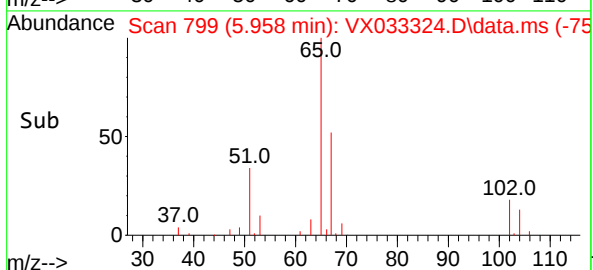
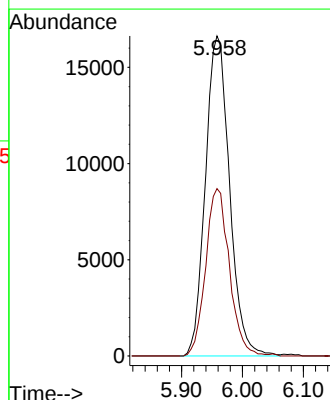
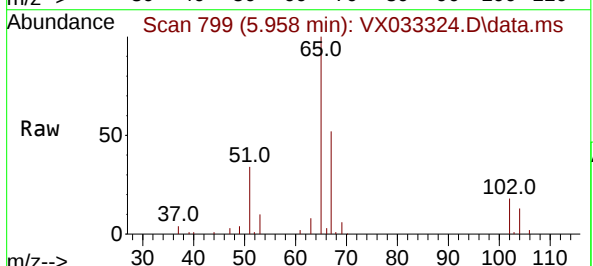


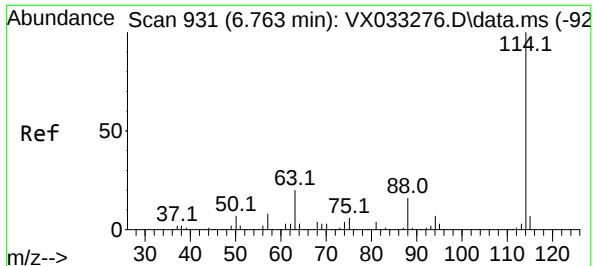

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28




Instrument :
MSVOA_X
ClientSampleId :
FB120522


Tgt Ion:114 Resp: 232083
Ion Ratio Lower Upper
114 100
63 19.7 0.0 41.6
88 15.5 0.0 33.4

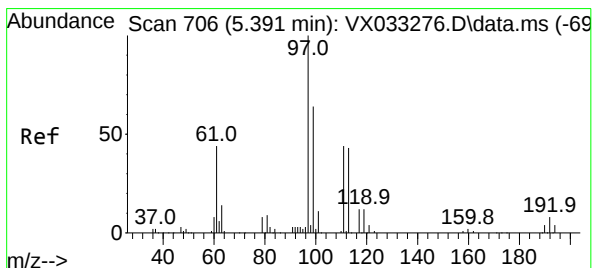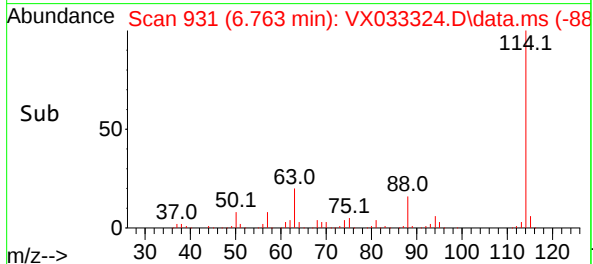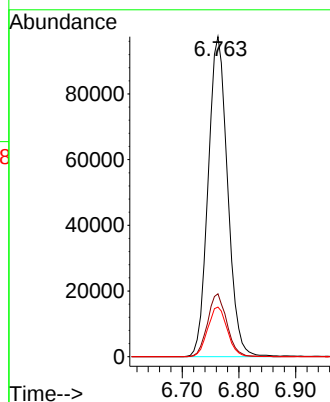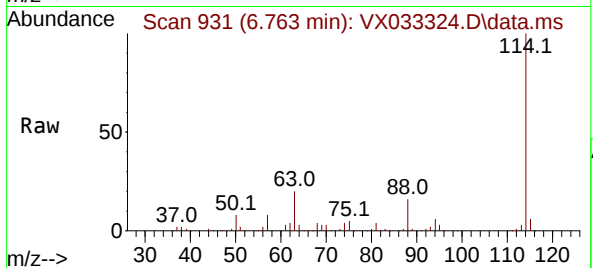

#35
Dibromofluoromethane
Concen: 46.980 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28

Tgt Ion:113 Resp: 49041
Ion Ratio Lower Upper
113 100
111 104.6 82.4 123.6
192 19.6 15.4 23.2

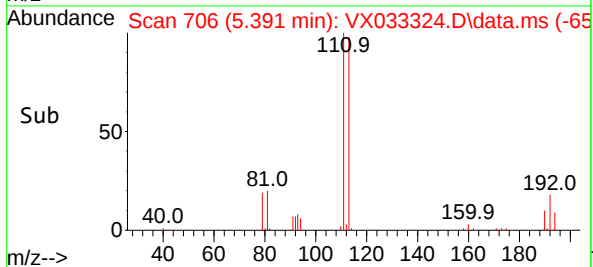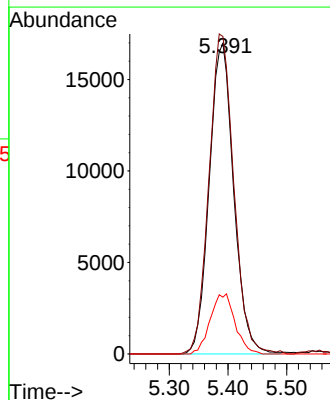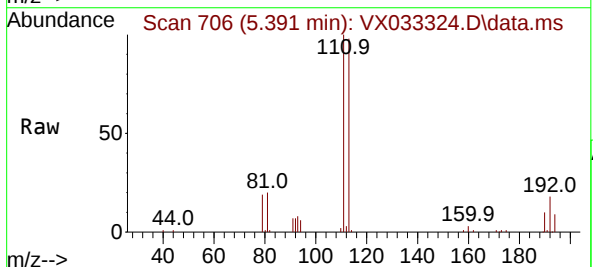

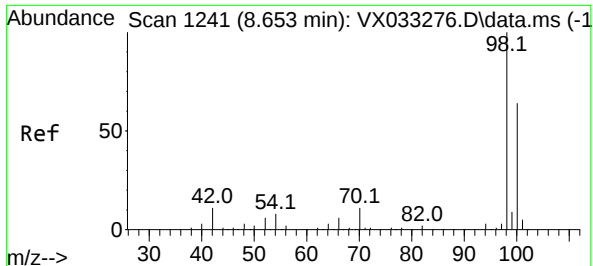

#50

Toluene-d8

Concen: 48.353 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX033324.D

Acq: 08 Dec 2022 15:28

Instrument :

MSVOA_X

ClientSampleId :





FB120522

Tgt Ion: 98 Resp: 105588

Ion Ratio Lower Upper

98 100

100 64.8 50.9 76.3

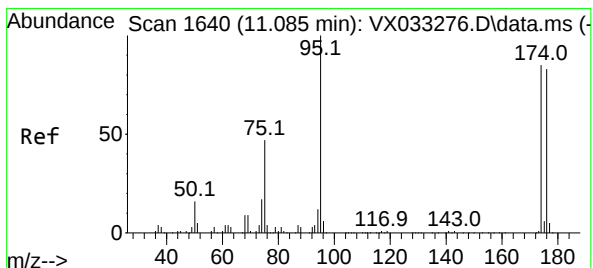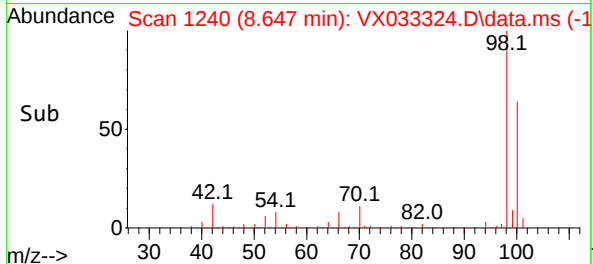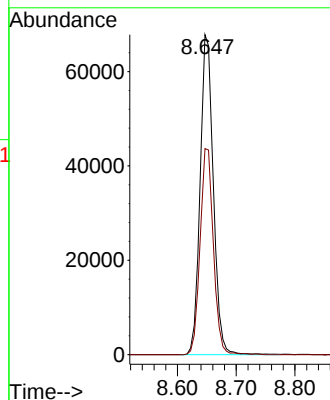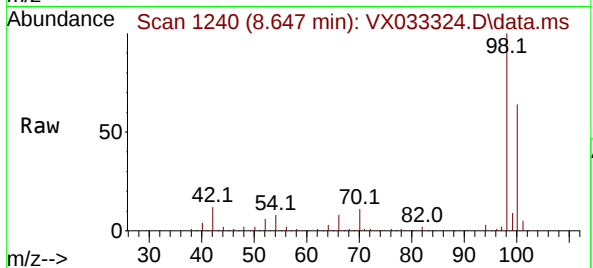

#62

4-Bromofluorobenzene

Concen: 48.089 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX033324.D

Acq: 08 Dec 2022 15:28




Tgt Ion: 95 Resp: 80294


Ion Ratio Lower Upper

95 100

174 81.3 0.0 164.0

176 78.6 0.0 154.4


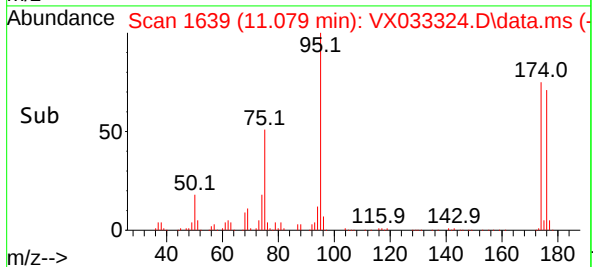
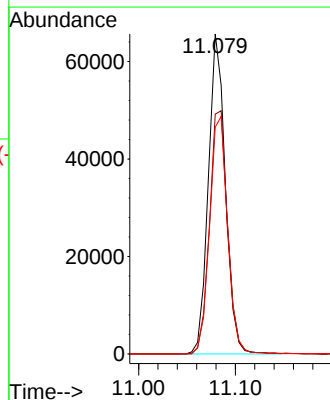
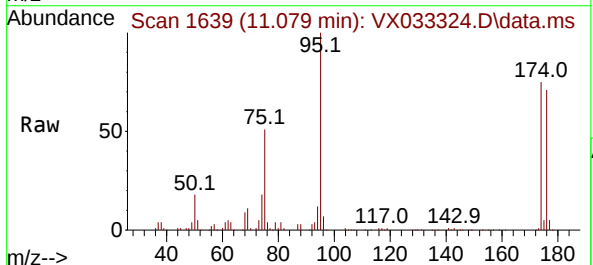


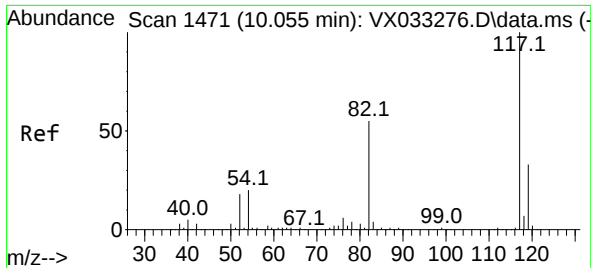

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28

Instrument :
MSVOA_X
ClientSampleId :
FB120522

Tgt Ion:117 Resp: 203976
Ion Ratio Lower Upper
117 100
82 53.6 44.3 66.5
119 32.1 25.7 38.5

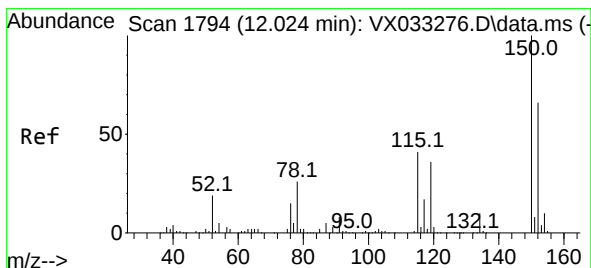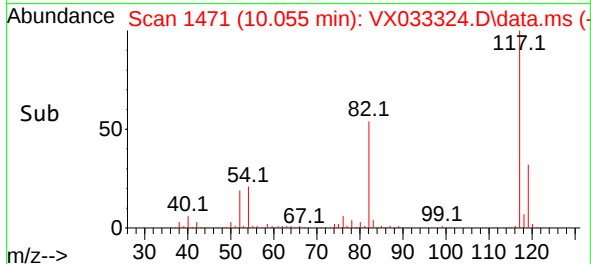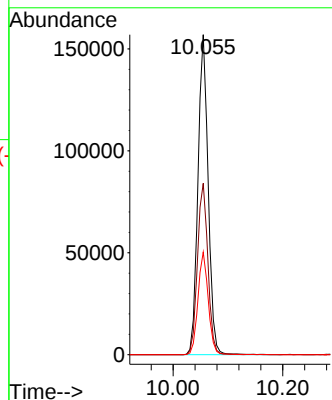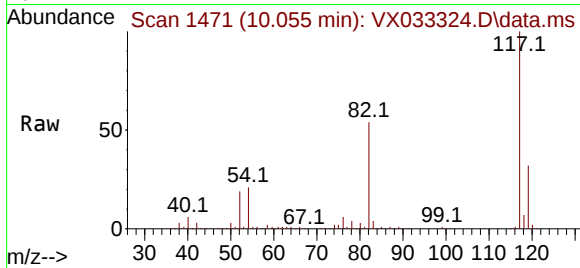

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033324.D
Acq: 08 Dec 2022 15:28

Tgt Ion:152 Resp: 92134
Ion Ratio Lower Upper
152 100
115 59.9 44.0 132.0
150 157.1 0.0 351.8

