

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120822\  
Data File : VX033327.D  
Acq On : 08 Dec 2022 16:41  
Operator : JC/MD  
Sample : N5890-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1827

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033327.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 719          | rBV      | 51602          | 150742        | 5.97%           | 2.709%        |
| 2         | 5.550       | 721           | 732         | 750          | rVV      | 151324         | 425818        | 16.86%          | 7.653%        |
| 3         | 5.952       | 787           | 798         | 815          | rBV      | 42140          | 110446        | 4.37%           | 1.985%        |
| 4         | 6.763       | 920           | 931         | 950          | rBV      | 218702         | 523088        | 20.71%          | 9.401%        |
| 5         | 8.647       | 1234          | 1240        | 1246         | rBV      | 160812         | 253374        | 10.03%          | 4.554%        |
| 6         | 8.720       | 1246          | 1252        | 1265         | rVB      | 1648004        | 2525953       | 100.00%         | 45.399%       |
| 7         | 9.275       | 1338          | 1343        | 1350         | rVB      | 28314          | 42356         | 1.68%           | 0.761%        |
| 8         | 10.055      | 1465          | 1471        | 1482         | rBV      | 450127         | 601738        | 23.82%          | 10.815%       |
| 9         | 11.079      | 1634          | 1639        | 1651         | rBV      | 291121         | 366760        | 14.52%          | 6.592%        |
| 10        | 12.024      | 1788          | 1794        | 1803         | rBV      | 445101         | 563647        | 22.31%          | 10.130%       |




Sum of corrected areas: 5563922

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120822\  
Data File : VX033327.D  
Acq On : 08 Dec 2022 16:41  
Operator : JC/MD  
Sample : N5890-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

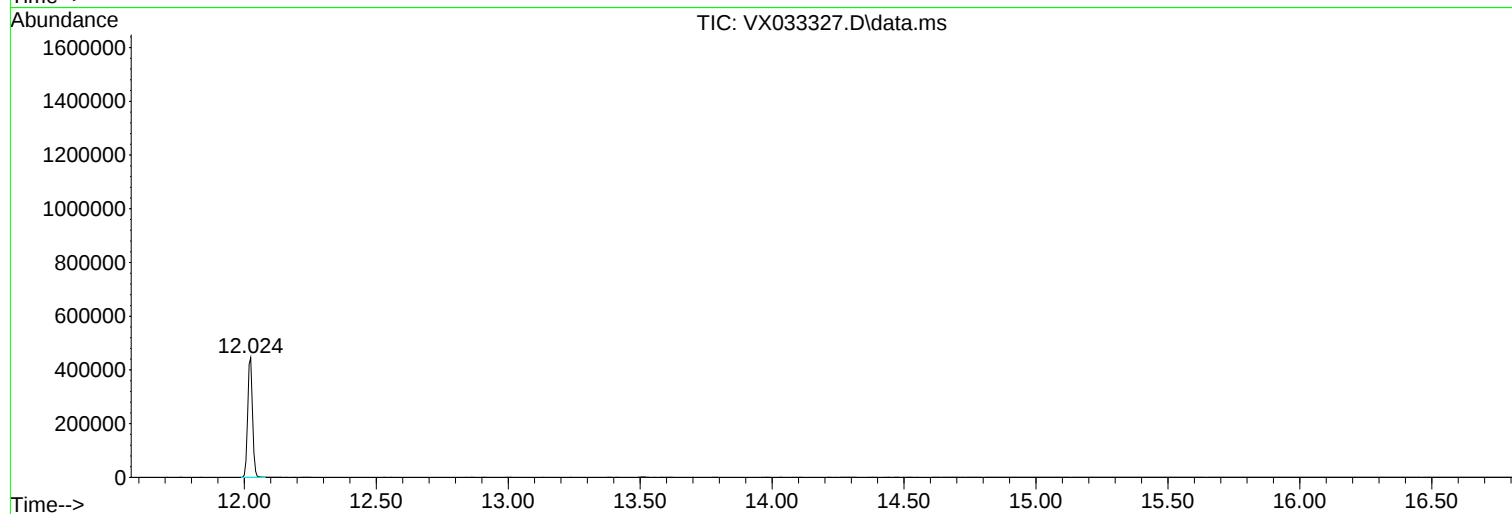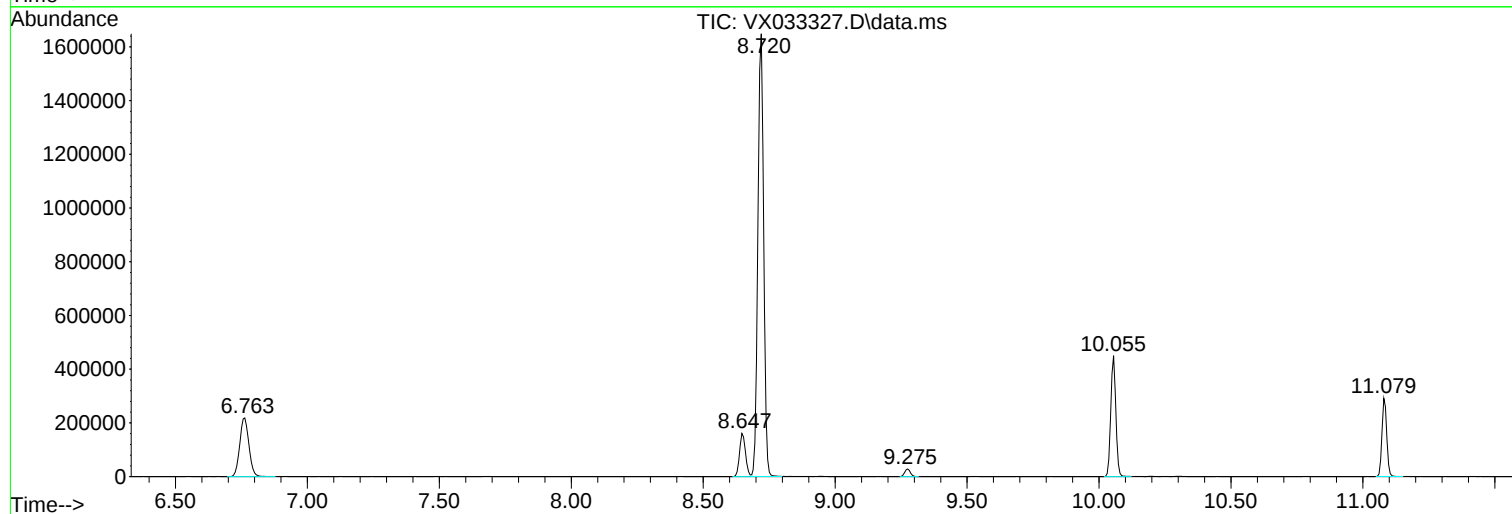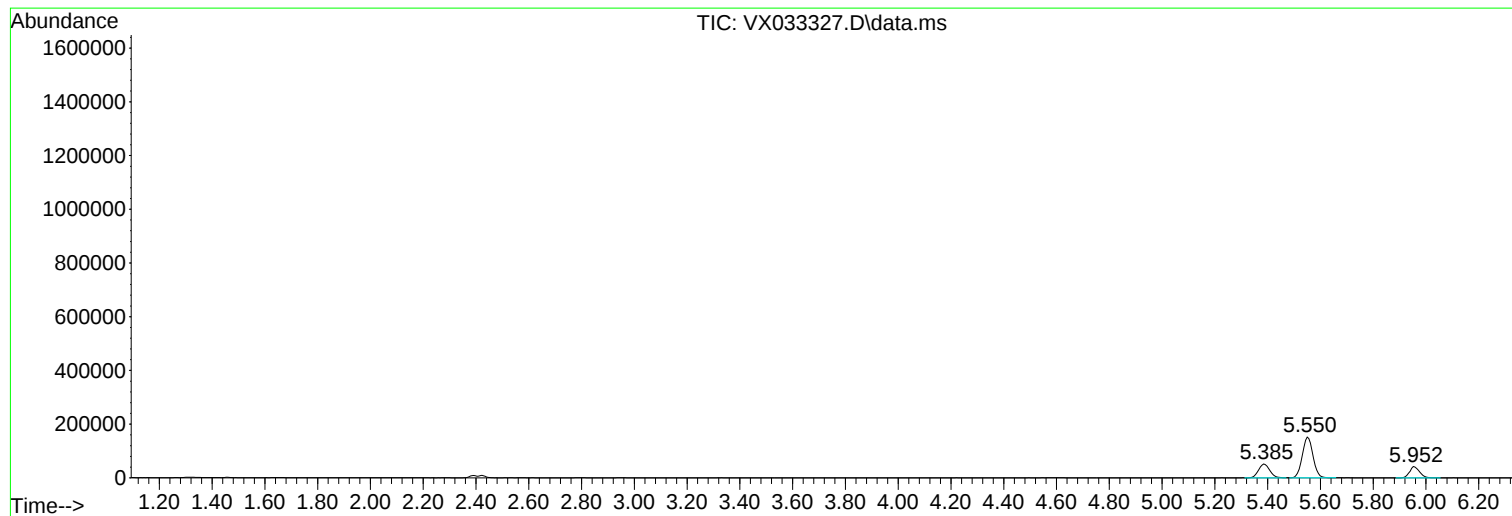

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120822\  
Data File : VX033327.D  
Acq On : 08 Dec 2022 16:41  
Operator : JC/MD  
Sample : N5890-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120822\  
Data File : VX033327.D  
Acq On : 08 Dec 2022 16:41  
Operator : JC/MD  
Sample : N5890-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1827

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|