

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
 Data File : VX033330.D
 Acq On : 08 Dec 2022 17:50
 Operator : JC/MD
 Sample : N5890-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1922

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.459	57	61	72	rVB	13573	18169	1.19%	0.093%
2	2.160	156	176	196	rBV2	29568	205084	13.39%	1.049%
3	2.392	206	214	230	rVB	41991	89055	5.81%	0.456%
4	2.599	237	248	261	rBV2	5797	29790	1.94%	0.152%
5	4.568	563	571	586	rBV	6456	20075	1.31%	0.103%
6	5.385	694	705	721	rBV	55211	163766	10.69%	0.838%
7	5.550	721	732	749	rVB	157976	449453	29.34%	2.299%
8	5.958	789	799	809	rBV2	44583	117646	7.68%	0.602%
9	6.763	921	931	945	rBV	235226	557101	36.37%	2.850%
10	8.647	1234	1240	1247	rVV	173740	276926	18.08%	1.417%
11	8.720	1247	1252	1263	rVB	124006	189678	12.38%	0.970%
12	9.518	1377	1383	1389	rBV	24773	38638	2.52%	0.198%
13	10.055	1465	1471	1479	rBV	487094	641304	41.87%	3.281%
14	10.195	1488	1494	1500	rBV	170356	217502	14.20%	1.113%
15	10.299	1504	1511	1519	rVV	608502	798008	52.10%	4.082%
16	10.640	1562	1567	1578	rVB	438844	545858	35.64%	2.792%
17	10.768	1583	1588	1598	rBV	17532	24349	1.59%	0.125%
18	10.963	1615	1620	1625	rBV	43938	53300	3.48%	0.273%
19	11.079	1634	1639	1645	rBV	324957	402054	26.25%	2.057%
20	11.305	1666	1676	1683	rBV	123630	149146	9.74%	0.763%
21	11.378	1683	1688	1696	rVV	598618	959930	62.67%	4.910%
22	11.451	1696	1700	1713	rVB	266749	325223	21.23%	1.664%
23	11.610	1721	1726	1732	rBV	322483	412034	26.90%	2.108%
24	11.750	1740	1749	1757	rBV	1279548	1531791	100.00%	7.836%
25	11.890	1769	1772	1776	rVB	30617	37288	2.43%	0.191%
26	11.969	1781	1785	1788	rBV	64909	75830	4.95%	0.388%
27	12.018	1788	1793	1799	rVV	506299	659276	43.04%	3.372%
28	12.085	1799	1804	1815	rVB	565400	681255	44.47%	3.485%
29	12.244	1822	1830	1838	rBV2	674961	1068639	69.76%	5.467%
30	12.317	1838	1842	1852	rVB3	261007	379479	24.77%	1.941%
31	12.402	1852	1856	1862	rBV	32892	42698	2.79%	0.218%
32	12.463	1862	1866	1872	rVB	98079	119967	7.83%	0.614%
33	12.530	1872	1877	1879	rBV	190232	235433	15.37%	1.204%
34	12.554	1879	1881	1885	rVB	169132	170463	11.13%	0.872%
35	12.609	1885	1890	1893	rBV	245334	302505	19.75%	1.547%
36	12.646	1893	1896	1900	rVB	101043	119159	7.78%	0.610%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
 Data File : VX033330.D
 Acq On : 08 Dec 2022 17:50
 Operator : JC/MD
 Sample : N5890-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1922

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

37	12.701	1900	1905	1913	rBV2	292062	436602	28.50%	2.233%
38	12.798	1917	1921	1924	rBV2	19023	20434	1.33%	0.105%
39	12.847	1924	1929	1934	rVB2	110733	141094	9.21%	0.722%
40	12.920	1934	1941	1944	rBV	159205	194762	12.71%	0.996%
41	12.963	1944	1948	1954	rVB	255787	315120	20.57%	1.612%
42	13.024	1954	1958	1960	rBV	30821	42814	2.80%	0.219%
43	13.140	1973	1977	1978	rBV2	30657	36168	2.36%	0.185%
44	13.170	1978	1982	1986	rVV	380161	484507	31.63%	2.478%
45	13.213	1986	1989	1992	rVB2	26934	31388	2.05%	0.161%
46	13.256	1992	1996	1997	rBV2	40266	50804	3.32%	0.260%
47	13.292	1997	2002	2008	rVV2	851949	1098946	71.74%	5.622%
48	13.371	2012	2015	2018	rVV	21017	24375	1.59%	0.125%
49	13.420	2018	2023	2032	rVB	714043	875340	57.14%	4.478%
50	13.506	2032	2037	2040	rBV2	51177	70800	4.62%	0.362%
51	13.542	2040	2043	2046	rVV	108014	141013	9.21%	0.721%
52	13.585	2046	2050	2055	rVV3	117841	213022	13.91%	1.090%
53	13.640	2056	2059	2060	rVV	65240	76722	5.01%	0.392%
54	13.664	2060	2063	2069	rVB2	124812	177787	11.61%	0.909%
55	13.774	2074	2081	2089	rVB	227186	297684	19.43%	1.523%
56	13.853	2089	2094	2099	rVB	122574	153779	10.04%	0.787%
57	13.926	2099	2106	2110	rBV2	157259	208682	13.62%	1.067%
58	13.969	2110	2113	2117	rVB	53728	62052	4.05%	0.317%
59	14.073	2126	2130	2135	rBV	102140	131262	8.57%	0.671%
60	14.231	2148	2156	2163	rBV	350274	540469	35.28%	2.765%
61	14.322	2167	2171	2175	rBV	28885	37963	2.48%	0.194%
62	14.371	2175	2179	2184	rVB	97213	116833	7.63%	0.598%
63	14.420	2184	2187	2192	rVB	11681	15705	1.03%	0.080%
64	14.481	2192	2197	2202	rBV	234715	298766	19.50%	1.528%
65	14.633	2214	2222	2226	rBV2	239354	384148	25.08%	1.965%
66	14.670	2226	2228	2233	rVB	41647	49378	3.22%	0.253%
67	14.731	2233	2238	2241	rBV3	13475	20853	1.36%	0.107%
68	14.780	2241	2246	2250	rVV	147023	186825	12.20%	0.956%
69	14.816	2250	2252	2255	rVV2	25912	35152	2.29%	0.180%
70	14.847	2255	2257	2262	rVB2	21007	23342	1.52%	0.119%
71	14.902	2262	2266	2273	rBV3	26285	47184	3.08%	0.241%
72	15.048	2283	2290	2295	rBV2	11108	19684	1.29%	0.101%
73	15.182	2307	2312	2315	rBV	53035	89324	5.83%	0.457%
74	15.377	2338	2344	2347	rBV	18344	29223	1.91%	0.149%
75	15.475	2353	2360	2365	rBV	42804	76253	4.98%	0.390%
76	15.523	2365	2368	2373	rVV2	13835	26127	1.71%	0.134%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
Data File : VX033330.D
Acq On : 08 Dec 2022 17:50
Operator : JC/MD
Sample : N5890-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1922

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Title : SW846 8260

77	15.615	2377	2383	2386	rVV	50395	86312	5.63%	0.442%
78	15.651	2386	2389	2397	rVB2	27859	43770	2.86%	0.224%
79	15.840	2409	2420	2425	rBV4	12220	28524	1.86%	0.146%




Sum of corrected areas: 19548864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
Data File : VX033330.D
Acq On : 08 Dec 2022 17:50
Operator : JC/MD
Sample : N5890-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1922

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

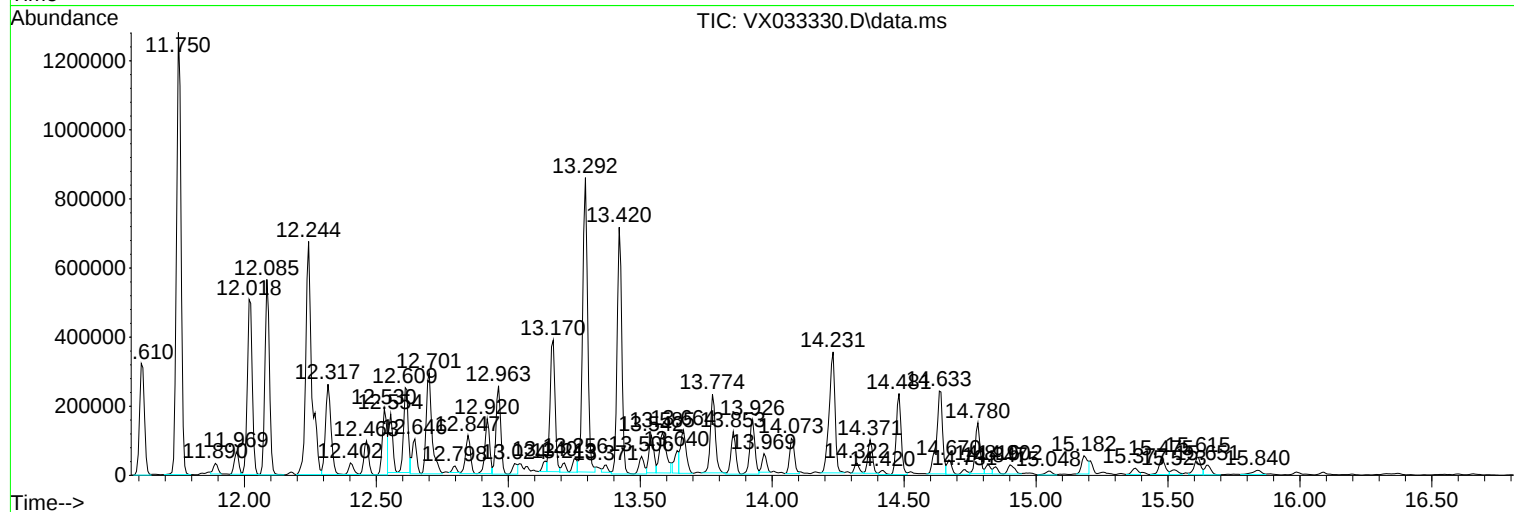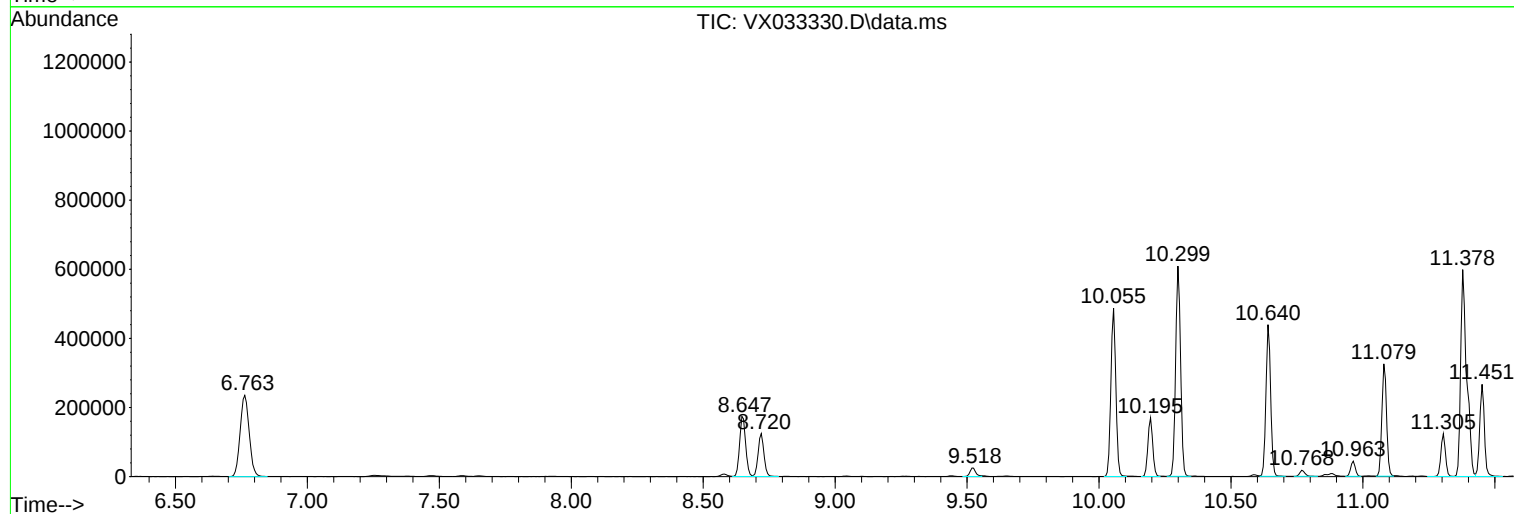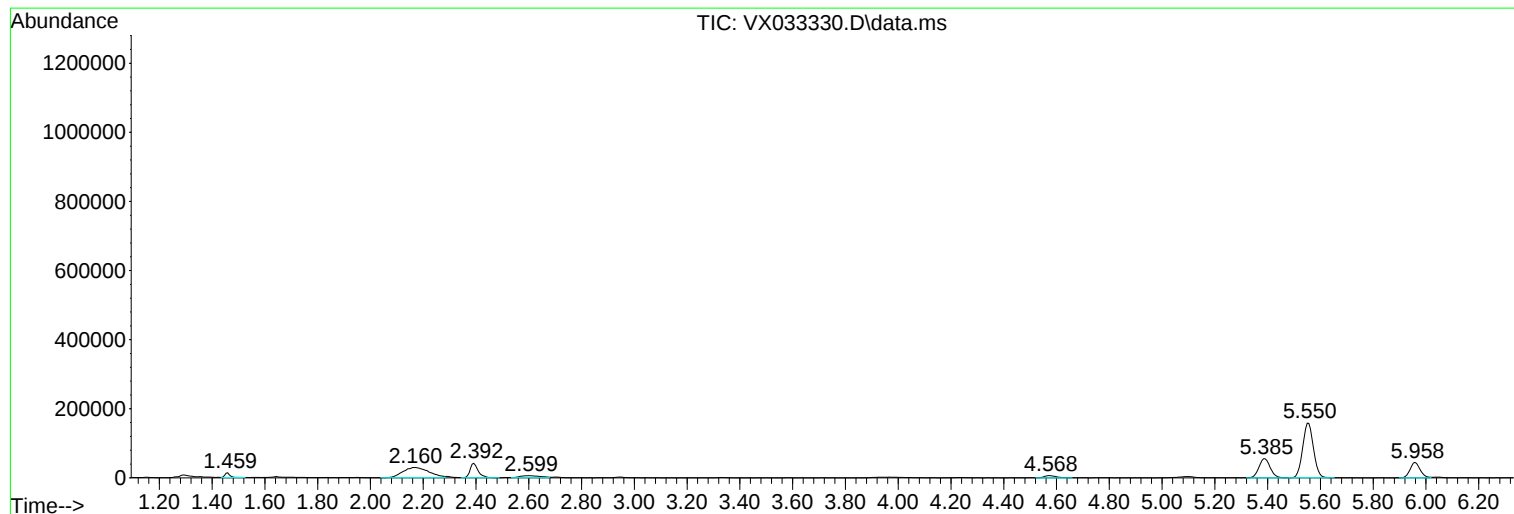

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
Data File : VX033330.D
Acq On : 08 Dec 2022 17:50
Operator : JC/MD
Sample : N5890-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1922

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120822\
Data File : VX033330.D
Acq On : 08 Dec 2022 17:50
Operator : JC/MD
Sample : N5890-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1922

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc