
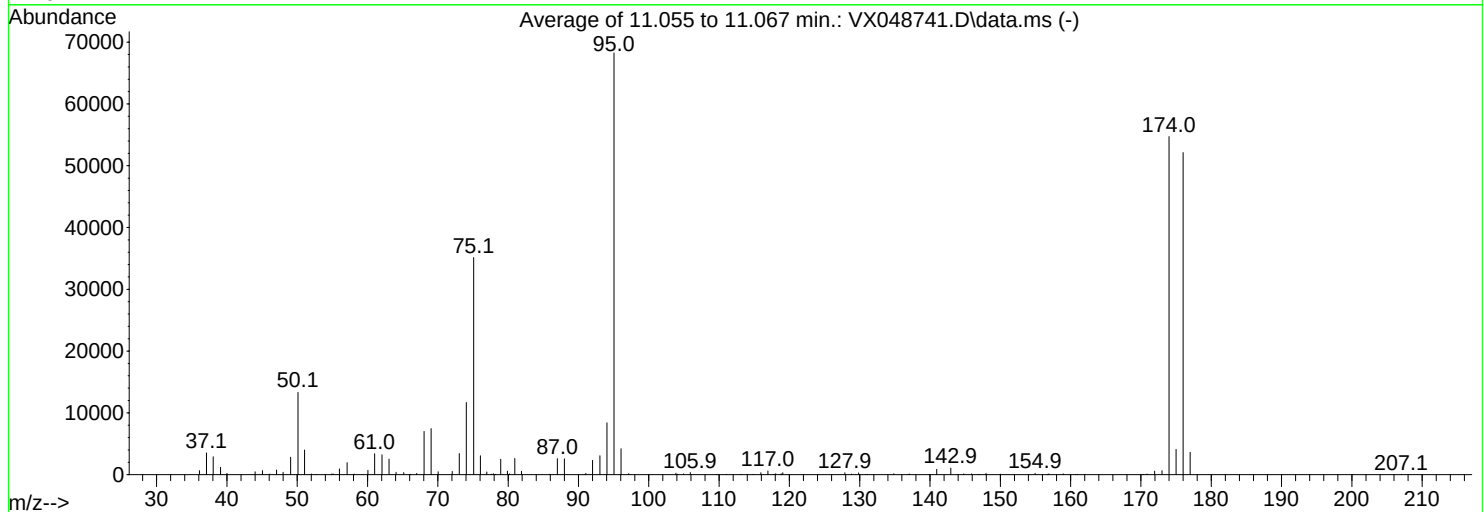


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120825\
Data File : VX048741.D
Acq On : 08 Dec 2025 08:17
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Title : SW846 8260
Last Update : Fri Dec 05 03:27:34 2025

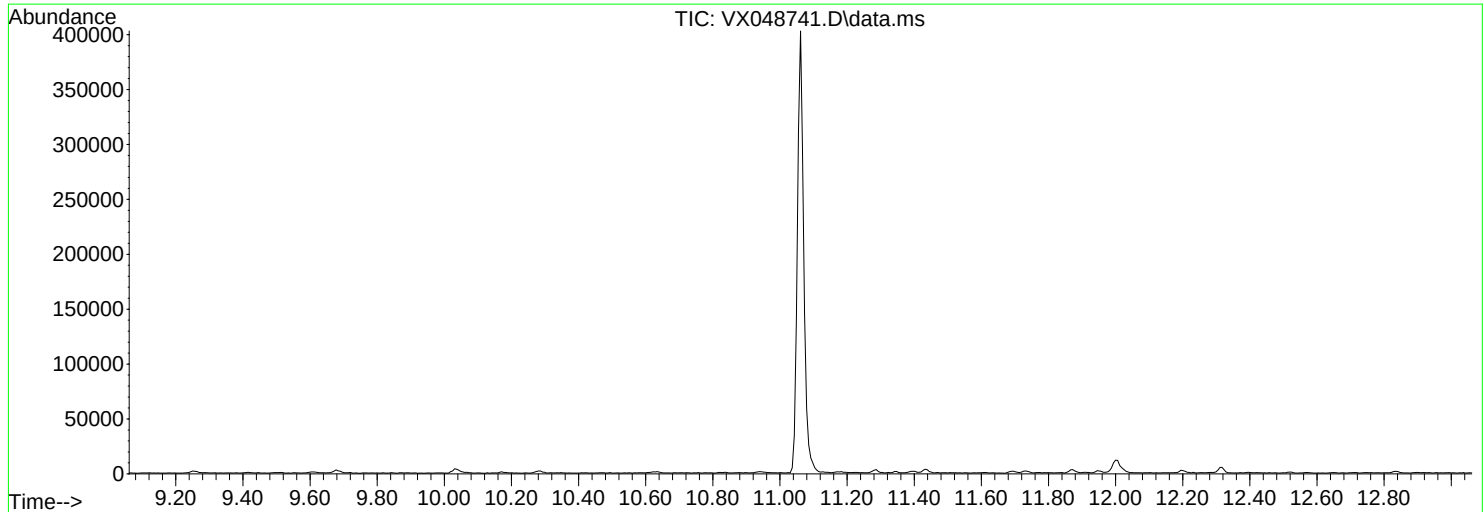

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	13323	PASS
75	95	30	60	51.5	35152	PASS
95	95	100	100	100.0	68272	PASS
96	95	5	9	6.2	4205	PASS
173	174	0.00	2	1.2	656	PASS
174	95	50	100	80.1	54717	PASS
175	174	5	9	7.5	4103	PASS
176	174	95	101	95.3	52133	PASS
177	176	5	9	7.0	3634	PASS