

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120919\
 Data File : VX0137859.D
 Acq On : 09 Dec 2019 18:30
 Operator : JC/SP
 Sample : K6185-17
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 10 03:28:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 26 15:53:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	612377	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	936100	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	839530	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	357222	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	340959	47.97	ug/l	0.00
Spiked Amount			Recovery	=	95.94%	
35) Dibromofluoromethane	5.49	113	279420	48.28	ug/l	0.00
Spiked Amount			Recovery	=	96.56%	
50) Toluene-d8	8.71	98	1107222	49.11	ug/l	0.00
Spiked Amount			Recovery	=	98.22%	
62) 4-Bromofluorobenzene	11.14	95	366757	45.11	ug/l	0.00
Spiked Amount			Recovery	=	90.22%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	1828	0.239	ug/l #	78
5) Bromomethane	1.65	94	1627	0.281	ug/l #	69
6) Chloroethane	1.82	64	1183	0.242	ug/l #	55
9) 1,1,2-Trichlorotrifluoroet	2.37	101	88058	15.082	ug/l	99
11) Tert butyl alcohol	3.00	59	573	0.327	ug/l #	1
12) 1,1-Dichloroethene	2.37	96	20468	3.512	ug/l	97
13) Acrolein	2.26	56	816	6.682	ug/l #	15
16) Acetone	2.44	43	16218	4.621	ug/l	92
20) Methylene Chloride	2.85	84	1480	0.220	ug/l #	85
24) 1,1-Dichloroethane	3.69	63	10004	0.899	ug/l #	96
27) cis-1,2-Dichloroethene	4.59	96	15354	2.106	ug/l	92
29) Tetrahydrofuran	5.01	42	964	0.300	ug/l	94
30) Chloroform	5.20	83	22370	1.981	ug/l	87
32) 1,1,1-Trichloroethane	5.48	97	3139	0.333	ug/l #	23
36) 1,1-Dichloropropene	5.65	75	41654	4.902	ug/l #	52
38) Carbon Tetrachloride	5.78	117	10512	1.342	ug/l #	91
39) Methylcyclohexane	7.21	83	57414	5.466	ug/l #	1
42) 1,2-Dichloroethane	6.19	62	2662	0.302	ug/l	99
44) Trichloroethene	7.21	130	518968	730.652	ug/l	99
47) Bromodichloromethane	7.89	83	1747	0.210	ug/l #	75
49) 1,4-Dioxane	7.76	88	802	4.699	ug/l #	72
55) 1,1,2-Trichloroethane	9.21	97	4087	0.631	ug/l #	90
64) Tetrachloroethene	9.33	164	8764	1.400	ug/l	91
76) 1,2,3-Trichloropropane	11.14	75	179362	22.324	ug/l #	39
81) trans-1,4-Dichloro-2-buten	11.14	75	179362	61.074	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	12.97	75	479	0.253	ug/l #	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120919\
Data File : VX0137859.D
Acq On : 09 Dec 2019 18:30
Operator : JC/SP
Sample : K6185-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 10 03:28:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 26 15:53:00 2019
Response via : Initial Calibration

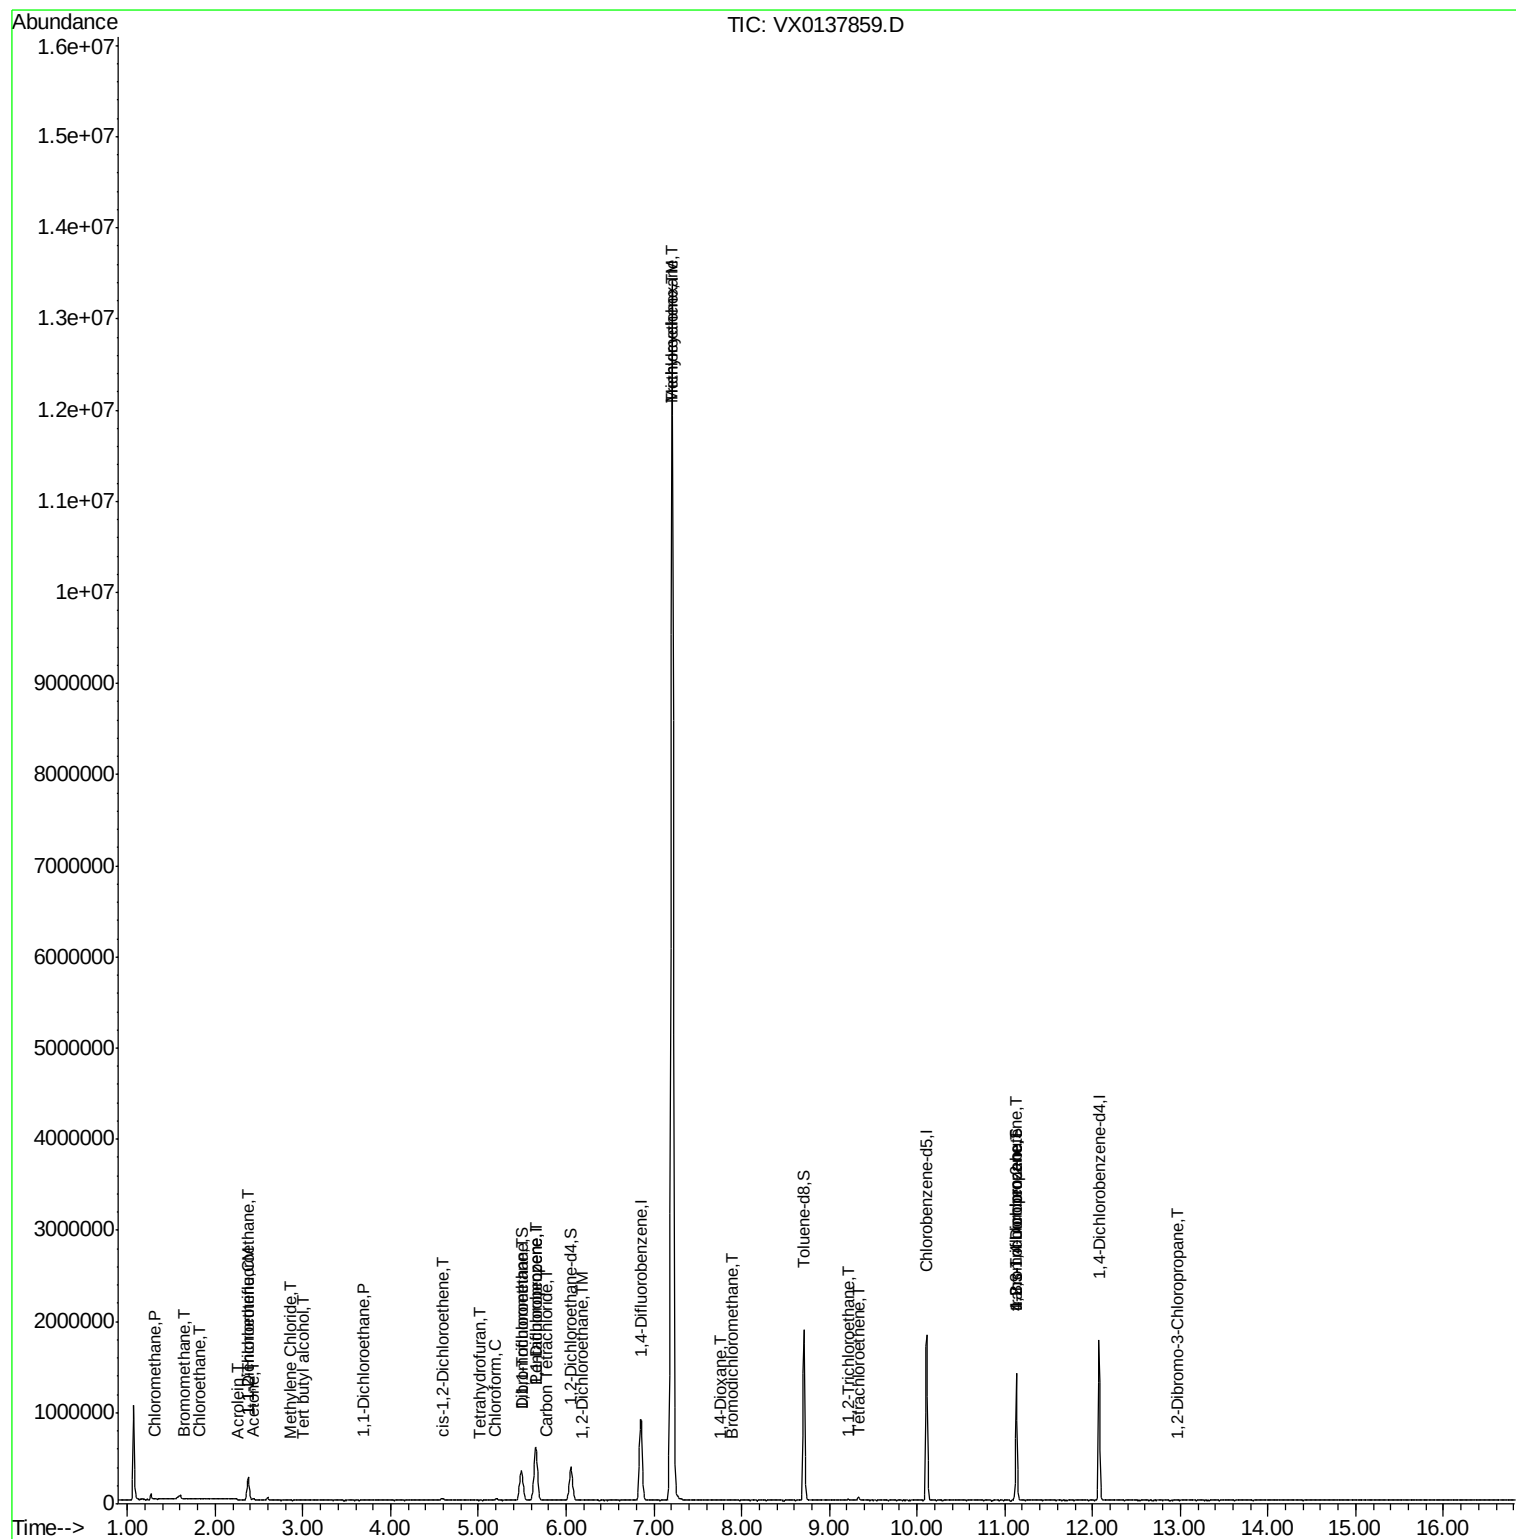



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:168 Resp: 612377

Ion Ratio Lower Upper

168 100

99 47.8 39.8 59.8

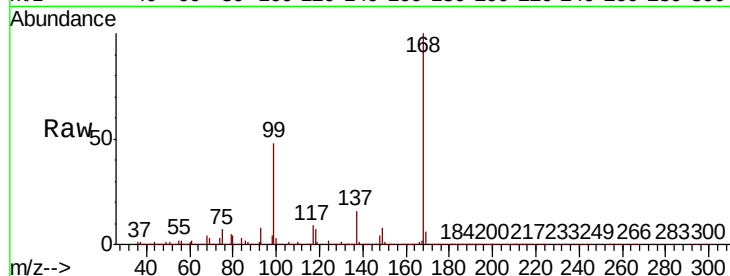

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

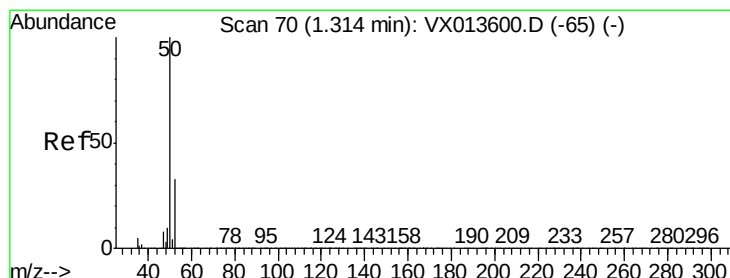

#3

Chloromethane

Concen: 0.239 ug/l

RT: 1.32 min Scan# 71

Delta R.T. 0.01 min

Lab File: VX0137859.D


Acq: 09 Dec 2019 18:30

Tgt Ion: 50 Resp: 1828

Ion Ratio Lower Upper

50 100

52 20.1 26.0 39.0#

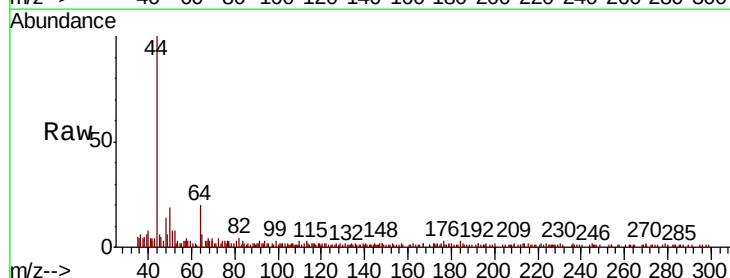

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.32

1500


1000


500

0

Time-->

1.30 1.35





#5

Bromomethane

Concen: 0.281 ug/l

RT: 1.65 min Scan# 125

Delta R.T. 0.02 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 94 Resp: 1627

Ion Ratio Lower Upper

94 100

96 65.6 77.0 115.4#

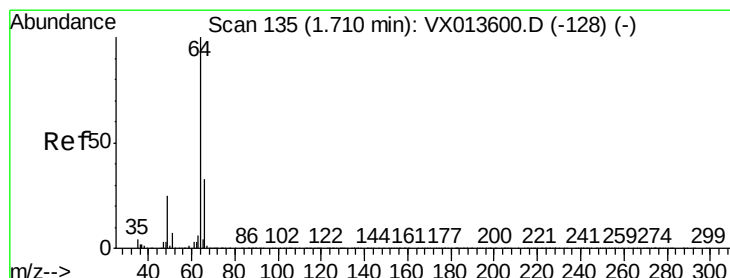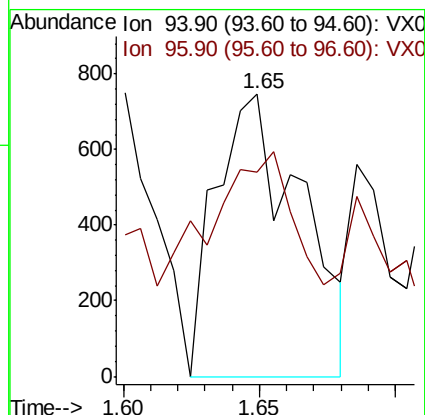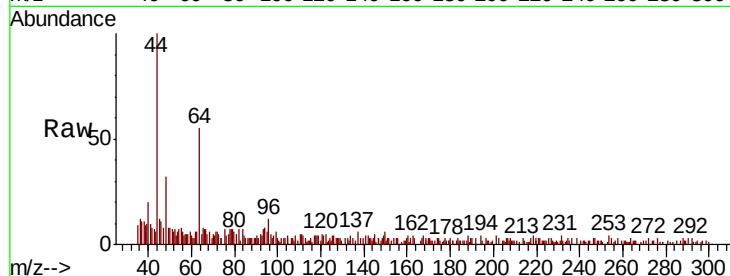

#6

Chloroethane

Concen: 0.242 ug/l

RT: 1.82 min Scan# 153

Delta R.T. 0.11 min

Lab File: VX0137859.D




Acq: 09 Dec 2019 18:30


Tgt Ion: 64 Resp: 1183

Ion Ratio Lower Upper

64 100

66 7.9 26.7 40.1#

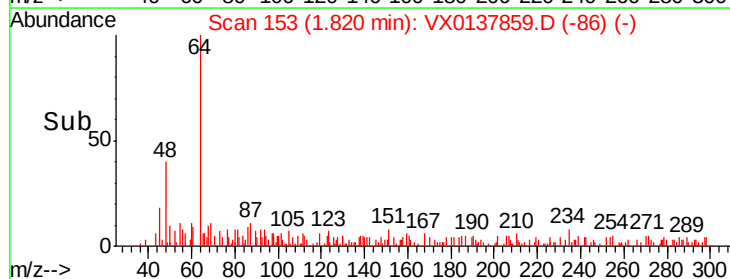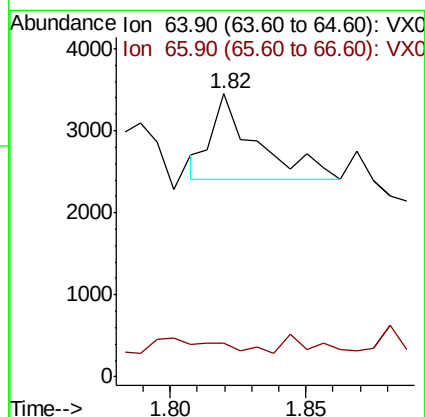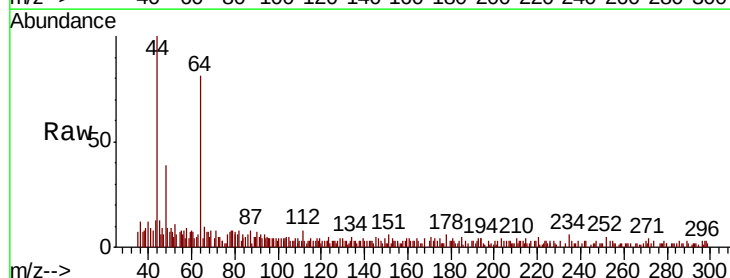

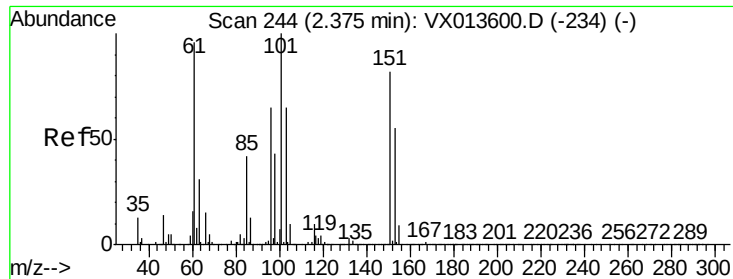

#9

1,1,2-Trichlorotrifluoroethane

Concen: 15.082 ug/l

RT: 2.37 min Scan# 244

Delta R.T. -0.00 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampled :


Tot Ion:101 Resp: 88058

Ion Ratio Lower Upper

101 100

85 42.8 33.9 50.9




151 81.5 64.2 96.2

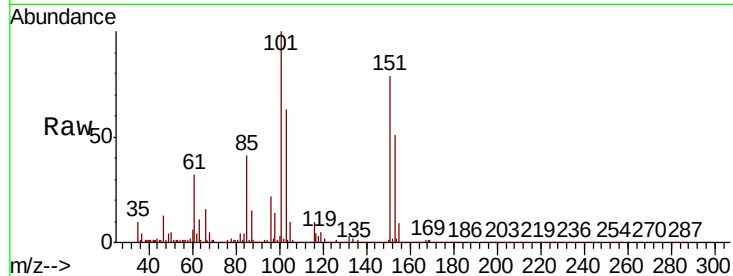

Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

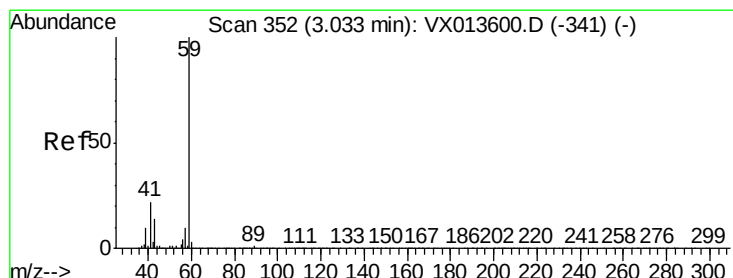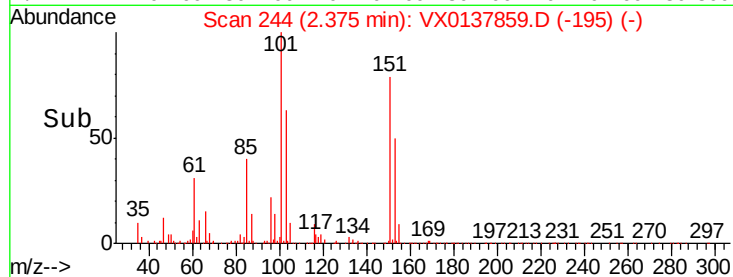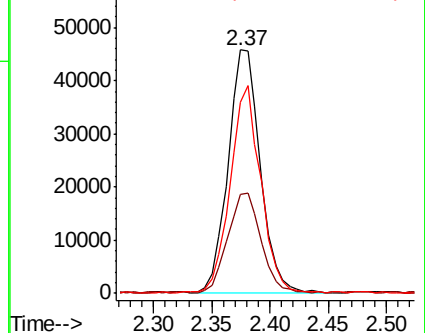

#11

Tert butyl alcohol

Concen: 0.327 ug/l

RT: 3.00 min Scan# 346

Delta R.T. -0.04 min

Lab File: VX0137859.D


Acq: 09 Dec 2019 18:30

Tgt Ion: 59 Resp: 573

Ion Ratio Lower Upper



59 100


57 229.5 7.8 11.6#

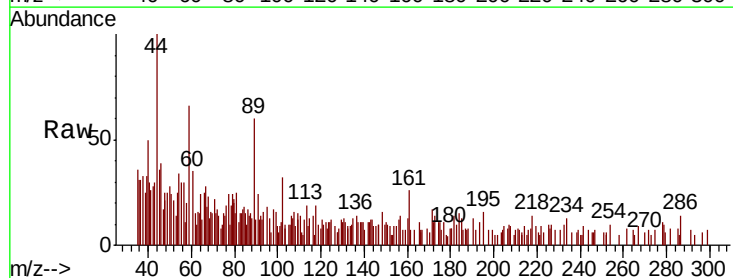

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

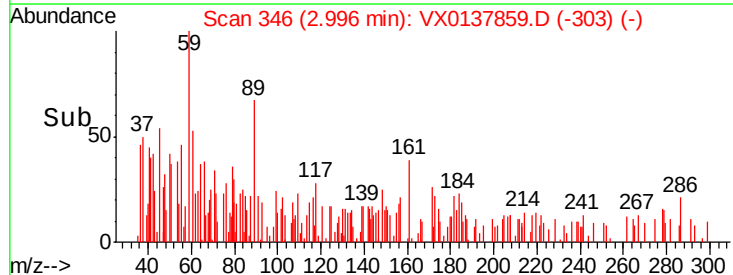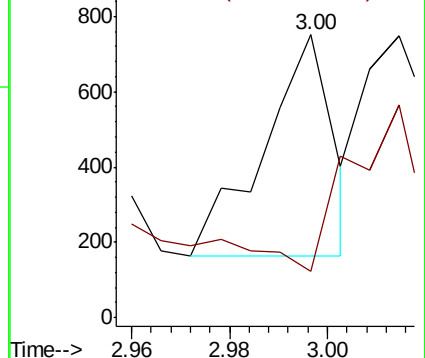

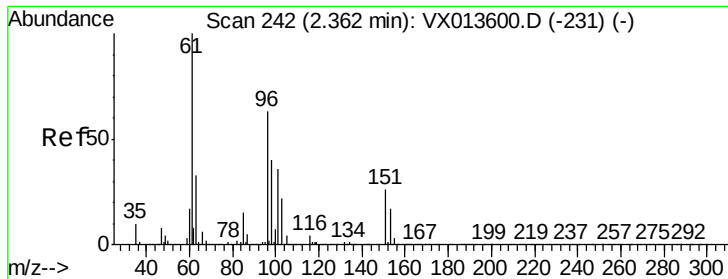

#12

1,1-Dichloroethene

Concen: 3.512 ug/l

RT: 2.37 min Scan# 243

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :
MSVOA_X
ClientSampled :





Tot Ion: 96 Resp: 20468

Ion Ratio Lower Upper

96 100

61 159.9 126.6 190.0

98 67.7 50.6 76.0

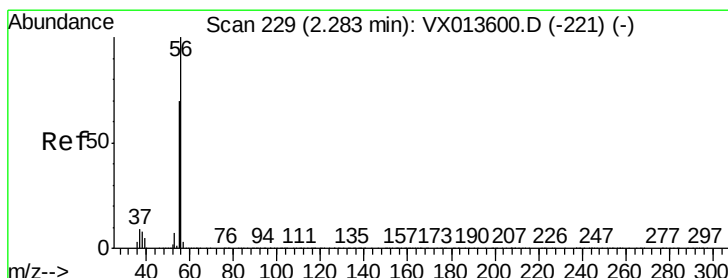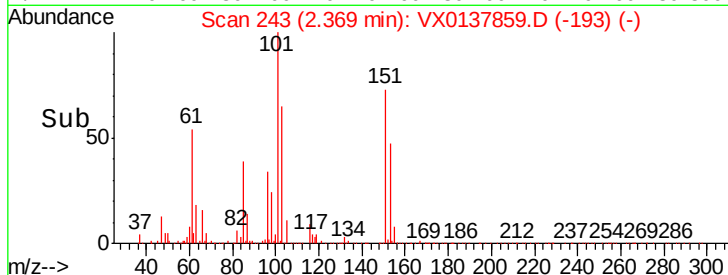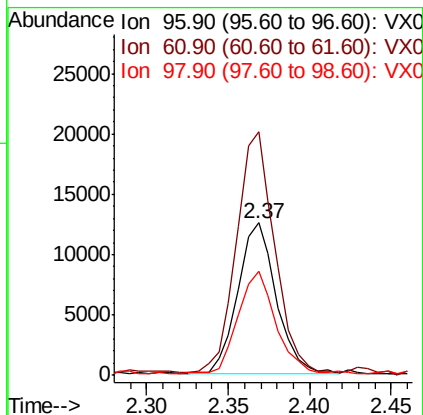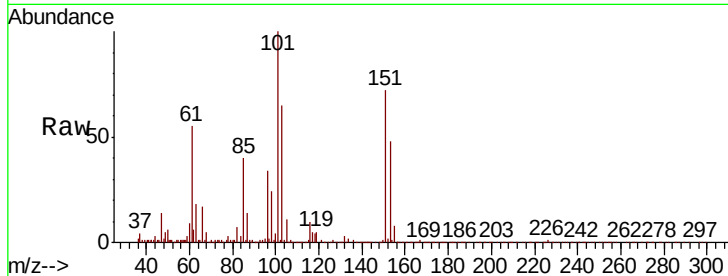

#13

Acrolein

Concen: 6.682 ug/l

RT: 2.26 min Scan# 225

Delta R.T. -0.02 min

Lab File: VX0137859.D




Acq: 09 Dec 2019 18:30


Tgt Ion: 56 Resp: 816

Ion Ratio Lower Upper

56 100

55 0.0 56.2 84.4#


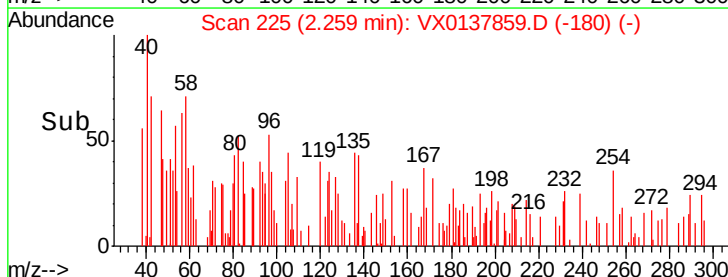
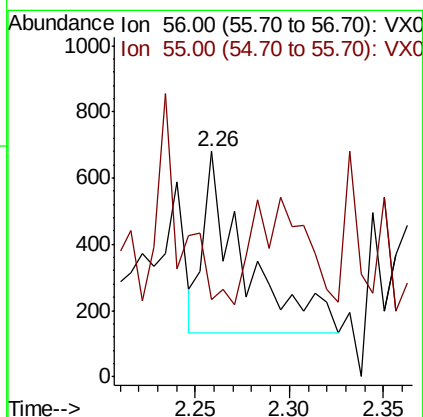
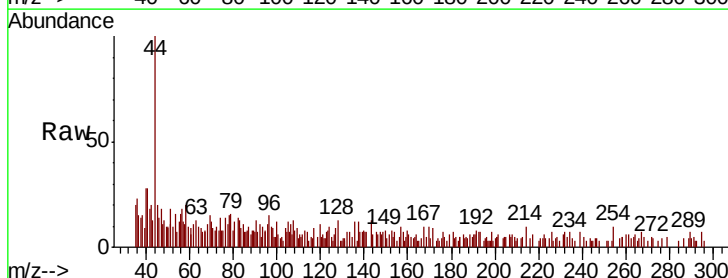


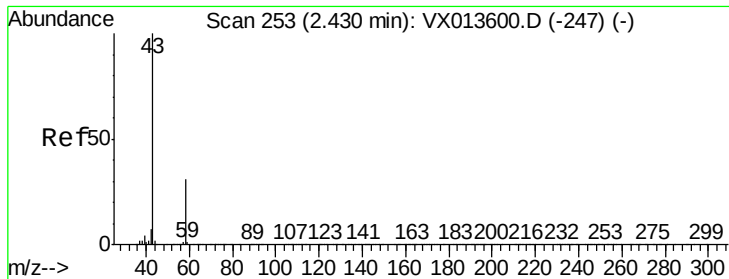

#16
Acetone
Concen: 4.621 ug/l
RT: 2.44 min Scan# 254
Delta R.T. 0.01 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 43 Resp: 16218
Ion Ratio Lower Upper
43 100
58 26.3 24.6 36.8

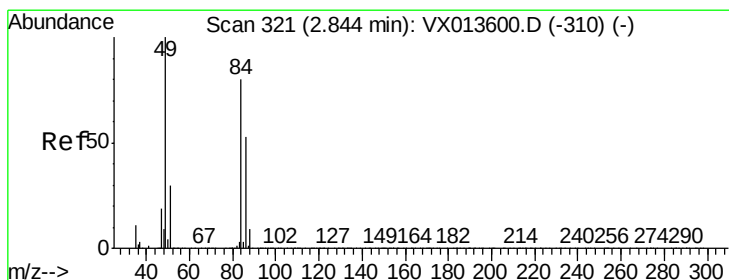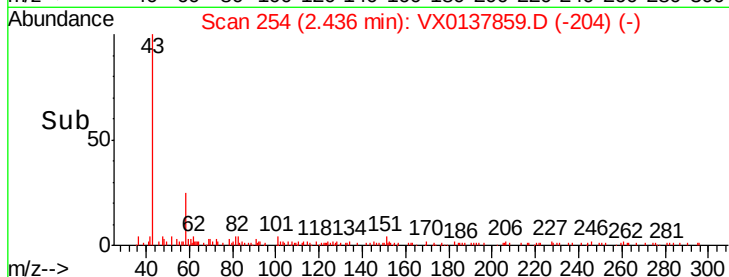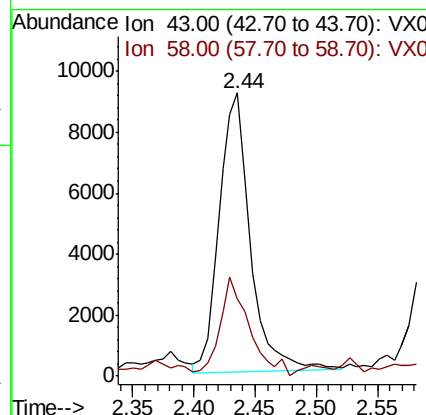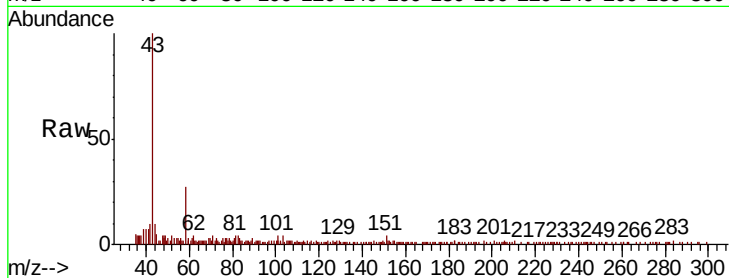

#20
Methylene Chloride
Concen: 0.220 ug/l
RT: 2.85 min Scan# 322
Delta R.T. 0.01 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30

Tgt Ion: 84 Resp: 1480
Ion Ratio Lower Upper
84 100
49 108.5 99.7 149.5
51 15.9 29.9 44.9#
86 69.5 52.2 78.4

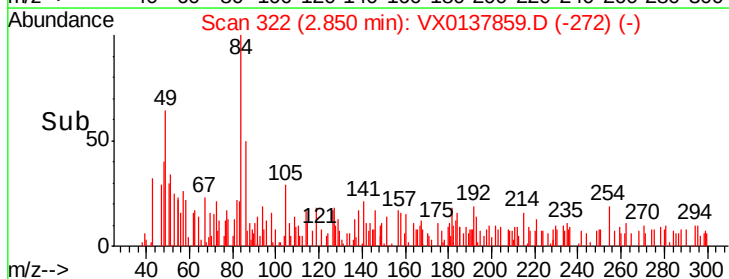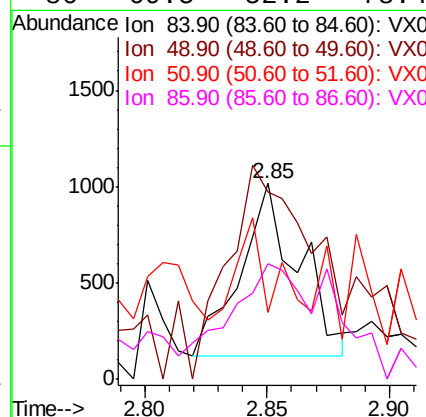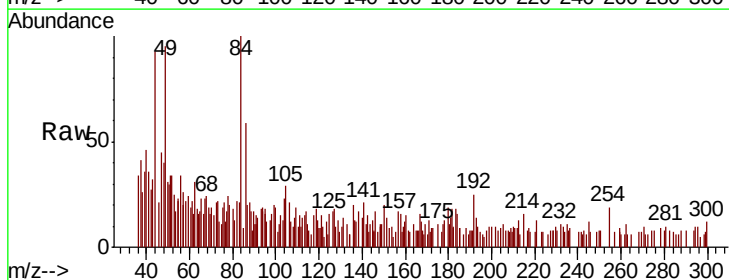



#24

1,1-Dichloroethane

Concen: 0.899 ug/l

RT: 3.69 min Scan# 460

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 63 Resp: 10004

Ion Ratio Lower Upper

63 100

98 6.2 3.5 10.4




100 6.6 2.1 6.3#

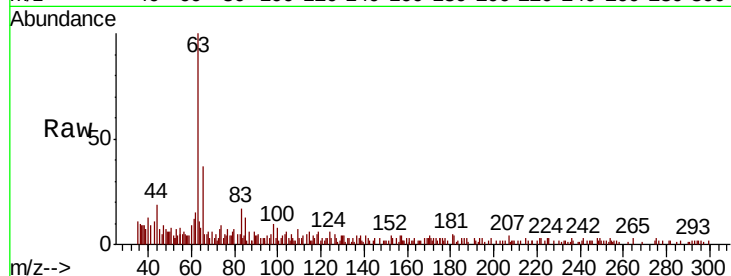

Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

Ion 99.90 (99.60 to 100.60): VX0

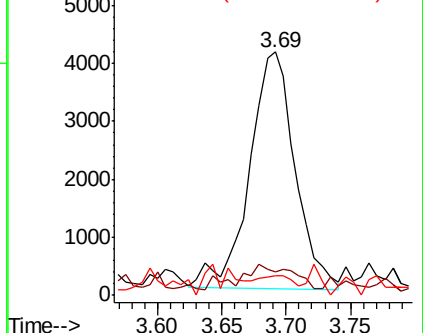

#27

cis-1,2-Dichloroethene

Concen: 2.106 ug/l

RT: 4.59 min Scan# 608

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30


Tgt Ion: 96 Resp: 15354

Ion Ratio Lower Upper

96 100

61 133.5 0.0 286.4



98 69.7 0.0 127.4




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0



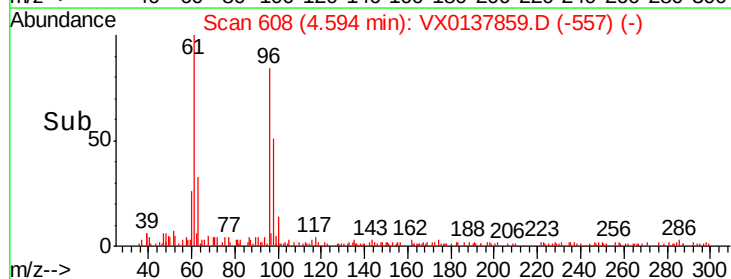
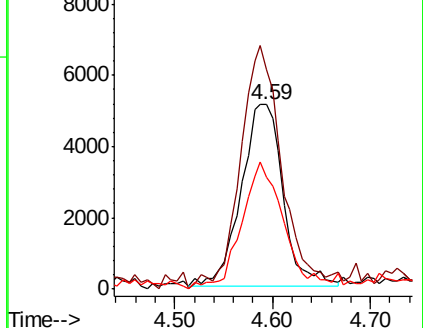


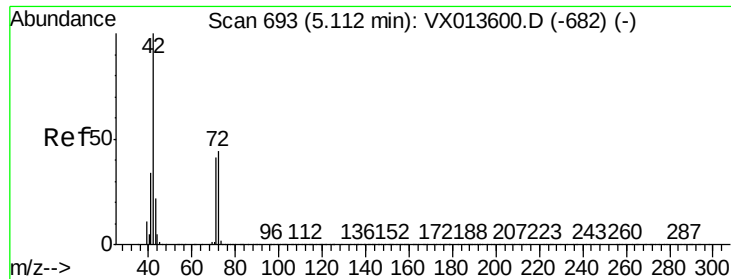

#29
Tetrahydrofuran
Concen: 0.300 ug/l
RT: 5.01 min Scan# 677
Delta R.T. -0.10 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 42 Resp: 964
Ion Ratio Lower Upper
42 100
72 43.7 36.3 54.5
71 48.1 33.2 49.8

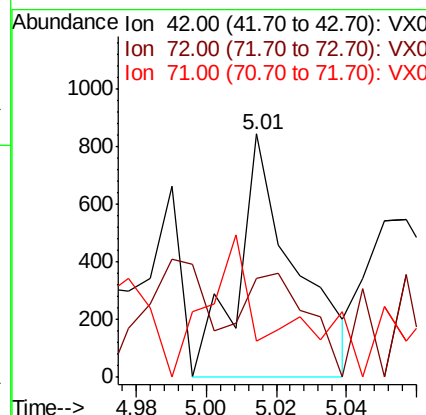

#30
Chloroform
Concen: 1.981 ug/l
RT: 5.20 min Scan# 708
Delta R.T. 0.01 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30

Tgt Ion: 83 Resp: 22370
Ion Ratio Lower Upper
83 100
85 52.6 50.2 75.4

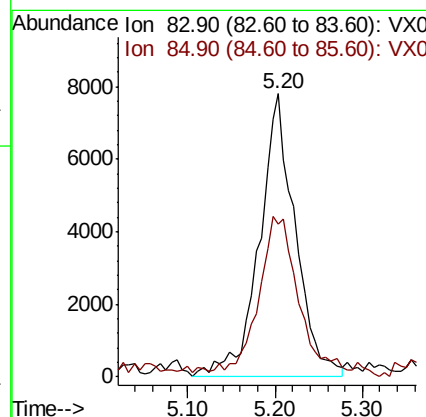



#32

1,1,1-Trichloroethane

Concen: 0.333 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.00 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 97 Resp: 3139

Ion Ratio Lower Upper

97 100

99 0.0 51.6 77.4#




61 0.0 36.1 54.1#



Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

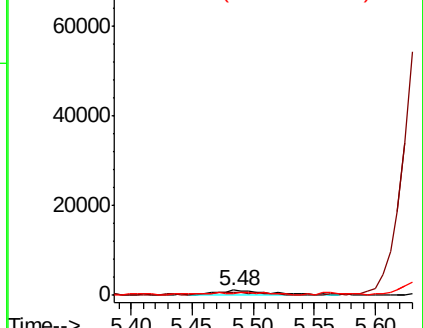

#33

1,2-Dichloroethane-d4

Concen: 47.966 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX0137859.D


Acq: 09 Dec 2019 18:30

Tgt Ion: 65 Resp: 340959

Ion Ratio Lower Upper



65 100


67 53.1 0.0 104.4



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

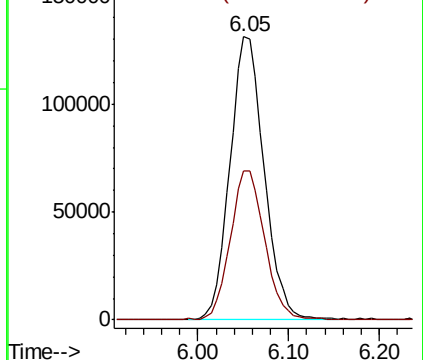



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampled :


Tot Ion:114 Resp: 936100

Ion Ratio Lower Upper

114 100

63 20.3 0.0 39.6




88 15.4 0.0 31.4

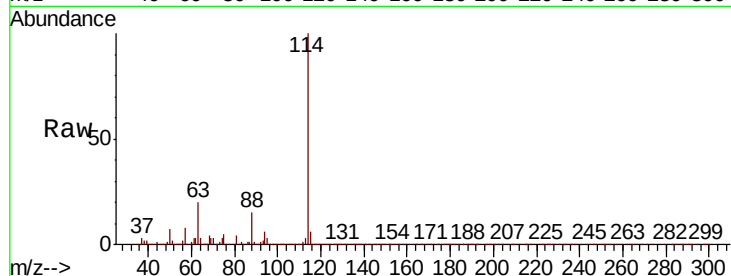

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

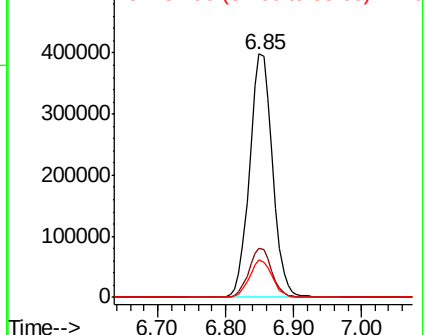

#35

Dibromofluoromethane

Concen: 48.283 ug/l

RT: 5.49 min Scan# 755

Delta R.T. -0.00 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30


Tgt Ion:113 Resp: 279420

Ion Ratio Lower Upper

113 100

111 102.5 83.6 125.4



192 24.1 19.2 28.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

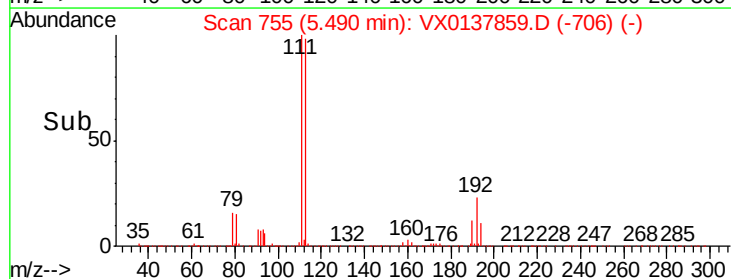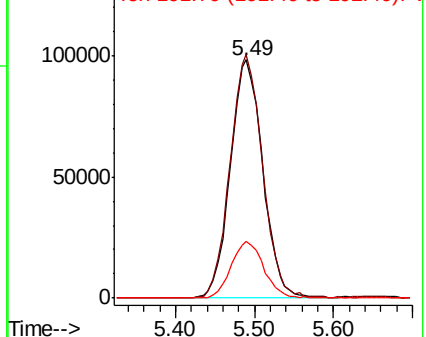



#36

1,1-Dichloropropene

Concen: 4.902 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.13 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 75 Resp: 41654

Ion Ratio Lower Upper

75 100

110 11.2 18.1 54.1#




77 0.6 24.5 36.7#

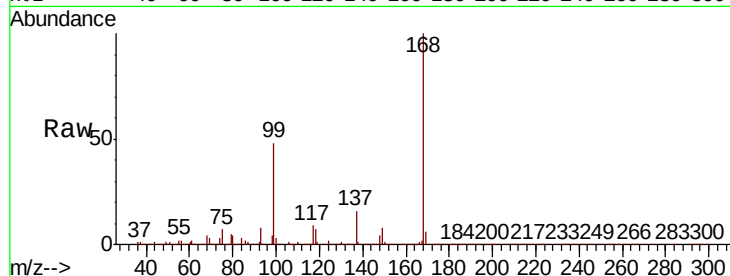

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

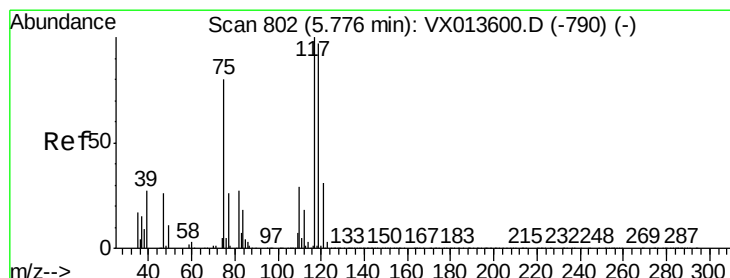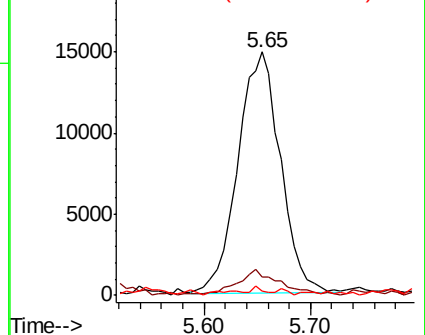

#38

Carbon Tetrachloride

Concen: 1.342 ug/l

RT: 5.78 min Scan# 803

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30


Tgt Ion: 117 Resp: 10512

Ion Ratio Lower Upper

117 100

119 91.1 77.5 116.3



121 20.2 25.0 37.6#

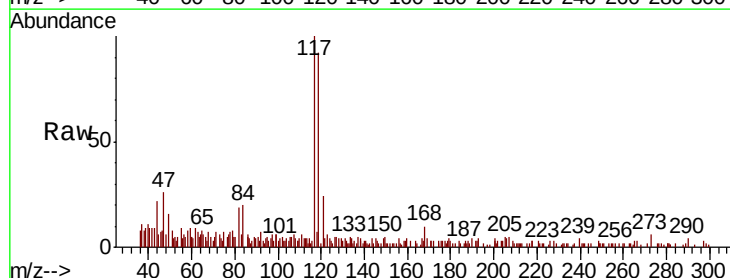


Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

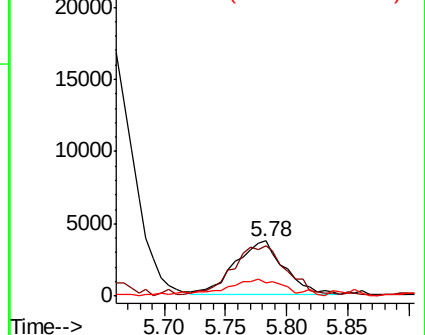

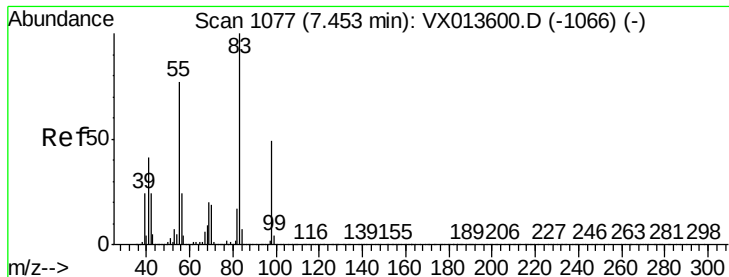

#39

Methylcyclohexane

Concen: 5.466 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. -0.24 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampleId :





Tot Ion: 83 Resp: 57414

Ion Ratio Lower Upper

83 100

55 0.5 61.9 92.9#

98 205.6 39.4 59.0#

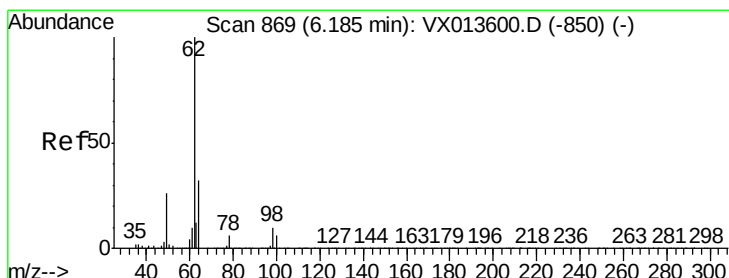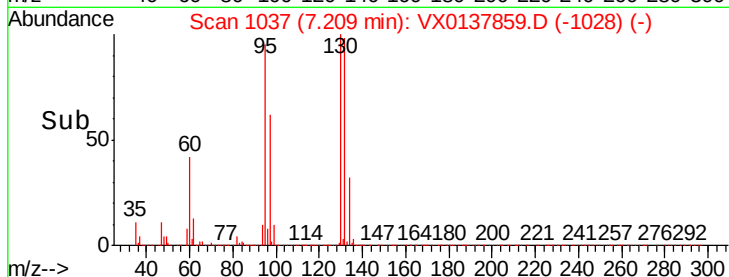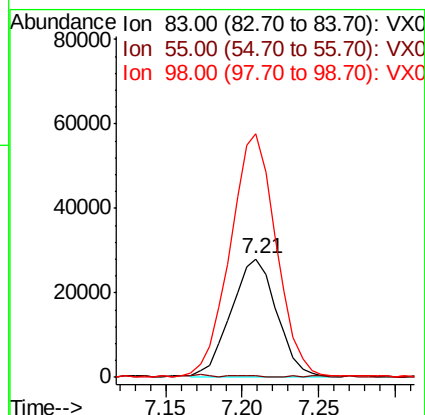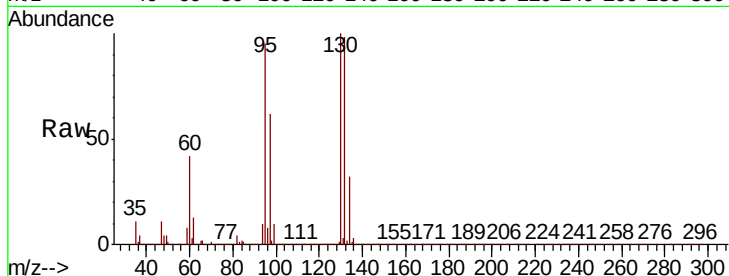

#42

1,2-Dichloroethane

Concen: 0.302 ug/l

RT: 6.19 min Scan# 870

Delta R.T. 0.01 min

Lab File: VX0137859.D




Acq: 09 Dec 2019 18:30


Tgt Ion: 62 Resp: 2662

Ion Ratio Lower Upper

62 100

98 10.0 0.0 20.8

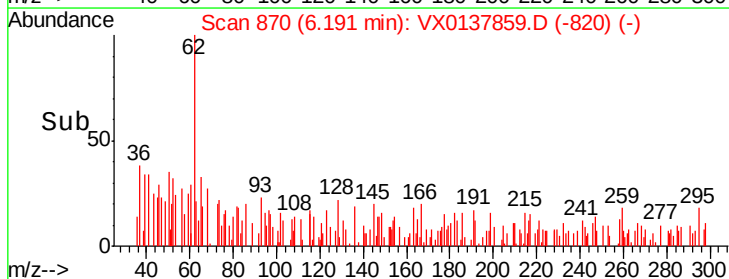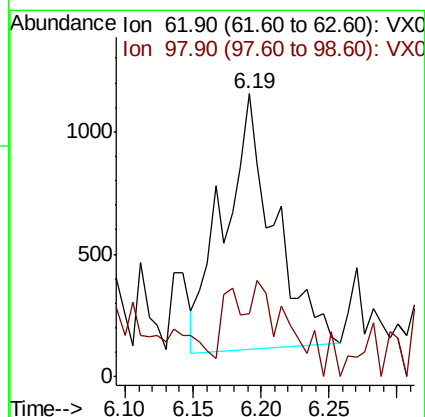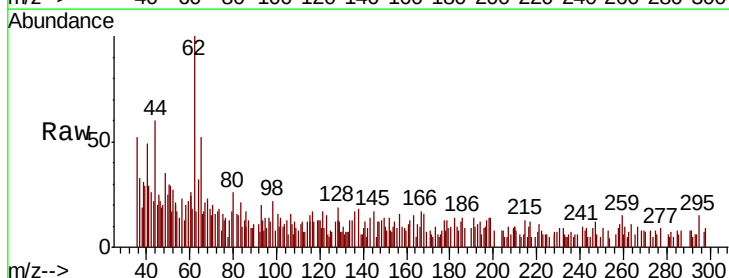

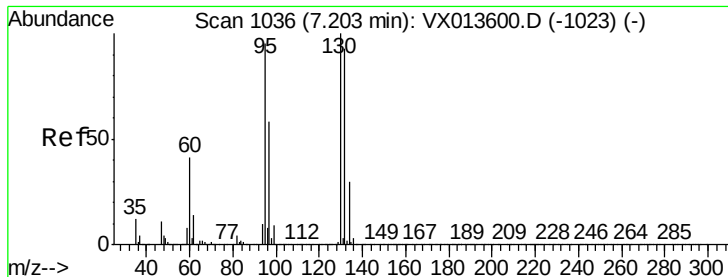

#44

Trichloroethene

Concen: 730.652 ug/l

RT: 7.21 min Scan# 1037

Delta R.T. 0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:130 Resp: 5189668

Ion Ratio Lower Upper




130 100

95 94.8 0.0 190.8

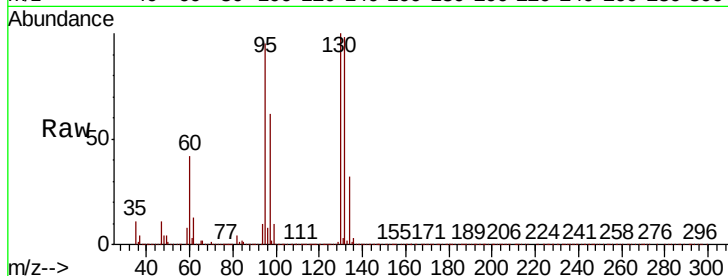

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

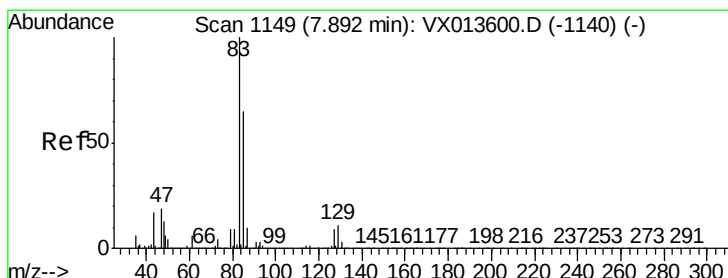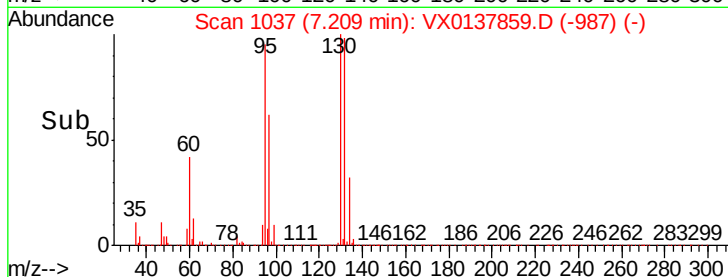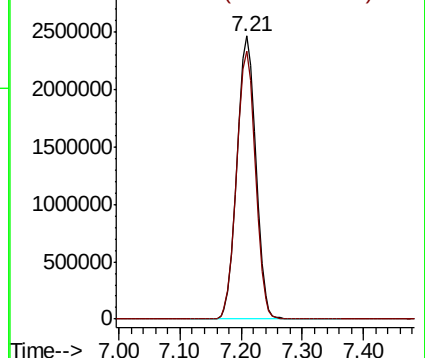

#47

Bromodichloromethane

Concen: 0.210 ug/l

RT: 7.89 min Scan# 1148

Delta R.T. -0.01 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30


Tgt Ion: 83 Resp: 1747

Ion Ratio Lower Upper

83 100

85 47.3 52.1 78.1#



127 23.9 7.0 10.4#

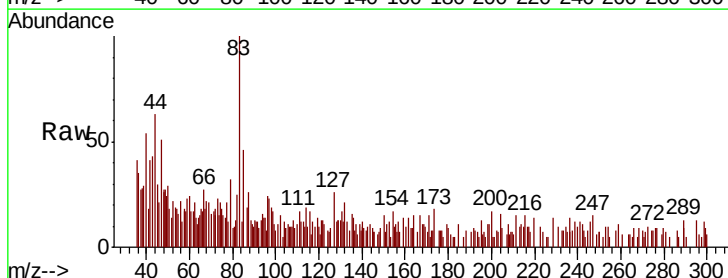


Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 126.80 (126.50 to 127.50): V

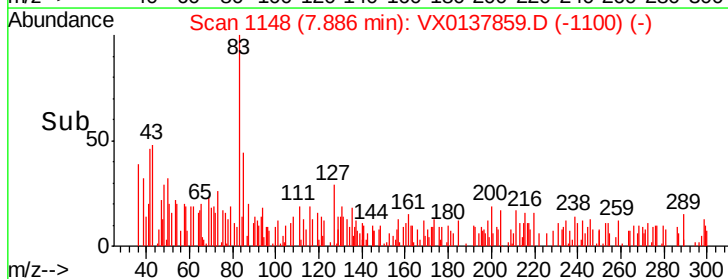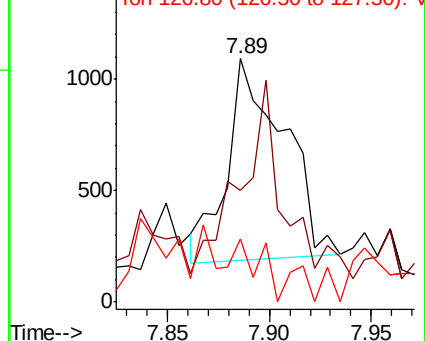



#49

1,4-Dioxane

Concen: 4.699 ug/l

RT: 7.76 min Scan# 1127

Delta R.T. 0.02 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampled :





Tot Ion: 88 Resp: 802

Ion Ratio Lower Upper

88 100

43 47.8 25.8 38.6#

58 45.5 54.6 82.0#

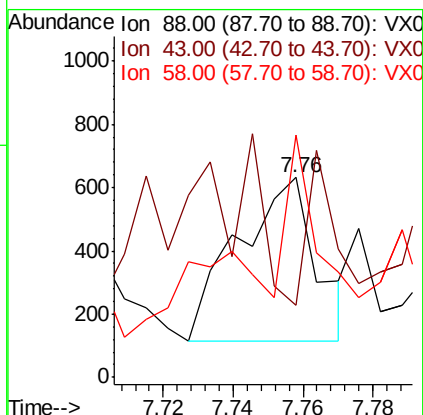

#50

Toluene-d8

Concen: 49.107 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX0137859.D




Acq: 09 Dec 2019 18:30


Tgt Ion: 98 Resp: 1107222

Ion Ratio Lower Upper

98 100

100 66.0 53.1 79.7



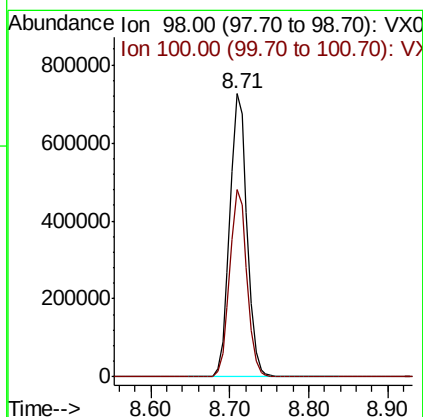



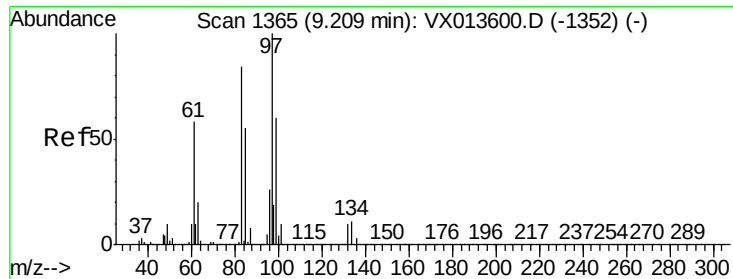

#55
 1,1,2-Trichloroethane
 Concen: 0.631 ug/l
 RT: 9.21 min Scan# 1365
 Delta R.T. -0.00 min
 Lab File: VX0137859.D
 Acq: 09 Dec 2019 18:30




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion:	97	Resp:	4087
Ion	Ratio	Lower	Upper
97	100		
83	81.6	67.3	100.9
85	45.0	43.6	65.4
99	47.9	48.2	72.4#

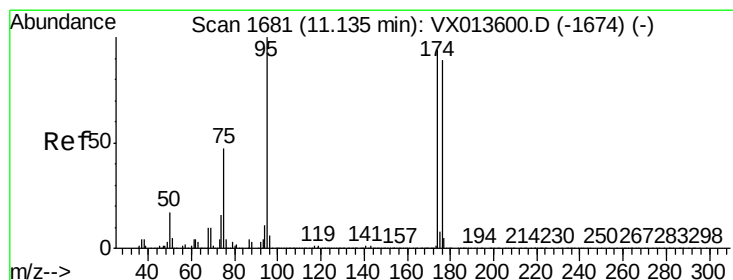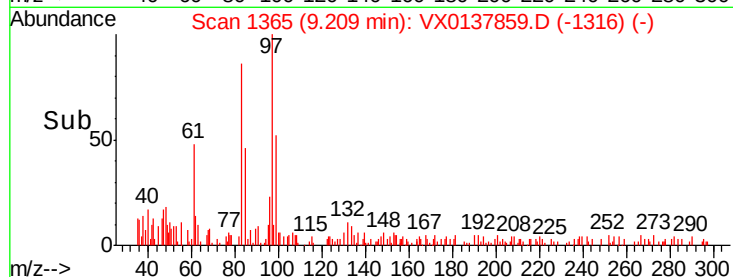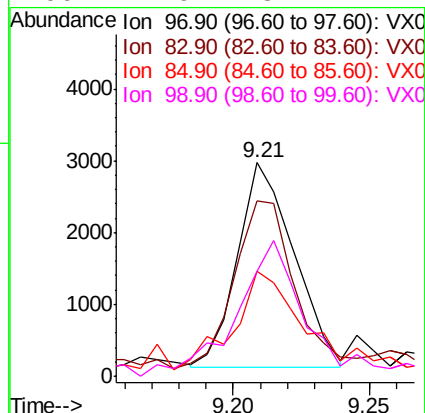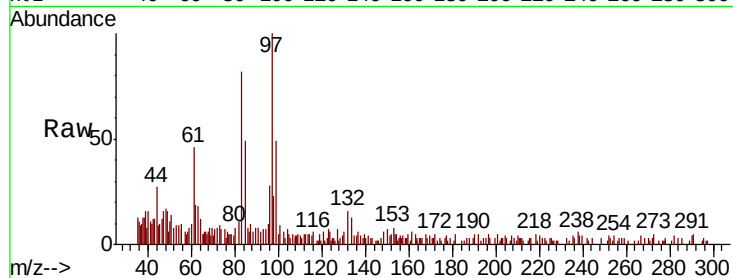

#62
 4-Bromofluorobenzene
 Concen: 45.108 ug/l
 RT: 11.14 min Scan# 1681
 Delta R.T. -0.00 min
 Lab File: VX0137859.D
 Acq: 09 Dec 2019 18:30

Tgt Ion:	95	Resp:	366757
Ion	Ratio	Lower	Upper
95	100		
174	88.6	0.0	180.0
176	85.8	0.0	173.6


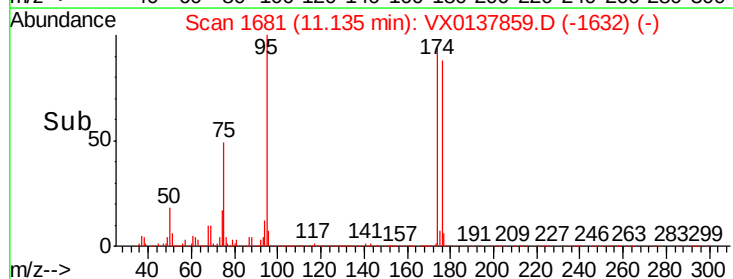
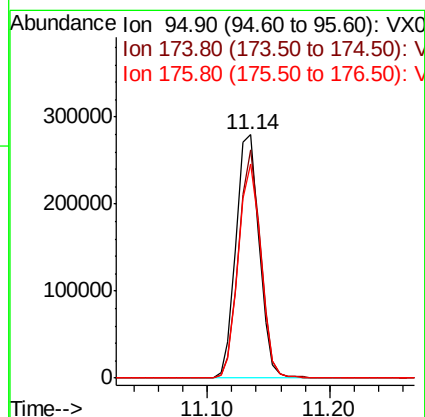
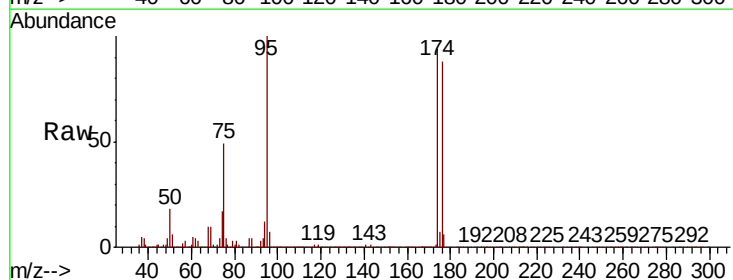


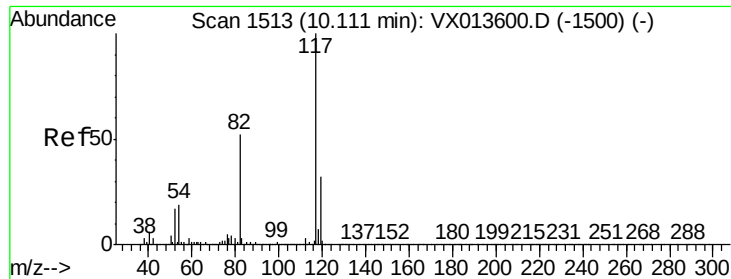

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
117	100		
82	52.8	41.8	62.8
119	32.6	25.8	38.8

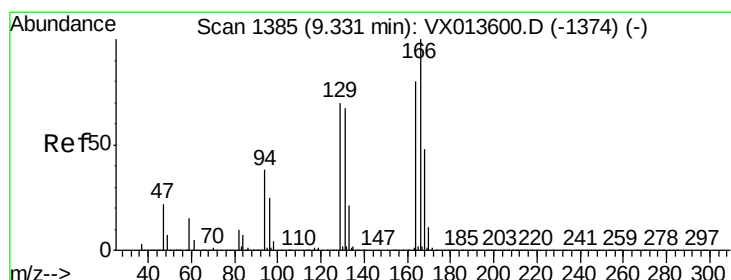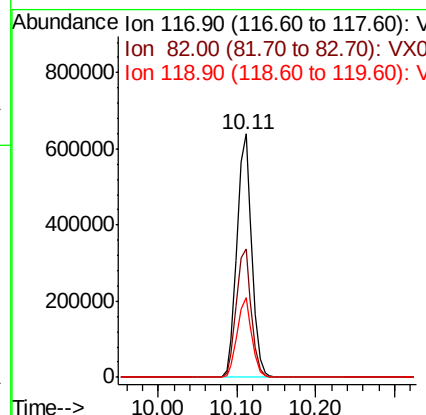

#64
Tetrachloroethene
Concen: 1.400 ug/l
RT: 9.33 min Scan# 1385
Delta R.T. -0.00 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30

Tgt Ion	Ratio	Lower	Upper
164	100		
166	110.0	99.7	149.5
129	93.1	70.1	105.1
131	89.0	66.9	100.3

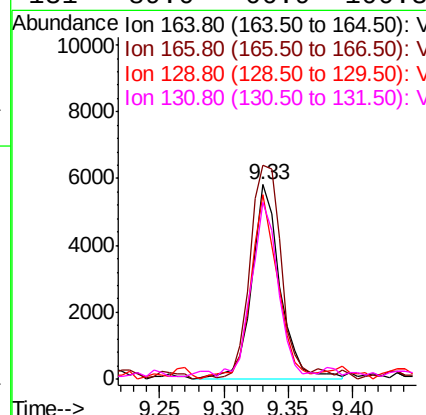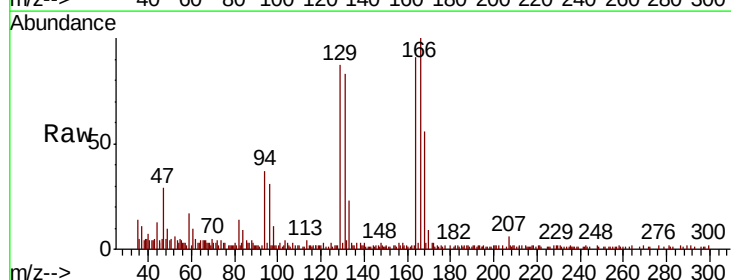







#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30

Instrument :
MSVOA_X
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
152	100		
115	56.4	38.4	115.1
150	157.5	0.0	346.8

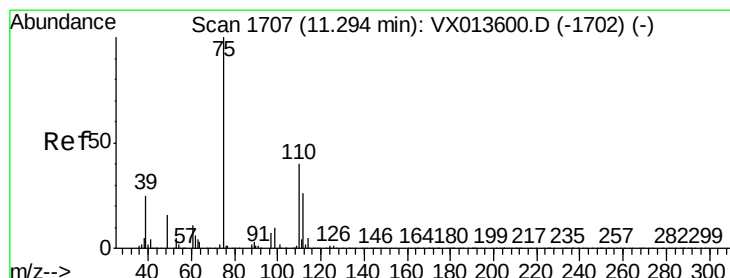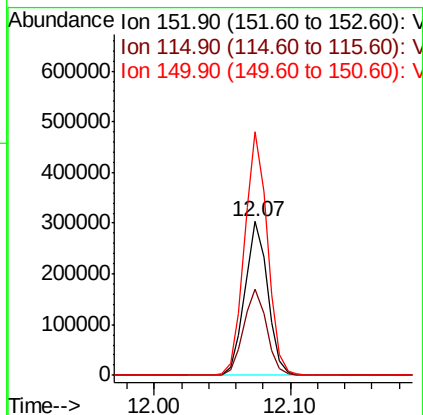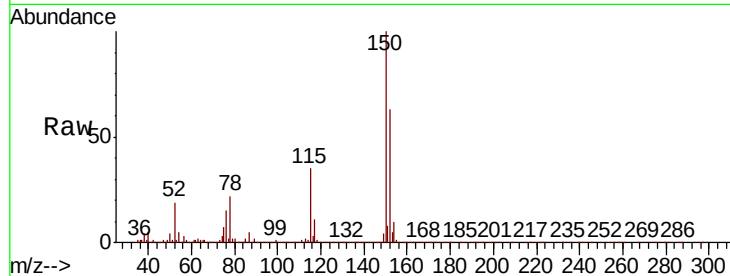


#76

1,2,3-Trichloropropane
Concen: 22.324 ug/l
RT: 11.14 min Scan# 1681
Delta R.T. -0.16 min
Lab File: VX0137859.D
Acq: 09 Dec 2019 18:30

Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.6	19.1	57.5#

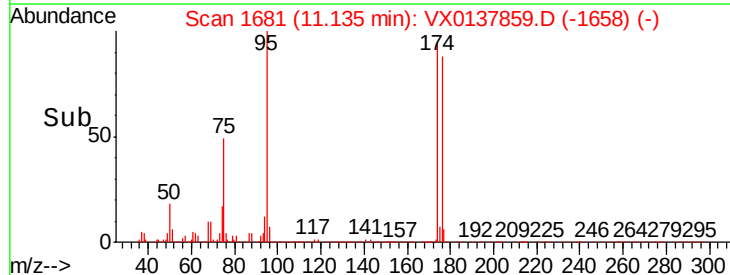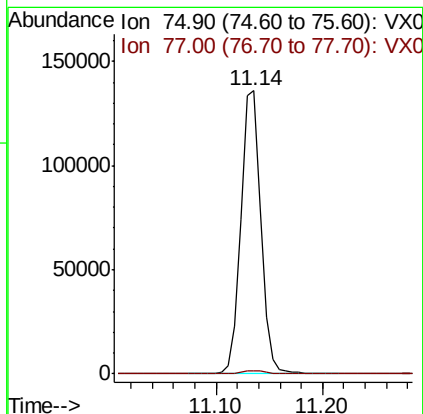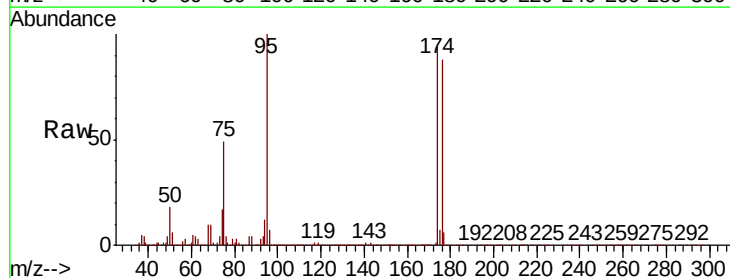



#81

trans-1,4-Dichloro-2-butene

Concen: 61.074 ug/l

RT: 11.14 min Scan# 1681

Delta R.T. 0.07 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Instrument :

MSVOA_X

ClientSampleId :





Tot Ion: 75 Resp: 179362

Ion Ratio Lower Upper

75 100

53 0.1 78.2 117.2#

89 0.2 35.4 53.2#

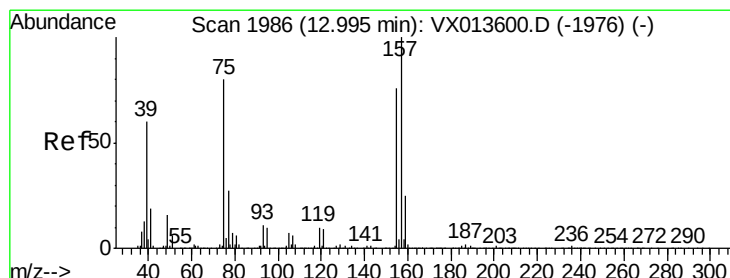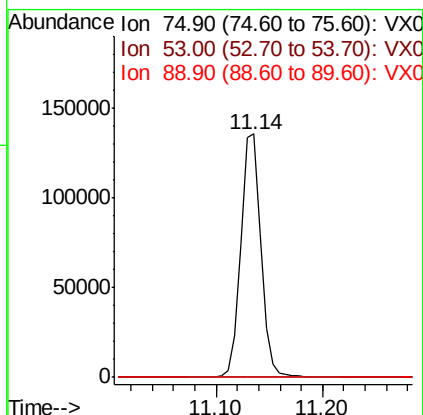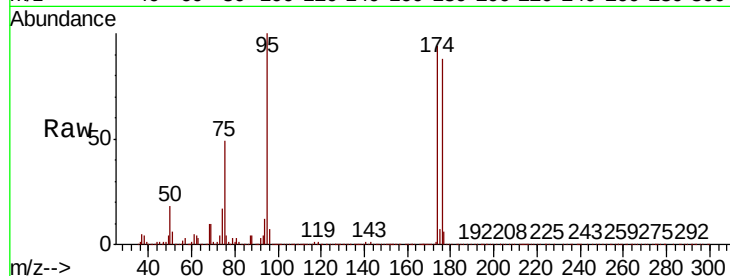

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.253 ug/l

RT: 12.97 min Scan# 1982

Delta R.T. -0.02 min

Lab File: VX0137859.D

Acq: 09 Dec 2019 18:30

Tgt Ion: 75 Resp: 479

Ion Ratio Lower Upper

75 100

155 52.8 47.6 142.8

157 33.0 62.1 186.2#

