

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120919\
 Data File : VX013847.D
 Acq On : 09 Dec 2019 13:21
 Operator : JC/SP
 Sample : VX1209WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1209WBL01

Quant Time: Dec 10 03:46:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 26 15:53:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	614301	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	941182	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	836596	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	380177	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	341531	47.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.80%	
35) Dibromofluoromethane	5.48	113	280625	48.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.46%	
50) Toluene-d8	8.71	98	1111585	49.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.06%	
62) 4-Bromofluorobenzene	11.13	95	382032	46.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.46%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120919\
Data File : VX013847.D
Acq On : 09 Dec 2019 13:21
Operator : JC/SP
Sample : VX1209WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1209WBL01

Quant Time: Dec 10 03:46:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 26 15:53:00 2019
Response via : Initial Calibration

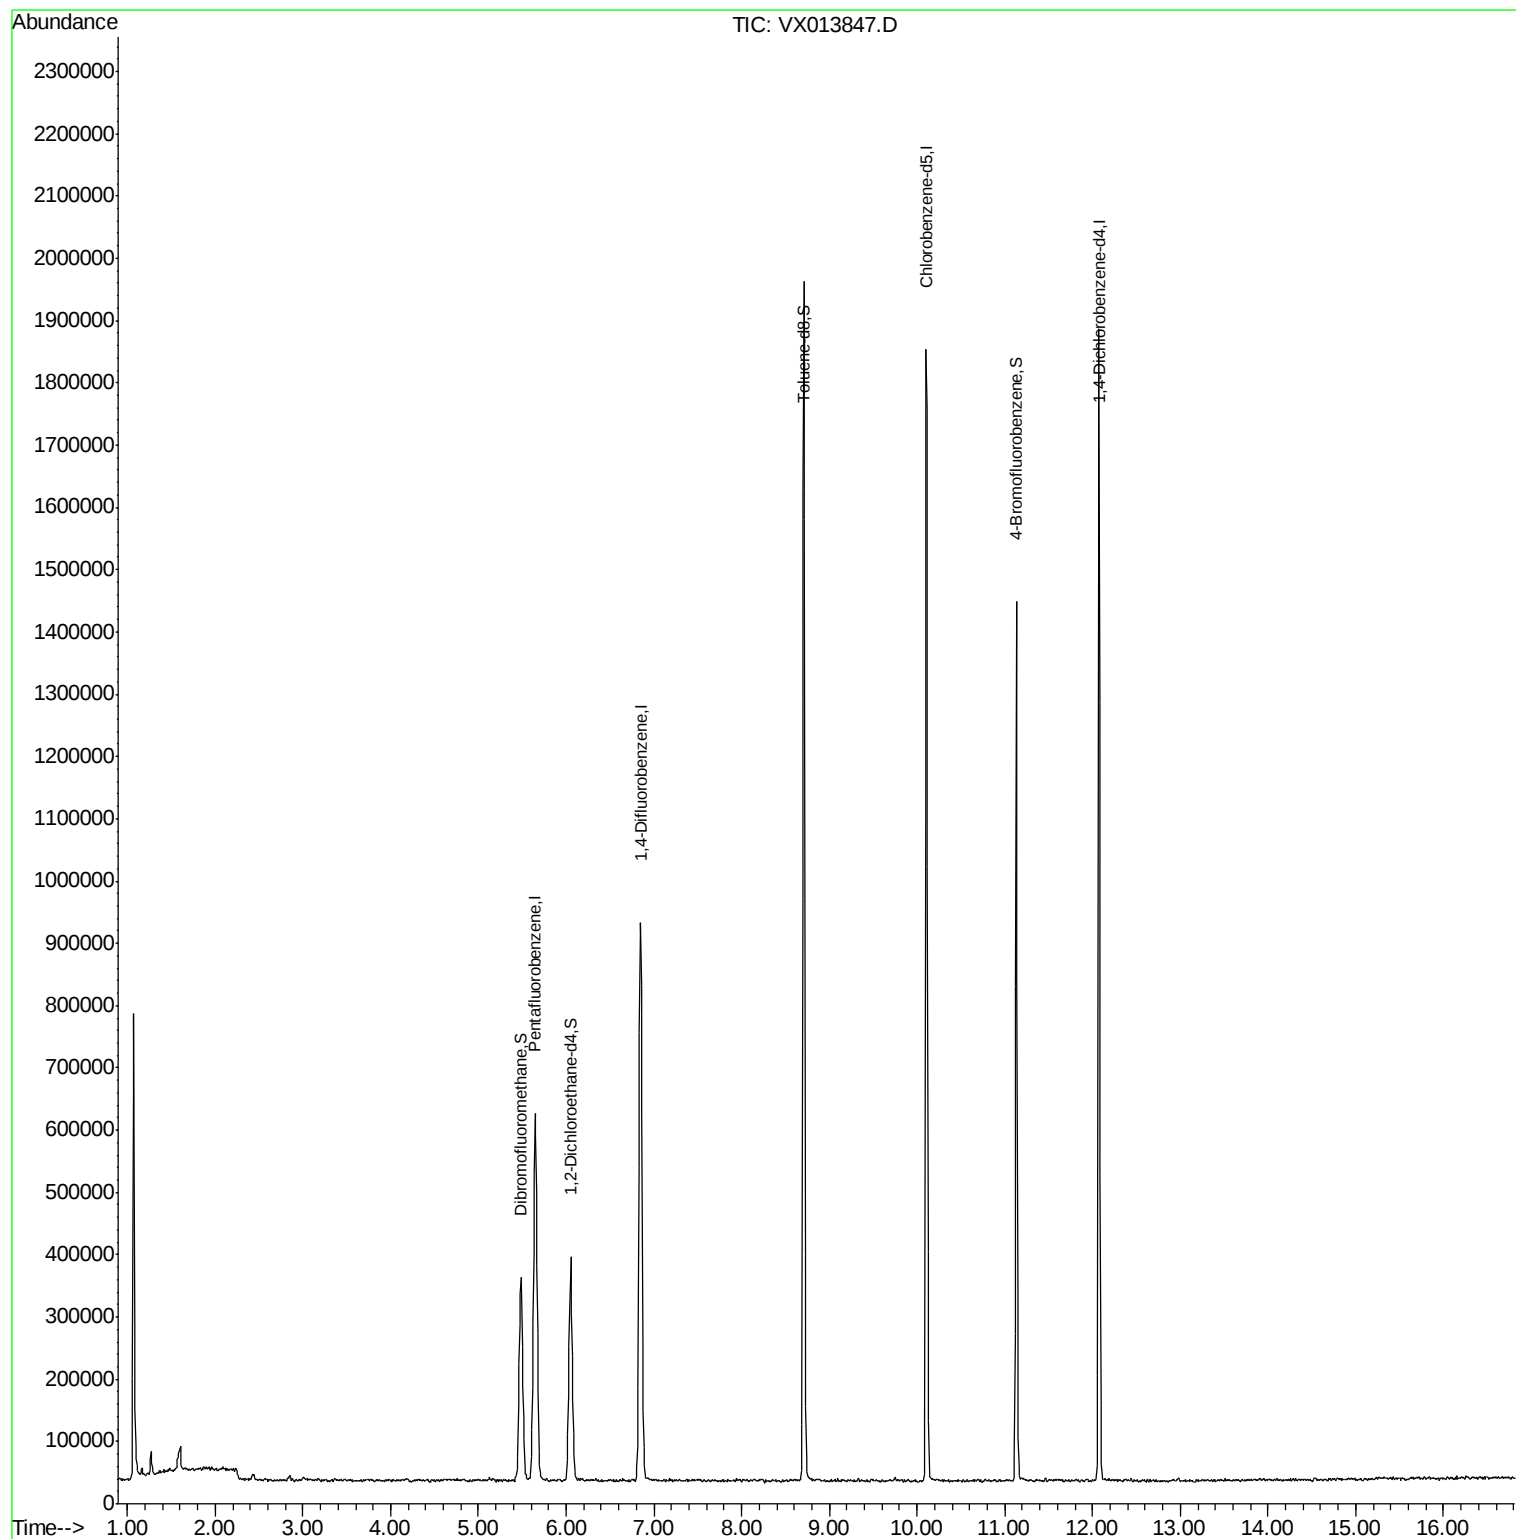

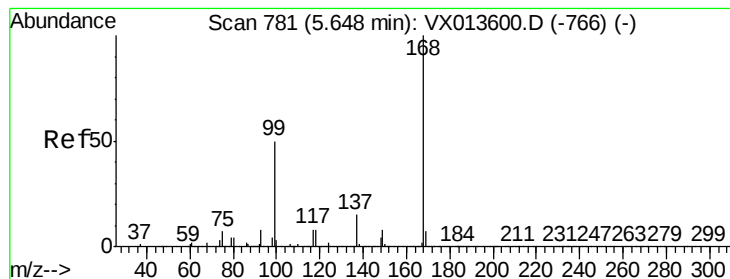

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. 0.00 min

Lab File: VX013847.D

Acq: 09 Dec 2019 13:21

Instrument :

MSVOA_X

ClientSampleId :


VX1209WBL01

Tot Ion:168 Resp: 614301

Ion Ratio Lower Upper

168 100

99 51.1 39.8 59.8

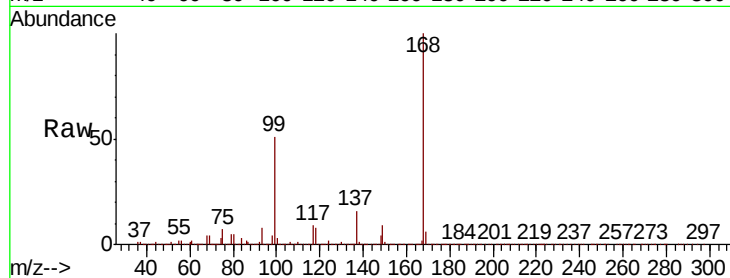

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000



150000

100000

50000

0

Time-->

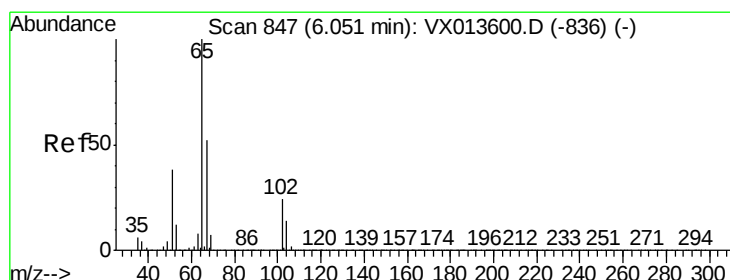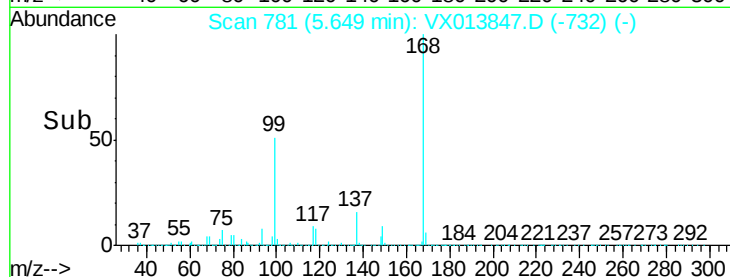

#33

1,2-Dichloroethane-d4

Concen: 47.896 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX013847.D


Acq: 09 Dec 2019 13:21

Tgt Ion: 65 Resp: 341531

Ion Ratio Lower Upper

65 100

67 53.4 0.0 104.4

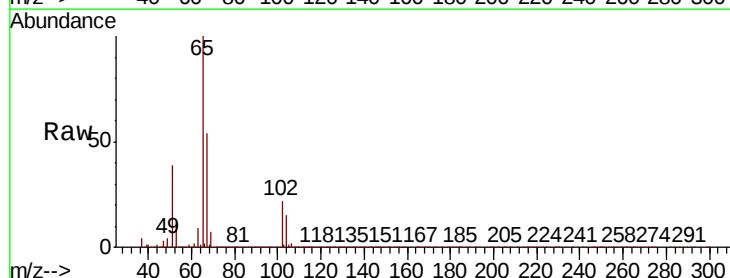

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0


150000


100000

50000

0

Time-->

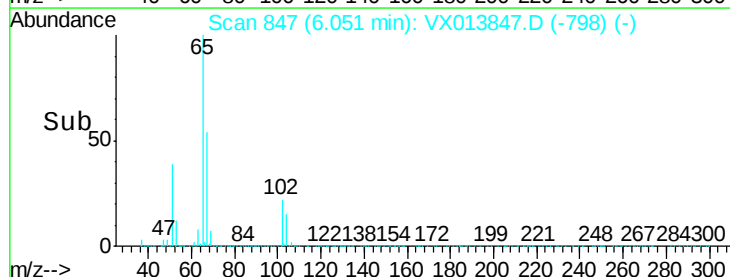

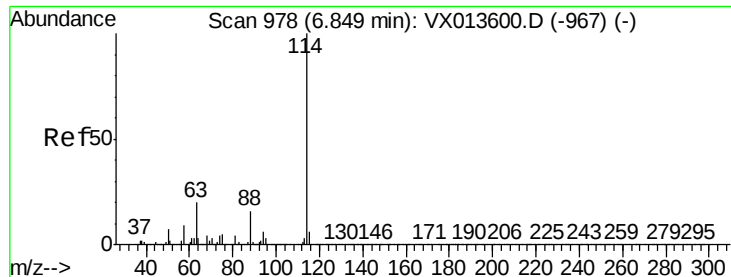

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX013847.D

Acq: 09 Dec 2019 13:21

Instrument :

MSVOA_X

ClientSampleId :

VX1209WBL01


Tot Ion:114 Resp: 941182

Ion Ratio Lower Upper

114 100

63 19.4 0.0 39.6




88 15.0 0.0 31.4

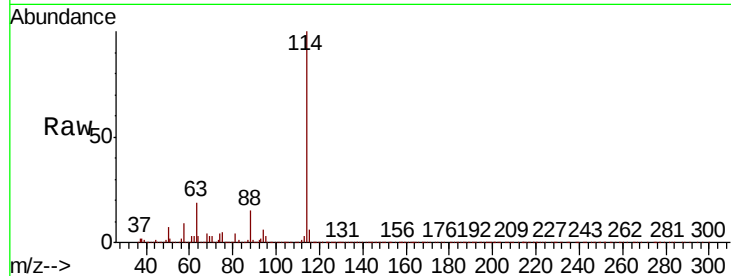

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

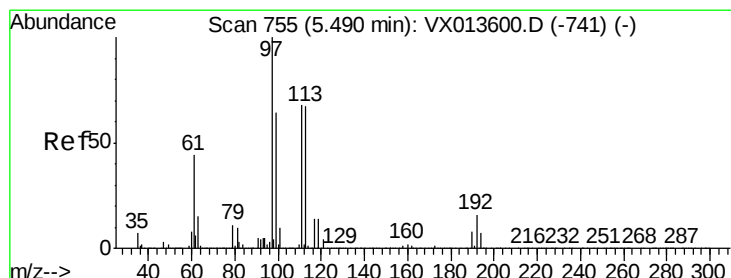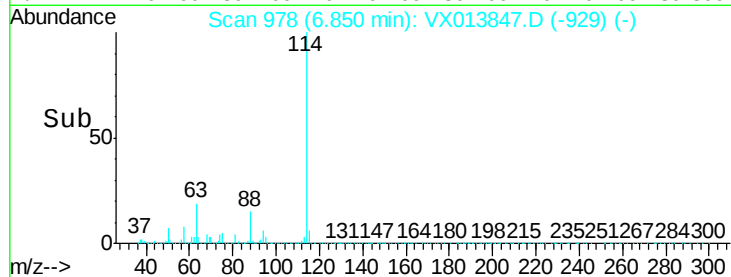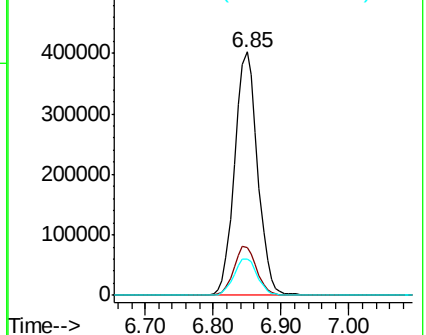

#35

Dibromofluoromethane

Concen: 48.230 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.01 min

Lab File: VX013847.D

Acq: 09 Dec 2019 13:21


Tgt Ion:113 Resp: 280625

Ion Ratio Lower Upper

113 100

111 103.3 83.6 125.4



192 22.9 19.2 28.8

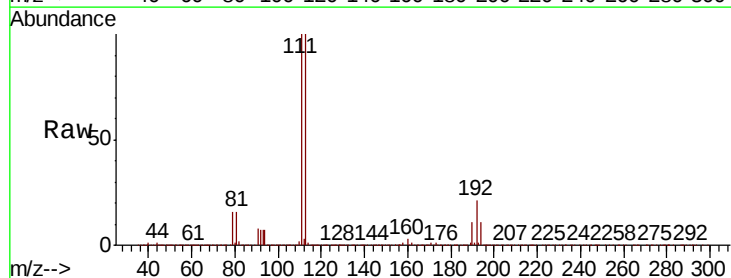


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

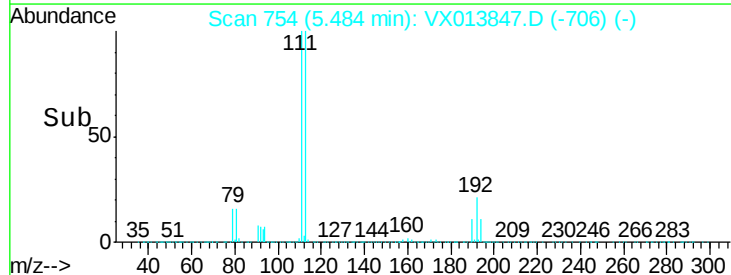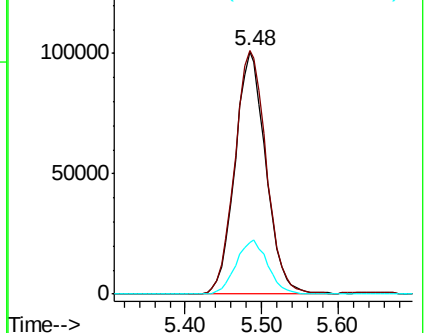

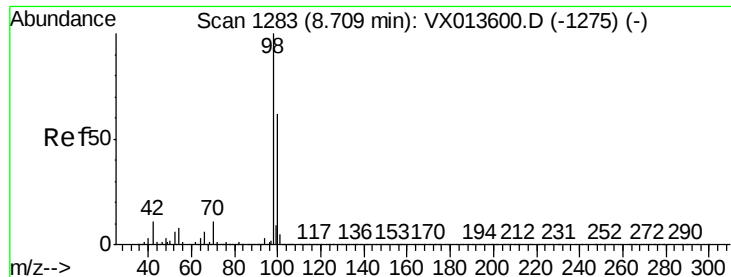

#50

Toluene-d8

Concen: 49.034 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX013847.D

Acq: 09 Dec 2019 13:21

Instrument :

MSVOA_X

ClientSampleId :





VX1209WBL01

Tot Ion: 98 Resp: 1111585

Ion Ratio Lower Upper

98 100

100 66.1 53.1 79.7

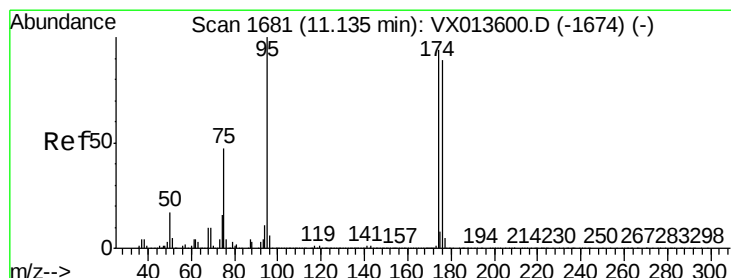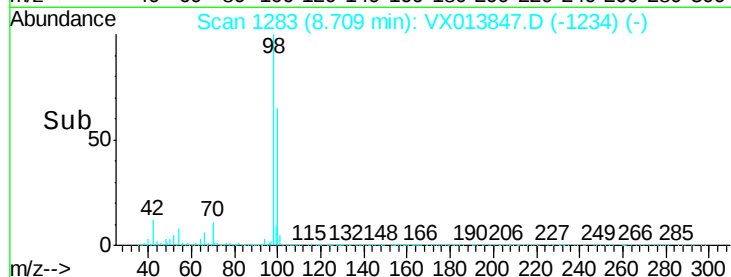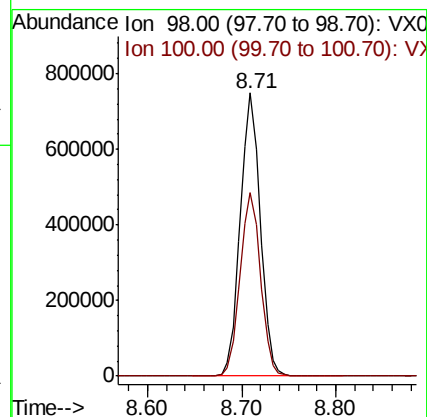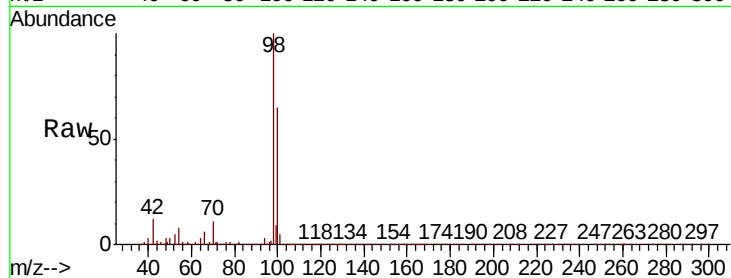

#62

4-Bromofluorobenzene

Concen: 46.733 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX013847.D

Acq: 09 Dec 2019 13:21




Tgt Ion: 95 Resp: 382032


Ion Ratio Lower Upper

95 100

174 87.9 0.0 180.0

176 85.3 0.0 173.6


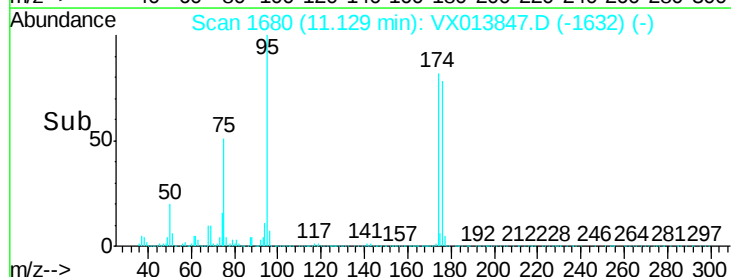
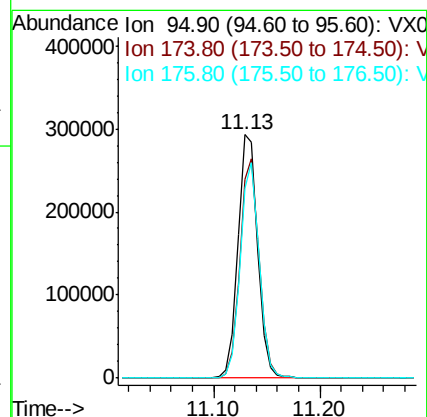
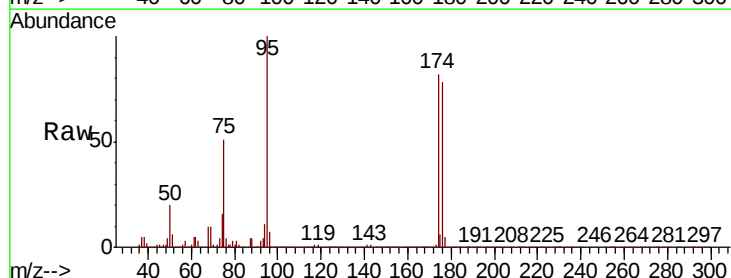


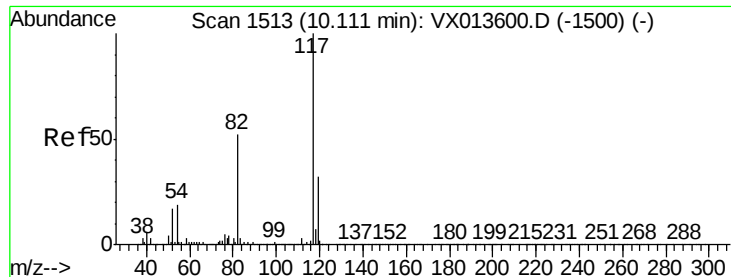

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013847.D
Acq: 09 Dec 2019 13:21

Instrument :
MSVOA_X
ClientSampleId :
VX1209WBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	58.0	41.8	62.8
119	32.2	25.8	38.8

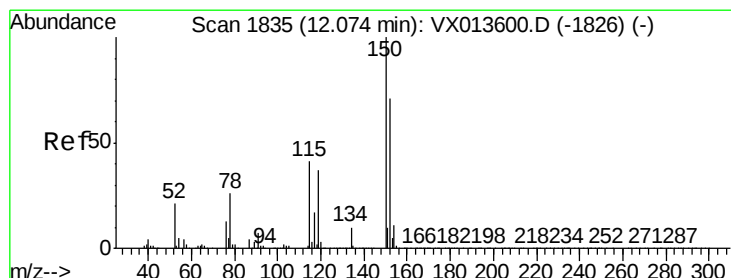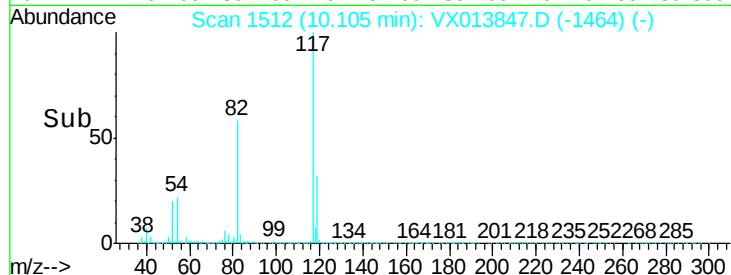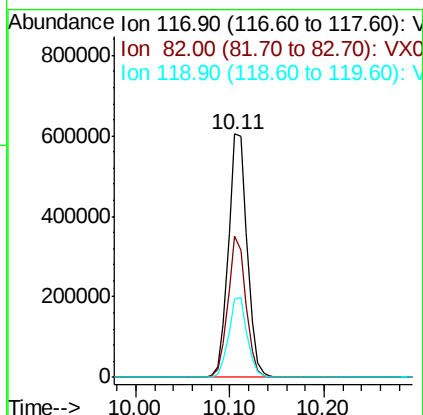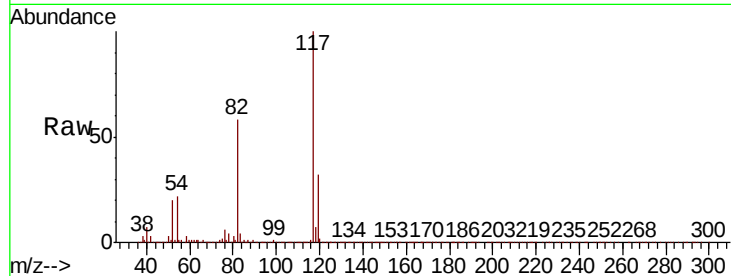

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX013847.D
Acq: 09 Dec 2019 13:21

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.0	38.4	115.1
150	158.0	0.0	346.8

