

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120720\
 Data File : BG047625.D
 Acq On : 7 Dec 2020 20:06
 Operator : CG/JU
 Sample : PB133251BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	11	12	15	rBV3	2170	1798	0.15%	0.016%
2	3.470	20	22	24	rBV3	2457	1785	0.15%	0.016%
3	3.541	30	34	39	rBV3	6317	9172	0.78%	0.083%
4	3.723	63	65	67	rBV2	2295	1718	0.15%	0.016%
5	4.240	151	153	158	rVB	1465	1920	0.16%	0.017%
6	4.322	163	167	168	rBV2	1678	2102	0.18%	0.019%
7	4.451	185	189	191	rBV	1595	2041	0.17%	0.019%
8	4.510	195	199	201	rVV	3163	3528	0.30%	0.032%
9	4.528	201	202	205	rVB	2761	1858	0.16%	0.017%
10	4.692	229	230	235	rBV	1390	1882	0.16%	0.017%
11	4.986	278	280	282	rVB	1803	1780	0.15%	0.016%
12	5.385	345	348	351	rBV	1982	1944	0.16%	0.018%
13	5.615	385	387	390	rVB	1448	1640	0.14%	0.015%
14	5.662	394	395	400	rBV	1791	2217	0.19%	0.020%
15	6.026	454	457	460	rVB	1656	1690	0.14%	0.015%
16	6.461	528	531	535	rBV	2111	2526	0.21%	0.023%
17	6.608	554	556	560	rVB	1252	1715	0.15%	0.016%
18	6.696	568	571	572	rBV	1849	1813	0.15%	0.016%
19	6.725	574	576	578	rVB	2441	1663	0.14%	0.015%
20	7.354	676	683	690	rBV	162007	280908	23.82%	2.555%
21	7.465	699	702	705	rVB	2300	2370	0.20%	0.022%
22	7.524	705	712	721	rBV	94798	166301	14.10%	1.512%
23	7.741	739	749	758	rBV2	157464	286424	24.29%	2.605%
24	8.217	822	830	837	rVB2	111587	189781	16.09%	1.726%
25	8.353	850	853	855	rBV2	1634	1843	0.16%	0.017%
26	8.911	939	948	956	rBV2	192474	339171	28.76%	3.085%
27	8.999	961	963	966	rVB	1783	1771	0.15%	0.016%
28	9.381	1020	1028	1037	rBV	163359	288408	24.46%	2.623%
29	10.109	1144	1152	1162	rBV	156909	289664	24.56%	2.634%
30	10.650	1237	1244	1253	rBV2	217697	382475	32.43%	3.479%
31	10.832	1274	1275	1280	rBV2	1223	1622	0.14%	0.015%
32	11.044	1304	1311	1324	rVB	138395	246735	20.92%	2.244%
33	11.167	1324	1332	1339	rBV	187388	344720	29.23%	3.135%
34	11.549	1392	1397	1399	rBV	1198	1636	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120720\
 Data File : BG047625.D
 Acq On : 7 Dec 2020 20:06
 Operator : CG/JU
 Sample : PB133251BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	12.036	1477	1480	1483	rBV	1535	2397	0.20%	0.022%
36	12.424	1543	1546	1550	rVB	1491	2044	0.17%	0.019%
37	12.606	1573	1577	1582	rVB2	2992	4665	0.40%	0.042%
38	12.994	1641	1643	1645	rVB2	1894	1642	0.14%	0.015%
39	13.552	1737	1738	1742	rVB2	2208	1894	0.16%	0.017%
40	13.770	1773	1775	1777	rBV2	1876	1773	0.15%	0.016%
41	13.946	1802	1805	1808	rBV2	1791	2399	0.20%	0.022%
42	13.993	1812	1813	1817	rBV2	1431	1895	0.16%	0.017%
43	14.228	1845	1853	1862	rBV	427946	621863	52.74%	5.656%
44	14.534	1897	1905	1912	rBV	400377	627651	53.23%	5.708%
45	14.833	1950	1956	1963	rBV	223874	359446	30.48%	3.269%
46	15.004	1978	1985	1992	rBV	201330	331322	28.10%	3.013%
47	15.092	1997	2000	2001	rVV3	3530	3525	0.30%	0.032%
48	15.133	2004	2007	2011	rVB	2649	3151	0.27%	0.029%
49	15.262	2027	2029	2033	rBV	2051	2323	0.20%	0.021%
50	15.820	2117	2124	2132	rVB	539749	805336	68.29%	7.324%
51	15.926	2136	2142	2150	rVV	205437	315719	26.77%	2.871%
52	15.979	2150	2151	2158	rVB	2035	3196	0.27%	0.029%
53	16.061	2161	2165	2169	rBV	7967	11535	0.98%	0.105%
54	16.220	2190	2192	2198	rVV	1967	1920	0.16%	0.017%
55	16.267	2198	2200	2205	rVB	1404	2109	0.18%	0.019%
56	16.502	2232	2240	2245	rBV	1859	3606	0.31%	0.033%
57	16.602	2253	2257	2261	rBV2	3870	5029	0.43%	0.046%
58	16.749	2280	2282	2286	rVB2	1513	2045	0.17%	0.019%
59	16.954	2313	2317	2318	rVB	2066	2035	0.17%	0.019%
60	16.978	2320	2321	2326	rVB	2023	2375	0.20%	0.022%
61	17.066	2334	2336	2339	rBV	1697	2098	0.18%	0.019%
62	17.142	2348	2349	2352	rVB	2230	1935	0.16%	0.018%
63	17.177	2352	2355	2356	rBV	2104	2276	0.19%	0.021%
64	17.360	2383	2386	2390	rVB	3788	3470	0.29%	0.032%
65	17.430	2396	2398	2401	rVB	1571	1603	0.14%	0.015%
66	17.571	2416	2422	2429	rBV	320457	499283	42.34%	4.541%
67	17.671	2432	2439	2445	rBV2	611617	932325	79.06%	8.479%
68	17.918	2478	2481	2482	rBV	2213	1959	0.17%	0.018%
69	18.100	2510	2512	2514	rBV	2442	1947	0.17%	0.018%
70	18.358	2554	2556	2560	rVB2	2398	2414	0.20%	0.022%
71	18.417	2565	2566	2571	rVB2	2164	1996	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120720\
 Data File : BG047625.D
 Acq On : 7 Dec 2020 20:06
 Operator : CG/JU
 Sample : PB133251BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

72	18.746	2619	2622	2625	rBV2	1328	1764	0.15%	0.016%
73	18.793	2627	2630	2633	rBV	2398	3416	0.29%	0.031%
74	18.917	2645	2651	2652	rBV	2743	3094	0.26%	0.028%
75	19.005	2663	2666	2669	rBV	2282	3095	0.26%	0.028%
76	19.052	2672	2674	2676	rBV	3225	3772	0.32%	0.034%
77	19.128	2683	2687	2688	rBV3	2235	2741	0.23%	0.025%
78	19.263	2706	2710	2713	rBV3	2999	4208	0.36%	0.038%
79	19.293	2713	2715	2716	rVV	2864	2017	0.17%	0.018%
80	19.475	2743	2746	2747	rBV	1776	1983	0.17%	0.018%
81	19.575	2760	2763	2768	rVB3	10142	12017	1.02%	0.109%
82	19.798	2799	2801	2803	rBV	3418	3136	0.27%	0.029%
83	19.939	2819	2825	2831	rBV	833012	1179219	100.00%	10.725%
84	20.421	2905	2907	2909	rBV3	4195	3904	0.33%	0.036%
85	20.967	2998	3000	3001	rVB2	5815	2567	0.22%	0.023%
86	21.843	3143	3149	3158	rVB2	342928	601554	51.01%	5.471%
87	24.980	3672	3683	3697	rBV3	355118	1066024	90.40%	9.695%
88	25.209	3713	3722	3735	rVB2	193889	596325	50.57%	5.424%
89	26.425	3922	3929	3936	rBV10	19001	56443	4.79%	0.513%
90	27.248	4067	4069	4071	rBV2	6864	5032	0.43%	0.046%


Sum of corrected areas: 10995133

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120720\
Data File : BG047625.D
Acq On : 7 Dec 2020 20:06
Operator : CG/JU
Sample : PB133251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

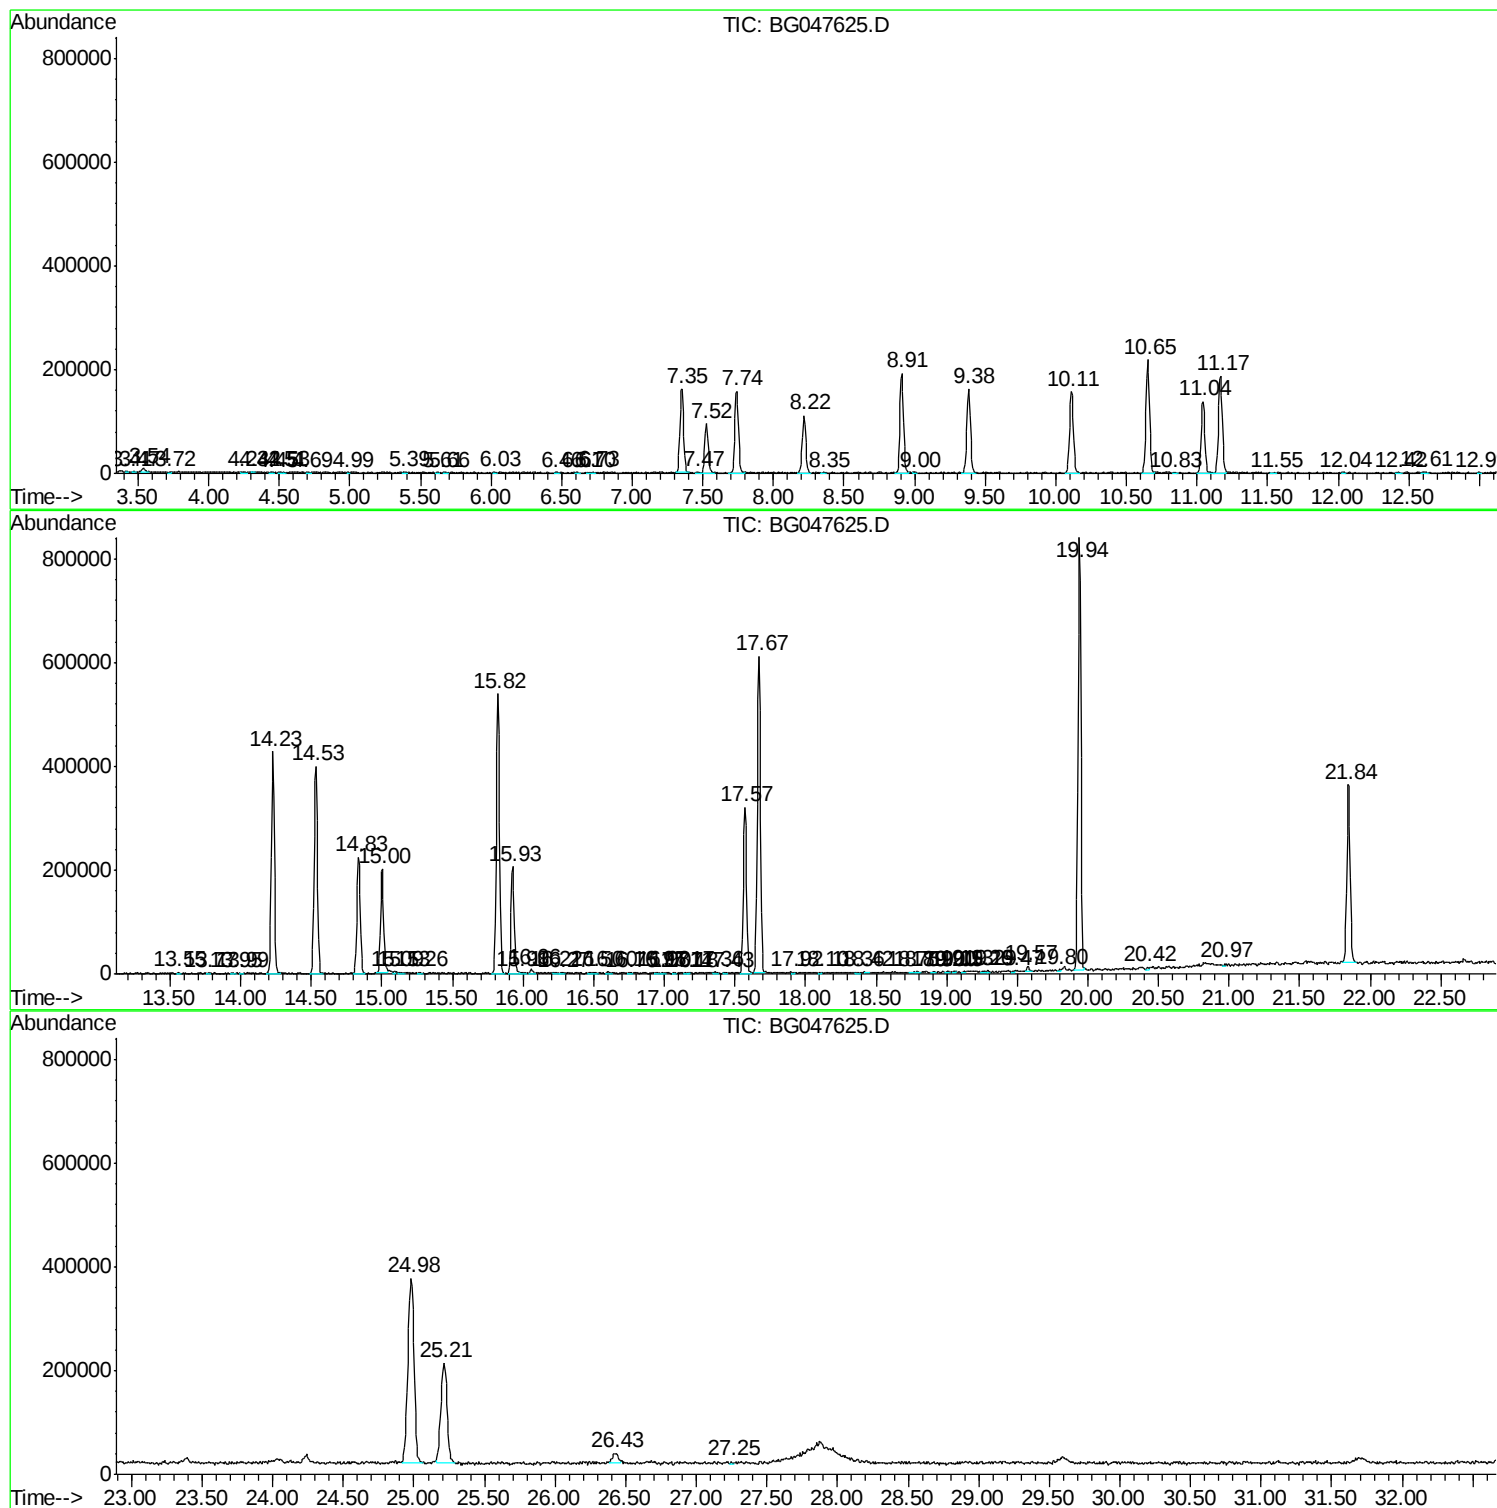

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120720\
Data File : BG047625.D
Acq On : 7 Dec 2020 20:06
Operator : CG/JU
Sample : PB133251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120720\
Data File : BG047625.D
Acq On : 7 Dec 2020 20:06
Operator : CG/JU
Sample : PB133251BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc