


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120920\  
Data File : VX019794.D  
Acq On : 09 Dec 2020 21:59  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X120420W.M  
Title : SW846 8260  
Last Update : Fri Dec 04 15:32:53 2020

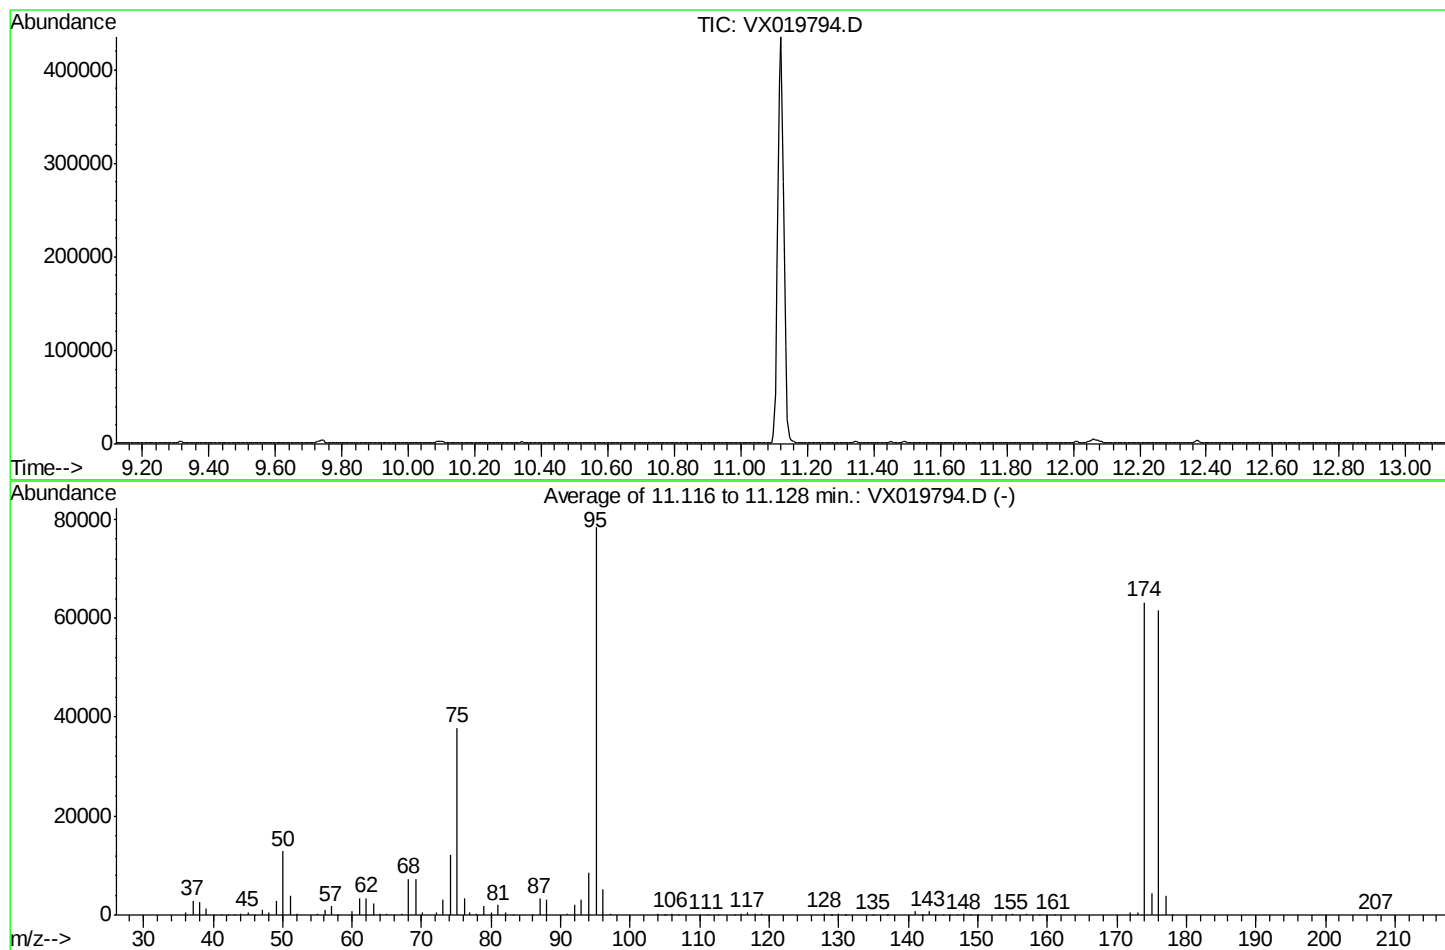

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.5      | 12893   | PASS             |
| 75          | 95           | 30           | 60           | 48.2      | 37802   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 78365   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 5302    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.7       | 453     | PASS             |
| 174         | 95           | 50           | 100          | 80.6      | 63200   | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 4481    | PASS             |
| 176         | 174          | 95           | 101          | 97.4      | 61536   | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 3818    | PASS             |