

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025658.D
 Acq On : 09 Dec 2021 14:29
 Operator : JC/MD
 Sample : VIBLK615
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	43637	42807	11.29%	1.274%
2	1.666	91	95	104	rBV	39247	52678	13.89%	1.568%
3	2.306	194	200	210	rVB	65670	107996	28.48%	3.214%
4	2.471	225	227	229	rVB	499	342	0.09%	0.010%
5	2.666	258	259	261	rVV	335	202	0.05%	0.006%
6	2.794	274	280	287	rBV3	3272	6152	1.62%	0.183%
7	2.940	299	304	308	rBV2	1443	3046	0.80%	0.091%
8	3.136	335	336	338	rBV	304	241	0.06%	0.007%
9	3.312	363	365	367	rBV2	280	321	0.08%	0.010%
10	3.349	369	371	373	rBV2	331	350	0.09%	0.010%
11	3.489	392	394	396	rVB	392	241	0.06%	0.007%
12	3.532	399	401	403	rBV	364	336	0.09%	0.010%
13	3.776	436	441	442	rBV2	337	656	0.17%	0.020%
14	3.818	447	448	453	rVV	292	373	0.10%	0.011%
15	4.026	481	482	484	rVB	484	225	0.06%	0.007%
16	4.050	484	486	489	rBV	264	392	0.10%	0.012%
17	4.190	508	509	511	rBV2	246	231	0.06%	0.007%
18	4.452	543	552	568	rBV	39775	111257	29.34%	3.311%
19	4.940	630	632	634	rBV	275	211	0.06%	0.006%
20	5.056	640	651	667	rVB	51376	163382	43.09%	4.862%
21	5.214	673	677	679	rBV	233	210	0.06%	0.006%
22	5.495	721	723	725	rVB	309	238	0.06%	0.007%
23	5.531	728	729	730	rBV	392	256	0.07%	0.008%
24	5.629	743	745	750	rVB2	264	256	0.07%	0.008%
25	5.702	755	757	759	rVB	394	278	0.07%	0.008%
26	5.733	759	762	765	rBV	286	345	0.09%	0.010%
27	5.763	765	767	770	rBV	312	327	0.09%	0.010%
28	5.867	782	784	786	rBV	312	255	0.07%	0.008%
29	5.970	790	801	817	rVB2	123053	367647	96.97%	10.941%
30	6.190	835	837	838	rBV	280	261	0.07%	0.008%
31	6.300	854	855	858	rVV2	305	222	0.06%	0.007%
32	6.385	866	869	871	rVB2	262	305	0.08%	0.009%
33	6.409	871	873	879	rBV2	236	434	0.11%	0.013%
34	6.483	883	885	888	rBV2	236	282	0.07%	0.008%
35	6.550	892	896	897	rVB3	353	386	0.10%	0.011%
36	6.641	909	911	914	rBV2	235	224	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025658.D
 Acq On : 09 Dec 2021 14:29
 Operator : JC/MD
 Sample : VIBLK615
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	6.763	920	931	944	rBV	131530	317132	83.64%	9.438%
38	6.891	951	952	954	rBV	305	208	0.05%	0.006%
39	6.909	954	955	958	rVB	433	311	0.08%	0.009%
40	6.958	961	963	965	rBV	408	299	0.08%	0.009%
41	7.025	971	974	977	rVB2	258	305	0.08%	0.009%
42	7.117	979	989	998	rVV6	6322	16451	4.34%	0.490%
43	7.220	1004	1006	1009	rBV2	391	385	0.10%	0.011%
44	7.312	1011	1021	1031	rBV	80104	175872	46.39%	5.234%
45	7.501	1051	1052	1055	rVB2	404	289	0.08%	0.009%
46	7.537	1055	1058	1060	rBV	411	563	0.15%	0.017%
47	7.805	1100	1102	1104	rVV2	352	278	0.07%	0.008%
48	7.824	1104	1105	1108	rVB	512	392	0.10%	0.012%
49	7.879	1112	1114	1115	rBV2	251	238	0.06%	0.007%
50	7.927	1119	1122	1125	rBV2	379	485	0.13%	0.014%
51	8.025	1135	1138	1139	rBV	356	236	0.06%	0.007%
52	8.068	1142	1145	1147	rVB2	304	283	0.07%	0.008%
53	8.190	1163	1165	1166	rBV	353	247	0.07%	0.007%
54	8.232	1170	1172	1175	rBV2	240	254	0.07%	0.008%
55	8.324	1181	1187	1195	rBV	56207	90172	23.78%	2.684%
56	8.592	1229	1231	1234	rVV	209	245	0.06%	0.007%
57	8.647	1234	1240	1248	rVV	168848	271683	71.66%	8.085%
58	8.714	1249	1251	1256	rVB	1819	2763	0.73%	0.082%
59	8.891	1279	1280	1283	rVB2	355	257	0.07%	0.008%
60	8.952	1284	1290	1298	rVV	39998	57450	15.15%	1.710%
61	9.086	1310	1312	1315	rVV2	208	209	0.06%	0.006%
62	9.153	1320	1323	1325	rBV2	157	206	0.05%	0.006%
63	9.275	1339	1343	1349	rVB3	2815	4080	1.08%	0.121%
64	9.336	1352	1353	1355	rBV	302	202	0.05%	0.006%
65	9.384	1355	1361	1375	rBV	169055	237485	62.64%	7.068%
66	9.519	1381	1383	1385	rBV	362	340	0.09%	0.010%
67	9.830	1432	1434	1435	rBV	228	207	0.05%	0.006%
68	9.951	1452	1454	1456	rBV	343	232	0.06%	0.007%
69	10.055	1465	1471	1483	rBV	283207	379151	100.00%	11.284%
70	10.171	1488	1490	1497	rVB2	279	424	0.11%	0.013%
71	10.226	1497	1499	1502	rBV	323	308	0.08%	0.009%
72	10.421	1529	1531	1533	rBV2	236	227	0.06%	0.007%
73	10.567	1551	1555	1557	rBV2	214	362	0.10%	0.011%
74	10.640	1564	1567	1571	rBV	390	474	0.13%	0.014%
75	10.811	1593	1595	1599	rVB2	239	291	0.08%	0.009%
76	10.939	1613	1616	1621	rBV2	224	441	0.12%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025658.D
 Acq On : 09 Dec 2021 14:29
 Operator : JC/MD
 Sample : VIBLK615
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	11.195	1652	1658	1665	rVV	177690	228131	60.17%	6.789%
78	11.415	1693	1694	1696	rBV2	427	392	0.10%	0.012%
79	11.500	1703	1708	1709	rBV	324	410	0.11%	0.012%
80	11.512	1709	1710	1713	rVV2	243	310	0.08%	0.009%
81	11.555	1715	1717	1719	rVB	280	238	0.06%	0.007%
82	11.750	1745	1749	1753	rBV2	520	846	0.22%	0.025%
83	12.024	1788	1794	1804	rVB	297179	372800	98.32%	11.095%
84	12.189	1819	1821	1823	rBV	370	353	0.09%	0.011%
85	12.323	1837	1843	1852	rBV	244722	305631	80.61%	9.096%
86	12.475	1866	1868	1869	rBV	297	308	0.08%	0.009%
87	12.609	1888	1890	1893	rBV	262	224	0.06%	0.007%
88	12.884	1920	1935	1937	rBV3	4424	13564	3.58%	0.404%
89	13.042	1959	1961	1965	rBV2	293	322	0.08%	0.010%
90	13.603	2052	2053	2058	rBV	313	325	0.09%	0.010%
91	13.780	2078	2082	2086	rVB	5592	7167	1.89%	0.213%
92	14.140	2137	2141	2144	rBV4	933	1499	0.40%	0.045%
93	14.865	2259	2260	2263	rBV	363	315	0.08%	0.009%
94	15.188	2311	2313	2315	rBV2	352	284	0.07%	0.008%
95	15.365	2340	2342	2346	rBV2	257	387	0.10%	0.012%
96	15.505	2364	2365	2367	rVB	304	218	0.06%	0.006%
97	15.938	2434	2436	2439	rBV2	309	392	0.10%	0.012%
98	16.084	2457	2460	2461	rBV2	588	524	0.14%	0.016%
99	16.633	2548	2550	2553	rBV3	387	502	0.13%	0.015%
100	16.658	2553	2554	2555	rBV	435	221	0.06%	0.007%




Sum of corrected areas: 3360165

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025658.D
Acq On : 09 Dec 2021 14:29
Operator : JC/MD
Sample : VIBLK615
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

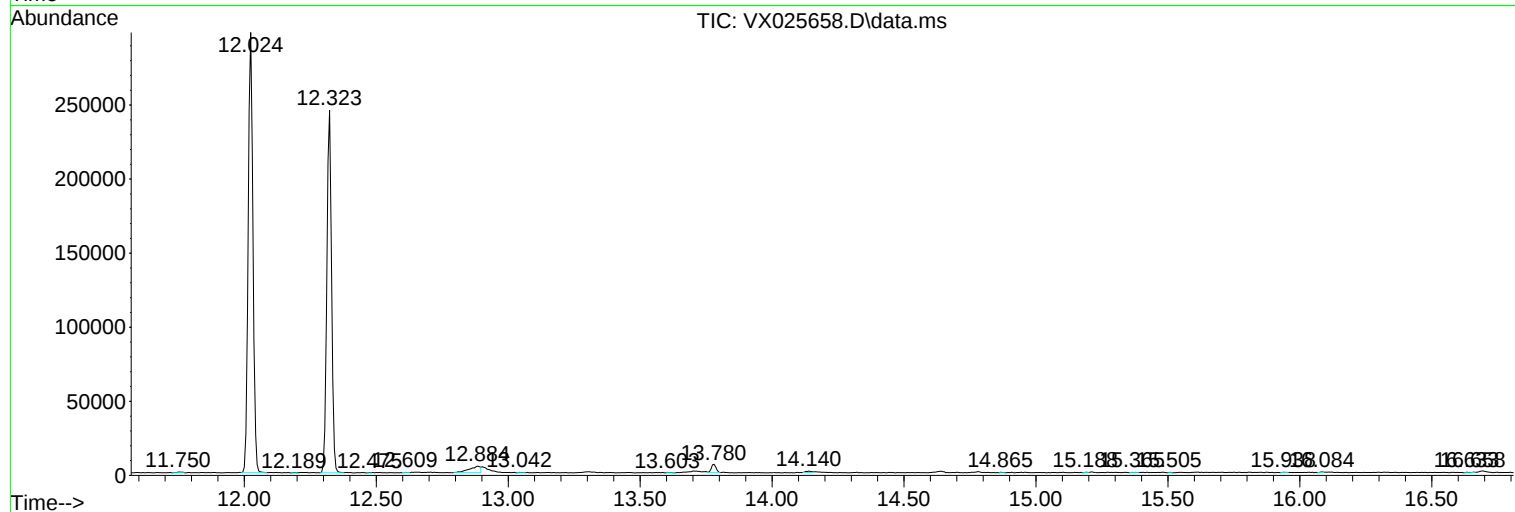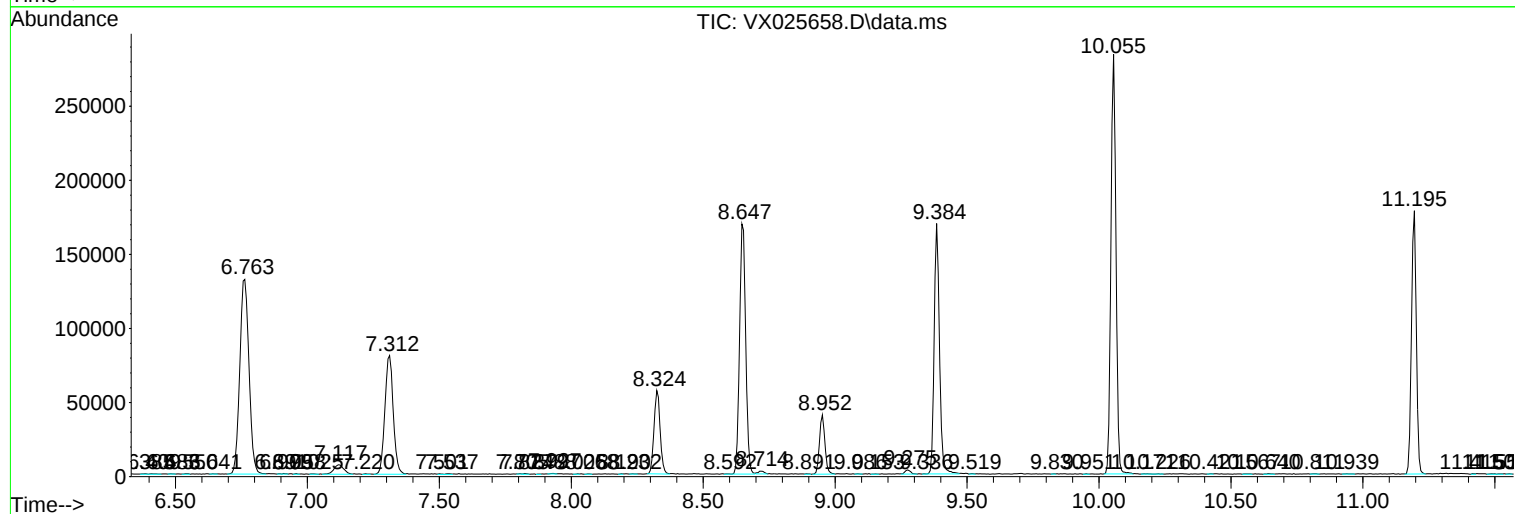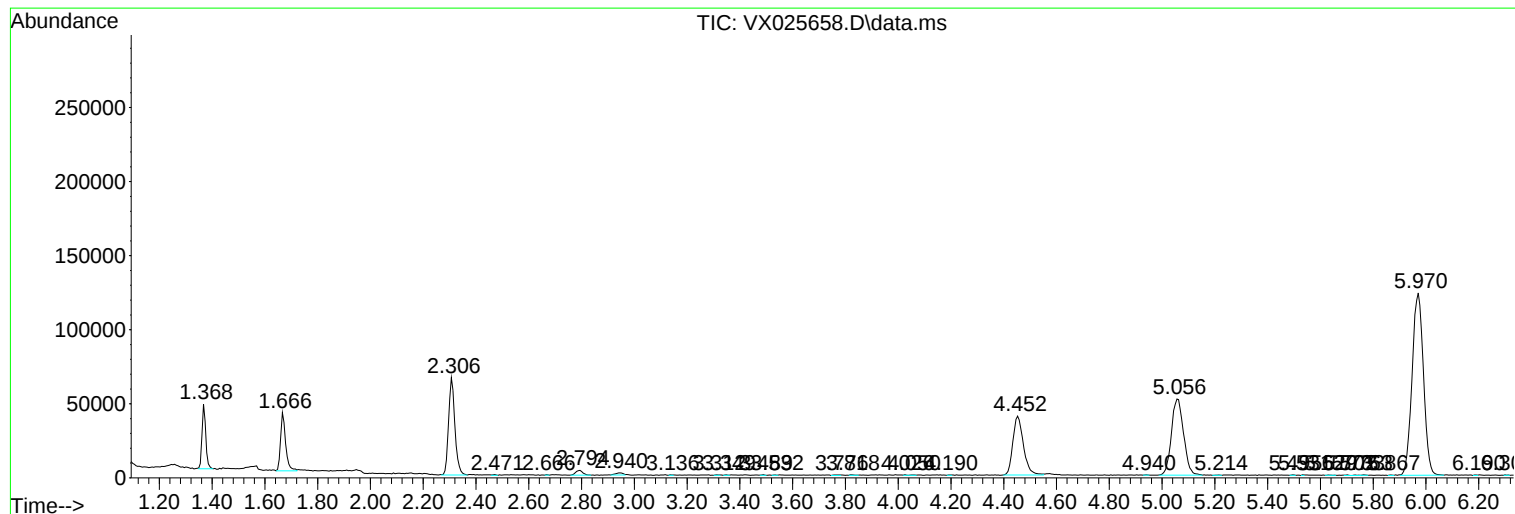

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025658.D
Acq On : 09 Dec 2021 14:29
Operator : JC/MD
Sample : VIBLK615
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025658.D
Acq On : 09 Dec 2021 14:29
Operator : JC/MD
Sample : VIBLK615
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc