

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025666.D
 Acq On : 09 Dec 2021 17:52
 Operator : JC/MD
 Sample : VX1209MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	75859	70593	16.52%	2.061%
2	1.666	91	95	105	rVB	47560	64119	15.01%	1.872%
3	2.307	194	200	211	rVB	101938	163304	38.22%	4.768%
4	2.666	257	259	263	rVB2	217	226	0.05%	0.007%
5	2.770	274	276	277	rBV	297	276	0.06%	0.008%
6	2.788	277	279	287	rVB4	991	1417	0.33%	0.041%
7	2.947	297	305	313	rBV2	2704	6839	1.60%	0.200%
8	3.069	322	325	328	rBV	267	343	0.08%	0.010%
9	3.239	350	353	355	rBV2	335	376	0.09%	0.011%
10	3.392	375	378	380	rBV2	218	224	0.05%	0.007%
11	4.099	491	494	496	rBB	309	309	0.07%	0.009%
12	4.123	496	498	501	rBV	304	321	0.08%	0.009%
13	4.190	506	509	511	rBV2	353	376	0.09%	0.011%
14	4.453	544	552	564	rBV	31312	89199	20.87%	2.604%
15	4.690	587	591	592	rBV	363	343	0.08%	0.010%
16	4.739	597	599	601	rVV	338	264	0.06%	0.008%
17	4.757	601	602	607	rVB	289	351	0.08%	0.010%
18	4.818	610	612	614	rBV	260	245	0.06%	0.007%
19	5.056	637	651	668	rBV	54814	172907	40.46%	5.048%
20	5.446	714	715	718	rVB	281	213	0.05%	0.006%
21	5.544	728	731	732	rBV	309	350	0.08%	0.010%
22	5.556	732	733	735	rVB	589	336	0.08%	0.010%
23	5.666	748	751	752	rBV	336	311	0.07%	0.009%
24	5.684	752	754	757	rVB	272	330	0.08%	0.010%
25	5.727	757	761	763	rBV	271	434	0.10%	0.013%
26	5.971	789	801	815	rBV2	144064	427313	100.00%	12.475%
27	6.373	864	867	871	rBV2	246	496	0.12%	0.014%
28	6.702	919	921	922	rBV	286	290	0.07%	0.008%
29	6.763	922	931	942	rVV	119838	284146	66.50%	8.295%
30	6.885	950	951	952	rBV	553	264	0.06%	0.008%
31	6.958	962	963	966	rVB	496	317	0.07%	0.009%
32	7.050	975	978	980	rBV	370	523	0.12%	0.015%
33	7.117	982	989	994	rVB6	1985	4985	1.17%	0.146%
34	7.312	1012	1021	1035	rVB	84235	189350	44.31%	5.528%
35	7.440	1041	1042	1046	rBV	334	279	0.07%	0.008%
36	7.592	1065	1067	1070	rBV	335	332	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025666.D
 Acq On : 09 Dec 2021 17:52
 Operator : JC/MD
 Sample : VX1209MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.757	1092	1094	1096	rVB	356	262	0.06%	0.008%
38	8.043	1138	1141	1145	rBV	480	830	0.19%	0.024%
39	8.074	1145	1146	1148	rBV	271	225	0.05%	0.007%
40	8.324	1180	1187	1196	rBV	63180	104752	24.51%	3.058%
41	8.647	1234	1240	1249	rVV	230871	364382	85.27%	10.638%
42	8.720	1249	1252	1258	rVB3	3363	4994	1.17%	0.146%
43	8.872	1273	1277	1278	rBV2	275	340	0.08%	0.010%
44	8.915	1282	1284	1285	rBV	255	267	0.06%	0.008%
45	8.952	1285	1290	1299	rVV	45277	65485	15.32%	1.912%
46	9.037	1303	1304	1305	rBV	372	231	0.05%	0.007%
47	9.275	1340	1343	1347	rVB2	1507	1911	0.45%	0.056%
48	9.336	1351	1353	1355	rBV	344	361	0.08%	0.011%
49	9.385	1356	1361	1373	rBV	142384	198436	46.44%	5.793%
50	9.537	1385	1386	1389	rBV	414	262	0.06%	0.008%
51	9.696	1411	1412	1418	rVB2	624	756	0.18%	0.022%
52	9.824	1430	1433	1434	rBV	232	206	0.05%	0.006%
53	9.866	1438	1440	1441	rBV	246	220	0.05%	0.006%
54	9.915	1445	1448	1450	rBV	388	370	0.09%	0.011%
55	9.982	1457	1459	1462	rBV	335	362	0.08%	0.011%
56	10.006	1462	1463	1465	rVV	359	324	0.08%	0.009%
57	10.055	1465	1471	1484	rVV	253598	341606	79.94%	9.973%
58	10.165	1487	1489	1491	rVB	353	277	0.06%	0.008%
59	10.195	1491	1494	1495	rBV2	396	441	0.10%	0.013%
60	10.299	1510	1511	1513	rBV	583	400	0.09%	0.012%
61	10.391	1522	1526	1527	rBV2	335	417	0.10%	0.012%
62	10.458	1535	1537	1540	rBV	293	279	0.07%	0.008%
63	10.512	1545	1546	1550	rBV2	264	300	0.07%	0.009%
64	10.677	1571	1573	1574	rBV	241	260	0.06%	0.008%
65	10.793	1590	1592	1594	rVB	352	248	0.06%	0.007%
66	11.122	1640	1646	1650	rBV2	1841	2648	0.62%	0.077%
67	11.195	1652	1658	1665	rVB	156640	201712	47.20%	5.889%
68	11.311	1675	1677	1678	rBV2	434	336	0.08%	0.010%
69	11.451	1698	1700	1702	rBV2	345	361	0.08%	0.011%
70	11.476	1702	1704	1708	rVB3	475	551	0.13%	0.016%
71	11.549	1714	1716	1718	rBV	263	234	0.05%	0.007%
72	11.683	1733	1738	1739	rBV2	232	331	0.08%	0.010%
73	11.750	1745	1749	1753	rVV3	1729	2205	0.52%	0.064%
74	11.884	1767	1771	1774	rBV	208	298	0.07%	0.009%
75	11.933	1777	1779	1783	rVB3	682	871	0.20%	0.025%
76	12.024	1789	1794	1801	rBV	256047	321851	75.32%	9.396%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025666.D
 Acq On : 09 Dec 2021 17:52
 Operator : JC/MD
 Sample : VX1209MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.152	1812	1815	1819	rVB	1333	1559	0.36%	0.046%
78	12.323	1837	1843	1851	rVB	234910	305144	71.41%	8.908%
79	12.427	1857	1860	1863	rBV3	655	818	0.19%	0.024%
80	12.482	1867	1869	1872	rVB	345	290	0.07%	0.008%
81	12.622	1889	1892	1893	rBV	260	274	0.06%	0.008%
82	13.207	1986	1988	1991	rVB	405	348	0.08%	0.010%
83	13.244	1991	1994	1995	rBV2	356	420	0.10%	0.012%
84	13.280	1998	2000	2001	rBV	393	264	0.06%	0.008%
85	13.414	2020	2022	2024	rBV2	292	228	0.05%	0.007%
86	13.524	2036	2040	2043	rVB2	334	455	0.11%	0.013%
87	13.585	2048	2050	2055	rBV3	582	905	0.21%	0.026%
88	13.670	2060	2064	2065	rBV2	496	558	0.13%	0.016%
89	13.780	2078	2082	2089	rVB2	2749	3993	0.93%	0.117%
90	13.847	2089	2093	2094	rBV	229	330	0.08%	0.010%
91	13.926	2105	2106	2108	rBV	302	220	0.05%	0.006%
92	13.994	2115	2117	2118	rBV	356	245	0.06%	0.007%
93	14.012	2118	2120	2123	rVV2	237	238	0.06%	0.007%
94	14.085	2130	2132	2134	rVB	312	223	0.05%	0.007%
95	14.146	2134	2142	2145	rBV5	1542	3955	0.93%	0.115%
96	14.786	2243	2247	2249	rBV2	474	734	0.17%	0.021%
97	15.597	2378	2380	2381	rBV	349	278	0.07%	0.008%
98	15.749	2404	2405	2406	rBV	414	202	0.05%	0.006%
99	15.810	2413	2415	2419	rBV2	290	463	0.11%	0.014%
100	16.383	2507	2509	2511	rVB2	405	272	0.06%	0.008%


Sum of corrected areas: 3425319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025666.D
Acq On : 09 Dec 2021 17:52
Operator : JC/MD
Sample : VX1209MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK648

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

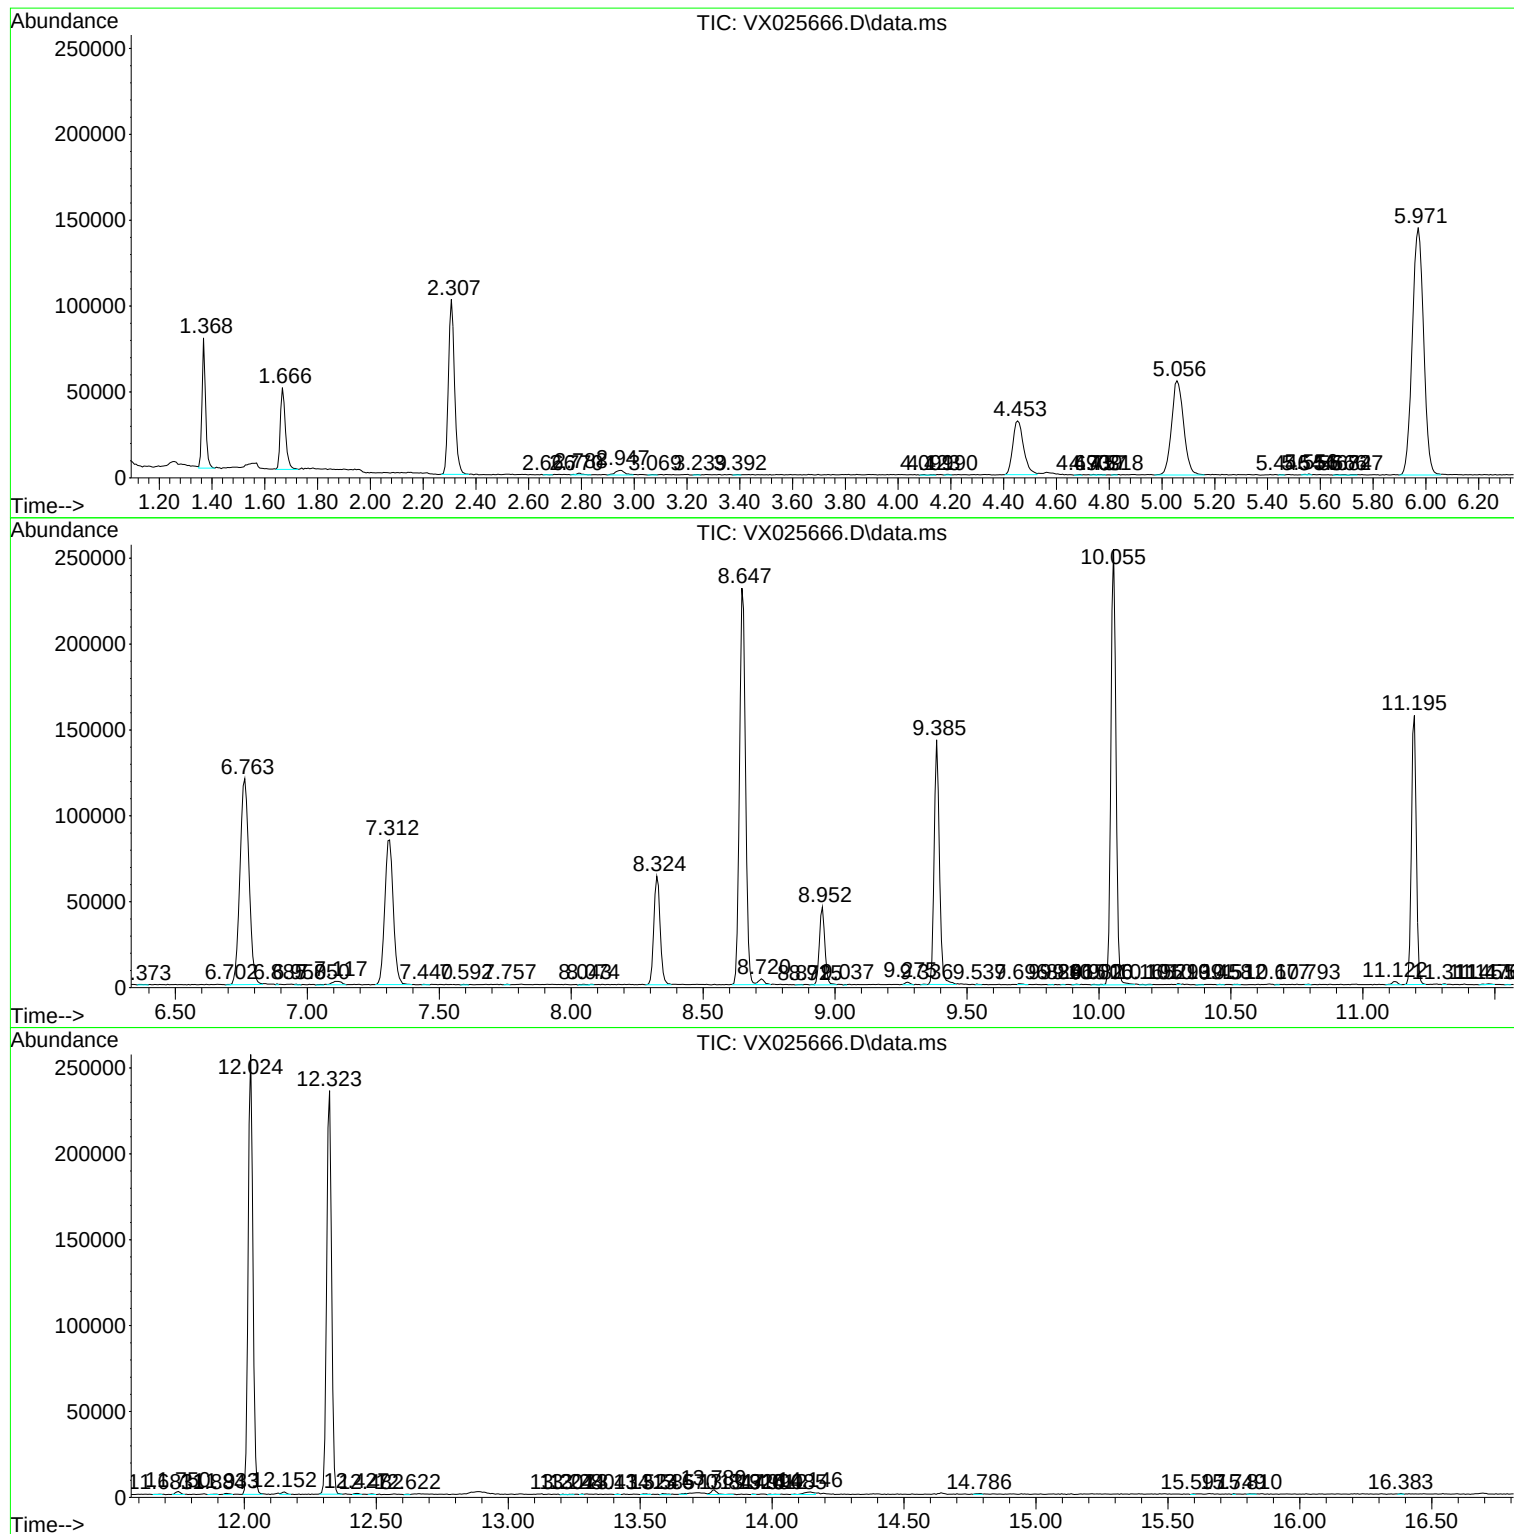

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025666.D
Acq On : 09 Dec 2021 17:52
Operator : JC/MD
Sample : VX1209MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK648

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025666.D
Acq On : 09 Dec 2021 17:52
Operator : JC/MD
Sample : VX1209MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK648

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc