

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025670.D
 Acq On : 09 Dec 2021 19:30
 Operator : JC/MD
 Sample : M4975-13ME
 Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rBV	48054	56677	13.64%	1.747%
2	1.648	88	92	98	rVB	32586	38557	9.28%	1.188%
3	2.282	190	196	206	rBV	91601	149068	35.88%	4.595%
4	2.514	232	234	235	rBV2	380	234	0.06%	0.007%
5	2.642	253	255	258	rBV	428	369	0.09%	0.011%
6	2.672	258	260	263	rBV2	562	553	0.13%	0.017%
7	2.947	300	305	312	rBV	3386	6928	1.67%	0.214%
8	4.489	549	558	576	rBV	17773	72890	17.54%	2.247%
9	4.788	605	607	610	rVB	333	178	0.04%	0.005%
10	5.068	642	653	670	rVB	52395	167474	40.31%	5.162%
11	5.257	682	684	687	rBV	205	206	0.05%	0.006%
12	5.330	694	696	697	rVB	331	175	0.04%	0.005%
13	5.355	697	700	701	rBV2	305	227	0.05%	0.007%
14	5.544	729	731	732	rBV	238	185	0.04%	0.006%
15	5.696	754	756	758	rBV	360	341	0.08%	0.011%
16	5.763	765	767	769	rBV	250	170	0.04%	0.005%
17	5.970	790	801	819	rBV2	145385	415509	100.00%	12.807%
18	6.263	848	849	852	rBV2	370	455	0.11%	0.014%
19	6.324	857	859	860	rBV	317	200	0.05%	0.006%
20	6.367	860	866	873	rBV5	1518	4461	1.07%	0.138%
21	6.763	922	931	943	rBV	111910	283537	68.24%	8.739%
22	7.007	969	971	974	rBV2	265	318	0.08%	0.010%
23	7.117	983	989	999	rVB8	1704	4807	1.16%	0.148%
24	7.220	999	1006	1012	rBV3	795	2175	0.52%	0.067%
25	7.312	1012	1021	1036	rVV	77051	181497	43.68%	5.594%
26	7.452	1040	1044	1046	rBV2	269	348	0.08%	0.011%
27	7.659	1075	1078	1079	rBV	207	212	0.05%	0.007%
28	7.708	1084	1086	1088	rVV	371	290	0.07%	0.009%
29	7.763	1092	1095	1099	rVB	168	284	0.07%	0.009%
30	7.921	1119	1121	1122	rBV	279	210	0.05%	0.006%
31	7.988	1130	1132	1134	rVB	253	210	0.05%	0.006%
32	8.013	1134	1136	1137	rBV	302	214	0.05%	0.007%
33	8.055	1141	1143	1145	rBV	273	230	0.06%	0.007%
34	8.250	1173	1175	1179	rVB2	226	203	0.05%	0.006%
35	8.330	1181	1188	1199	rVV	52511	93688	22.55%	2.888%
36	8.482	1211	1213	1216	rVB2	254	220	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025670.D
 Acq On : 09 Dec 2021 19:30
 Operator : JC/MD
 Sample : M4975-13ME
 Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.519	1216	1219	1220	rBV	247	225	0.05%	0.007%
38	8.549	1222	1224	1227	rBV2	177	200	0.05%	0.006%
39	8.580	1227	1229	1231	rVB	301	174	0.04%	0.005%
40	8.653	1234	1241	1248	rBV	215251	347662	83.67%	10.716%
41	8.811	1264	1267	1268	rBV	201	242	0.06%	0.007%
42	8.848	1271	1273	1276	rBV	204	316	0.08%	0.010%
43	8.909	1281	1283	1285	rVV	196	168	0.04%	0.005%
44	8.958	1285	1291	1299	rVB	34187	57068	13.73%	1.759%
45	9.073	1306	1310	1311	rBV2	308	463	0.11%	0.014%
46	9.159	1321	1324	1325	rBV2	330	269	0.06%	0.008%
47	9.202	1328	1331	1332	rBV2	232	236	0.06%	0.007%
48	9.275	1339	1343	1347	rVB2	5028	7069	1.70%	0.218%
49	9.323	1347	1351	1352	rBV	162	179	0.04%	0.006%
50	9.397	1357	1363	1375	rBV	105878	167410	40.29%	5.160%
51	9.531	1384	1385	1388	rBV2	345	224	0.05%	0.007%
52	9.659	1403	1406	1409	rBV	405	528	0.13%	0.016%
53	9.708	1411	1414	1417	rBV2	334	511	0.12%	0.016%
54	9.817	1428	1432	1434	rBV	290	333	0.08%	0.010%
55	10.061	1466	1472	1484	rVB	227749	340374	81.92%	10.491%
56	10.201	1493	1495	1501	rVB2	406	560	0.13%	0.017%
57	10.274	1506	1507	1509	rBV	343	193	0.05%	0.006%
58	10.305	1511	1512	1516	rBV	449	371	0.09%	0.011%
59	10.463	1535	1538	1539	rBV	244	234	0.06%	0.007%
60	10.646	1567	1568	1573	rVB2	208	174	0.04%	0.005%
61	10.707	1577	1578	1580	rVB	274	174	0.04%	0.005%
62	10.726	1580	1581	1583	rVB2	383	259	0.06%	0.008%
63	11.024	1627	1630	1632	rBV2	312	431	0.10%	0.013%
64	11.122	1641	1646	1650	rVV2	1773	2579	0.62%	0.079%
65	11.195	1653	1658	1667	rVV	143033	188548	45.38%	5.812%
66	11.372	1686	1687	1690	rBV	257	240	0.06%	0.007%
67	11.457	1699	1701	1702	rBV	222	176	0.04%	0.005%
68	11.750	1743	1749	1753	rBV3	1391	1981	0.48%	0.061%
69	11.786	1753	1755	1757	rVB	250	174	0.04%	0.005%
70	11.805	1757	1758	1761	rBV2	232	190	0.05%	0.006%
71	11.933	1776	1779	1782	rBV3	658	825	0.20%	0.025%
72	11.981	1785	1787	1789	rBV	172	183	0.04%	0.006%
73	12.024	1789	1794	1801	rBV	274872	331656	79.82%	10.223%
74	12.128	1807	1811	1812	rBV2	617	801	0.19%	0.025%
75	12.323	1838	1843	1850	rVB	239733	297253	71.54%	9.162%
76	12.433	1857	1861	1866	rVB2	587	800	0.19%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025670.D
 Acq On : 09 Dec 2021 19:30
 Operator : JC/MD
 Sample : M4975-13ME
 Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.548	1878	1880	1884	rBV	279	472	0.11%	0.015%
78	12.670	1897	1900	1901	rBV	593	608	0.15%	0.019%
79	12.768	1913	1916	1921	rVB2	446	549	0.13%	0.017%
80	12.872	1929	1933	1934	rBV2	200	262	0.06%	0.008%
81	13.280	1998	2000	2002	rBV	236	236	0.06%	0.007%
82	13.408	2019	2021	2022	rBV	264	209	0.05%	0.006%
83	13.481	2032	2033	2038	rBV	321	468	0.11%	0.014%
84	13.524	2038	2040	2041	rVB	325	203	0.05%	0.006%
85	13.542	2041	2043	2046	rBV	338	337	0.08%	0.010%
86	13.719	2070	2072	2076	rVB	285	229	0.06%	0.007%
87	13.786	2078	2083	2088	rBV3	557	1281	0.31%	0.039%
88	13.963	2109	2112	2114	rBV2	357	378	0.09%	0.012%
89	13.987	2114	2116	2119	rVB2	314	349	0.08%	0.011%
90	14.018	2119	2121	2122	rVB	380	191	0.05%	0.006%
91	14.042	2122	2125	2127	rBV2	283	417	0.10%	0.013%
92	14.091	2130	2133	2136	rVV2	328	422	0.10%	0.013%
93	14.127	2137	2139	2144	rVB2	696	929	0.22%	0.029%
94	14.249	2157	2159	2163	rBV	256	243	0.06%	0.007%
95	14.713	2233	2235	2236	rBV	302	203	0.05%	0.006%
96	14.810	2249	2251	2253	rVB	392	374	0.09%	0.012%
97	15.249	2321	2323	2325	rBV	331	253	0.06%	0.008%
98	15.633	2384	2386	2390	rBV2	305	312	0.08%	0.010%
99	15.792	2410	2412	2415	rBV3	443	440	0.11%	0.014%
100	16.548	2534	2536	2537	rBV	356	225	0.05%	0.007%




Sum of corrected areas: 3244343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025670.D
Acq On : 09 Dec 2021 19:30
Operator : JC/MD
Sample : M4975-13ME
Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

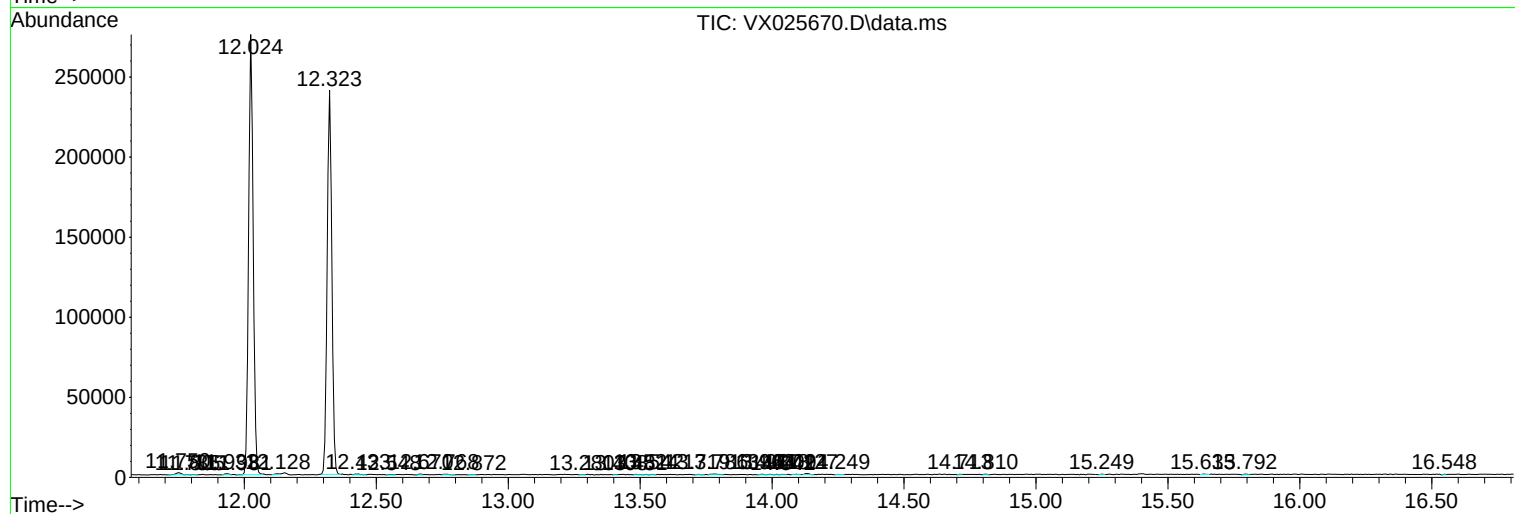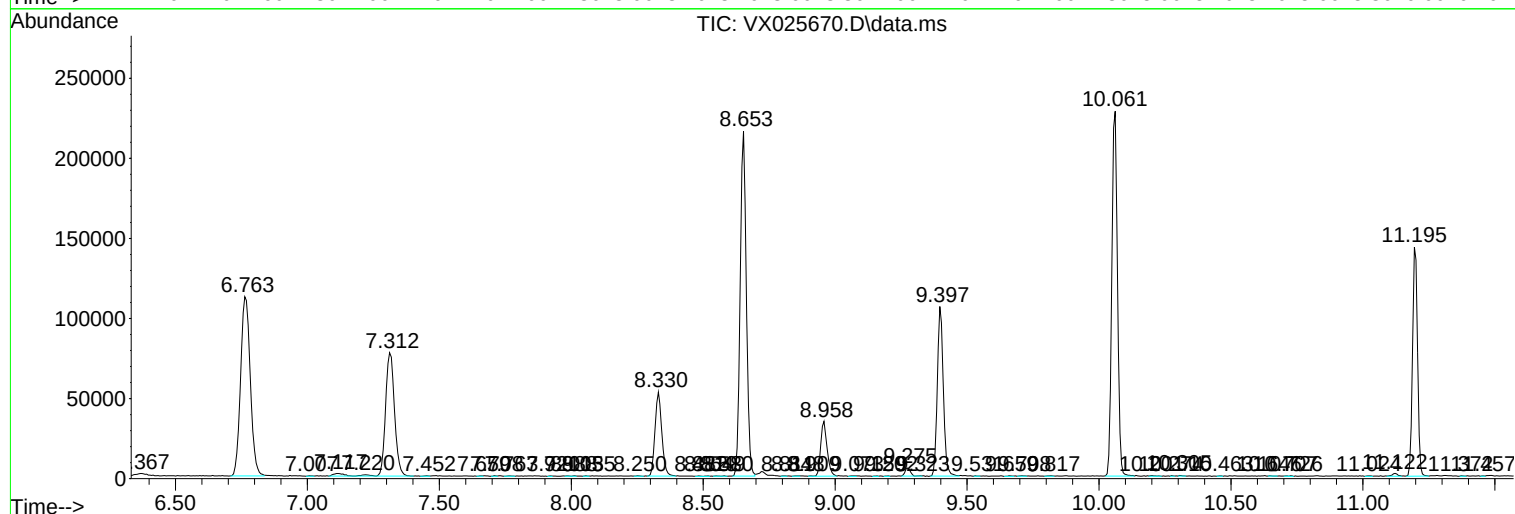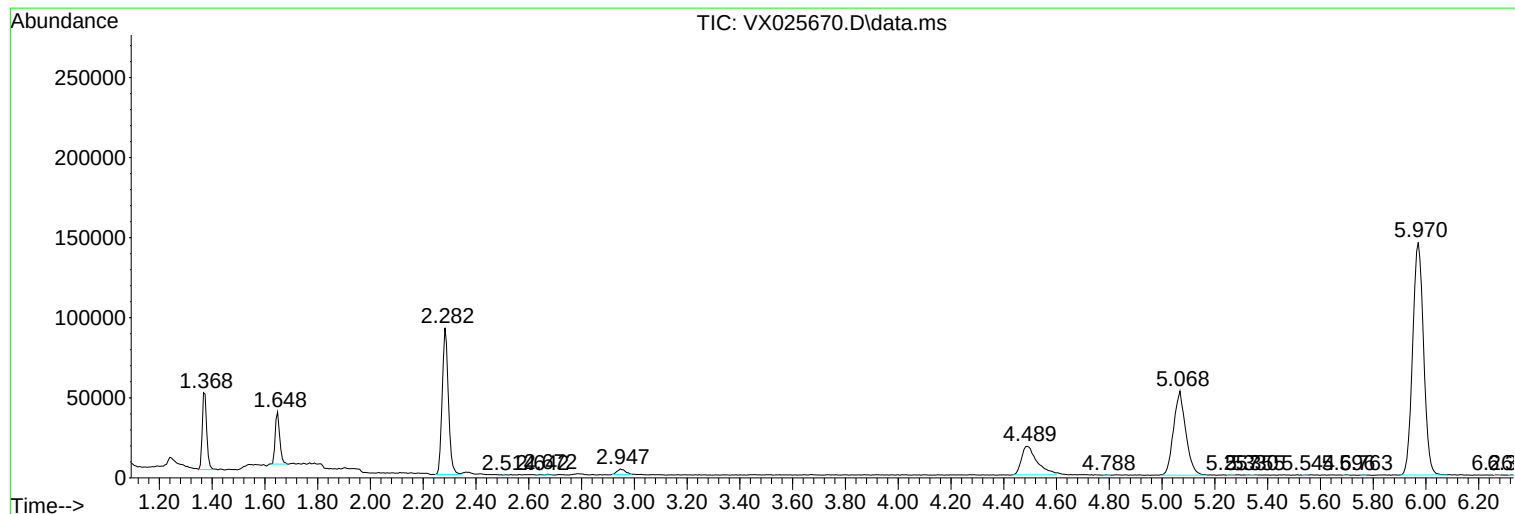

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025670.D
Acq On : 09 Dec 2021 19:30
Operator : JC/MD
Sample : M4975-13ME
Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025670.D
Acq On : 09 Dec 2021 19:30
Operator : JC/MD
Sample : M4975-13ME
Misc : 6.54g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc