

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025672.D
 Acq On : 09 Dec 2021 20:17
 Operator : JC/MD
 Sample : M4975-08DL 10X
 Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	61698	59389	8.80%	1.500%
2	1.660	90	94	101	rBV	45543	56898	8.43%	1.437%
3	2.306	192	200	211	rBV	92717	152478	22.60%	3.851%
4	2.501	231	232	236	rVB2	302	373	0.06%	0.009%
5	2.776	275	277	278	rBV	715	692	0.10%	0.017%
6	2.940	298	304	313	rBV	5869	14221	2.11%	0.359%
7	3.050	320	322	325	rBV2	306	312	0.05%	0.008%
8	3.453	387	388	390	rBV2	346	274	0.04%	0.007%
9	3.514	395	398	400	rBV2	223	248	0.04%	0.006%
10	3.611	406	414	426	rVB	28823	68858	10.21%	1.739%
11	3.965	471	472	475	rBV	304	336	0.05%	0.008%
12	4.032	481	483	489	rVB2	304	443	0.07%	0.011%
13	4.318	528	530	534	rBV	267	317	0.05%	0.008%
14	4.458	543	553	566	rBV	28259	80916	11.99%	2.044%
15	4.647	582	584	587	rBV2	216	293	0.04%	0.007%
16	5.062	640	652	667	rVV	49558	155518	23.05%	3.928%
17	5.281	686	688	690	rVB	318	270	0.04%	0.007%
18	5.300	690	691	693	rBV	316	230	0.03%	0.006%
19	5.385	700	705	706	rBV3	675	1141	0.17%	0.029%
20	5.720	759	760	761	rBV	449	251	0.04%	0.006%
21	5.970	790	801	816	rVV2	130777	387966	57.51%	9.798%
22	6.318	857	858	860	rBV2	328	311	0.05%	0.008%
23	6.403	870	872	873	rBV2	278	254	0.04%	0.006%
24	6.556	894	897	899	rBV	270	299	0.04%	0.008%
25	6.598	903	904	907	rVB	313	232	0.03%	0.006%
26	6.763	921	931	943	rBV	106740	253442	37.57%	6.401%
27	6.995	965	969	970	rBV	231	252	0.04%	0.006%
28	7.129	982	991	1007	rBV	307901	674643	100.00%	17.038%
29	7.312	1013	1021	1033	rVB	79379	172208	25.53%	4.349%
30	7.482	1047	1049	1053	rBV2	280	435	0.06%	0.011%
31	7.513	1053	1054	1058	rVB	238	217	0.03%	0.005%
32	7.751	1091	1093	1095	rBV	232	249	0.04%	0.006%
33	8.019	1134	1137	1138	rBV2	296	296	0.04%	0.007%
34	8.055	1141	1143	1146	rBV2	258	285	0.04%	0.007%
35	8.324	1181	1187	1200	rVV	54369	90641	13.44%	2.289%
36	8.604	1230	1233	1234	rBV	286	255	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025672.D
 Acq On : 09 Dec 2021 20:17
 Operator : JC/MD
 Sample : M4975-08DL 10X
 Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rVV	209719	328155	48.64%	8.288%
38	8.720	1248	1252	1261	rVB	21012	32222	4.78%	0.814%
39	8.903	1280	1282	1284	rBV	305	362	0.05%	0.009%
40	8.952	1285	1290	1298	rVB	38277	55504	8.23%	1.402%
41	9.128	1317	1319	1321	rVV2	314	238	0.04%	0.006%
42	9.275	1337	1343	1351	rVB	85102	123846	18.36%	3.128%
43	9.384	1356	1361	1378	rVV	117322	177323	26.28%	4.478%
44	9.714	1411	1415	1419	rVB3	540	871	0.13%	0.022%
45	9.836	1433	1435	1439	rBV2	327	394	0.06%	0.010%
46	9.872	1439	1441	1445	rVB	308	314	0.05%	0.008%
47	10.055	1465	1471	1484	rVB	225881	304221	45.09%	7.683%
48	10.195	1492	1494	1497	rVB2	382	340	0.05%	0.009%
49	10.299	1509	1511	1515	rVB2	417	523	0.08%	0.013%
50	10.750	1582	1585	1588	rBV2	193	239	0.04%	0.006%
51	10.957	1615	1619	1620	rBV	279	388	0.06%	0.010%
52	11.091	1638	1641	1643	rBV	434	371	0.05%	0.009%
53	11.122	1643	1646	1650	rVB3	1730	2138	0.32%	0.054%
54	11.195	1652	1658	1666	rVB	147277	181801	26.95%	4.591%
55	11.457	1698	1701	1702	rBV	242	259	0.04%	0.007%
56	11.585	1719	1722	1723	rBV2	307	307	0.05%	0.008%
57	11.628	1728	1729	1731	rBV	362	247	0.04%	0.006%
58	11.652	1731	1733	1735	rBV	222	213	0.03%	0.005%
59	11.671	1735	1736	1741	rVV	230	265	0.04%	0.007%
60	11.750	1745	1749	1753	rVB3	1400	1918	0.28%	0.048%
61	11.890	1768	1772	1774	rBV	258	433	0.06%	0.011%
62	11.933	1777	1779	1782	rVB	738	736	0.11%	0.019%
63	11.963	1782	1784	1786	rBV	318	233	0.03%	0.006%
64	12.024	1789	1794	1803	rVB	227675	283778	42.06%	7.167%
65	12.122	1807	1810	1812	rBV2	632	757	0.11%	0.019%
66	12.231	1826	1828	1830	rBV2	278	219	0.03%	0.006%
67	12.262	1832	1833	1836	rVB	309	220	0.03%	0.006%
68	12.323	1836	1843	1854	rBV	214135	274365	40.67%	6.929%
69	12.402	1854	1856	1858	rBV	225	214	0.03%	0.005%
70	12.433	1858	1861	1862	rVB	304	324	0.05%	0.008%
71	12.652	1893	1897	1900	rBV2	363	664	0.10%	0.017%
72	12.695	1902	1904	1909	rBV2	312	468	0.07%	0.012%
73	12.737	1909	1911	1912	rVV2	229	216	0.03%	0.005%
74	12.762	1913	1915	1920	rVB2	623	665	0.10%	0.017%
75	12.872	1931	1933	1938	rVB2	253	392	0.06%	0.010%
76	13.061	1960	1964	1966	rBV2	281	286	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025672.D
 Acq On : 09 Dec 2021 20:17
 Operator : JC/MD
 Sample : M4975-08DL 10X
 Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKT2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	13.122	1971	1974	1976	rBV	151	222	0.03%	0.006%
78	13.146	1976	1978	1979	rVB	365	219	0.03%	0.006%
79	13.170	1979	1982	1984	rBV2	362	533	0.08%	0.013%
80	13.329	2006	2008	2010	rBV	318	388	0.06%	0.010%
81	13.353	2010	2012	2016	rVV	258	264	0.04%	0.007%
82	13.463	2027	2030	2031	rBV	294	245	0.04%	0.006%
83	13.500	2034	2036	2039	rVB2	287	246	0.04%	0.006%
84	13.579	2047	2049	2051	rVB	266	239	0.04%	0.006%
85	13.628	2051	2057	2058	rBV2	242	372	0.06%	0.009%
86	13.884	2097	2099	2102	rVB	400	364	0.05%	0.009%
87	14.048	2124	2126	2129	rBV	365	290	0.04%	0.007%
88	14.091	2129	2133	2134	rBV	297	380	0.06%	0.010%
89	14.201	2149	2151	2156	rBV2	299	520	0.08%	0.013%
90	14.365	2174	2178	2179	rBV	315	332	0.05%	0.008%
91	14.384	2179	2181	2185	rVV2	334	412	0.06%	0.010%
92	14.420	2185	2187	2190	rVV	374	310	0.05%	0.008%
93	14.493	2195	2199	2200	rBV2	249	269	0.04%	0.007%
94	14.615	2215	2219	2221	rVB2	298	411	0.06%	0.010%
95	14.670	2226	2228	2230	rBV2	233	241	0.04%	0.006%
96	15.146	2304	2306	2309	rVB2	246	287	0.04%	0.007%
97	15.231	2319	2320	2324	rBV2	232	268	0.04%	0.007%
98	15.920	2431	2433	2434	rBV	308	250	0.04%	0.006%
99	16.316	2496	2498	2502	rBV	242	339	0.05%	0.009%
100	16.365	2505	2506	2509	rBV	299	268	0.04%	0.007%




Sum of corrected areas: 3959541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025672.D
Acq On : 09 Dec 2021 20:17
Operator : JC/MD
Sample : M4975-08DL 10X
Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

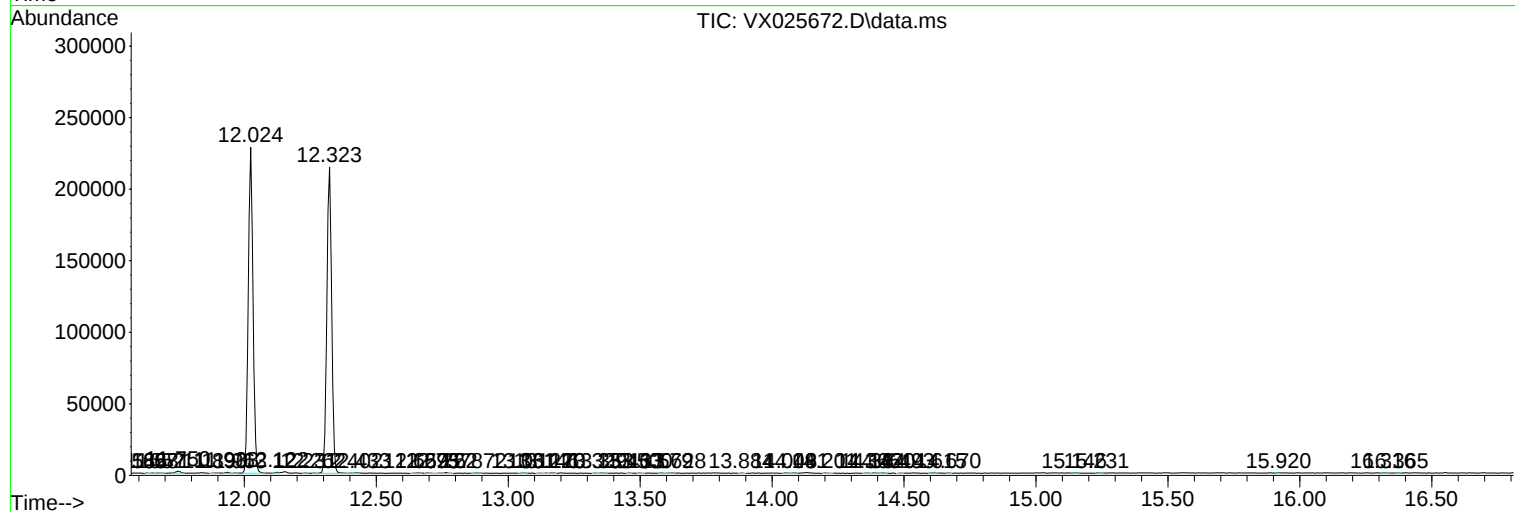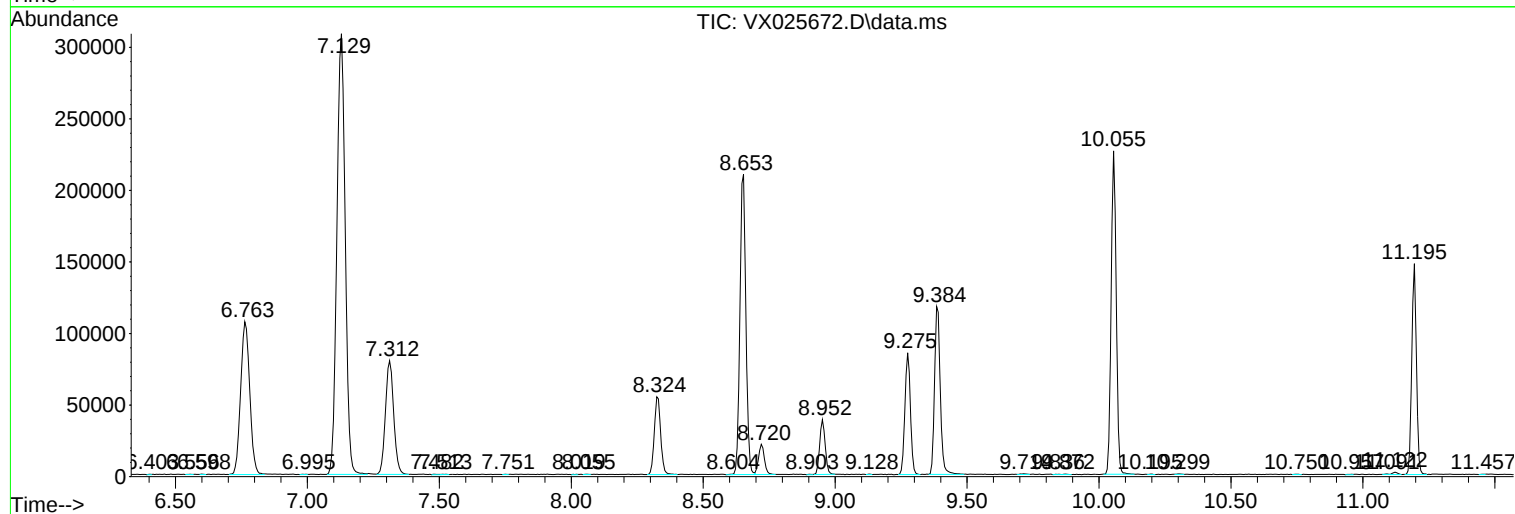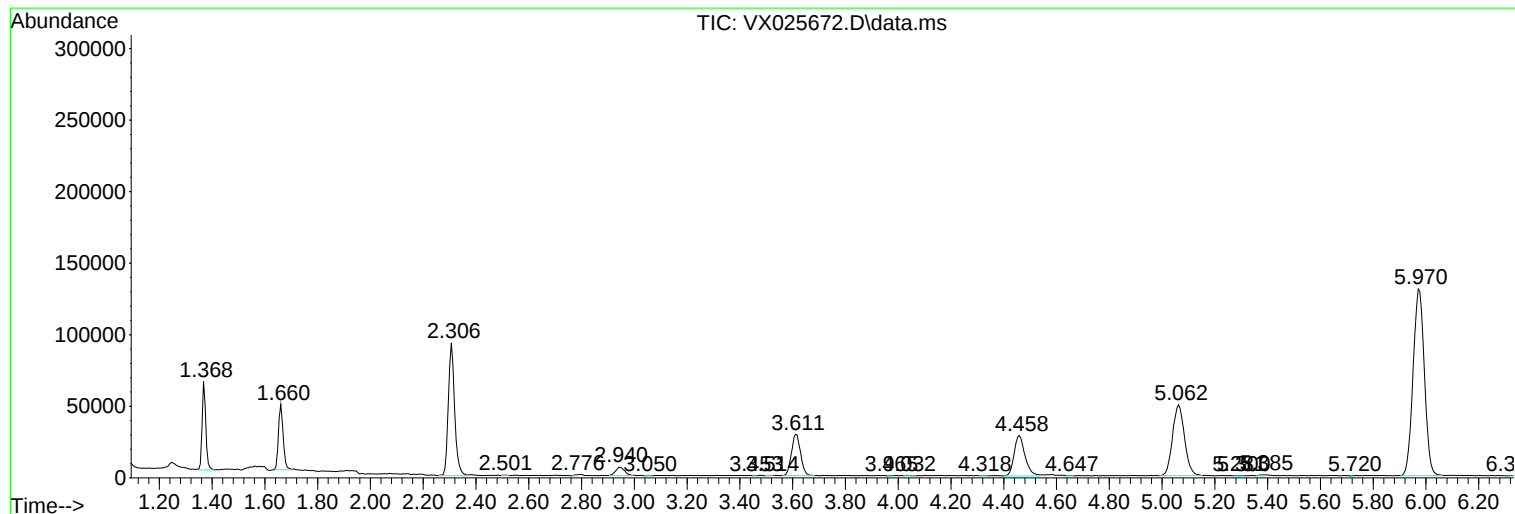

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025672.D
Acq On : 09 Dec 2021 20:17
Operator : JC/MD
Sample : M4975-08DL 10X
Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025672.D
Acq On : 09 Dec 2021 20:17
Operator : JC/MD
Sample : M4975-08DL 10X
Misc : 6.39g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKT2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc