

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025686.D
 Acq On : 10 Dec 2021 01:42
 Operator : JC/MD
 Sample : M5004-14 20X
 Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	56140	55481	15.17%	1.928%
2	1.660	90	94	101	rBV	43317	53398	14.61%	1.856%
3	2.307	194	200	211	rVB	88313	137627	37.64%	4.783%
4	2.428	219	220	223	rBV	375	436	0.12%	0.015%
5	2.508	232	233	235	rBV	325	234	0.06%	0.008%
6	2.745	271	272	276	rBV	283	269	0.07%	0.009%
7	2.794	276	280	284	rVB4	679	1078	0.29%	0.037%
8	2.947	298	305	317	rVB	8376	19701	5.39%	0.685%
9	3.093	327	329	332	rBV	279	339	0.09%	0.012%
10	3.373	374	375	378	rVB	441	408	0.11%	0.014%
11	3.477	391	392	396	rBV2	335	371	0.10%	0.013%
12	3.739	431	435	437	rVB	338	342	0.09%	0.012%
13	4.001	475	478	480	rVV2	263	308	0.08%	0.011%
14	4.117	494	497	504	rBV2	438	849	0.23%	0.030%
15	4.172	504	506	507	rBV	292	246	0.07%	0.009%
16	4.379	537	540	544	rVB	355	658	0.18%	0.023%
17	4.459	544	553	566	rBV	26142	73895	20.21%	2.568%
18	4.769	602	604	606	rVV2	301	236	0.06%	0.008%
19	4.818	611	612	615	rBV	383	342	0.09%	0.012%
20	4.934	628	631	633	rBV2	289	386	0.11%	0.013%
21	4.952	633	634	636	rVV	410	253	0.07%	0.009%
22	5.062	639	652	668	rVV2	46217	147173	40.25%	5.115%
23	5.556	727	733	736	rBV2	553	838	0.23%	0.029%
24	5.647	745	748	749	rBV2	255	286	0.08%	0.010%
25	5.971	789	801	816	rBV2	123330	365608	100.00%	12.707%
26	6.153	829	831	834	rVB	509	577	0.16%	0.020%
27	6.196	836	838	839	rBV2	311	282	0.08%	0.010%
28	6.361	862	865	868	rBV	240	309	0.08%	0.011%
29	6.428	874	876	877	rBV2	307	259	0.07%	0.009%
30	6.763	922	931	944	rVB	100735	239644	65.55%	8.329%
31	6.897	951	953	959	rVB2	428	527	0.14%	0.018%
32	7.013	970	972	976	rVB2	278	318	0.09%	0.011%
33	7.117	982	989	996	rVB2	2231	4964	1.36%	0.173%
34	7.312	1013	1021	1034	rVB2	74710	161600	44.20%	5.617%
35	7.428	1037	1040	1044	rBV	372	593	0.16%	0.021%
36	7.745	1088	1092	1093	rBV2	170	227	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025686.D
 Acq On : 10 Dec 2021 01:42
 Operator : JC/MD
 Sample : M5004-14 20X
 Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.921	1118	1121	1123	rBV2	296	238	0.07%	0.008%
38	7.982	1129	1131	1132	rBV2	286	233	0.06%	0.008%
39	8.001	1132	1134	1137	rVB2	391	381	0.10%	0.013%
40	8.031	1137	1139	1140	rBV	279	250	0.07%	0.009%
41	8.123	1151	1154	1155	rBV2	243	232	0.06%	0.008%
42	8.141	1155	1157	1159	rVV	233	253	0.07%	0.009%
43	8.190	1163	1165	1168	rVB	338	360	0.10%	0.013%
44	8.220	1168	1170	1172	rBV	375	305	0.08%	0.011%
45	8.324	1181	1187	1196	rBV	51912	85063	23.27%	2.956%
46	8.440	1205	1206	1209	rBV	335	266	0.07%	0.009%
47	8.507	1215	1217	1218	rBV	333	232	0.06%	0.008%
48	8.525	1218	1220	1223	rBV2	374	474	0.13%	0.016%
49	8.555	1223	1225	1227	rBV2	249	236	0.06%	0.008%
50	8.653	1234	1241	1248	rBV	191508	303603	83.04%	10.552%
51	8.720	1249	1252	1260	rVB2	2892	4504	1.23%	0.157%
52	8.781	1260	1262	1264	rBV2	379	389	0.11%	0.014%
53	8.952	1285	1290	1300	rVV	36463	53273	14.57%	1.852%
54	9.092	1310	1313	1314	rBV2	240	247	0.07%	0.009%
55	9.128	1317	1319	1322	rVB	362	241	0.07%	0.008%
56	9.275	1338	1343	1347	rBV2	1683	2151	0.59%	0.075%
57	9.385	1356	1361	1375	rBV	110159	161710	44.23%	5.620%
58	9.903	1444	1446	1448	rVB2	354	301	0.08%	0.010%
59	9.927	1448	1450	1451	rBV	337	219	0.06%	0.008%
60	10.055	1465	1471	1481	rBV	218120	290164	79.36%	10.085%
61	10.165	1488	1489	1492	rBV2	261	303	0.08%	0.011%
62	10.384	1522	1525	1527	rVB2	434	507	0.14%	0.018%
63	10.793	1590	1592	1595	rVB	275	255	0.07%	0.009%
64	10.823	1595	1597	1599	rBV	217	276	0.08%	0.010%
65	10.860	1601	1603	1606	rBV	266	265	0.07%	0.009%
66	10.890	1606	1608	1610	rBV2	235	221	0.06%	0.008%
67	10.915	1610	1612	1614	rBV	283	237	0.06%	0.008%
68	11.122	1641	1646	1652	rBV3	1262	1756	0.48%	0.061%
69	11.195	1652	1658	1666	rVV	134885	169751	46.43%	5.900%
70	11.415	1689	1694	1696	rBV2	282	580	0.16%	0.020%
71	11.585	1721	1722	1727	rBV	386	540	0.15%	0.019%
72	11.744	1746	1748	1752	rVV2	1052	1343	0.37%	0.047%
73	11.793	1754	1756	1760	rVB	339	395	0.11%	0.014%
74	11.835	1762	1763	1767	rBV2	250	262	0.07%	0.009%
75	11.933	1776	1779	1783	rVB	726	806	0.22%	0.028%
76	12.024	1789	1794	1801	rBV	215412	265372	72.58%	9.223%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025686.D
 Acq On : 10 Dec 2021 01:42
 Operator : JC/MD
 Sample : M5004-14 20X
 Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BGKX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.128	1809	1811	1813	rBV3	492	606	0.17%	0.021%
78	12.189	1820	1821	1824	rBV	415	327	0.09%	0.011%
79	12.323	1836	1843	1852	rBV	197070	250662	68.56%	8.712%
80	12.482	1865	1869	1871	rBV2	278	358	0.10%	0.012%
81	12.671	1896	1900	1901	rVV3	281	255	0.07%	0.009%
82	13.042	1956	1961	1962	rBV2	293	372	0.10%	0.013%
83	13.305	2002	2004	2005	rBV2	235	243	0.07%	0.008%
84	13.652	2060	2061	2064	rVB	364	245	0.07%	0.009%
85	13.798	2084	2085	2089	rVB2	231	225	0.06%	0.008%
86	13.884	2098	2099	2102	rVB	418	284	0.08%	0.010%
87	14.134	2136	2140	2143	rBV3	583	952	0.26%	0.033%
88	14.213	2151	2153	2155	rVV	427	346	0.09%	0.012%
89	14.609	2215	2218	2219	rVB2	309	288	0.08%	0.010%
90	15.115	2298	2301	2303	rBV2	341	348	0.10%	0.012%
91	15.371	2341	2343	2344	rBV2	326	316	0.09%	0.011%
92	15.646	2386	2388	2391	rBV2	253	259	0.07%	0.009%
93	15.847	2419	2421	2424	rVB	244	255	0.07%	0.009%
94	16.060	2453	2456	2459	rBV2	341	499	0.14%	0.017%
95	16.085	2459	2460	2463	rBV	369	307	0.08%	0.011%
96	16.231	2482	2484	2486	rBV2	491	448	0.12%	0.016%
97	16.280	2491	2492	2494	rVV	418	340	0.09%	0.012%
98	16.328	2497	2500	2502	rBV2	304	379	0.10%	0.013%
99	16.347	2502	2503	2506	rBV	261	262	0.07%	0.009%
100	16.773	2570	2573	2575	rBV	356	404	0.11%	0.014%


Sum of corrected areas: 2877236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025686.D
Acq On : 10 Dec 2021 01:42
Operator : JC/MD
Sample : M5004-14 20X
Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

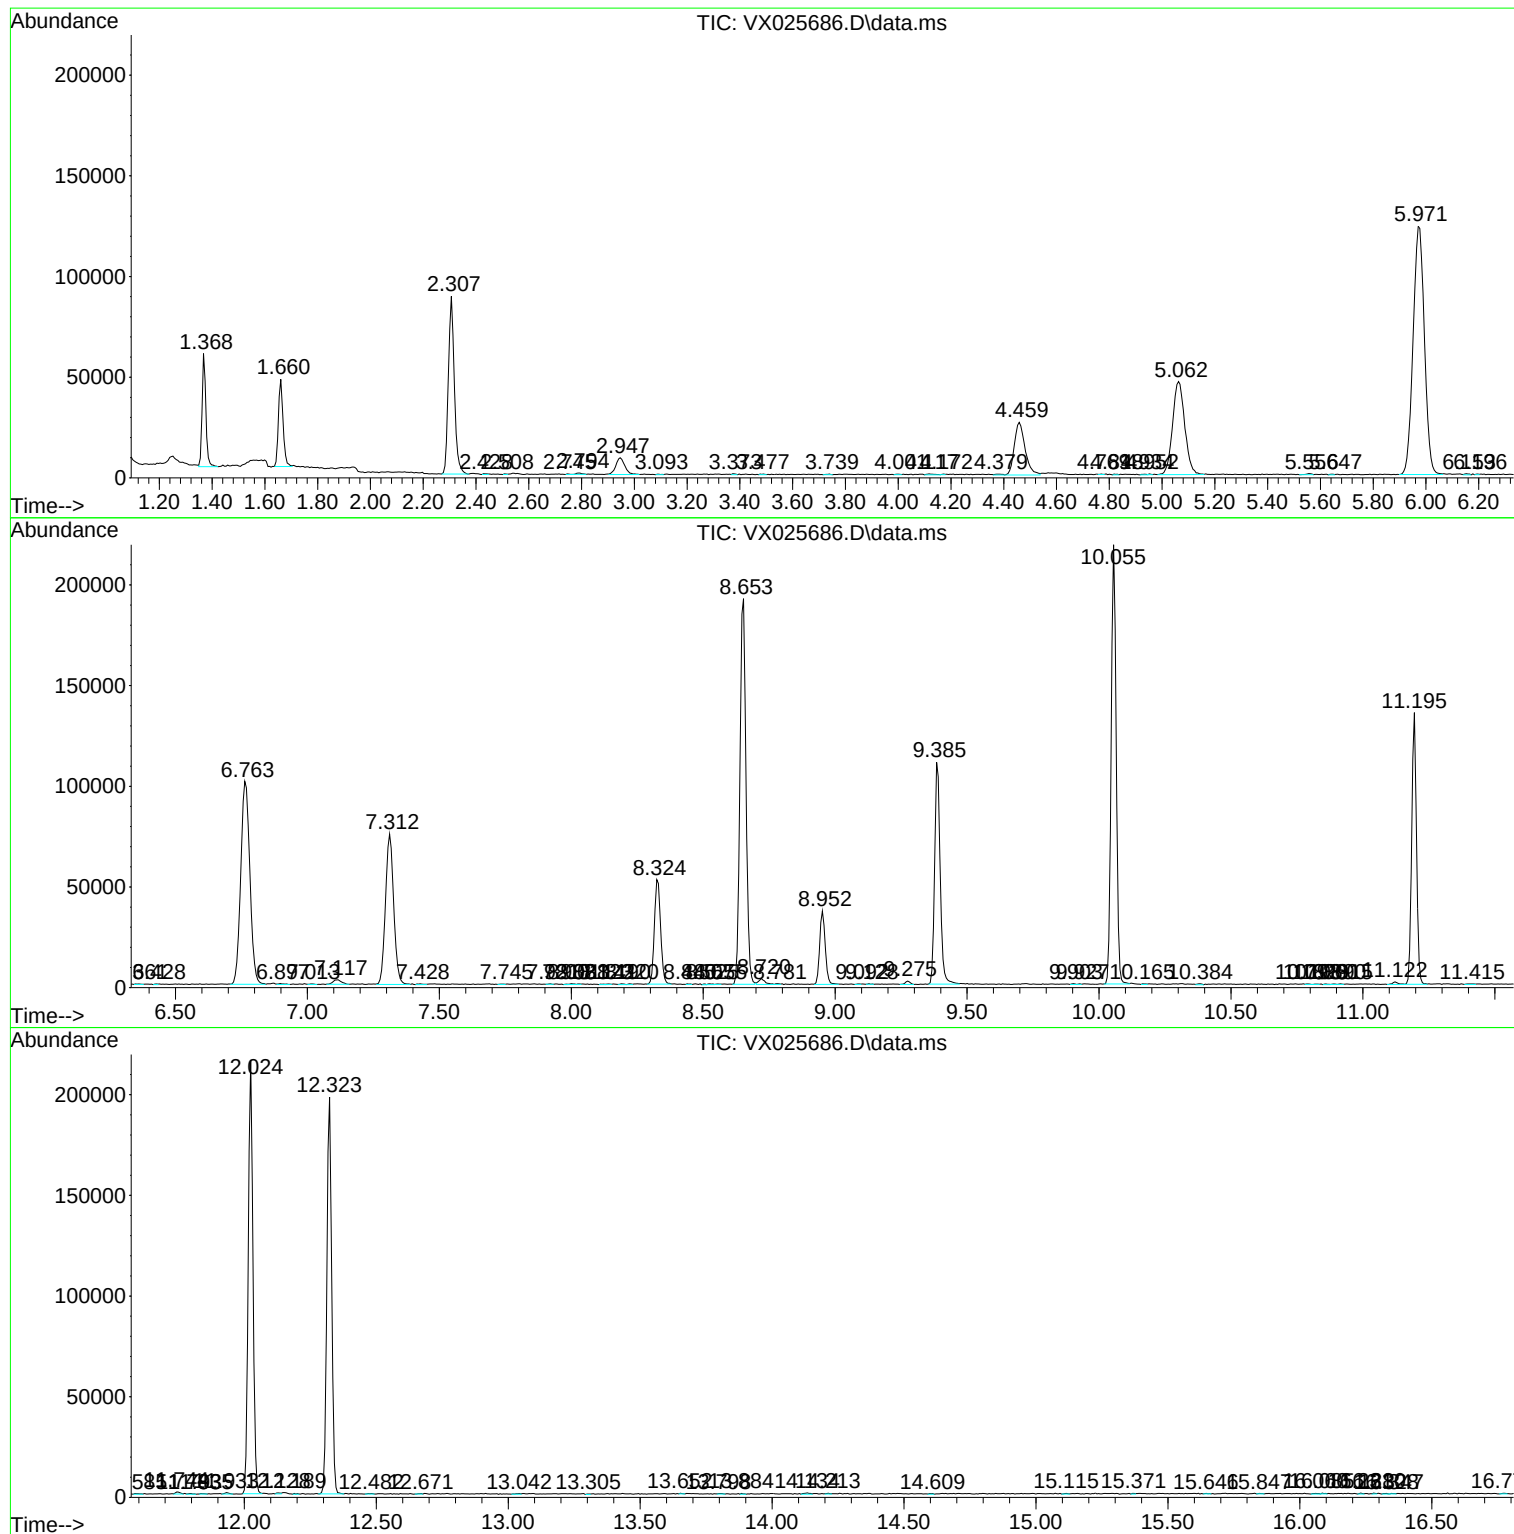

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025686.D
Acq On : 10 Dec 2021 01:42
Operator : JC/MD
Sample : M5004-14 20X
Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
Data File : VX025686.D
Acq On : 10 Dec 2021 01:42
Operator : JC/MD
Sample : M5004-14 20X
Misc : 6.88g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BGKX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc