
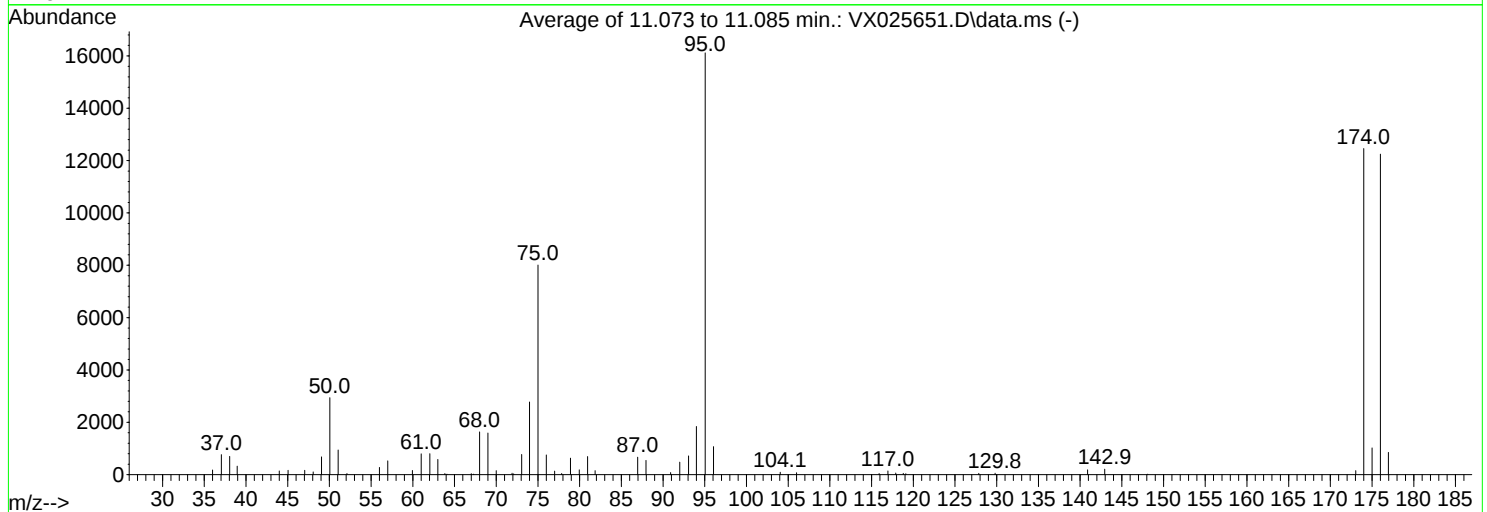


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120921\
 Data File : VX025651.D
 Acq On : 09 Dec 2021 10:07
 Operator : JC/MD
 Sample : BFB621
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB621

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Sun Dec 12 06:39:29 2021

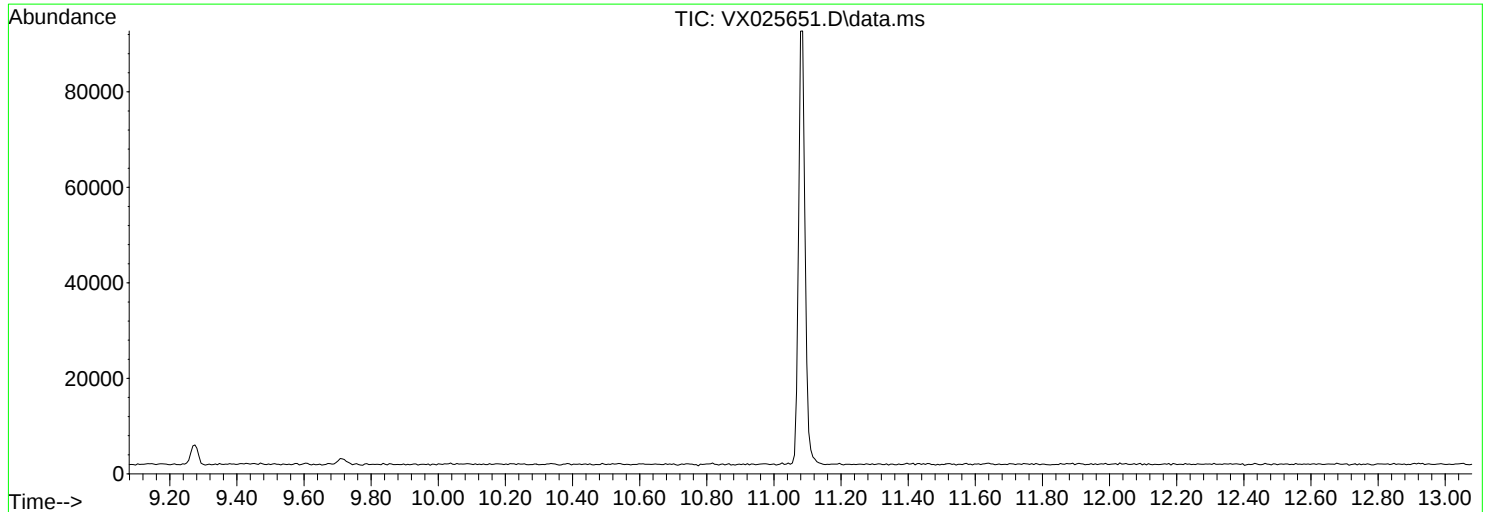

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	2941	PASS
75	95	30	80	49.7	8009	PASS
95	95	100	100	100.0	16116	PASS
96	95	5	9	6.6	1070	PASS
173	174	0.00	2	1.3	156	PASS
174	95	50	120	77.3	12458	PASS
175	174	5	9	8.2	1019	PASS
176	174	95	101	98.3	12247	PASS
177	176	5	9	7.0	852	PASS

Scan 1633 (11.043 min): VX025651.D\data.ms
BFB621

m/z	Abundance
40.00	2149.0
44.00	140.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.00	175.0
37.00	620.0
38.00	516.0
39.00	281.0
40.00	1842.0
44.10	264.0
45.10	133.0
47.20	190.0
48.00	96.0
49.10	477.0
50.00	2285.0
51.10	666.0
56.00	205.0
57.00	419.0
59.90	117.0
61.00	597.0
62.10	671.0
63.00	471.0
63.90	78.0
67.30	62.0
68.00	1224.0
69.00	1181.0
69.90	152.0
71.90	63.0
73.00	580.0
74.00	1807.0
75.00	5499.0
76.00	505.0
77.00	77.0
78.90	411.0
80.00	105.0
80.90	482.0
82.00	85.0
86.90	550.0
87.90	375.0
91.90	370.0
93.00	514.0
94.00	1303.0
95.10	10667.0
96.00	761.0
104.10	61.0
115.90	58.0
117.00	93.0
141.00	100.0
143.00	83.0
173.10	114.0
174.00	7018.0
175.00	598.0
176.00	6799.0
176.90	547.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.00	223.0
37.10	879.0
38.00	821.0
39.00	379.0
40.00	1800.0
44.00	264.0
45.00	196.0
47.00	156.0
48.10	103.0
49.00	885.0
50.10	3416.0
51.00	1129.0
52.10	62.0
55.90	356.0
57.00	636.0
60.00	201.0
61.00	914.0
62.00	892.0
63.00	689.0
64.10	61.0
67.00	55.0
68.00	1977.0
69.00	1975.0
70.00	150.0
71.90	99.0
73.00	943.0
74.00	3403.0
75.00	9478.0
76.00	938.0
76.90	207.0
77.80	64.0
78.90	804.0
80.00	223.0
81.00	779.0
81.80	197.0
87.00	652.0
88.00	624.0
90.90	140.0
92.00	529.0
93.10	791.0
94.00	2101.0
95.00	19416.0
96.10	1237.0
104.00	110.0
106.00	120.0
115.90	80.0
116.90	140.0
117.90	93.0
118.80	152.0
127.90	80.0
129.80	53.0
140.90	230.0
142.90	274.0
173.00	180.0
174.00	13923.0
175.00	1247.0
176.00	14272.0
177.00	912.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.00	136.0
37.00	799.0
38.10	758.0
38.90	311.0
40.00	1975.0
44.10	322.0
45.00	159.0
47.00	152.0
48.00	116.0
49.00	673.0
50.00	3122.0
51.00	1026.0
52.10	58.0
56.10	261.0
57.00	521.0
60.00	158.0
61.00	878.0
62.00	835.0
63.00	574.0
63.80	55.0
67.00	57.0
68.00	1692.0
69.00	1609.0
70.10	156.0
72.10	91.0
73.10	785.0
74.00	3116.0
75.00	9050.0
76.00	820.0
77.10	118.0
77.90	61.0
78.90	680.0
79.90	224.0
80.90	803.0
81.90	180.0
86.90	797.0
87.90	642.0
90.90	94.0
92.10	541.0
93.00	840.0
94.00	2119.0
95.00	18264.0
96.00	1212.0
104.00	98.0
106.00	106.0
116.90	188.0
117.90	92.0
119.10	105.0
127.80	63.0
129.80	114.0
140.80	222.0
143.00	272.0
148.10	52.0
173.00	174.0
174.00	16432.0
175.00	1212.0
176.00	15670.0
176.90	1096.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621