

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
 Data File : VX033360.D
 Acq On : 09 Dec 2022 20:03
 Operator : JC/MD
 Sample : N5972-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW9-PT-OUT-02-12082022

Quant Time: Dec 10 05:58:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 07 12:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	150298	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	240193	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	209534	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93353	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	45737	47.434	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.860%
35) Dibromofluoromethane	5.391	113	50425	46.675	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.360%
50) Toluene-d8	8.647	98	107081	47.381	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.760%
62) 4-Bromofluorobenzene	11.079	95	79825	46.194	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.380%
Target Compounds						
					Qvalue	
16) Acetone	2.398	43	230	0.322	ug/l #	45
31) Cyclohexane	5.550	56	2810	1.226	ug/l #	9
36) 1,1-Dichloropropene	5.556	75	11194	5.315	ug/l #	50
38) Carbon Tetrachloride	5.556	117	15566	6.596	ug/l #	15
51) 4-Methyl-2-Pentanone	8.647	43	432	0.213	ug/l #	1
76) 1,2,3-Trichloropropane	11.079	75	40951	21.561	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	40951	67.070	ug/l #	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033360.D
Acq On : 09 Dec 2022 20:03
Operator : JC/MD
Sample : N5972-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022

Quant Time: Dec 10 05:58:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 07 12:43:54 2022
Response via : Initial Calibration




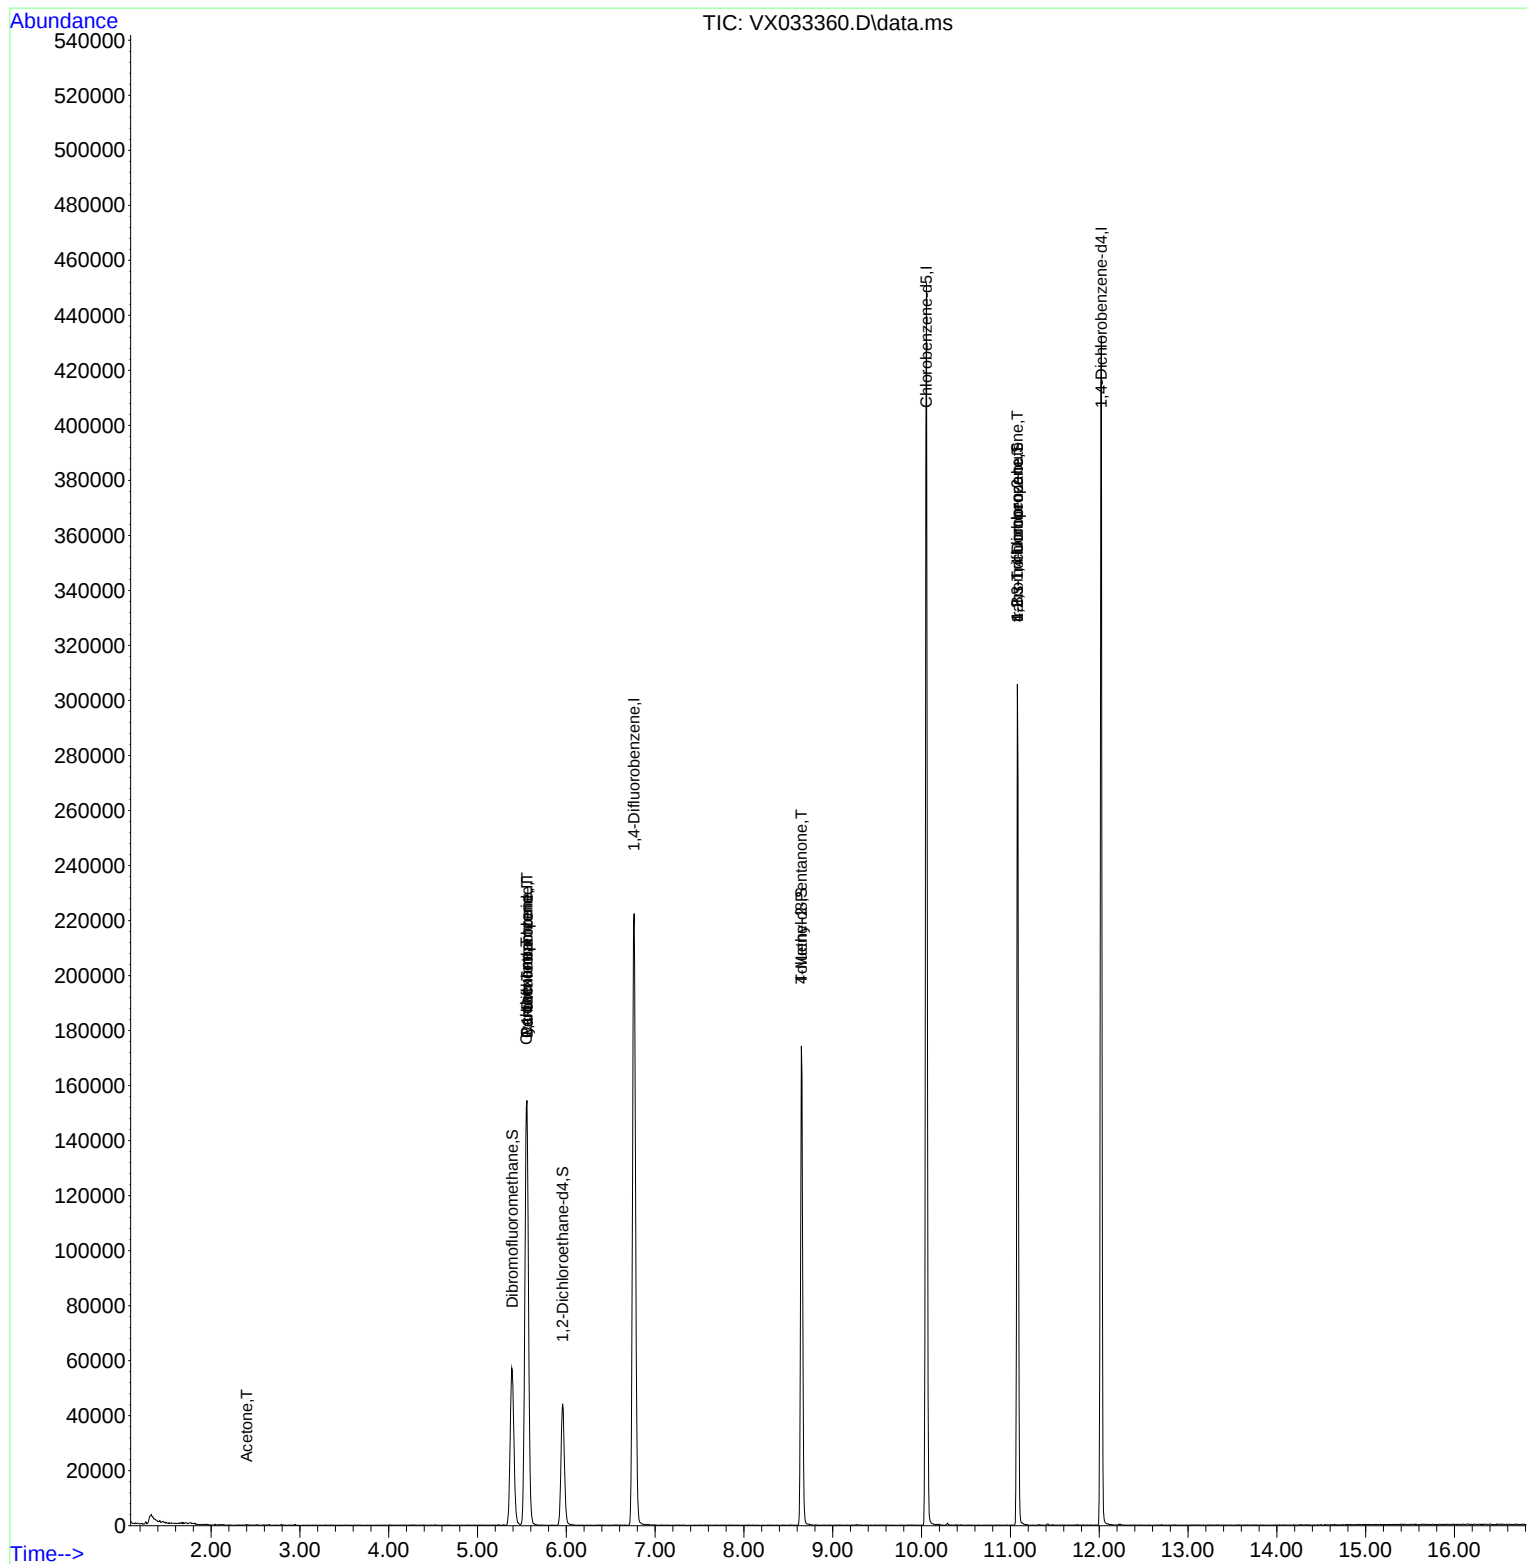


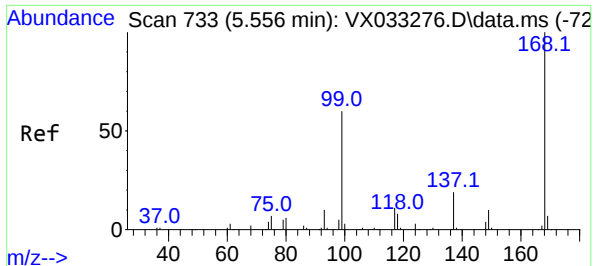

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03




Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022


Tgt Ion:168 Resp: 150298
Ion Ratio Lower Upper
168 100
99 56.7 46.1 69.1

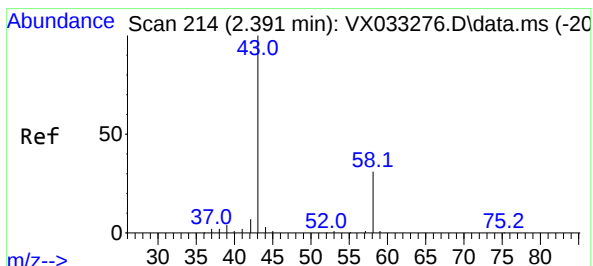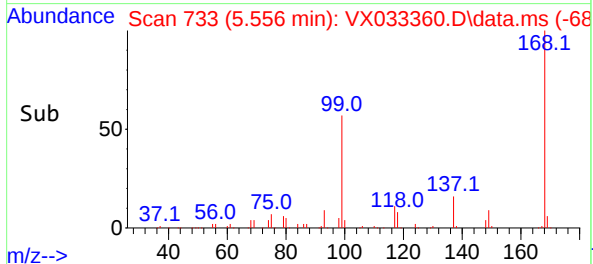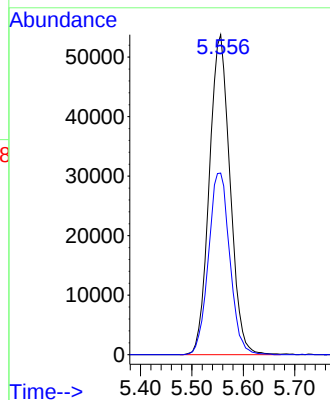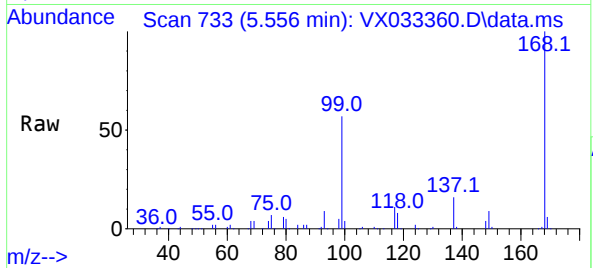

#16
Acetone
Concen: 0.322 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03


Tgt Ion: 43 Resp: 230
Ion Ratio Lower Upper
43 100
58 0.0 23.8 35.8#

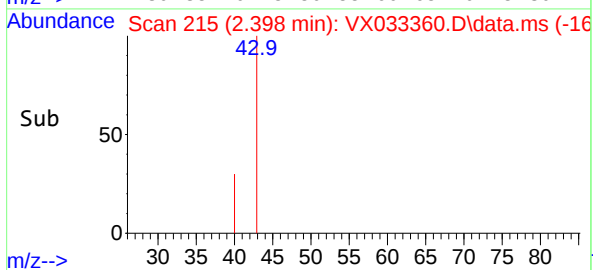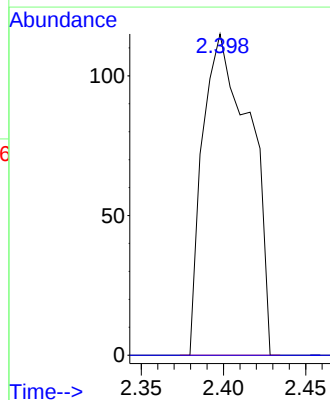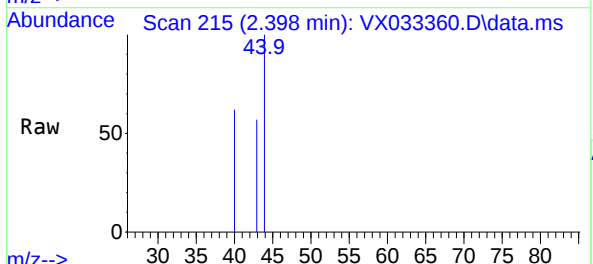



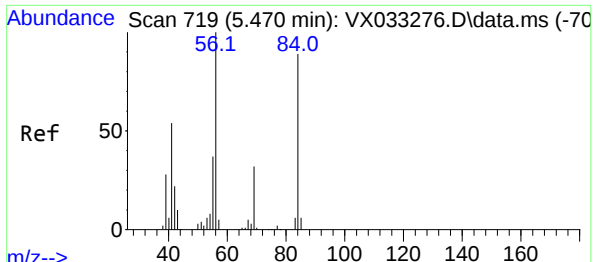


#31
Cyclohexane
Concen: 1.226 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.080 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022



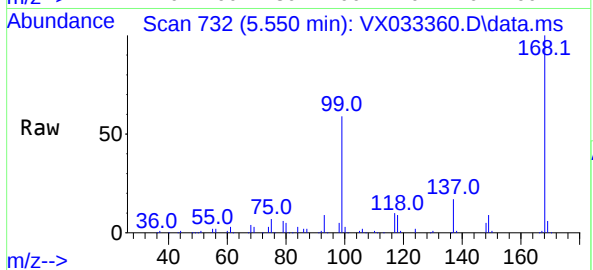



Tgt Ion: 56 Resp: 2810
Ion Ratio Lower Upper
56 100
69 145.4 24.1 36.1#
84 126.5 66.9 100.3#

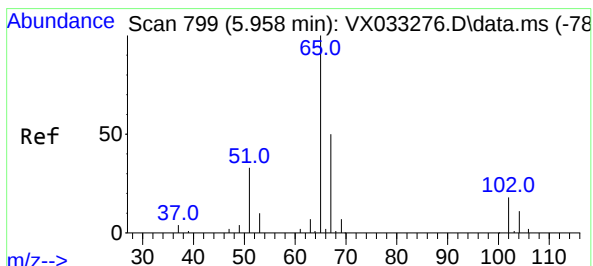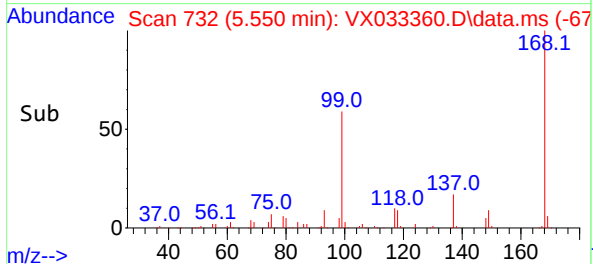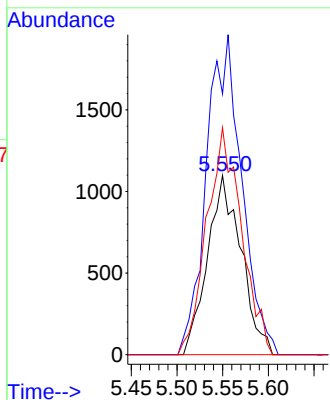

#33
1,2-Dichloroethane-d4
Concen: 47.434 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Tgt Ion: 65 Resp: 45737
Ion Ratio Lower Upper
65 100
67 49.9 0.0 101.8

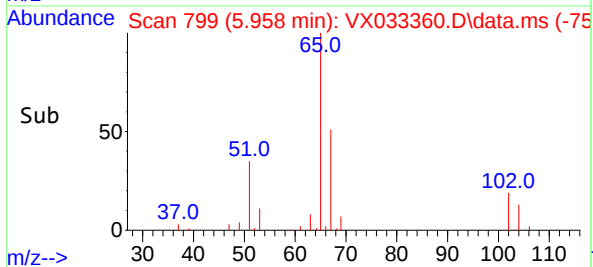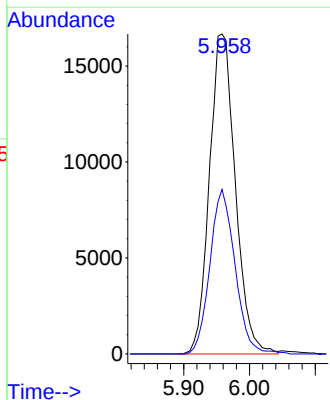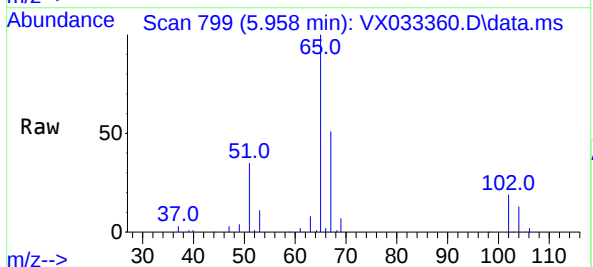




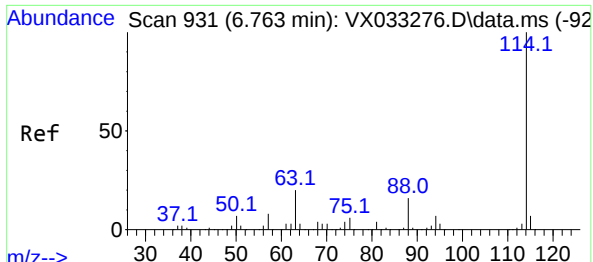


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022

Tgt Ion:114 Resp: 240193




Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	41.6
88	15.9	0.0	33.4

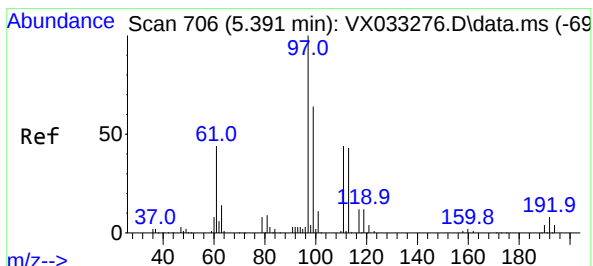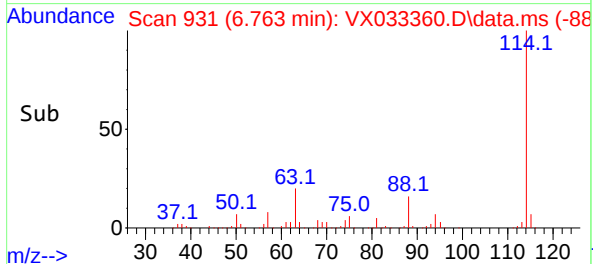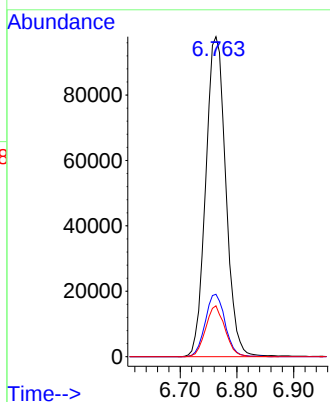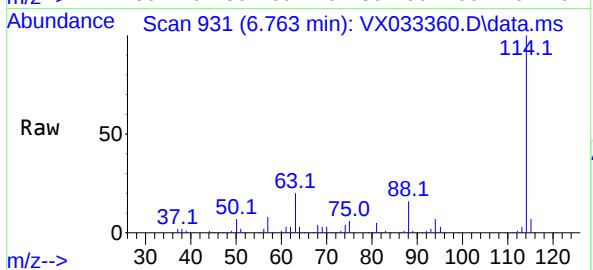


#35
Dibromofluoromethane
Concen: 46.675 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Tgt Ion:113 Resp: 50425

Ion	Ratio	Lower	Upper
113	100		
111	104.1	82.4	123.6
192	19.3	15.4	23.2


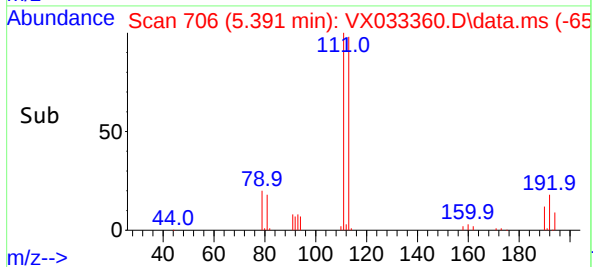
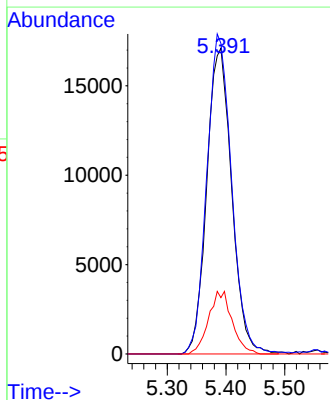
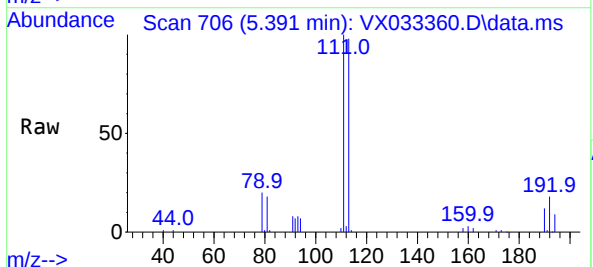


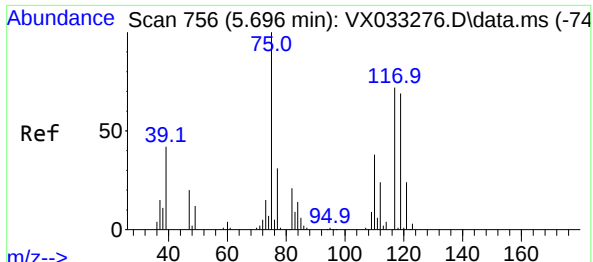

#36
1,1-Dichloropropene
Concen: 5.315 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.140 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03




Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022


Tgt Ion: 75 Resp: 11194
Ion Ratio Lower Upper
75 100
110 10.1 18.4 55.2#
77 0.0 24.5 36.7#

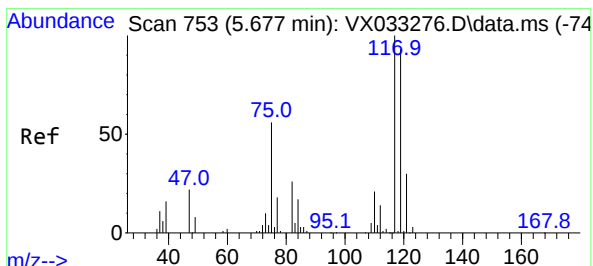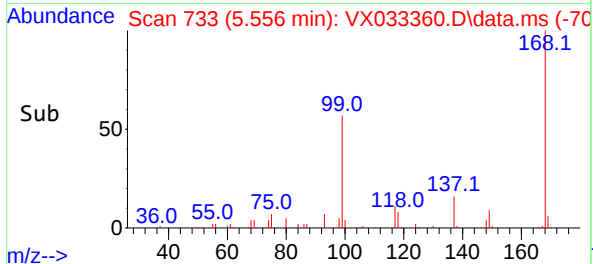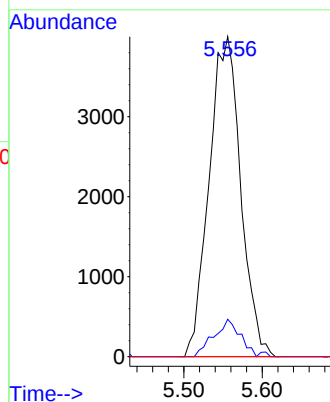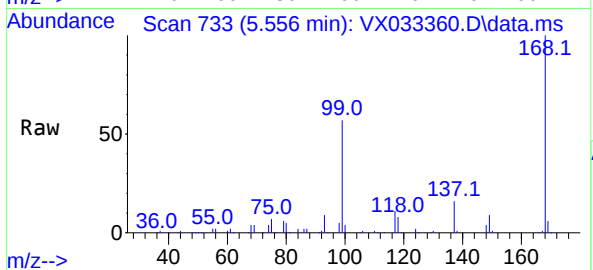

#38
Carbon Tetrachloride
Concen: 6.596 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.122 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Tgt Ion: 117 Resp: 15566
Ion Ratio Lower Upper
117 100
119 4.6 77.2 115.8#
121 0.0 25.8 38.6#

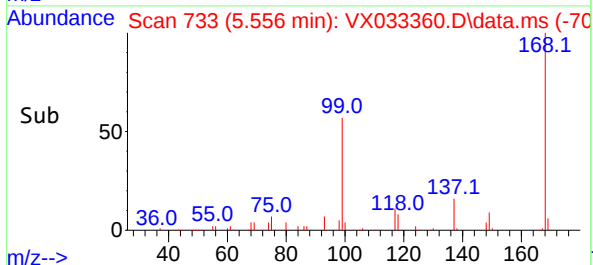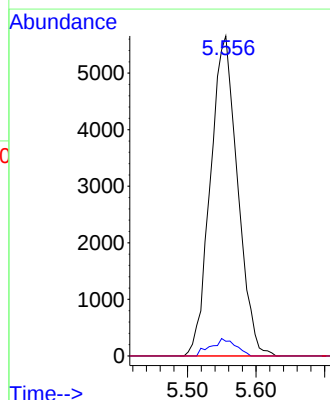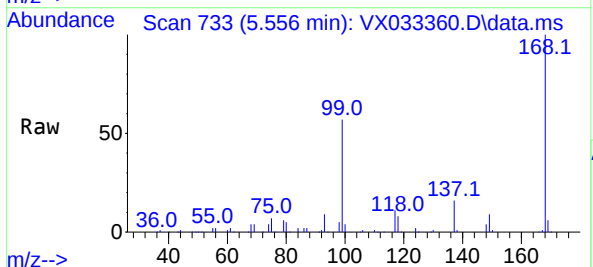

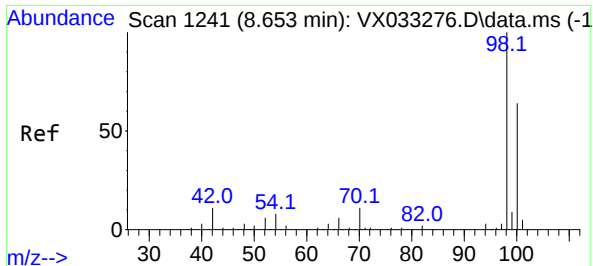

#50

Toluene-d8

Concen: 47.381 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX033360.D

Acq: 09 Dec 2022 20:03

Instrument :

MSVOA_X

ClientSampleId :





RW9-PT-OUT-02-12082022

Tgt Ion: 98 Resp: 107081

Ion Ratio Lower Upper

98 100

100 64.3 50.9 76.3

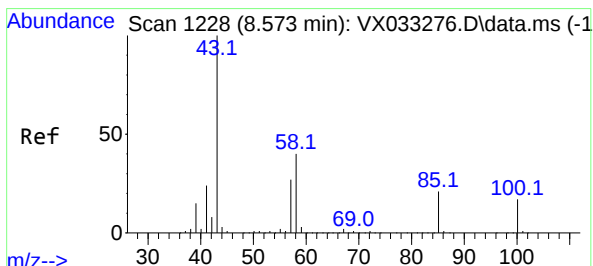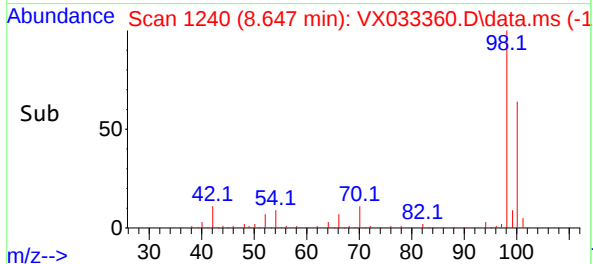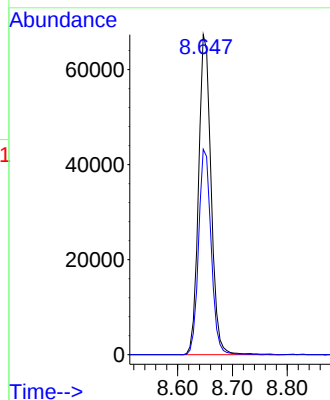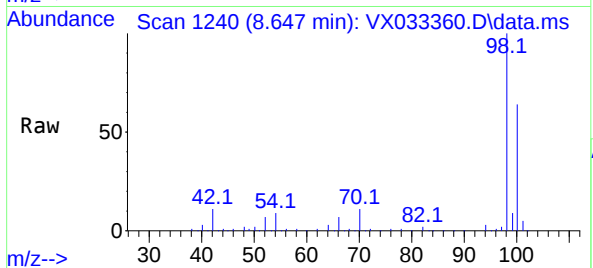

#51

4-Methyl-2-Pentanone

Concen: 0.213 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.073 min

Lab File: VX033360.D




Acq: 09 Dec 2022 20:03


Tgt Ion: 43 Resp: 432

Ion Ratio Lower Upper

43 100

58 181.0 30.9 46.3#


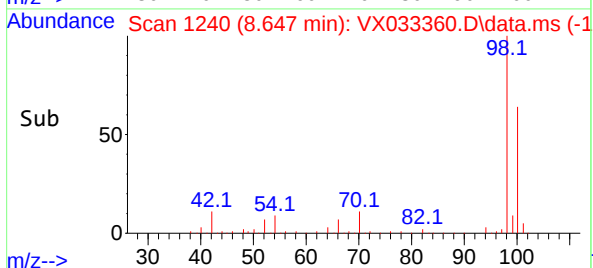
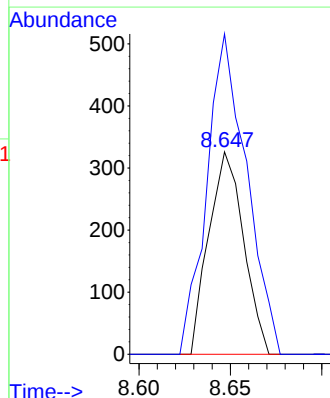
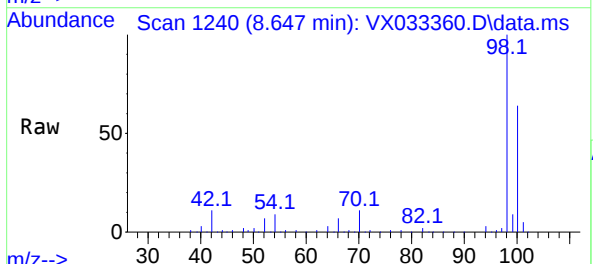


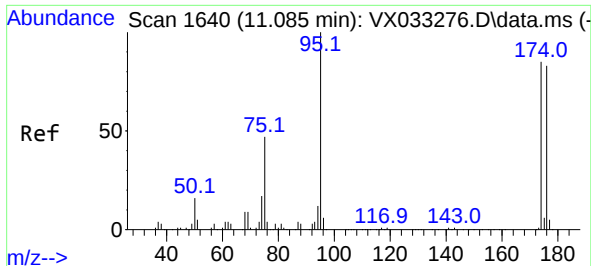

#62
4-Bromofluorobenzene
Concen: 46.194 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03




Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022


Tgt Ion: 95 Resp: 79825
Ion Ratio Lower Upper
95 100
174 82.3 0.0 164.0
176 79.4 0.0 154.4

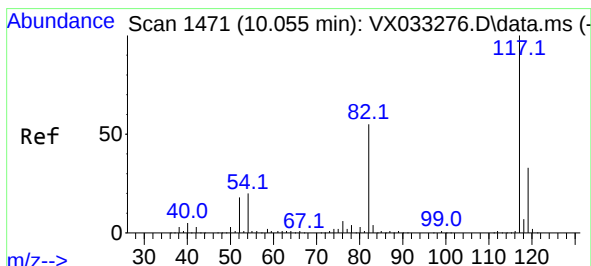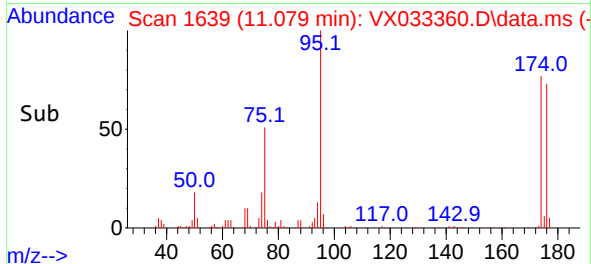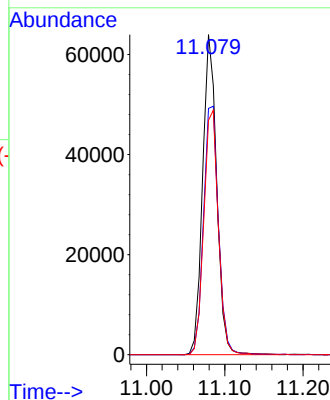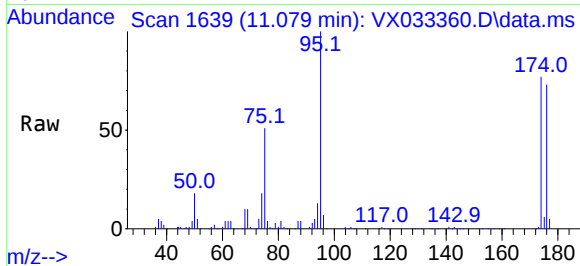

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Tgt Ion: 117 Resp: 209534
Ion Ratio Lower Upper
117 100
82 53.8 44.3 66.5
119 32.3 25.7 38.5


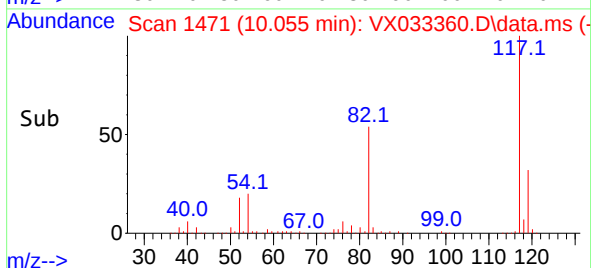
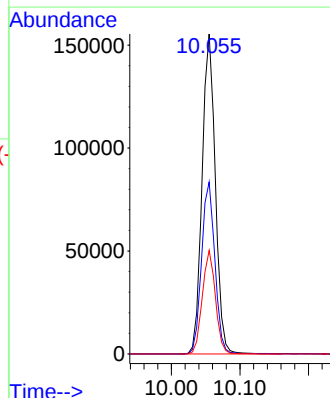
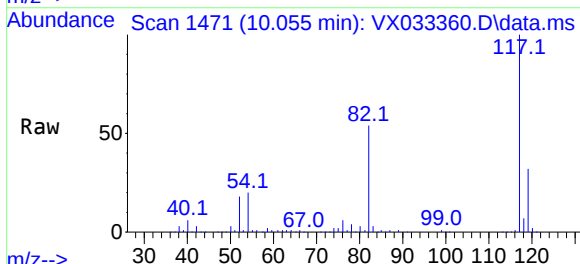


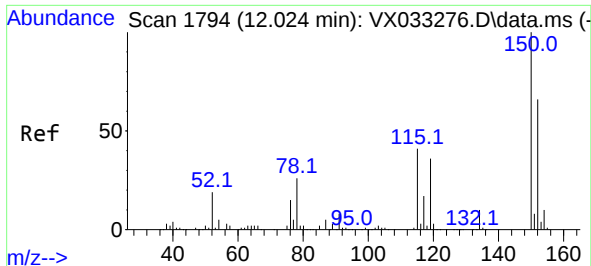

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03




Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022


Tgt Ion:152 Resp: 93353
Ion Ratio Lower Upper
152 100
115 59.3 44.0 132.0
150 155.1 0.0 351.8

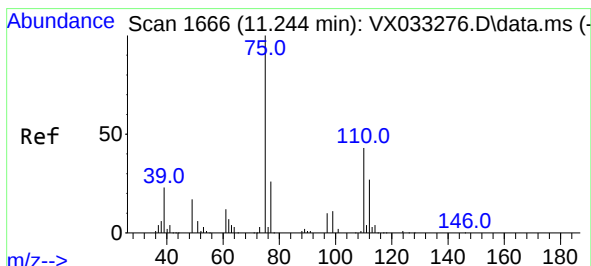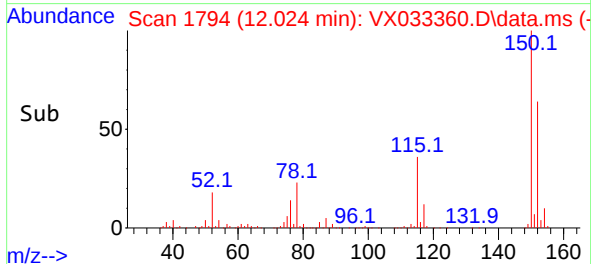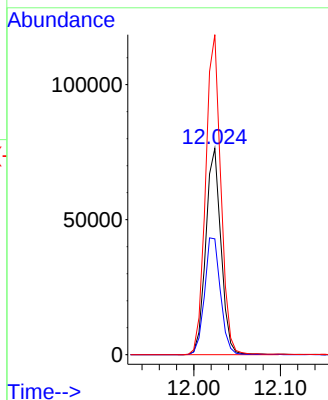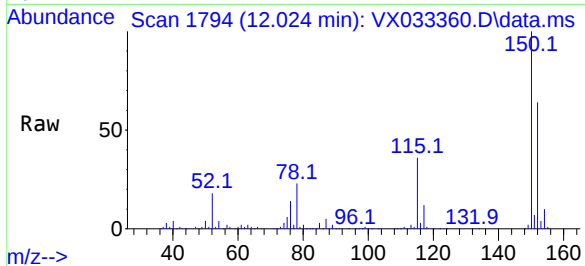

#76
1,2,3-Trichloropropane
Concen: 21.561 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.164 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03


Tgt Ion: 75 Resp: 40951
Ion Ratio Lower Upper
75 100
77 1.3 20.0 60.0#

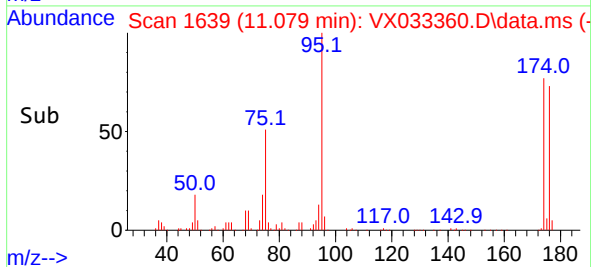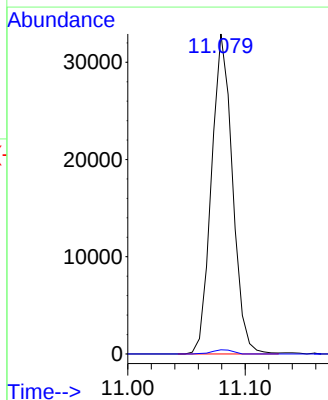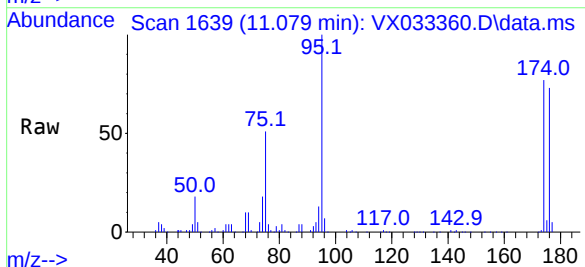

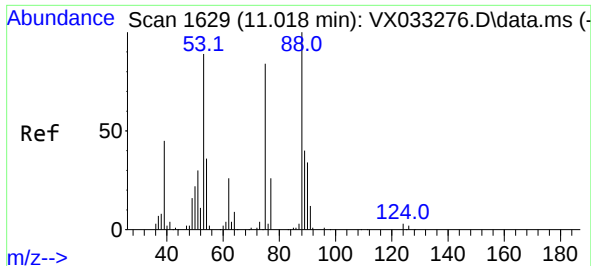

#81
trans-1,4-Dichloro-2-butene
Concen: 67.070 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX033360.D
Acq: 09 Dec 2022 20:03

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-OUT-02-12082022

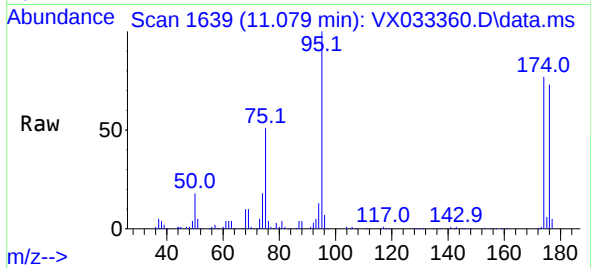

Tgt Ion: 75 Resp: 40951
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

