

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
 Data File : VX033349.D
 Acq On : 09 Dec 2022 15:50
 Operator : JC/MD
 Sample : N5947-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NYE-WATER-1208

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.300	31	35	42	rBV	3131	7749	1.24%	0.239%
2	5.025	638	646	656	rBV4	3070	10136	1.63%	0.313%
3	5.385	694	705	721	rBV	58681	169628	27.23%	5.232%
4	5.550	721	732	747	rVV	157137	447821	71.89%	13.813%
5	5.958	790	799	809	rBV	46069	118892	19.09%	3.667%
6	6.763	921	931	948	rBV	232069	549352	88.19%	16.944%
7	7.129	986	991	1001	rBV4	3150	6540	1.05%	0.202%
8	8.647	1234	1240	1248	rBV	172775	279326	44.84%	8.616%
9	8.720	1248	1252	1265	rVB2	11541	19025	3.05%	0.587%
10	9.275	1338	1343	1351	rVB2	6504	9068	1.46%	0.280%
11	10.055	1465	1471	1487	rBV	462056	622939	100.00%	19.214%
12	11.079	1634	1639	1651	rBV	314334	407655	65.44%	12.574%
13	12.024	1788	1794	1801	rBV	449138	587233	94.27%	18.113%
14	14.993	2275	2281	2289	rBV5	4246	6717	1.08%	0.207%




Sum of corrected areas: 3242081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033349.D
Acq On : 09 Dec 2022 15:50
Operator : JC/MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

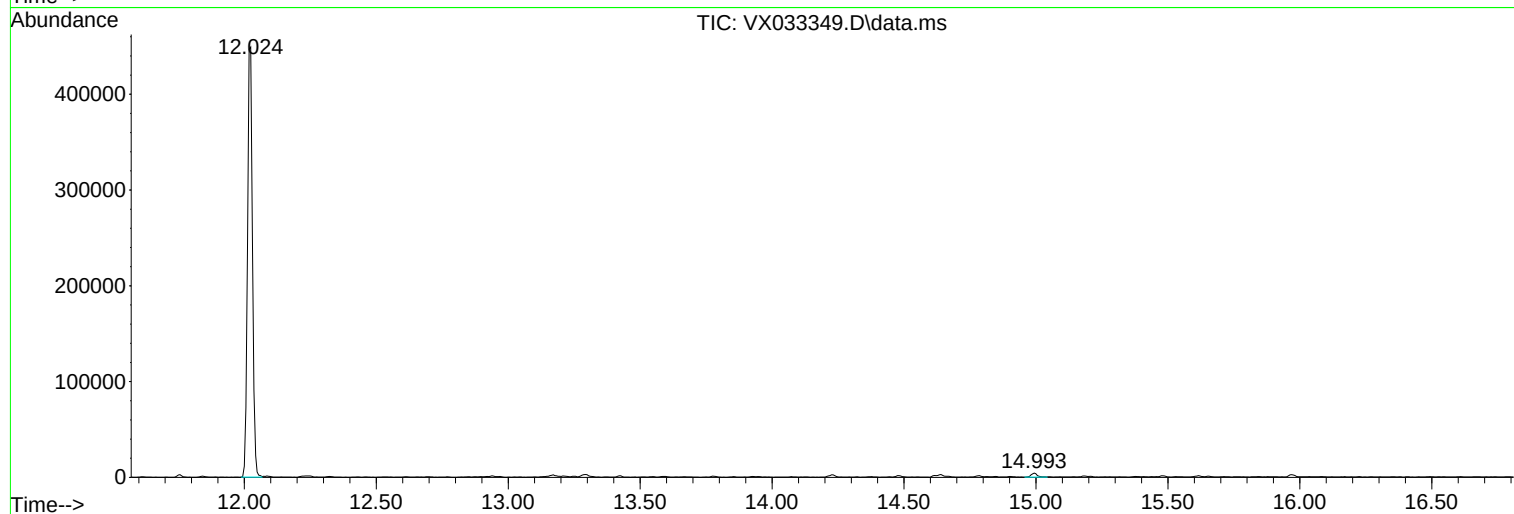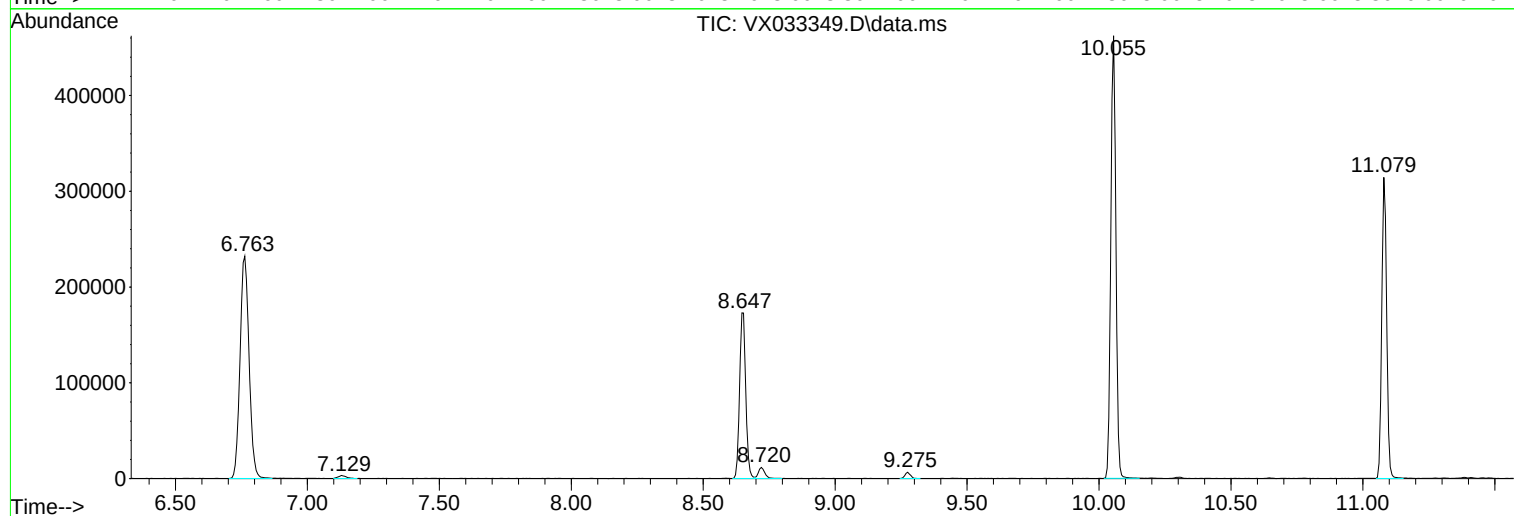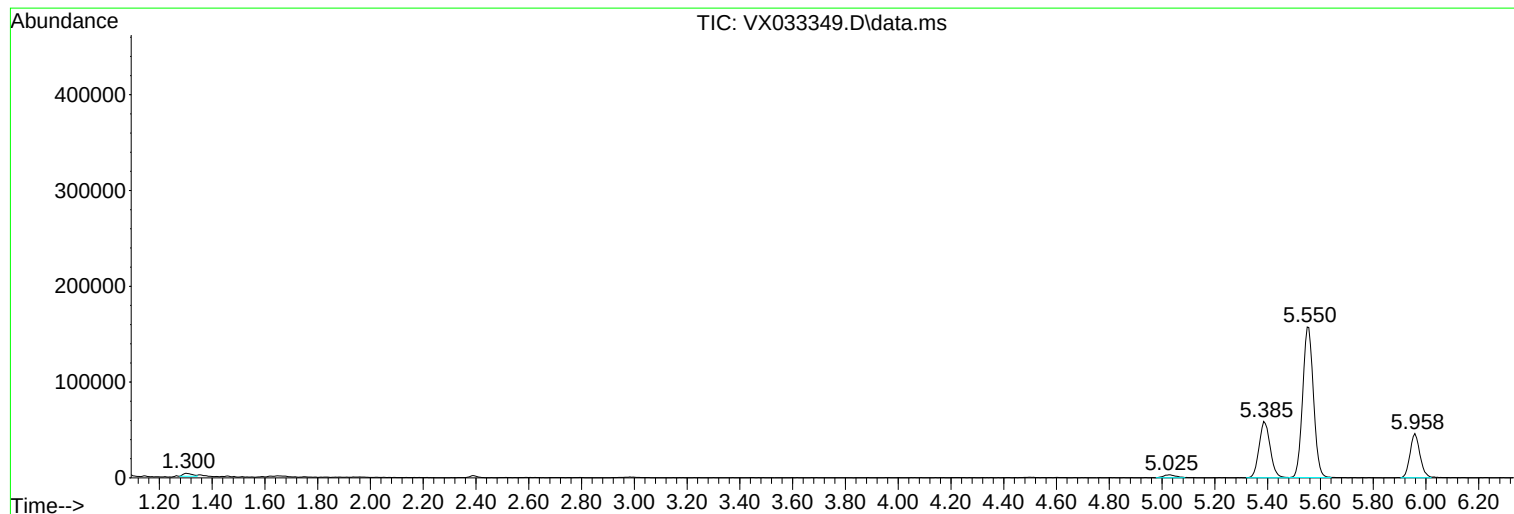

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033349.D
Acq On : 09 Dec 2022 15:50
Operator : JC/MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033349.D
Acq On : 09 Dec 2022 15:50
Operator : JC/MD
Sample : N5947-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NYE-WATER-1208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------