

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
 Data File : VX033350.D
 Acq On : 09 Dec 2022 16:13
 Operator : JC/MD
 Sample : N5906-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-23R

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.343	200	206	212	rBV3	4088	7660	1.21%	0.221%
2	2.782	269	278	284	rBV4	3663	7869	1.24%	0.227%
3	3.111	326	332	341	rBV2	3952	8360	1.32%	0.241%
4	4.428	540	548	561	rVB7	2246	6996	1.10%	0.202%
5	5.391	693	706	718	rBV2	57732	171086	26.96%	4.941%
6	5.550	722	732	755	rVB	158981	451966	71.21%	13.054%
7	5.958	789	799	810	rBV2	44994	120523	18.99%	3.481%
8	6.251	835	847	862	rBV3	15982	51676	8.14%	1.492%
9	6.763	919	931	944	rBV	231313	548771	86.47%	15.849%
10	7.988	1125	1132	1138	rVB6	2768	6605	1.04%	0.191%
11	8.110	1146	1152	1163	rVB3	4904	11128	1.75%	0.321%
12	8.427	1198	1204	1210	rBV	3996	7129	1.12%	0.206%
13	8.507	1210	1217	1230	rVB2	10500	18467	2.91%	0.533%
14	8.647	1230	1240	1250	rBV	179581	288467	45.45%	8.331%
15	8.842	1265	1272	1280	rBV2	11039	18293	2.88%	0.528%
16	8.958	1286	1291	1300	rVB	15097	25285	3.98%	0.730%
17	9.049	1300	1306	1312	rBV	16305	26114	4.11%	0.754%
18	10.055	1460	1471	1477	rBV	471118	634660	100.00%	18.330%
19	10.147	1483	1486	1491	rVB4	5267	7310	1.15%	0.211%
20	11.079	1634	1639	1649	rBV	329390	414830	65.36%	11.981%
21	12.024	1788	1794	1802	rBV	456852	582103	91.72%	16.812%
22	12.244	1823	1830	1837	rVB2	6822	9644	1.52%	0.279%
23	12.646	1892	1896	1900	rVB	9986	12395	1.95%	0.358%
24	13.664	2056	2063	2068	rVB	16031	25062	3.95%	0.724%




Sum of corrected areas: 3462399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033350.D
Acq On : 09 Dec 2022 16:13
Operator : JC/MD
Sample : N5906-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

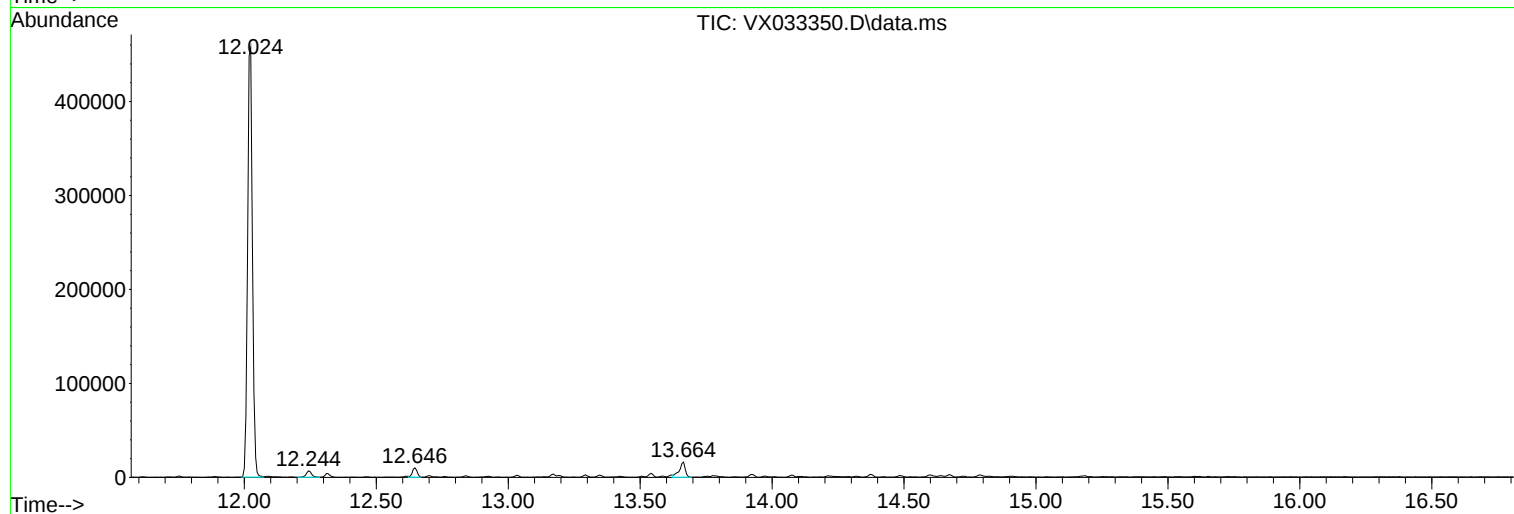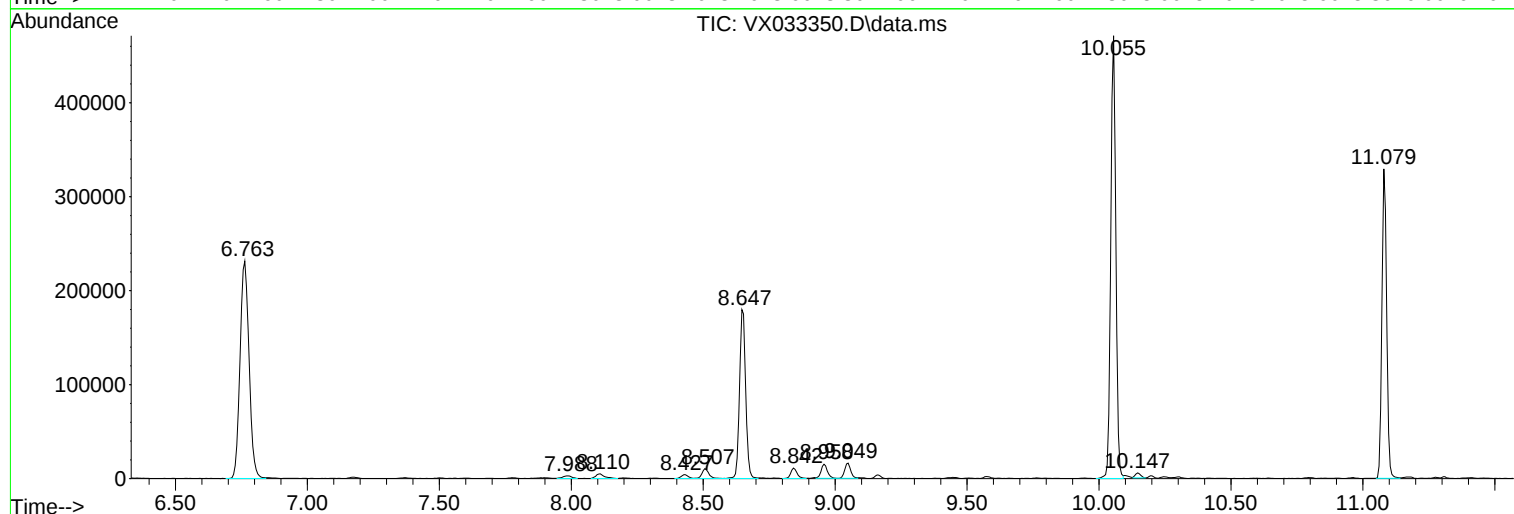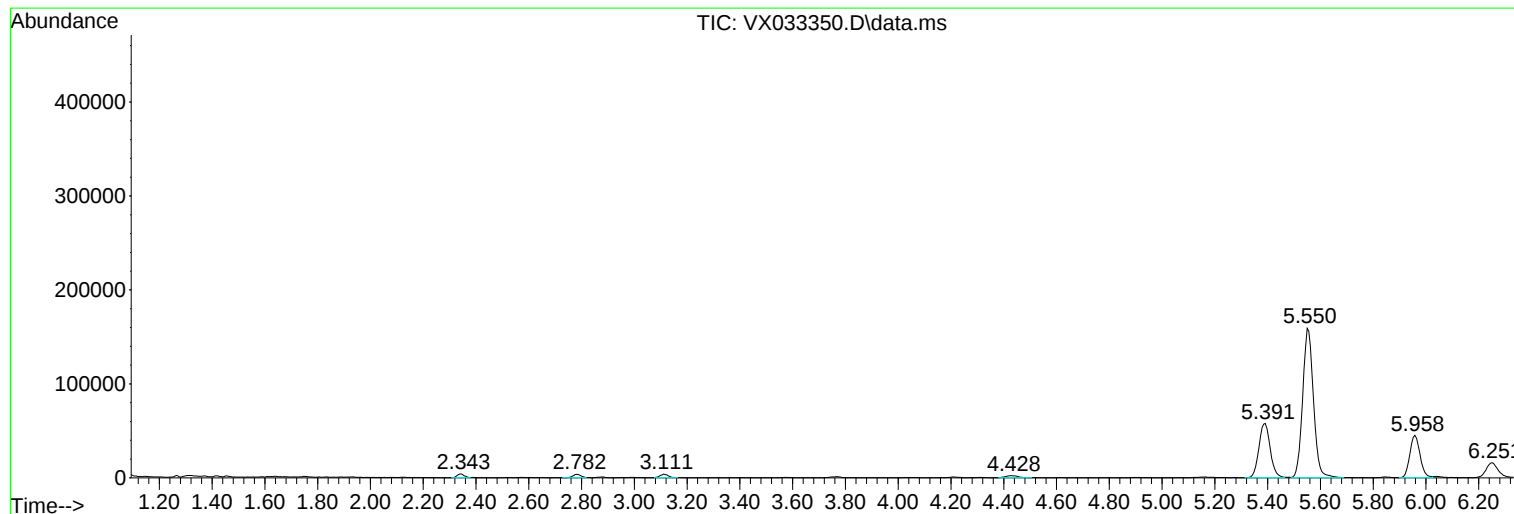

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033350.D
Acq On : 09 Dec 2022 16:13
Operator : JC/MD
Sample : N5906-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033350.D
Acq On : 09 Dec 2022 16:13
Operator : JC/MD
Sample : N5906-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------