

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033356.D
Acq On : 09 Dec 2022 18:31
Operator : JC/MD
Sample : N5976-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-1-2-3-4-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	25	33	42	rBV3	3662	11588	1.95%	0.376%
2	5.385	694	705	722	rBV	58067	172082	28.90%	5.585%
3	5.550	722	732	748	rVV	149380	424682	71.32%	13.783%
4	5.958	787	799	818	rBV	44514	121078	20.33%	3.929%
5	6.763	918	931	946	rBV	224963	527278	88.55%	17.112%
6	8.647	1234	1240	1249	rBV	177048	279890	47.00%	9.084%
7	10.055	1465	1471	1485	rBV	434388	595448	100.00%	19.325%
8	11.079	1634	1639	1649	rBV	315668	401396	67.41%	13.027%
9	12.024	1788	1794	1803	rBV	424268	547819	92.00%	17.779%




Sum of corrected areas: 3081261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033356.D
Acq On : 09 Dec 2022 18:31
Operator : JC/MD
Sample : N5976-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-1-2-3-4-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

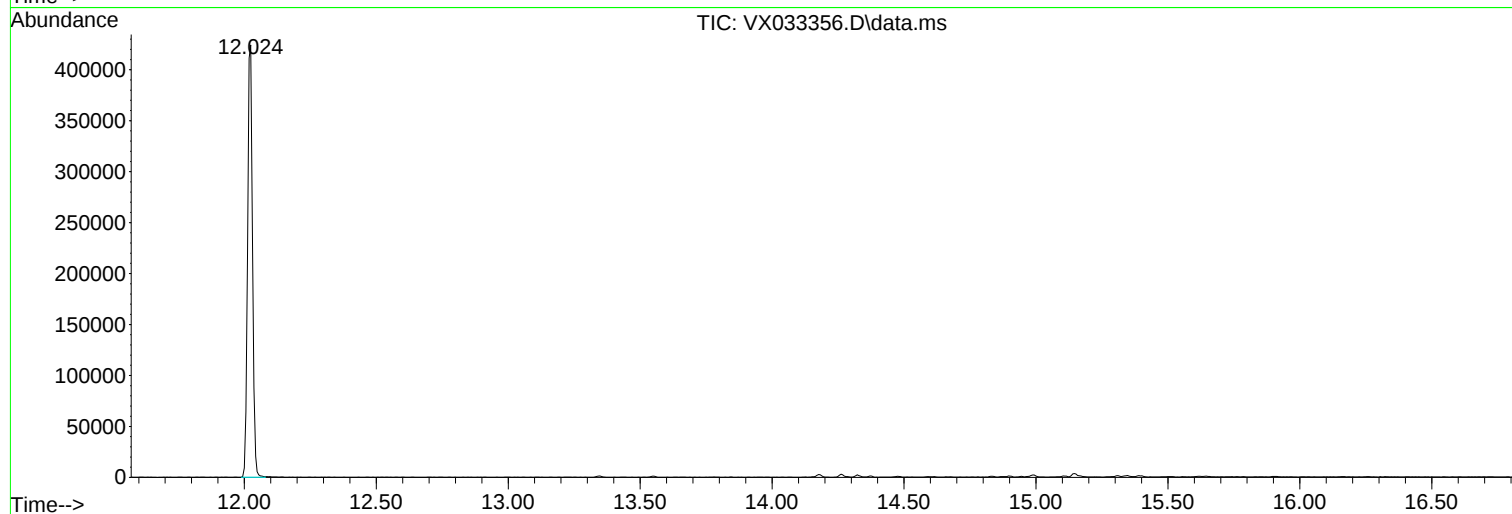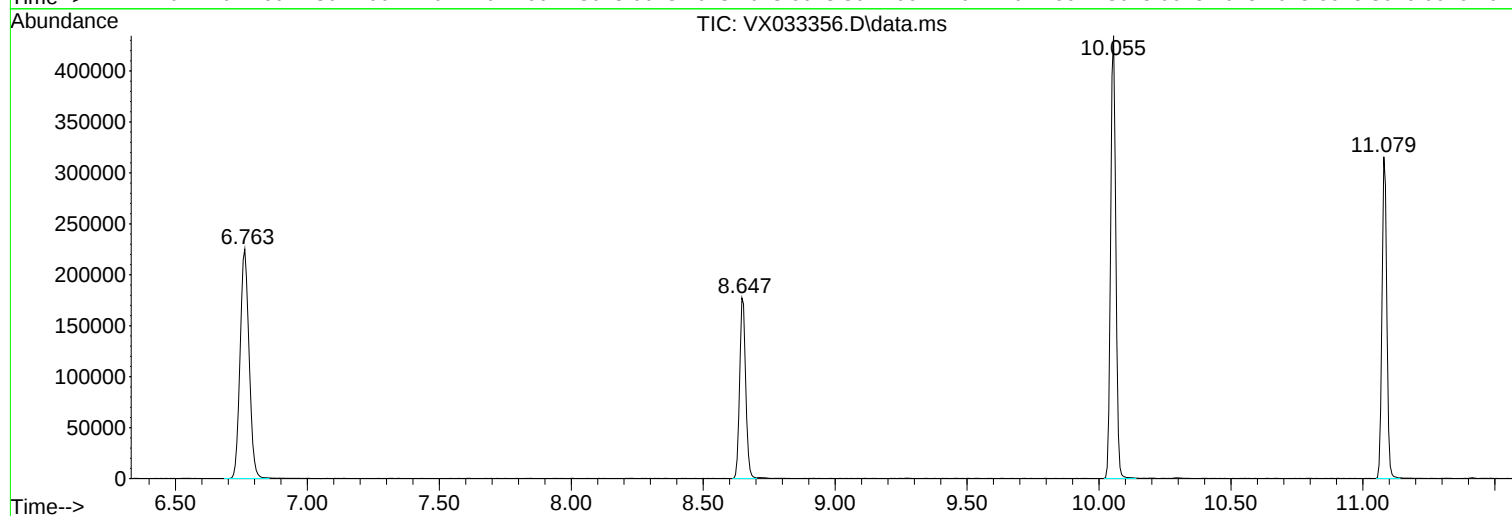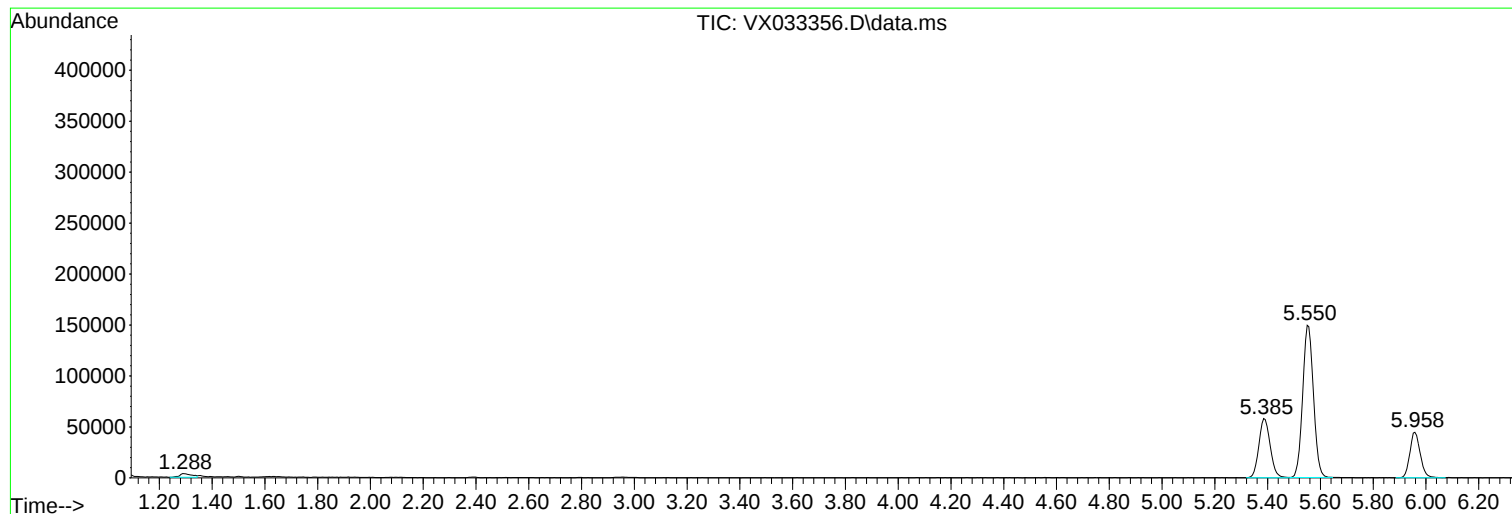

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033356.D
Acq On : 09 Dec 2022 18:31
Operator : JC/MD
Sample : N5976-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-1-2-3-4-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033356.D
Acq On : 09 Dec 2022 18:31
Operator : JC/MD
Sample : N5976-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-1-2-3-4-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc