

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
 Data File : VX033357.D
 Acq On : 09 Dec 2022 18:54
 Operator : JC/MD
 Sample : N5977-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-SAMPLE-TANK-6-7-8-9-16

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.502	64	68	73	rVB	5713	6489	1.08%	0.207%
2	2.568	236	243	258	rBV2	2108	7539	1.25%	0.241%
3	2.940	297	304	314	rBV2	4682	11302	1.88%	0.361%
4	5.385	695	705	719	rBV	56301	168062	27.95%	5.365%
5	5.556	721	733	750	rVV	151489	425814	70.83%	13.592%
6	5.958	789	799	815	rBV	44771	118871	19.77%	3.794%
7	6.763	921	931	947	rBV	221823	531130	88.34%	16.954%
8	8.647	1234	1240	1249	rBV	174530	275129	45.76%	8.782%
9	10.055	1465	1471	1487	rBV	449974	601201	100.00%	19.191%
10	11.079	1634	1639	1652	rBV	308589	397860	66.18%	12.700%
11	12.024	1788	1794	1805	rBV	435605	557363	92.71%	17.792%
12	14.176	2143	2147	2152	rVB	4827	6333	1.05%	0.202%
13	14.261	2156	2161	2167	rBV2	4792	6818	1.13%	0.218%
14	14.987	2277	2280	2286	rVB2	4486	6578	1.09%	0.210%
15	15.145	2302	2306	2314	rBV4	7557	12231	2.03%	0.390%




Sum of corrected areas: 3132720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033357.D
Acq On : 09 Dec 2022 18:54
Operator : JC/MD
Sample : N5977-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-6-7-8-9-16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

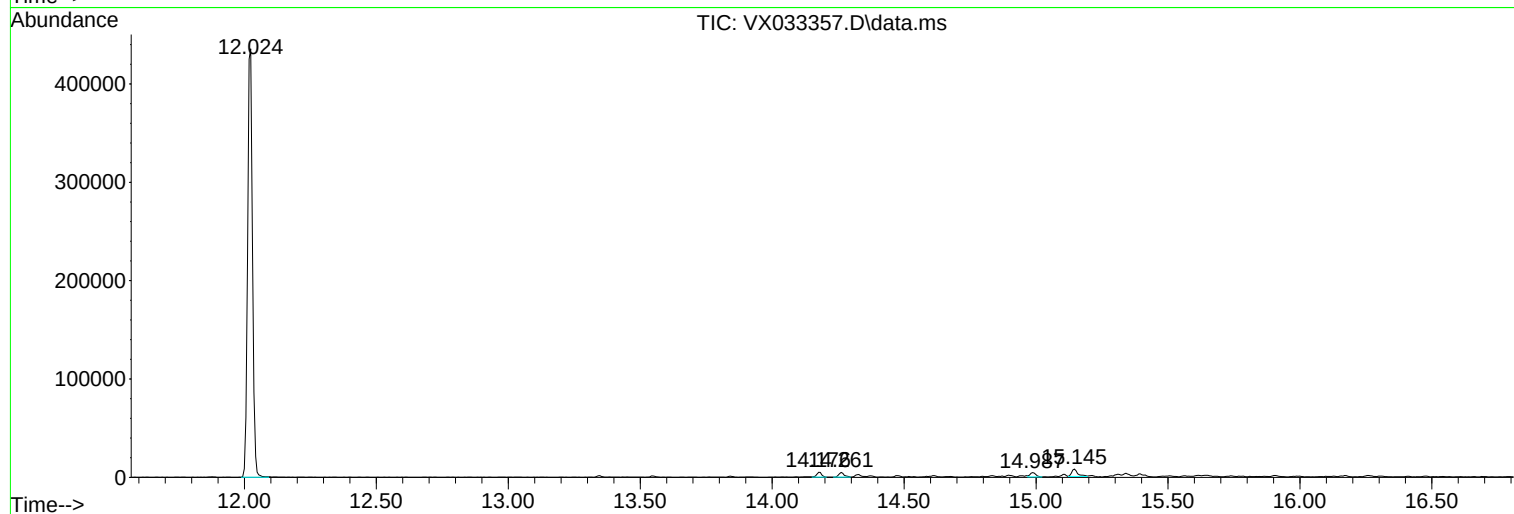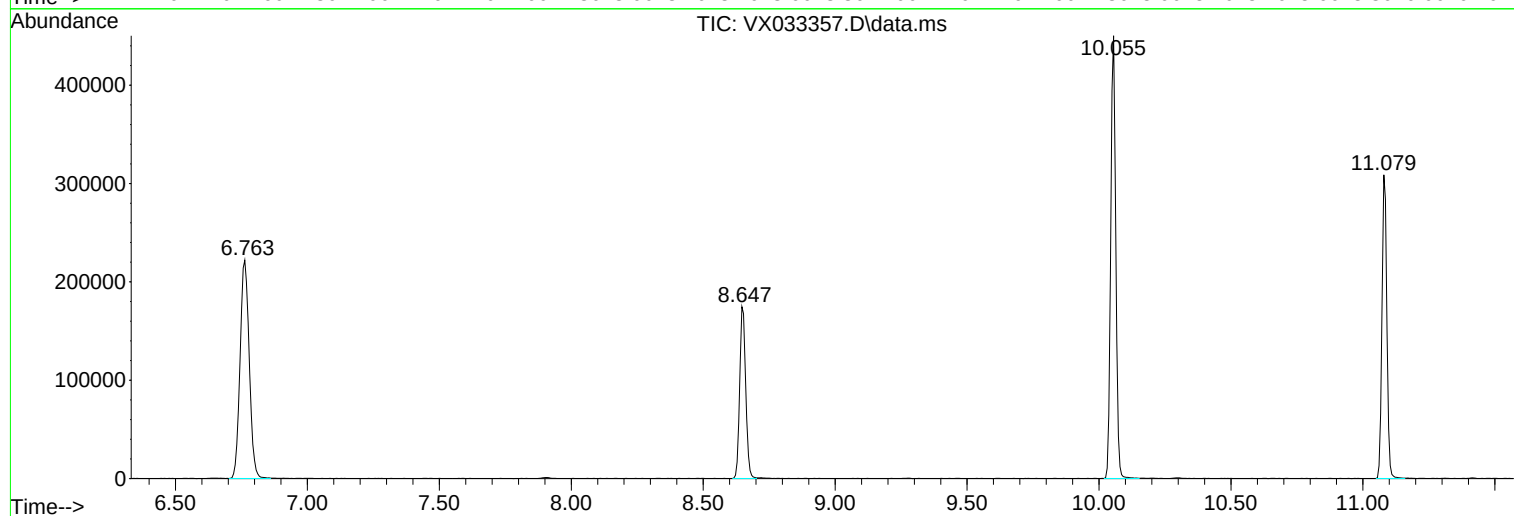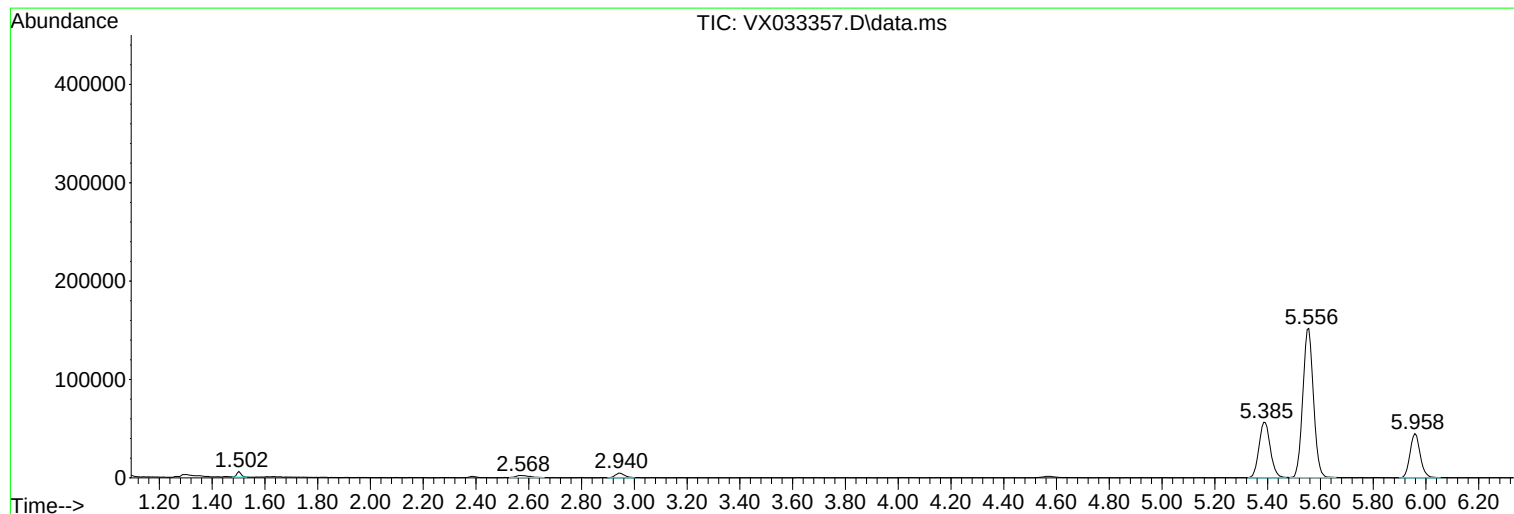

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033357.D
Acq On : 09 Dec 2022 18:54
Operator : JC/MD
Sample : N5977-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-6-7-8-9-16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120922\
Data File : VX033357.D
Acq On : 09 Dec 2022 18:54
Operator : JC/MD
Sample : N5977-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-6-7-8-9-16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------