

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039107.D
 Acq On : 08 Dec 2023 16:09
 Operator : JC/MD
 Sample : VX1209WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	24	26	27	rBV2	2706	2689	0.25%	0.032%
2	1.368	42	46	57	rVB	142827	151184	14.11%	1.787%
3	1.447	57	59	63	rVB2	1969	2424	0.23%	0.029%
4	1.502	67	68	72	rVB	2881	3102	0.29%	0.037%
5	1.569	75	79	81	rBV	3210	3541	0.33%	0.042%
6	1.666	91	95	104	rBV	95560	132449	12.36%	1.566%
7	1.825	119	121	124	rVB2	1988	2256	0.21%	0.027%
8	1.886	129	131	134	rVB2	2406	2629	0.25%	0.031%
9	1.929	134	138	139	rBV3	1143	1724	0.16%	0.020%
10	2.069	159	161	163	rVB2	1473	1154	0.11%	0.014%
11	2.179	176	179	181	rBV2	821	1086	0.10%	0.013%
12	2.307	194	200	212	rVB	230072	367975	34.35%	4.349%
13	2.514	230	234	237	rBV2	2991	4253	0.40%	0.050%
14	2.544	237	239	243	rVB	1296	1167	0.11%	0.014%
15	2.703	262	265	268	rBV	1698	2921	0.27%	0.035%
16	2.947	298	305	307	rBV3	4513	7654	0.71%	0.090%
17	3.032	313	319	322	rBV	1976	3665	0.34%	0.043%
18	3.648	418	420	423	rBV	1277	1797	0.17%	0.021%
19	3.800	443	445	446	rVB	1652	1155	0.11%	0.014%
20	3.831	446	450	451	rBV	1725	1954	0.18%	0.023%
21	4.032	482	483	485	rVV	1890	1195	0.11%	0.014%
22	4.056	485	487	488	rVV	1953	1393	0.13%	0.016%
23	4.075	488	490	492	rVV	2257	1898	0.18%	0.022%
24	4.099	492	494	495	rVB	2142	1290	0.12%	0.015%
25	4.446	543	551	564	rBV	99827	283453	26.46%	3.350%
26	4.794	607	608	611	rBV	1476	1681	0.16%	0.020%
27	4.891	621	624	626	rVB	1776	1532	0.14%	0.018%
28	5.050	639	650	664	rBV	141185	422222	39.41%	4.991%
29	5.208	672	676	677	rBV	1161	1345	0.13%	0.016%
30	5.422	710	711	713	rVB	2170	1232	0.11%	0.015%
31	5.849	779	781	783	rBV	1353	1238	0.12%	0.015%
32	5.964	789	800	816	rBV2	355390	1071346	100.00%	12.663%
33	6.288	851	853	855	rVB	2118	1528	0.14%	0.018%
34	6.312	855	857	859	rBV	1714	1884	0.18%	0.022%
35	6.410	871	873	876	rBV	1212	1070	0.10%	0.013%
36	6.647	911	912	917	rVB	1683	1551	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039107.D
 Acq On : 08 Dec 2023 16:09
 Operator : JC/MD
 Sample : VX1209WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	6.757	921	930	942	rBV	261595	627541	58.58%	7.417%
38	7.025	972	974	977	rVB	2169	2459	0.23%	0.029%
39	7.092	982	985	986	rBV	1435	1705	0.16%	0.020%
40	7.184	998	1000	1005	rBV	1239	1211	0.11%	0.014%
41	7.306	1012	1020	1035	rBV	218386	491742	45.90%	5.812%
42	7.513	1052	1054	1056	rVB	1983	1401	0.13%	0.017%
43	7.592	1064	1067	1068	rBV	2234	1930	0.18%	0.023%
44	7.629	1071	1073	1076	rVV	1417	1553	0.14%	0.018%
45	7.976	1128	1130	1131	rBV	1149	1153	0.11%	0.014%
46	8.043	1140	1141	1144	rBV	1684	1789	0.17%	0.021%
47	8.080	1146	1147	1150	rBV	1501	1424	0.13%	0.017%
48	8.165	1158	1161	1165	rBV2	1222	1864	0.17%	0.022%
49	8.257	1174	1176	1181	rVB	1348	1784	0.17%	0.021%
50	8.324	1181	1187	1197	rBV	157849	267917	25.01%	3.167%
51	8.452	1204	1208	1212	rVB2	1290	2348	0.22%	0.028%
52	8.488	1212	1214	1217	rBV	1785	1377	0.13%	0.016%
53	8.586	1228	1230	1233	rBV	1391	1601	0.15%	0.019%
54	8.647	1233	1240	1255	rBV	541016	856262	79.92%	10.121%
55	8.946	1284	1289	1297	rBV	115850	176979	16.52%	2.092%
56	9.043	1304	1305	1307	rBV	1375	1144	0.11%	0.014%
57	9.318	1348	1350	1351	rVB	2293	1279	0.12%	0.015%
58	9.378	1355	1360	1371	rBV	465823	673197	62.84%	7.957%
59	9.702	1409	1413	1416	rVV2	2176	3676	0.34%	0.043%
60	10.055	1465	1471	1485	rVV	529064	765536	71.46%	9.049%
61	10.250	1501	1503	1506	rVB	2127	1364	0.13%	0.016%
62	10.305	1510	1512	1515	rBV	1536	1304	0.12%	0.015%
63	10.525	1546	1548	1549	rBV2	1675	1683	0.16%	0.020%
64	10.647	1566	1568	1569	rBV	1631	1316	0.12%	0.016%
65	10.738	1581	1583	1586	rVB	1553	1366	0.13%	0.016%
66	10.762	1586	1587	1591	rBV	1633	1672	0.16%	0.020%
67	10.915	1611	1612	1615	rBV	1938	1510	0.14%	0.018%
68	10.964	1618	1620	1622	rVV3	1633	1409	0.13%	0.017%
69	11.018	1628	1629	1631	rBV	1552	1211	0.11%	0.014%
70	11.189	1652	1657	1666	rBV	418767	532645	49.72%	6.296%
71	11.482	1704	1705	1708	rBV	2169	1524	0.14%	0.018%
72	11.506	1708	1709	1714	rBV	1280	1722	0.16%	0.020%
73	11.671	1734	1736	1737	rBV	1752	1206	0.11%	0.014%
74	11.750	1748	1749	1754	rVV2	1763	1562	0.15%	0.018%
75	11.811	1758	1759	1761	rVB	2088	1276	0.12%	0.015%
76	11.841	1761	1764	1766	rBV	1461	1913	0.18%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039107.D
 Acq On : 08 Dec 2023 16:09
 Operator : JC/MD
 Sample : VX1209WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK641

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	11.866	1766	1768	1770	rBV	2036	1434	0.13%	0.017%
78	11.963	1782	1784	1785	rBV	1774	1802	0.17%	0.021%
79	12.018	1788	1793	1803	rVB	583473	762201	71.14%	9.009%
80	12.317	1837	1842	1851	rVB	566189	713611	66.61%	8.435%
81	12.561	1881	1882	1885	rBV	1458	1501	0.14%	0.018%
82	13.049	1959	1962	1964	rBV	1593	2192	0.20%	0.026%
83	13.091	1966	1969	1970	rBV	1920	1983	0.19%	0.023%
84	13.116	1970	1973	1975	rVB	2078	2184	0.20%	0.026%
85	13.250	1994	1995	1998	rVV	1735	1248	0.12%	0.015%
86	13.280	1998	2000	2003	rBV	1037	1142	0.11%	0.013%
87	13.390	2017	2018	2022	rBV	1903	2420	0.23%	0.029%
88	13.780	2078	2082	2086	rVB	5772	6386	0.60%	0.075%
89	13.963	2109	2112	2116	rVB2	4548	4643	0.43%	0.055%
90	14.219	2152	2154	2159	rVB	1507	2256	0.21%	0.027%
91	14.439	2188	2190	2192	rBV	1838	1279	0.12%	0.015%
92	14.524	2202	2204	2207	rBV	1389	1404	0.13%	0.017%
93	14.621	2217	2220	2223	rVB	1725	2074	0.19%	0.025%
94	14.652	2223	2225	2227	rVB	1594	1304	0.12%	0.015%
95	14.670	2227	2228	2232	rBV	2116	2599	0.24%	0.031%
96	14.743	2238	2240	2243	rBV	2035	2033	0.19%	0.024%
97	15.195	2312	2314	2317	rBV	1815	2350	0.22%	0.028%
98	15.896	2425	2429	2432	rBV	2032	3249	0.30%	0.038%
99	16.456	2520	2521	2524	rBV	1691	1656	0.15%	0.020%
100	16.652	2551	2553	2555	rBV	1541	1173	0.11%	0.014%




Sum of corrected areas: 8460316

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039107.D
Acq On : 08 Dec 2023 16:09
Operator : JC/MD
Sample : VX1209WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

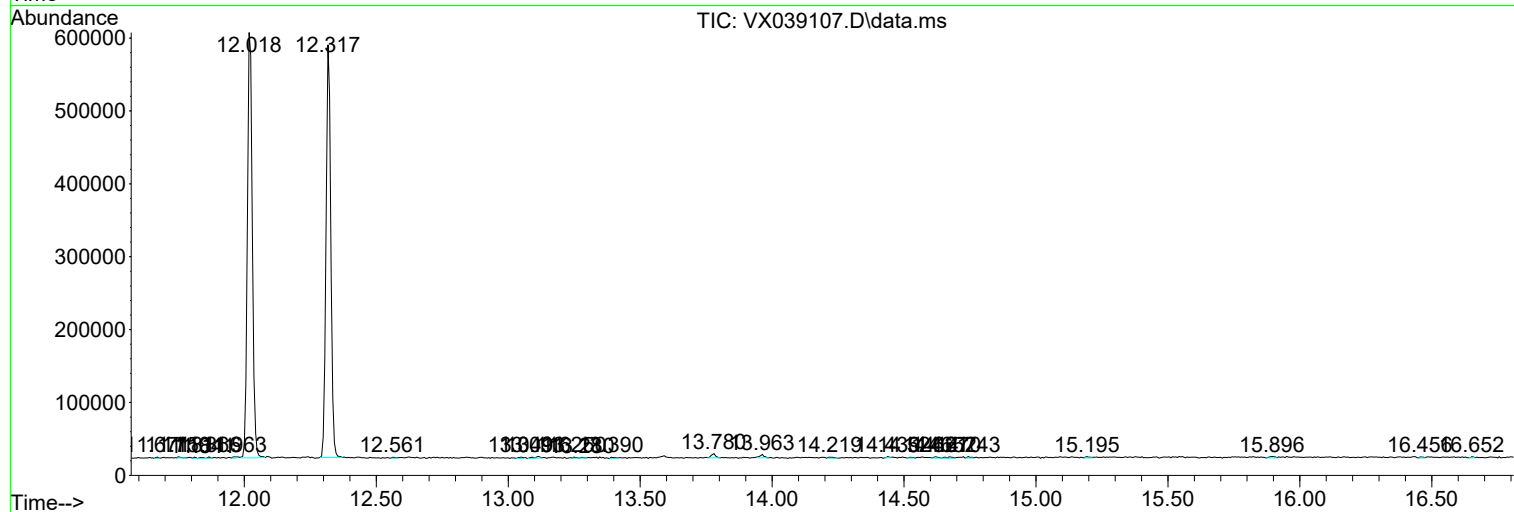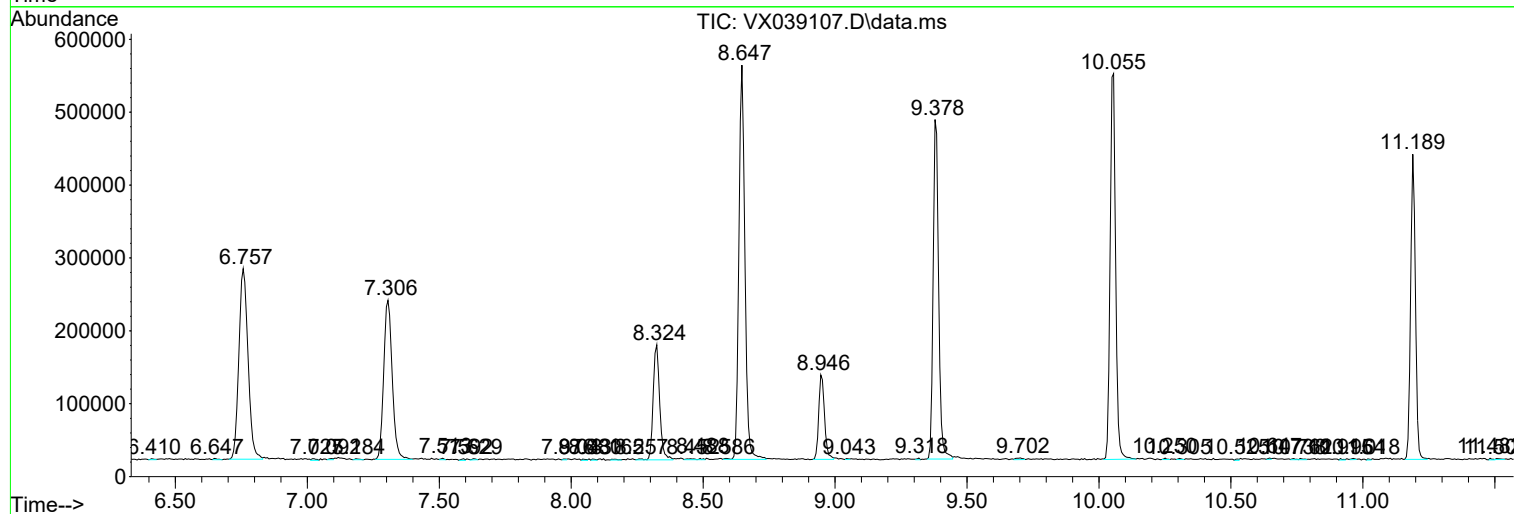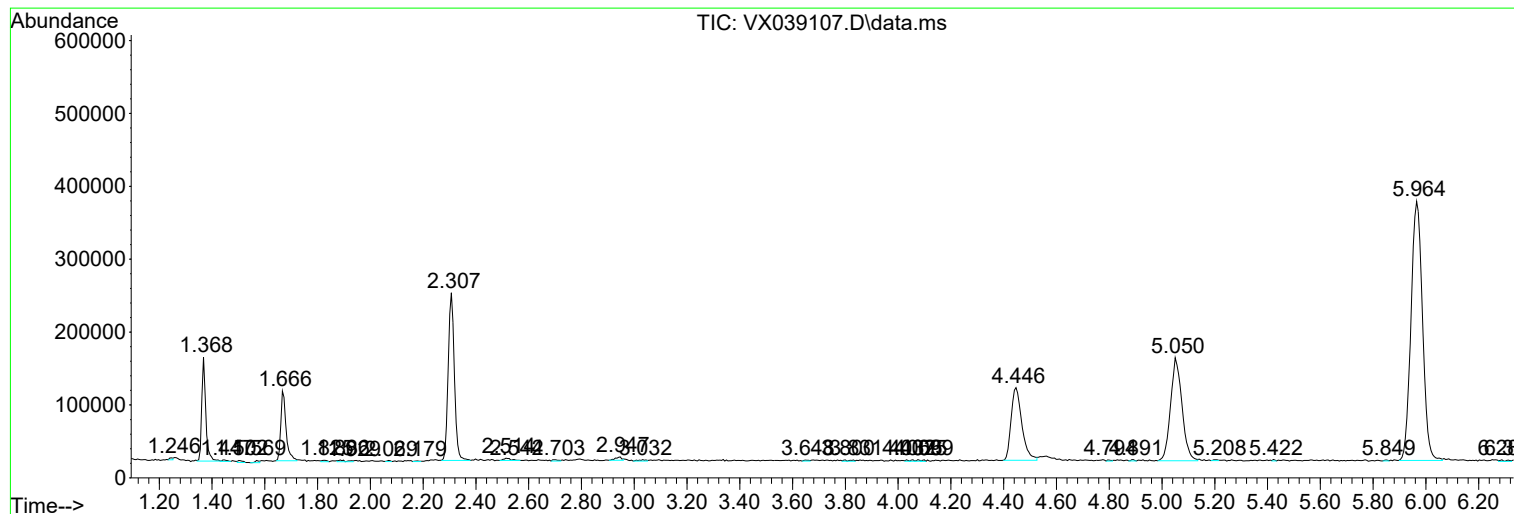

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039107.D
Acq On : 08 Dec 2023 16:09
Operator : JC/MD
Sample : VX1209WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039107.D
Acq On : 08 Dec 2023 16:09
Operator : JC/MD
Sample : VX1209WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK641

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc