

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039108.D
 Acq On : 08 Dec 2023 16:32
 Operator : JC/MD
 Sample : VX1209MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rBV	134506	139728	13.67%	1.737%
2	1.477	62	64	65	rBV	1102	870	0.09%	0.011%
3	1.575	75	80	82	rBV2	4369	8050	0.79%	0.100%
4	1.593	82	83	85	rVV	1929	1558	0.15%	0.019%
5	1.672	91	96	106	rBV	93101	132862	13.00%	1.652%
6	1.788	113	115	117	rVB2	1530	937	0.09%	0.012%
7	2.014	150	152	153	rBV	1649	742	0.07%	0.009%
8	2.038	153	156	158	rBV	1939	2427	0.24%	0.030%
9	2.227	184	187	188	rBV	2231	2288	0.22%	0.028%
10	2.306	194	200	211	rVB	216256	340582	33.32%	4.234%
11	2.514	231	234	239	rVB	3604	5850	0.57%	0.073%
12	2.599	246	248	249	rBV	1482	1347	0.13%	0.017%
13	2.776	275	277	278	rBV	2135	1800	0.18%	0.022%
14	2.867	290	292	295	rBV2	1385	1418	0.14%	0.018%
15	2.934	301	303	305	rBV2	2979	2718	0.27%	0.034%
16	3.087	326	328	329	rBV	1753	933	0.09%	0.012%
17	3.257	354	356	357	rBV	1562	862	0.08%	0.011%
18	3.379	374	376	379	rVB	1963	1822	0.18%	0.023%
19	3.495	393	395	397	rBV	1413	1363	0.13%	0.017%
20	3.568	406	407	411	rBV	1959	2149	0.21%	0.027%
21	3.837	449	451	452	rBV	1860	1202	0.12%	0.015%
22	3.952	468	470	471	rVB	1363	575	0.06%	0.007%
23	4.208	510	512	515	rBV	1405	1691	0.17%	0.021%
24	4.446	543	551	564	rBV	92428	265751	26.00%	3.304%
25	4.751	599	601	604	rBV2	1420	1532	0.15%	0.019%
26	4.812	609	611	614	rVB	2460	1926	0.19%	0.024%
27	4.928	629	630	632	rVB	1350	848	0.08%	0.011%
28	4.952	632	634	637	rBV	1509	1497	0.15%	0.019%
29	5.056	640	651	664	rVV2	127411	397548	38.89%	4.942%
30	5.519	725	727	728	rBV	1227	545	0.05%	0.007%
31	5.855	780	782	784	rVB	1424	1032	0.10%	0.013%
32	5.970	789	801	818	rVV2	335100	1022211	100.00%	12.707%
33	6.251	846	847	850	rVB	1863	804	0.08%	0.010%
34	6.373	865	867	871	rVB	2356	1523	0.15%	0.019%
35	6.537	890	894	896	rBV	1280	1627	0.16%	0.020%
36	6.592	901	903	904	rBV	1801	977	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039108.D
 Acq On : 08 Dec 2023 16:32
 Operator : JC/MD
 Sample : VX1209MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.757	922	930	943	rBV	255874	615983	60.26%	7.657%
38	7.056	977	979	980	rBV	1384	1139	0.11%	0.014%
39	7.110	986	988	990	rBV	2410	2835	0.28%	0.035%
40	7.305	1012	1020	1033	rBV	211876	475333	46.50%	5.909%
41	7.494	1049	1051	1055	rBV	1997	2245	0.22%	0.028%
42	7.866	1109	1112	1113	rBV	2105	1531	0.15%	0.019%
43	7.927	1120	1122	1124	rVB	1960	1076	0.11%	0.013%
44	8.122	1152	1154	1157	rBV	1446	1685	0.16%	0.021%
45	8.159	1158	1160	1166	rVV	1543	2364	0.23%	0.029%
46	8.324	1181	1187	1195	rBV	147915	245571	24.02%	3.053%
47	8.647	1234	1240	1252	rBV	496369	794729	77.75%	9.879%
48	8.945	1284	1289	1299	rBV	108174	168981	16.53%	2.101%
49	9.128	1317	1319	1321	rBV	1425	1391	0.14%	0.017%
50	9.171	1324	1326	1327	rBV	1575	1143	0.11%	0.014%
51	9.330	1351	1352	1353	rBV	1119	438	0.04%	0.005%
52	9.384	1355	1361	1372	rVV	420927	634661	62.09%	7.889%
53	9.701	1408	1413	1417	rBV	3973	7456	0.73%	0.093%
54	9.781	1424	1426	1428	rBV	1503	1433	0.14%	0.018%
55	10.055	1465	1471	1482	rBV	528542	761307	74.48%	9.464%
56	10.311	1510	1513	1516	rBV2	2062	2714	0.27%	0.034%
57	10.506	1543	1545	1546	rBV	1686	927	0.09%	0.012%
58	11.079	1637	1639	1643	rBV3	1767	1671	0.16%	0.021%
59	11.189	1652	1657	1669	rVB	395927	508534	49.75%	6.322%
60	11.274	1669	1671	1674	rVB	1945	1905	0.19%	0.024%
61	11.305	1674	1676	1677	rBV	1425	1057	0.10%	0.013%
62	11.756	1748	1750	1752	rBV	1553	1402	0.14%	0.017%
63	12.018	1788	1793	1802	rBV	560931	745299	72.91%	9.265%
64	12.201	1821	1823	1824	rBV	1298	736	0.07%	0.009%
65	12.317	1837	1842	1851	rBV	531025	676304	66.16%	8.407%
66	12.530	1875	1877	1878	rBV	1329	630	0.06%	0.008%
67	12.573	1883	1884	1887	rBV	1675	1745	0.17%	0.022%
68	13.182	1983	1984	1986	rBV	2301	1951	0.19%	0.024%
69	13.268	1996	1998	1999	rBV	1460	1015	0.10%	0.013%
70	13.347	2009	2011	2013	rBV	1441	1440	0.14%	0.018%
71	13.713	2069	2071	2073	rVB	2249	2088	0.20%	0.026%
72	13.743	2073	2076	2078	rBV	1926	2801	0.27%	0.035%
73	13.871	2095	2097	2100	rVB	2423	2675	0.26%	0.033%
74	13.938	2106	2108	2109	rBV2	1301	776	0.08%	0.010%
75	14.030	2122	2123	2124	rBV	1417	546	0.05%	0.007%
76	14.079	2128	2131	2132	rBV	1533	1644	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039108.D
 Acq On : 08 Dec 2023 16:32
 Operator : JC/MD
 Sample : VX1209MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

77	14.359	2175	2177	2178	rBV	1696	1136	0.11%	0.014%
78	14.627	2219	2221	2223	rBV	2549	2585	0.25%	0.032%
79	14.761	2241	2243	2244	rBV	1869	1179	0.12%	0.015%
80	14.987	2279	2280	2281	rBV	2158	1107	0.11%	0.014%
81	15.078	2294	2295	2296	rBV	2123	1263	0.12%	0.016%
82	15.542	2369	2371	2373	rBV	1869	1644	0.16%	0.020%
83	15.871	2423	2425	2428	rVB	2628	2331	0.23%	0.029%
84	16.511	2528	2530	2531	rBV	2342	1758	0.17%	0.022%
85	16.767	2570	2572	2573	rVB	1688	755	0.07%	0.009%




Sum of corrected areas: 8044514

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039108.D
Acq On : 08 Dec 2023 16:32
Operator : JC/MD
Sample : VX1209MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

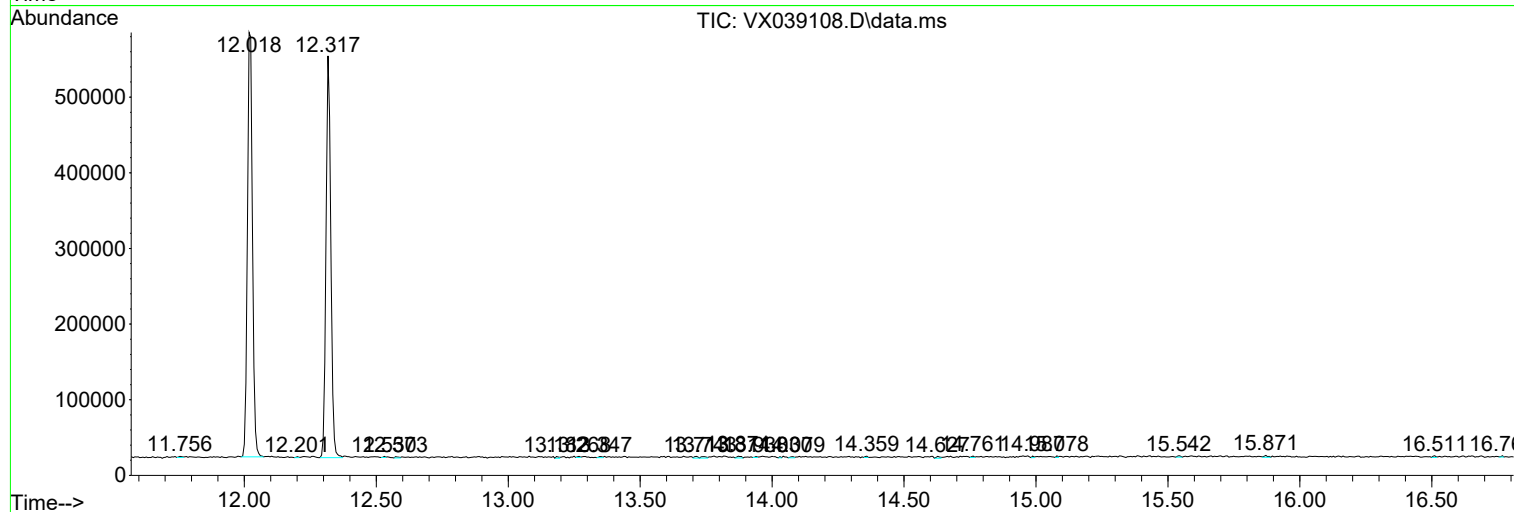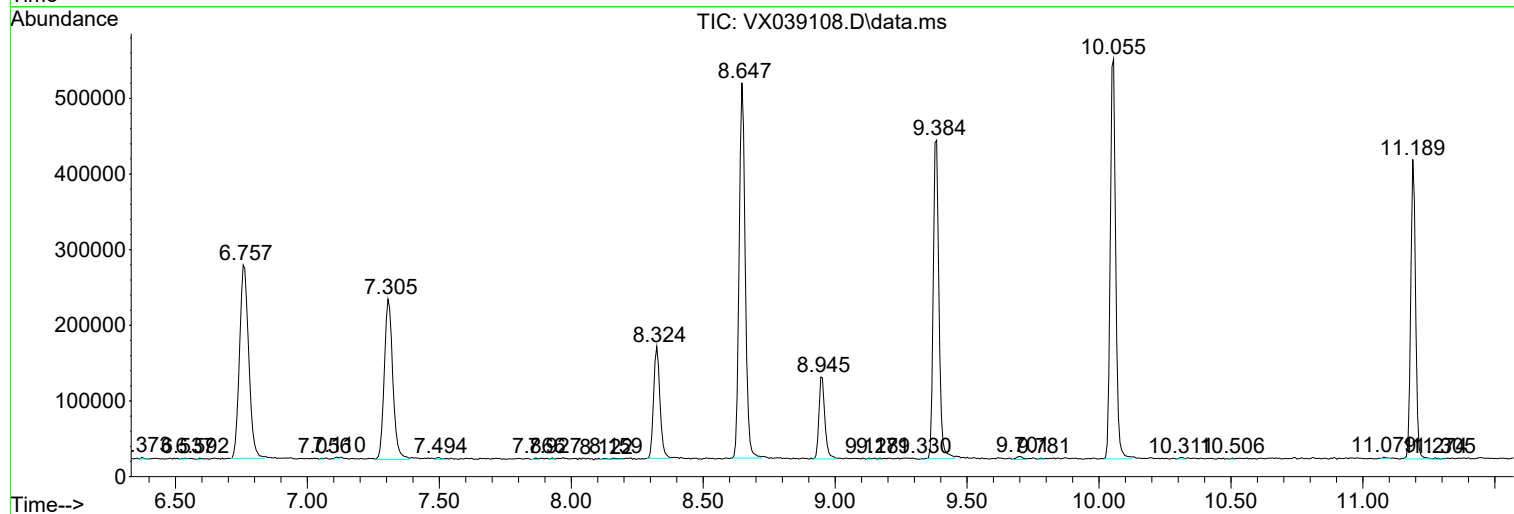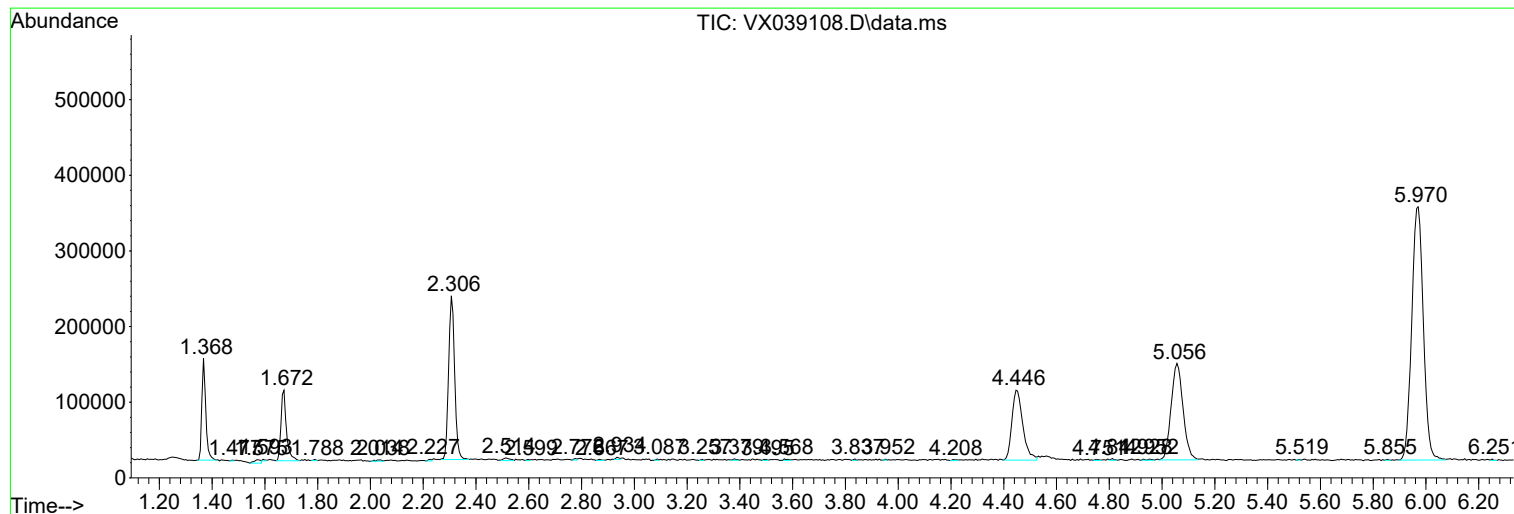

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039108.D
Acq On : 08 Dec 2023 16:32
Operator : JC/MD
Sample : VX1209MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039108.D
Acq On : 08 Dec 2023 16:32
Operator : JC/MD
Sample : VX1209MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc