

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039110.D
 Acq On : 08 Dec 2023 17:18
 Operator : JC/MD
 Sample : 05646-06ME
 Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	37	rVB4	5160	10977	0.73%	0.092%
2	1.368	42	46	57	rBV	155810	210298	14.04%	1.757%
3	1.545	71	75	76	rBV	3545	4170	0.28%	0.035%
4	1.563	76	78	81	rVB4	2611	2345	0.16%	0.020%
5	1.642	85	91	106	rBV2	56353	91968	6.14%	0.768%
6	1.746	106	108	112	rVB5	1454	1816	0.12%	0.015%
7	1.794	112	116	120	rBV	9963	18516	1.24%	0.155%
8	1.880	128	130	133	rVV2	1762	1680	0.11%	0.014%
9	1.929	136	138	140	rVV	2504	1818	0.12%	0.015%
10	2.063	159	160	164	rVB	1882	1526	0.10%	0.013%
11	2.105	164	167	170	rBV2	1379	1595	0.11%	0.013%
12	2.136	170	172	175	rVB2	1795	1509	0.10%	0.013%
13	2.221	181	186	190	rBV	3583	8663	0.58%	0.072%
14	2.288	191	197	208	rVB	325329	505747	33.77%	4.226%
15	2.404	215	216	219	rVB	2078	1295	0.09%	0.011%
16	2.666	257	259	261	rBV	1628	1468	0.10%	0.012%
17	2.709	261	266	270	rVV2	6725	11046	0.74%	0.092%
18	2.770	274	276	279	rVV3	1271	1432	0.10%	0.012%
19	2.819	283	284	287	rBV	1928	2430	0.16%	0.020%
20	2.947	298	305	311	rBV	10311	25854	1.73%	0.216%
21	3.032	317	319	322	rBV	1914	1929	0.13%	0.016%
22	3.087	327	328	331	rVB	2382	2066	0.14%	0.017%
23	3.160	336	340	341	rBV	1214	1319	0.09%	0.011%
24	3.325	366	367	368	rBV	2280	1412	0.09%	0.012%
25	3.380	374	376	379	rBV	1763	2199	0.15%	0.018%
26	3.648	418	420	421	rBV	1573	1327	0.09%	0.011%
27	3.782	440	442	444	rBV2	2066	2201	0.15%	0.018%
28	4.471	548	555	580	rVV	96152	371994	24.84%	3.108%
29	4.672	586	588	591	rBV	1363	1522	0.10%	0.013%
30	4.959	634	635	637	rBV	1549	1302	0.09%	0.011%
31	5.056	639	651	665	rBV	180693	578845	38.65%	4.837%
32	5.300	689	691	694	rBV	1766	1348	0.09%	0.011%
33	5.964	788	800	816	rBV2	517092	1497488	100.00%	12.513%
34	6.141	827	829	833	rBV	1447	1863	0.12%	0.016%
35	6.184	835	836	839	rBV	2039	1861	0.12%	0.016%
36	6.300	853	855	858	rVV	1334	1331	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039110.D
 Acq On : 08 Dec 2023 17:18
 Operator : JC/MD
 Sample : 05646-06ME
 Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.349	862	863	866	rVV	1758	1365	0.09%	0.011%
38	6.397	869	871	872	rBV	2495	1605	0.11%	0.013%
39	6.598	901	904	907	rVB	985	1325	0.09%	0.011%
40	6.757	921	930	943	rBV	385212	965942	64.50%	8.071%
41	6.903	952	954	959	rVB	1817	1704	0.11%	0.014%
42	7.025	971	974	976	rBV	1665	1761	0.12%	0.015%
43	7.056	978	979	981	rBV	1602	1296	0.09%	0.011%
44	7.086	983	984	985	rBV	2474	1363	0.09%	0.011%
45	7.104	985	987	988	rBV2	1903	1547	0.10%	0.013%
46	7.306	1011	1020	1034	rBV	302022	686161	45.82%	5.733%
47	7.464	1044	1046	1048	rBV	1815	1811	0.12%	0.015%
48	7.489	1048	1050	1052	rVB	2221	1442	0.10%	0.012%
49	7.610	1068	1070	1072	rVB	1662	1517	0.10%	0.013%
50	7.769	1094	1096	1098	rBV	1484	1401	0.09%	0.012%
51	7.836	1105	1107	1110	rVB	1707	1419	0.09%	0.012%
52	7.891	1112	1116	1119	rVV	1297	1892	0.13%	0.016%
53	7.921	1119	1121	1125	rVV	1135	1454	0.10%	0.012%
54	8.019	1134	1137	1140	rBV	1118	1628	0.11%	0.014%
55	8.068	1140	1145	1147	rBV	1662	1985	0.13%	0.017%
56	8.324	1181	1187	1197	rVV	219619	373095	24.91%	3.118%
57	8.513	1216	1218	1220	rVB	2212	1463	0.10%	0.012%
58	8.543	1220	1223	1225	rBV	2101	2223	0.15%	0.019%
59	8.647	1234	1240	1255	rBV	759329	1233071	82.34%	10.303%
60	8.787	1261	1263	1265	rVB	2178	1654	0.11%	0.014%
61	8.952	1284	1290	1302	rBV	155819	252972	16.89%	2.114%
62	9.159	1319	1324	1325	rBV	1483	1857	0.12%	0.016%
63	9.250	1336	1339	1341	rBV	1420	2044	0.14%	0.017%
64	9.311	1346	1349	1352	rBV	1212	2148	0.14%	0.018%
65	9.397	1356	1363	1377	rBV	512687	875974	58.50%	7.320%
66	9.714	1414	1415	1419	rVV2	2170	2000	0.13%	0.017%
67	9.903	1445	1446	1449	rBV	1161	1330	0.09%	0.011%
68	10.055	1465	1471	1486	rBV	792161	1144964	76.46%	9.567%
69	10.299	1509	1511	1513	rBV	1695	1660	0.11%	0.014%
70	10.433	1531	1533	1535	rBV	1854	2147	0.14%	0.018%
71	11.000	1624	1626	1629	rBV	1639	1893	0.13%	0.016%
72	11.104	1640	1643	1644	rVV	1676	1648	0.11%	0.014%
73	11.153	1648	1651	1652	rBV	1316	1564	0.10%	0.013%
74	11.195	1652	1658	1666	rVB	551213	731806	48.87%	6.115%
75	11.250	1666	1667	1669	rVB	2546	1308	0.09%	0.011%
76	11.293	1672	1674	1676	rBV	1579	1952	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039110.D
 Acq On : 08 Dec 2023 17:18
 Operator : JC/MD
 Sample : 05646-06ME
 Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	11.317	1676	1678	1680	rVB2	1936	1593	0.11%	0.013%
78	11.402	1690	1692	1694	rBV	1243	1543	0.10%	0.013%
79	11.494	1705	1707	1711	rBV	1272	1716	0.11%	0.014%
80	12.024	1788	1794	1801	rVV	918208	1155831	77.18%	9.658%
81	12.134	1810	1812	1815	rBV	1738	1769	0.12%	0.015%
82	12.323	1837	1843	1855	rVB	821828	1082488	72.29%	9.045%
83	12.890	1934	1936	1937	rVB	2004	1271	0.08%	0.011%
84	12.908	1937	1939	1942	rBV	1828	2391	0.16%	0.020%
85	13.006	1953	1955	1957	rVV2	1604	1272	0.08%	0.011%
86	13.042	1960	1961	1966	rVB	1071	1642	0.11%	0.014%
87	13.299	2001	2003	2006	rBV	1782	2396	0.16%	0.020%
88	13.561	2044	2046	2049	rBV	1002	1289	0.09%	0.011%
89	13.920	2103	2105	2106	rBV	1538	1258	0.08%	0.011%
90	13.987	2115	2116	2120	rBV	1365	1360	0.09%	0.011%
91	14.176	2142	2147	2149	rBV2	1672	2444	0.16%	0.020%
92	14.286	2162	2165	2166	rBV	1443	1422	0.09%	0.012%
93	14.445	2190	2191	2193	rBV	1644	1639	0.11%	0.014%
94	14.664	2225	2227	2228	rBV	1367	1274	0.09%	0.011%
95	14.871	2259	2261	2263	rVB	2048	1423	0.10%	0.012%
96	14.951	2272	2274	2276	rBV	1458	1344	0.09%	0.011%
97	15.127	2301	2303	2305	rVB	1675	1474	0.10%	0.012%
98	15.591	2376	2379	2383	rVB2	1374	1695	0.11%	0.014%
99	15.743	2402	2404	2405	rVV	1681	1336	0.09%	0.011%
100	16.536	2531	2534	2536	rBV	1436	2237	0.15%	0.019%




Sum of corrected areas: 11967658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039110.D
Acq On : 08 Dec 2023 17:18
Operator : JC/MD
Sample : 05646-06ME
Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

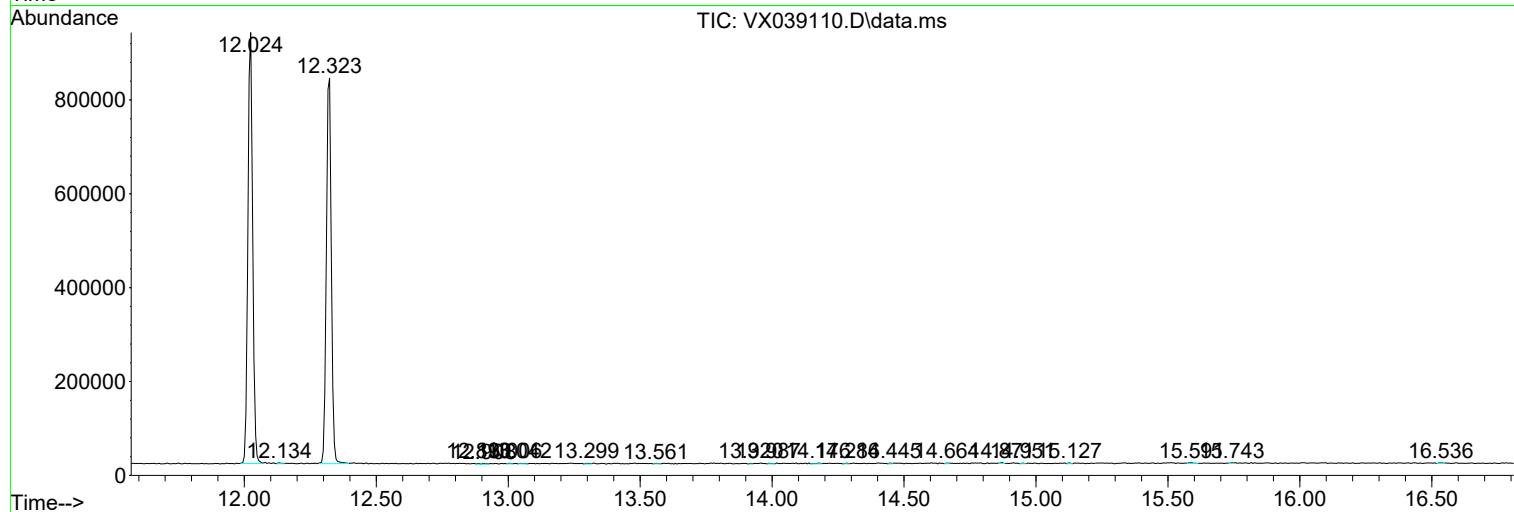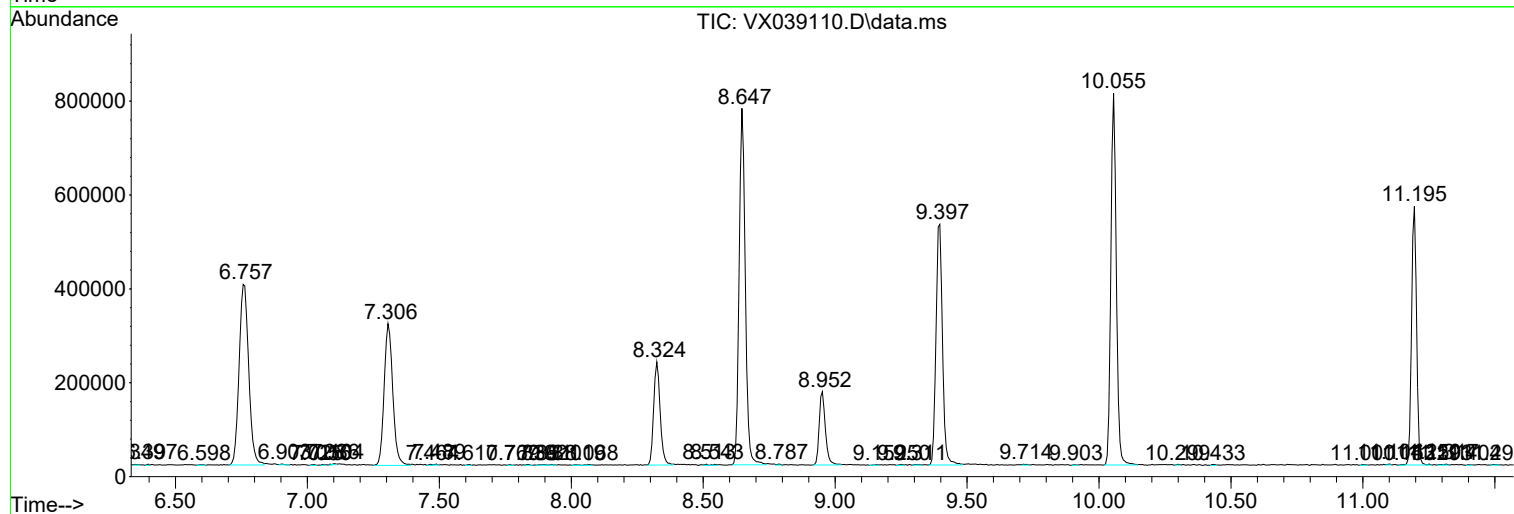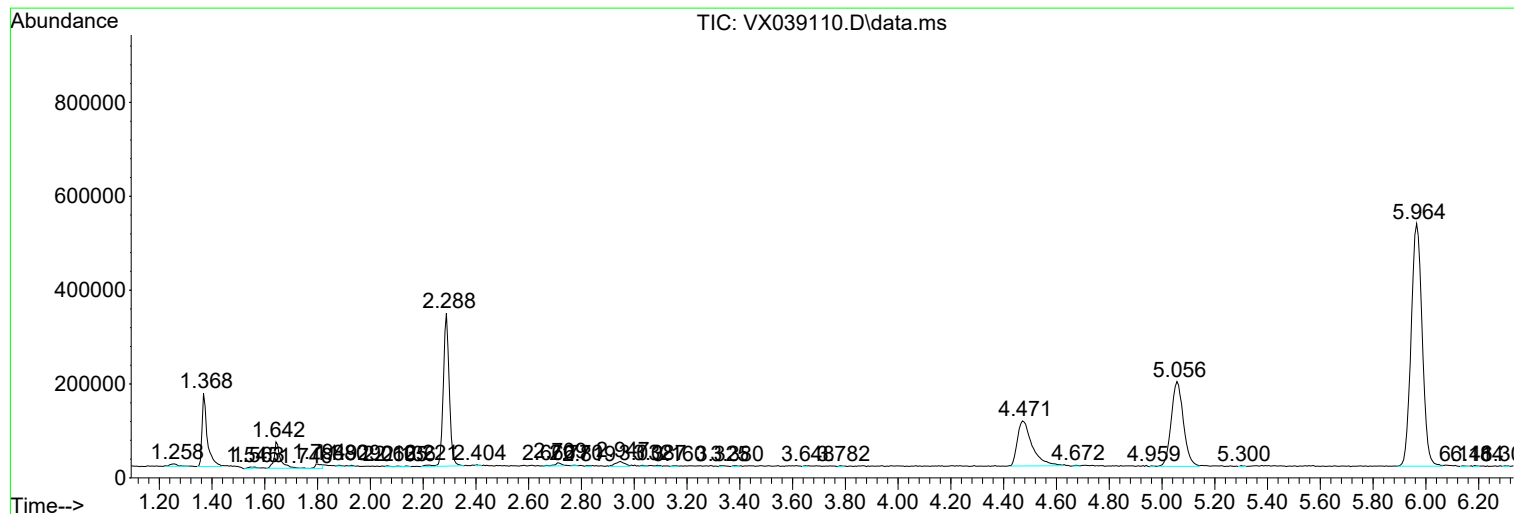

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039110.D
Acq On : 08 Dec 2023 17:18
Operator : JC/MD
Sample : 05646-06ME
Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039110.D
Acq On : 08 Dec 2023 17:18
Operator : JC/MD
Sample : 05646-06ME
Misc : 3.06g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc