

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039113.D
 Acq On : 08 Dec 2023 18:27
 Operator : JC/MD
 Sample : 05646-04ME
 Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	36	rVB3	5249	12023	0.95%	0.118%
2	1.331	38	40	42	rBV	1680	1091	0.09%	0.011%
3	1.368	42	46	57	rBV	134147	182152	14.37%	1.785%
4	1.490	65	66	72	rVB	5545	7060	0.56%	0.069%
5	1.532	72	73	74	rBV	2664	1714	0.14%	0.017%
6	1.557	74	77	81	rVB6	2308	2859	0.23%	0.028%
7	1.587	81	82	85	rVB3	2555	1665	0.13%	0.016%
8	1.642	85	91	103	rBV2	47571	82926	6.54%	0.813%
9	1.764	107	111	113	rBV5	1228	1474	0.12%	0.014%
10	1.788	113	115	120	rBV	11048	22777	1.80%	0.223%
11	2.008	145	151	153	rVB	2097	3529	0.28%	0.035%
12	2.209	180	184	185	rBV	4688	4783	0.38%	0.047%
13	2.288	191	197	206	rVB	273060	421518	33.26%	4.131%
14	2.721	263	268	271	rVV3	5802	10884	0.86%	0.107%
15	2.843	284	288	295	rVB2	8282	15987	1.26%	0.157%
16	2.934	299	303	304	rBV	2514	3488	0.28%	0.034%
17	3.166	339	341	342	rBV	1662	1646	0.13%	0.016%
18	3.197	344	346	348	rVV	1495	1313	0.10%	0.013%
19	3.227	348	351	355	rVB	1801	2724	0.21%	0.027%
20	3.398	377	379	381	rVV	1491	1131	0.09%	0.011%
21	3.794	443	444	445	rBV	2792	1389	0.11%	0.014%
22	4.471	543	555	574	rBV	87957	332468	26.23%	3.258%
23	4.806	608	610	612	rVV	1802	1444	0.11%	0.014%
24	5.056	641	651	671	rVB	151335	487109	38.43%	4.774%
25	5.190	671	673	674	rBV	1703	1308	0.10%	0.013%
26	5.343	695	698	700	rBV	1840	2699	0.21%	0.026%
27	5.477	717	720	721	rBV	1359	1101	0.09%	0.011%
28	5.684	752	754	757	rVV	1461	1286	0.10%	0.013%
29	5.818	774	776	777	rBV	1921	1194	0.09%	0.012%
30	5.964	789	800	808	rBV2	438791	1267442	100.00%	12.422%
31	6.196	836	838	841	rVB	1444	1293	0.10%	0.013%
32	6.275	850	851	853	rBV	1908	1646	0.13%	0.016%
33	6.501	886	888	889	rBV	1141	1239	0.10%	0.012%
34	6.580	899	901	905	rBV2	1893	3261	0.26%	0.032%
35	6.629	908	909	913	rVB2	2152	2414	0.19%	0.024%
36	6.665	913	915	917	rBV	1431	1605	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039113.D
 Acq On : 08 Dec 2023 18:27
 Operator : JC/MD
 Sample : 05646-04ME
 Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	6.757	921	930	950	rBV	308316	766045	60.44%	7.508%
38	7.190	999	1001	1002	rBV	1351	1091	0.09%	0.011%
39	7.245	1008	1010	1011	rBV	1399	1189	0.09%	0.012%
40	7.306	1012	1020	1031	rVV	254393	567077	44.74%	5.558%
41	7.641	1072	1075	1077	rBV	1947	2304	0.18%	0.023%
42	8.013	1134	1136	1137	rBV	2311	1252	0.10%	0.012%
43	8.165	1159	1161	1164	rVB	2067	1915	0.15%	0.019%
44	8.196	1164	1166	1169	rVB	2606	2797	0.22%	0.027%
45	8.226	1169	1171	1173	rBV	1423	1710	0.13%	0.017%
46	8.324	1181	1187	1196	rBV	181693	310413	24.49%	3.042%
47	8.415	1201	1202	1206	rBV	1483	1618	0.13%	0.016%
48	8.647	1234	1240	1252	rBV	632390	1025435	80.91%	10.050%
49	8.952	1284	1290	1301	rBV	132313	208124	16.42%	2.040%
50	9.104	1314	1315	1317	rBV	1573	1141	0.09%	0.011%
51	9.165	1324	1325	1328	rBV	1233	1487	0.12%	0.015%
52	9.391	1357	1362	1371	rBV	427994	733690	57.89%	7.191%
53	9.549	1387	1388	1391	rVV2	1896	1440	0.11%	0.014%
54	9.671	1406	1408	1411	rBV	1040	1108	0.09%	0.011%
55	9.726	1415	1417	1419	rVB	2358	1669	0.13%	0.016%
56	9.890	1442	1444	1445	rBV	1764	1531	0.12%	0.015%
57	9.927	1449	1450	1452	rVV	1947	1321	0.10%	0.013%
58	9.951	1452	1454	1457	rVV	1482	1836	0.14%	0.018%
59	10.055	1465	1471	1487	rVV2	631290	1203727	94.97%	11.797%
60	10.165	1487	1489	1492	rVB	1910	1704	0.13%	0.017%
61	10.445	1533	1535	1536	rBV	1909	1347	0.11%	0.013%
62	10.598	1556	1560	1561	rBV	1759	1566	0.12%	0.015%
63	11.195	1653	1658	1669	rVB	469405	604744	47.71%	5.927%
64	11.274	1669	1671	1673	rVB	1459	1098	0.09%	0.011%
65	11.360	1683	1685	1686	rBV	1786	1296	0.10%	0.013%
66	11.616	1725	1727	1728	rBV	1269	1337	0.11%	0.013%
67	11.786	1752	1755	1756	rBV	1738	1740	0.14%	0.017%
68	11.969	1782	1785	1788	rBV3	5362	7005	0.55%	0.069%
69	12.024	1788	1794	1802	rVV	711034	908573	71.69%	8.905%
70	12.201	1822	1823	1826	rBV	1837	1283	0.10%	0.013%
71	12.317	1837	1842	1850	rBV	660470	888189	70.08%	8.705%
72	12.414	1857	1858	1861	rVB	2281	2086	0.16%	0.020%
73	12.555	1880	1881	1883	rVB	2033	1227	0.10%	0.012%
74	12.579	1883	1885	1888	rBV	1466	1772	0.14%	0.017%
75	12.756	1912	1914	1915	rBV	2771	1491	0.12%	0.015%
76	13.042	1959	1961	1964	rVB	1348	1124	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039113.D
 Acq On : 08 Dec 2023 18:27
 Operator : JC/MD
 Sample : 05646-04ME
 Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAT8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.128	1973	1975	1977	rVV	1712	1192	0.09%	0.012%
78	13.146	1977	1978	1980	rVB	2196	1353	0.11%	0.013%
79	13.176	1980	1983	1984	rBV	1946	1971	0.16%	0.019%
80	13.207	1984	1988	1989	rVB	1441	1356	0.11%	0.013%
81	13.268	1996	1998	2001	rVB	2410	2194	0.17%	0.022%
82	13.305	2001	2004	2005	rBV	987	1325	0.10%	0.013%
83	13.542	2041	2043	2045	rBV	1936	1557	0.12%	0.015%
84	13.884	2097	2099	2104	rVB	2037	2577	0.20%	0.025%
85	14.493	2197	2199	2200	rBV	1610	1479	0.12%	0.014%
86	14.560	2209	2210	2215	rBV	1205	1198	0.09%	0.012%
87	14.627	2219	2221	2223	rVB	2279	1543	0.12%	0.015%
88	14.652	2223	2225	2229	rBV	1857	2354	0.19%	0.023%
89	14.865	2259	2260	2264	rBV	1556	2241	0.18%	0.022%
90	14.999	2280	2282	2285	rBV	1633	1585	0.13%	0.016%
91	15.133	2303	2304	2308	rVB	2170	2140	0.17%	0.021%
92	15.170	2308	2310	2315	rBV	2200	3117	0.25%	0.031%
93	15.243	2319	2322	2323	rBV	1417	1794	0.14%	0.018%
94	15.761	2403	2407	2408	rBV2	1419	1766	0.14%	0.017%
95	15.902	2428	2430	2433	rVB	1678	1911	0.15%	0.019%
96	16.011	2446	2448	2451	rVB	1810	1550	0.12%	0.015%
97	16.359	2504	2505	2507	rBV	2344	1567	0.12%	0.015%
98	16.578	2539	2541	2544	rBV	1882	2227	0.18%	0.022%
99	16.676	2556	2557	2561	rBV	1874	2430	0.19%	0.024%
100	16.779	2571	2574	2575	rBV	1748	1777	0.14%	0.017%




Sum of corrected areas: 10203348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039113.D
Acq On : 08 Dec 2023 18:27
Operator : JC/MD
Sample : 05646-04ME
Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

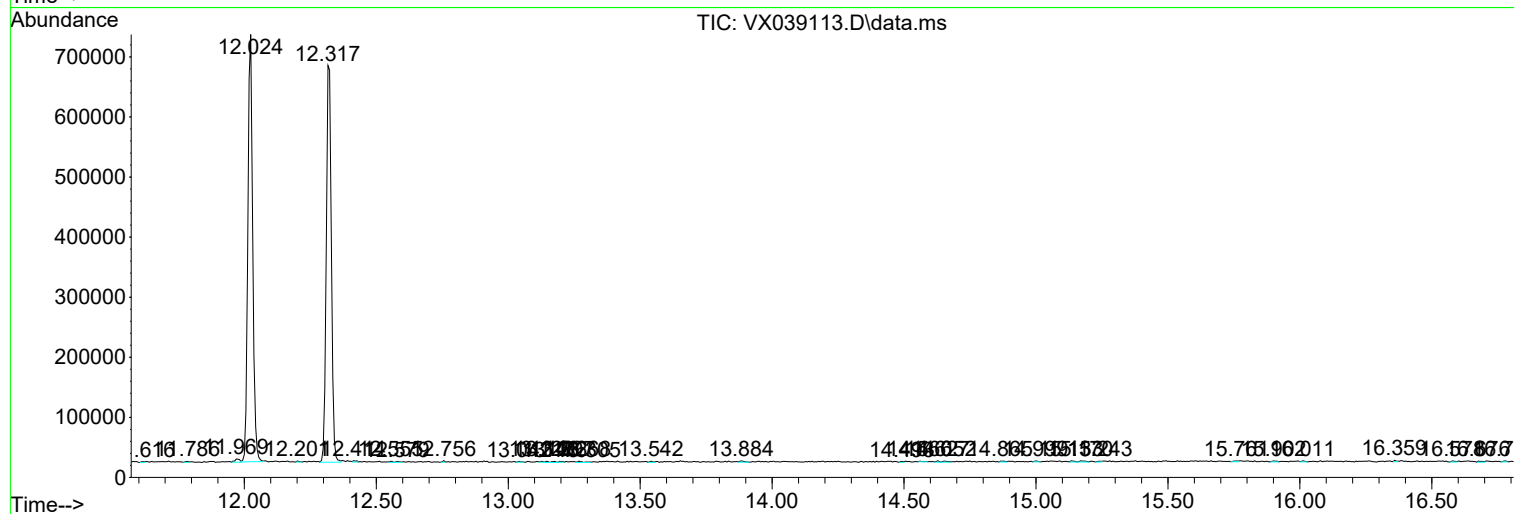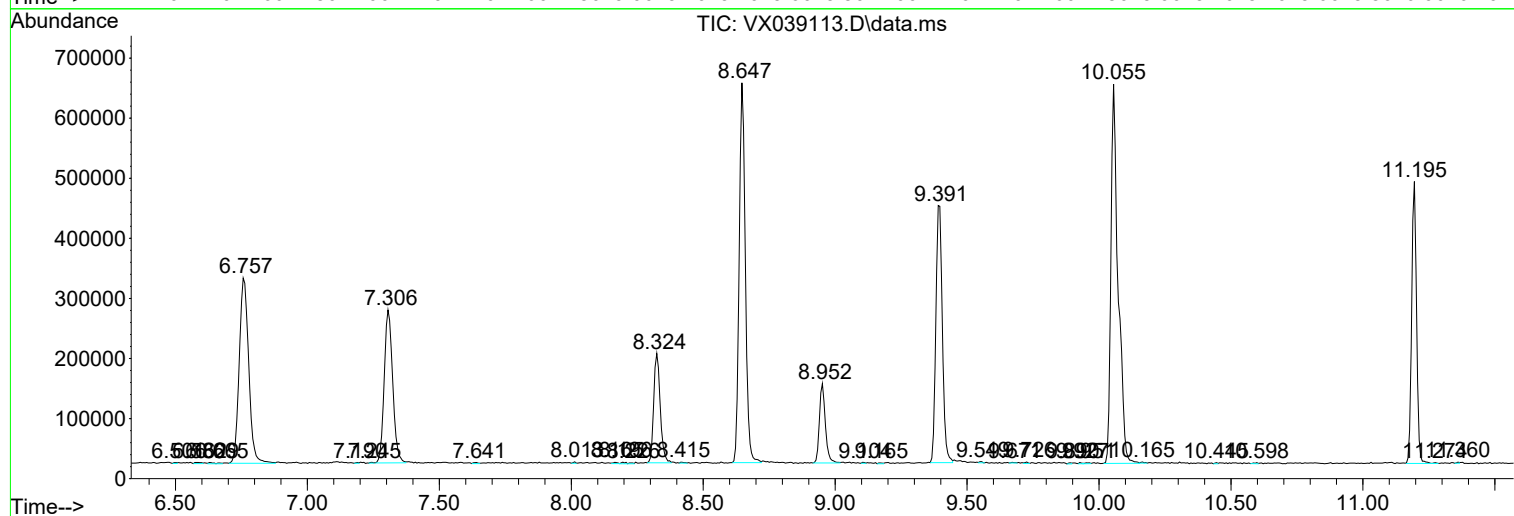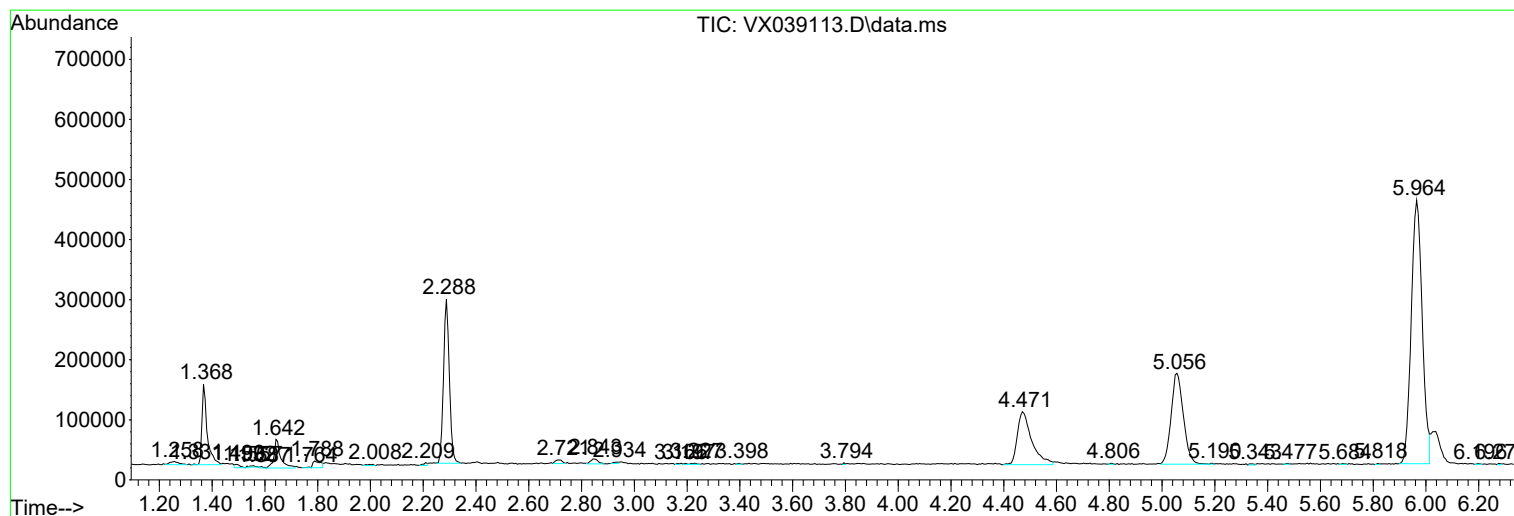

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039113.D
Acq On : 08 Dec 2023 18:27
Operator : JC/MD
Sample : 05646-04ME
Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039113.D
Acq On : 08 Dec 2023 18:27
Operator : JC/MD
Sample : 05646-04ME
Misc : 3.39g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc