

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039114.D
 Acq On : 08 Dec 2023 18:50
 Operator : JC/MD
 Sample : 05646-13ME 40X
 Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COASOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.203	17	19	22	rVB	1540	1442	0.03%	0.006%
2	1.246	22	26	28	rBV	5134	6319	0.12%	0.028%
3	1.368	43	46	55	rVB	151852	156563	3.06%	0.682%
4	1.563	74	78	79	rBV2	3133	4014	0.08%	0.017%
5	1.593	79	83	84	rVV2	3929	6202	0.12%	0.027%
6	1.636	88	90	91	rVV	4449	4163	0.08%	0.018%
7	1.666	91	95	106	rVV	104207	151111	2.96%	0.658%
8	1.764	110	111	112	rVV	2043	1344	0.03%	0.006%
9	1.782	112	114	115	rVV	2585	1809	0.04%	0.008%
10	2.063	158	160	162	rVB2	2153	1405	0.03%	0.006%
11	2.099	162	166	167	rBV2	1376	1772	0.03%	0.008%
12	2.191	178	181	182	rVB	1719	1705	0.03%	0.007%
13	2.203	182	183	184	rBV	2488	1492	0.03%	0.006%
14	2.227	185	187	190	rBV2	3106	4073	0.08%	0.018%
15	2.307	194	200	208	rBV	248532	389258	7.61%	1.696%
16	2.483	227	229	231	rBV	1424	1517	0.03%	0.007%
17	2.733	267	270	271	rBV	1657	1720	0.03%	0.007%
18	2.794	275	280	282	rBV3	2750	4563	0.09%	0.020%
19	2.947	298	305	314	rVB3	8749	21179	0.41%	0.092%
20	3.422	382	383	385	rBV	2079	1926	0.04%	0.008%
21	3.605	411	413	420	rVV	1619	3351	0.07%	0.015%
22	4.007	478	479	481	rVV	2239	1401	0.03%	0.006%
23	4.160	502	504	506	rBV	2155	1996	0.04%	0.009%
24	4.300	526	527	529	rVB	2461	1618	0.03%	0.007%
25	4.452	543	552	564	rBV	105195	299231	5.85%	1.303%
26	4.849	615	617	622	rBV	1311	1925	0.04%	0.008%
27	5.056	641	651	669	rVB	144013	451678	8.83%	1.967%
28	5.971	789	801	808	rBV2	394521	1196778	23.40%	5.213%
29	6.038	808	812	823	rVB	145031	355059	6.94%	1.547%
30	6.202	836	839	840	rBV	2399	2445	0.05%	0.011%
31	6.300	854	855	857	rVB	2166	1528	0.03%	0.007%
32	6.336	857	861	864	rBV	2610	3626	0.07%	0.016%
33	6.446	877	879	882	rBV	1849	2460	0.05%	0.011%
34	6.568	896	899	901	rBV	1270	1438	0.03%	0.006%
35	6.757	922	930	945	rBV	288952	700943	13.71%	3.053%
36	6.995	966	969	973	rBV	1738	3077	0.06%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039114.D
 Acq On : 08 Dec 2023 18:50
 Operator : JC/MD
 Sample : 05646-13ME 40X
 Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COASOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.086	981	984	985	rBV2	1606	2106	0.04%	0.009%
38	7.117	987	989	994	rVB	3624	3610	0.07%	0.016%
39	7.306	1012	1020	1031	rVV	238937	530159	10.37%	2.309%
40	7.708	1084	1086	1089	rVB	1972	2094	0.04%	0.009%
41	8.177	1161	1163	1167	rVB	1787	1336	0.03%	0.006%
42	8.275	1177	1179	1181	rBV	1612	1652	0.03%	0.007%
43	8.324	1181	1187	1200	rVV	174158	292931	5.73%	1.276%
44	8.647	1234	1240	1254	rVV	594603	941669	18.42%	4.102%
45	8.952	1284	1290	1296	rBV	124278	190606	3.73%	0.830%
46	9.171	1324	1326	1328	rBV	1346	1351	0.03%	0.006%
47	9.385	1355	1361	1374	rBV	470121	697816	13.65%	3.040%
48	9.513	1380	1382	1383	rVB	2501	1799	0.04%	0.008%
49	9.708	1410	1414	1419	rVB2	2826	4786	0.09%	0.021%
50	10.080	1465	1475	1493	rVV2	2857903	4839411	94.64%	21.079%
51	10.220	1496	1498	1503	rVV	1357	2029	0.04%	0.009%
52	10.287	1507	1509	1511	rVV	1538	1387	0.03%	0.006%
53	10.415	1526	1530	1531	rBV	1210	1923	0.04%	0.008%
54	10.464	1536	1538	1541	rVV	1779	1748	0.03%	0.008%
55	10.970	1619	1621	1624	rVB	1699	1347	0.03%	0.006%
56	11.189	1652	1657	1665	rVB	440249	561469	10.98%	2.446%
57	11.305	1675	1676	1680	rBV	1561	1342	0.03%	0.006%
58	11.366	1682	1686	1689	rVB3	9720	12624	0.25%	0.055%
59	11.457	1699	1701	1704	rBV3	1825	1742	0.03%	0.008%
60	11.707	1740	1742	1745	rVB	1443	1490	0.03%	0.006%
61	11.811	1756	1759	1760	rBV	2712	2644	0.05%	0.012%
62	11.969	1780	1785	1789	rVV	131383	166173	3.25%	0.724%
63	12.043	1789	1797	1806	rVB2	3334046	5113575	100.00%	22.274%
64	12.323	1837	1843	1853	rVV2	674064	1196266	23.39%	5.211%
65	12.396	1853	1855	1858	rVV	2184	2335	0.05%	0.010%
66	12.421	1858	1859	1862	rVV	1905	1539	0.03%	0.007%
67	12.738	1909	1911	1913	rBV	2151	1646	0.03%	0.007%
68	13.000	1953	1954	1956	rBV	1687	1427	0.03%	0.006%
69	13.055	1958	1963	1969	rVV2	39912	77180	1.51%	0.336%
70	13.109	1969	1972	1978	rVV3	9718	14129	0.28%	0.062%
71	13.195	1982	1986	1990	rBV3	3403	5422	0.11%	0.024%
72	13.378	2013	2016	2023	rVB4	4488	8536	0.17%	0.037%
73	13.585	2045	2050	2061	rVB	2245553	2703826	52.88%	11.777%
74	13.762	2077	2079	2081	rBV	1542	1779	0.03%	0.008%
75	13.920	2103	2105	2106	rVV	1661	1582	0.03%	0.007%
76	13.957	2106	2111	2119	rVV	945882	1218069	23.82%	5.306%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039114.D
 Acq On : 08 Dec 2023 18:50
 Operator : JC/MD
 Sample : 05646-13ME 40X
 Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COASOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.121	2136	2138	2140	rBV	1833	2155	0.04%	0.009%
78	14.170	2144	2146	2149	rVV	1767	1676	0.03%	0.007%
79	14.207	2149	2152	2153	rVV	1438	1438	0.03%	0.006%
80	14.231	2153	2156	2157	rVV	1935	1824	0.04%	0.008%
81	14.390	2178	2182	2184	rVV	1842	2493	0.05%	0.011%
82	14.542	2204	2207	2210	rVV2	3475	4488	0.09%	0.020%
83	14.621	2218	2220	2224	rVB3	8008	8062	0.16%	0.035%
84	14.780	2239	2246	2252	rVV2	65602	113394	2.22%	0.494%
85	14.963	2275	2276	2279	rVB	2306	1342	0.03%	0.006%
86	15.127	2301	2303	2306	rVB	1572	1768	0.03%	0.008%
87	15.158	2306	2308	2310	rBV	1491	1506	0.03%	0.007%
88	15.249	2317	2323	2330	rBV	258234	374071	7.32%	1.629%
89	15.377	2342	2344	2346	rBV	1993	2344	0.05%	0.010%
90	15.524	2366	2368	2370	rBV	1617	1588	0.03%	0.007%
91	15.585	2375	2378	2379	rVB	1804	1629	0.03%	0.007%
92	15.627	2381	2385	2387	rBV	1467	2089	0.04%	0.009%
93	15.682	2390	2394	2396	rBV	1520	1812	0.04%	0.008%
94	15.883	2425	2427	2430	rVB	1379	1795	0.04%	0.008%
95	16.414	2512	2514	2517	rVB	1890	1416	0.03%	0.006%
96	16.450	2519	2520	2523	rVV	1525	1404	0.03%	0.006%
97	16.499	2523	2528	2535	rVB5	9197	18562	0.36%	0.081%
98	16.548	2535	2536	2539	rBV	1341	1605	0.03%	0.007%
99	16.682	2556	2558	2562	rVB	2007	1492	0.03%	0.006%
100	16.712	2562	2563	2565	rBV	1694	1368	0.03%	0.006%




Sum of corrected areas: 22958007

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039114.D
Acq On : 08 Dec 2023 18:50
Operator : JC/MD
Sample : 05646-13ME 40X
Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COASOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

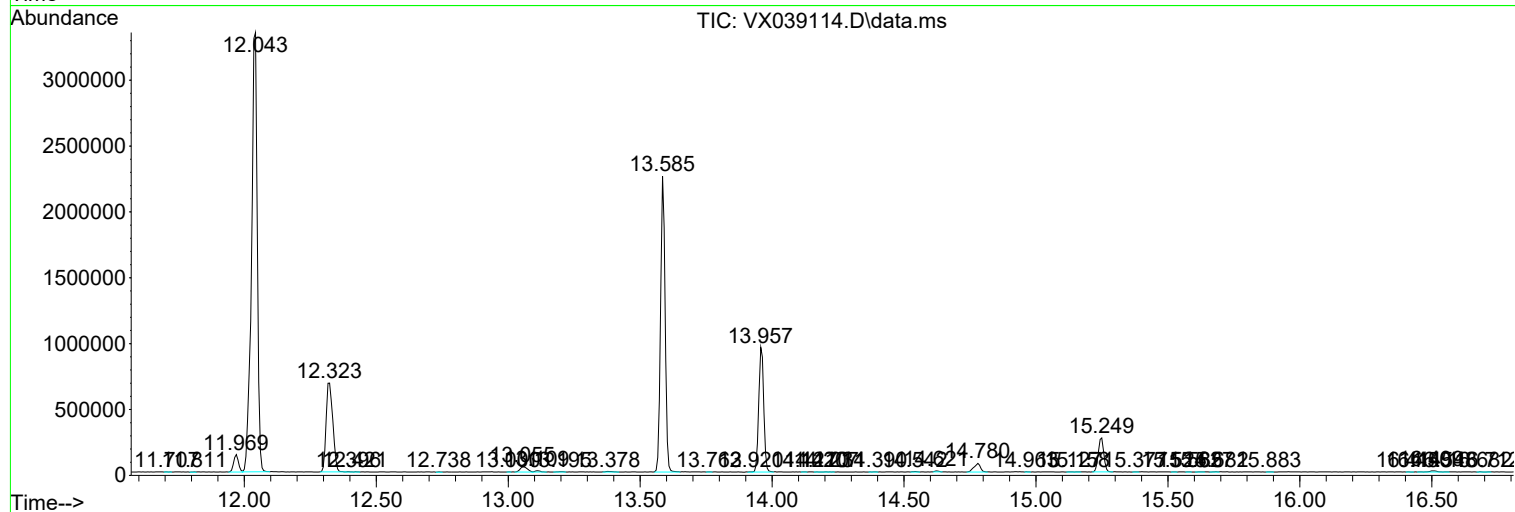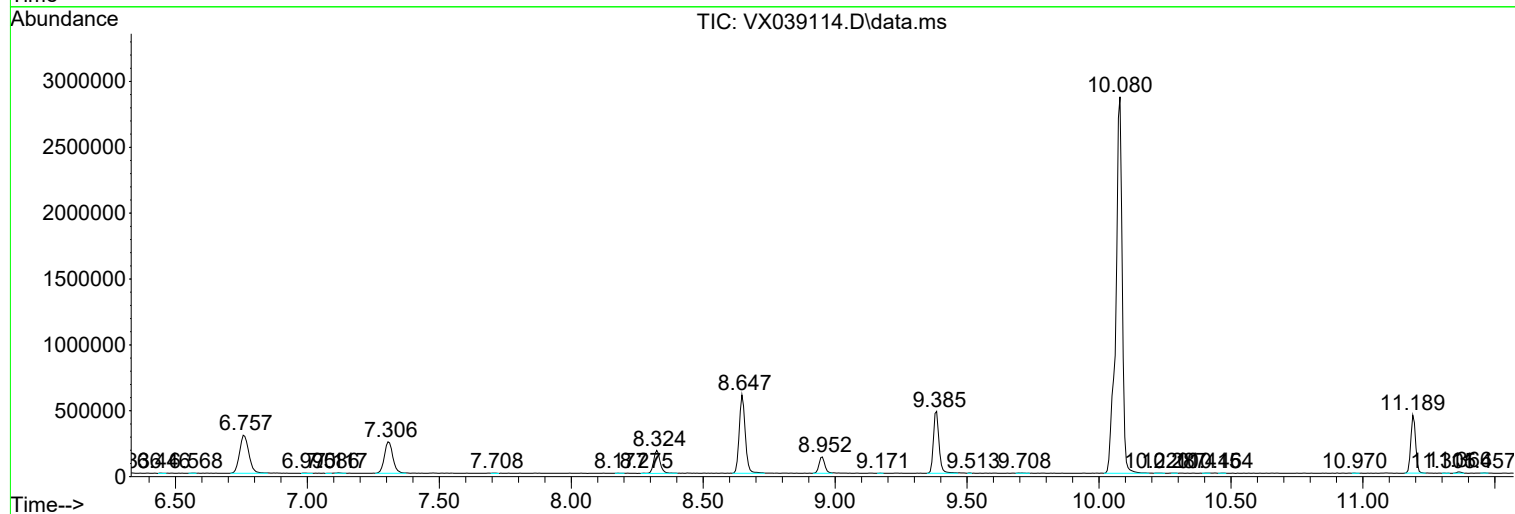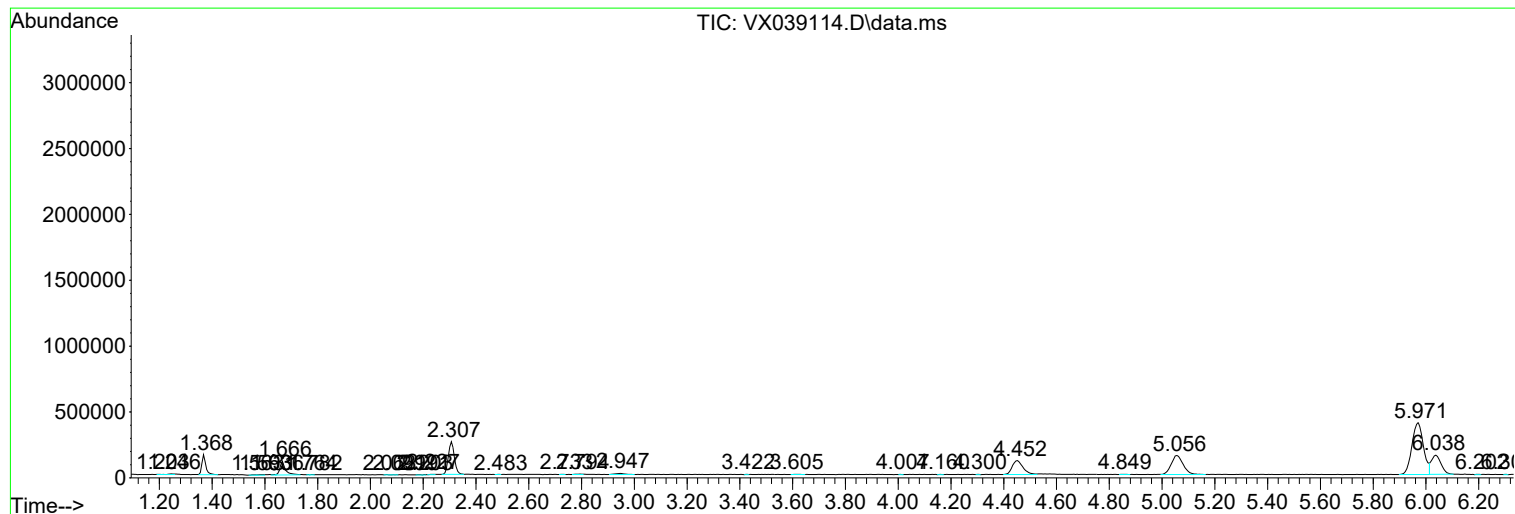

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039114.D
Acq On : 08 Dec 2023 18:50
Operator : JC/MD
Sample : 05646-13ME 40X
Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039114.D
Acq On : 08 Dec 2023 18:50
Operator : JC/MD
Sample : 05646-13ME 40X
Misc : 0.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc