

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039116.D
 Acq On : 08 Dec 2023 19:36
 Operator : JC/MD
 Sample : 05646-10 40X
 Misc : 3.25g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	24	26	29	rBV	4018	5353	0.11%	0.040%
2	1.368	41	46	53	rBV	144285	152698	3.00%	1.153%
3	1.569	74	79	80	rBV3	2143	2623	0.05%	0.020%
4	1.581	80	81	84	rVV2	2874	3581	0.07%	0.027%
5	1.624	86	88	90	rVV	2965	3900	0.08%	0.029%
6	1.666	91	95	109	rVB	93219	140595	2.76%	1.061%
7	1.874	127	129	130	rBV	1520	1058	0.02%	0.008%
8	2.002	149	150	153	rVB	1515	1042	0.02%	0.008%
9	2.075	160	162	166	rBV2	1322	1378	0.03%	0.010%
10	2.130	169	171	174	rVB2	1628	1732	0.03%	0.013%
11	2.160	174	176	179	rBV	1942	1961	0.04%	0.015%
12	2.227	182	187	188	rBV2	3801	4030	0.08%	0.030%
13	2.306	195	200	207	rVB	231635	357261	7.02%	2.697%
14	2.422	216	219	221	rBV	1490	1693	0.03%	0.013%
15	2.940	302	304	311	rVB2	7829	12181	0.24%	0.092%
16	3.050	320	322	324	rBV	1706	1251	0.02%	0.009%
17	3.385	376	377	378	rBV	1769	660	0.01%	0.005%
18	3.599	410	412	414	rBV	1803	1848	0.04%	0.014%
19	3.635	416	418	419	rVB	1697	830	0.02%	0.006%
20	3.678	424	425	426	rBV	1947	781	0.02%	0.006%
21	4.080	490	491	494	rBV	2008	1253	0.02%	0.009%
22	4.300	525	527	530	rBV	1356	1547	0.03%	0.012%
23	4.330	530	532	535	rBV	1584	2009	0.04%	0.015%
24	4.446	544	551	563	rBV2	97324	274698	5.40%	2.074%
25	4.971	635	637	638	rBV	2370	1267	0.02%	0.010%
26	5.056	642	651	665	rVB	143528	430463	8.46%	3.250%
27	5.970	790	801	808	rBV2	371423	1122327	22.05%	8.474%
28	6.220	840	842	843	rVB	1750	938	0.02%	0.007%
29	6.757	922	930	943	rBV	268381	647189	12.71%	4.886%
30	7.123	984	990	994	rBV2	3192	7398	0.15%	0.056%
31	7.305	1012	1020	1034	rBV	229378	504324	9.91%	3.808%
32	7.549	1058	1060	1062	rBV	1897	1979	0.04%	0.015%
33	7.787	1097	1099	1100	rBV	1604	969	0.02%	0.007%
34	7.915	1118	1120	1123	rBV	1606	1682	0.03%	0.013%
35	8.324	1181	1187	1195	rBV	163593	275902	5.42%	2.083%
36	8.647	1234	1240	1250	rBV	547721	879576	17.28%	6.641%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039116.D
 Acq On : 08 Dec 2023 19:36
 Operator : JC/MD
 Sample : 05646-10 40X
 Misc : 3.25g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.952	1284	1290	1300	rBV	120385	183443	3.60%	1.385%
38	9.293	1343	1346	1348	rBV	1800	2506	0.05%	0.019%
39	9.384	1355	1361	1375	rBV	446844	664750	13.06%	5.019%
40	9.610	1396	1398	1401	rVB	2090	1543	0.03%	0.012%
41	9.701	1411	1413	1417	rVB	2852	2839	0.06%	0.021%
42	9.890	1442	1444	1445	rBV	1402	832	0.02%	0.006%
43	10.079	1465	1475	1493	rBV2	3167939	5090465	100.00%	38.433%
44	10.238	1500	1501	1502	rVB	2318	847	0.02%	0.006%
45	10.256	1502	1504	1505	rBV	1344	851	0.02%	0.006%
46	10.390	1524	1526	1529	rBV	1582	1564	0.03%	0.012%
47	11.189	1652	1657	1664	rBV	434624	547214	10.75%	4.131%
48	11.366	1683	1686	1690	rVB3	4613	6698	0.13%	0.051%
49	11.463	1700	1702	1705	rVB2	2530	1855	0.04%	0.014%
50	11.543	1713	1715	1719	rVB	1547	1928	0.04%	0.015%
51	11.969	1780	1785	1789	rBV	62765	80438	1.58%	0.607%
52	12.018	1789	1793	1805	rVB2	602571	992659	19.50%	7.495%
53	12.317	1837	1842	1848	rBV	587938	755735	14.85%	5.706%
54	12.420	1857	1859	1860	rBV	1896	1652	0.03%	0.012%
55	13.061	1959	1964	1969	rBV3	15148	27127	0.53%	0.205%
56	13.109	1969	1972	1977	rBV2	8704	11253	0.22%	0.085%
57	13.591	2048	2051	2055	rVB2	4027	5770	0.11%	0.044%
58	13.737	2072	2075	2077	rBV	1945	2517	0.05%	0.019%
59	13.993	2115	2117	2122	rBV	1647	1902	0.04%	0.014%
60	14.859	2257	2259	2260	rVB	1926	938	0.02%	0.007%
61	15.310	2331	2333	2334	rBV	2601	1522	0.03%	0.011%
62	15.847	2419	2421	2423	rBV	1887	1985	0.04%	0.015%
63	16.042	2452	2453	2454	rBV	2390	1127	0.02%	0.009%
64	16.499	2526	2528	2532	rBV	1971	3012	0.06%	0.023%




Sum of corrected areas: 13244949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039116.D
Acq On : 08 Dec 2023 19:36
Operator : JC/MD
Sample : 05646-10 40X
Misc : 3.25g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

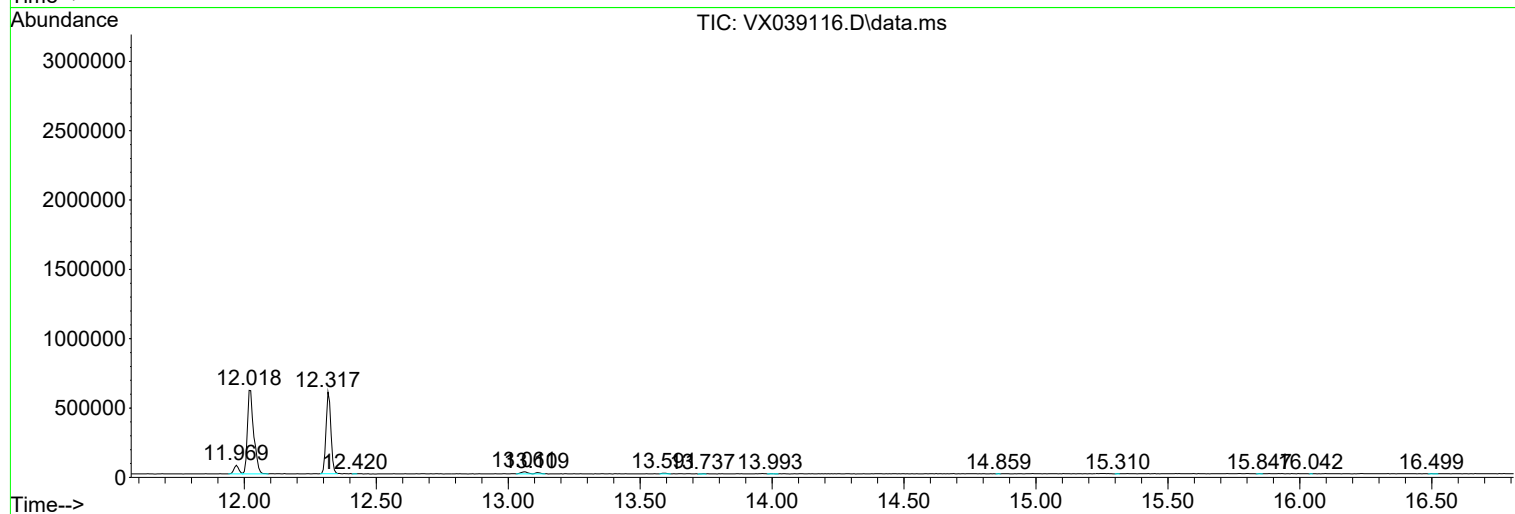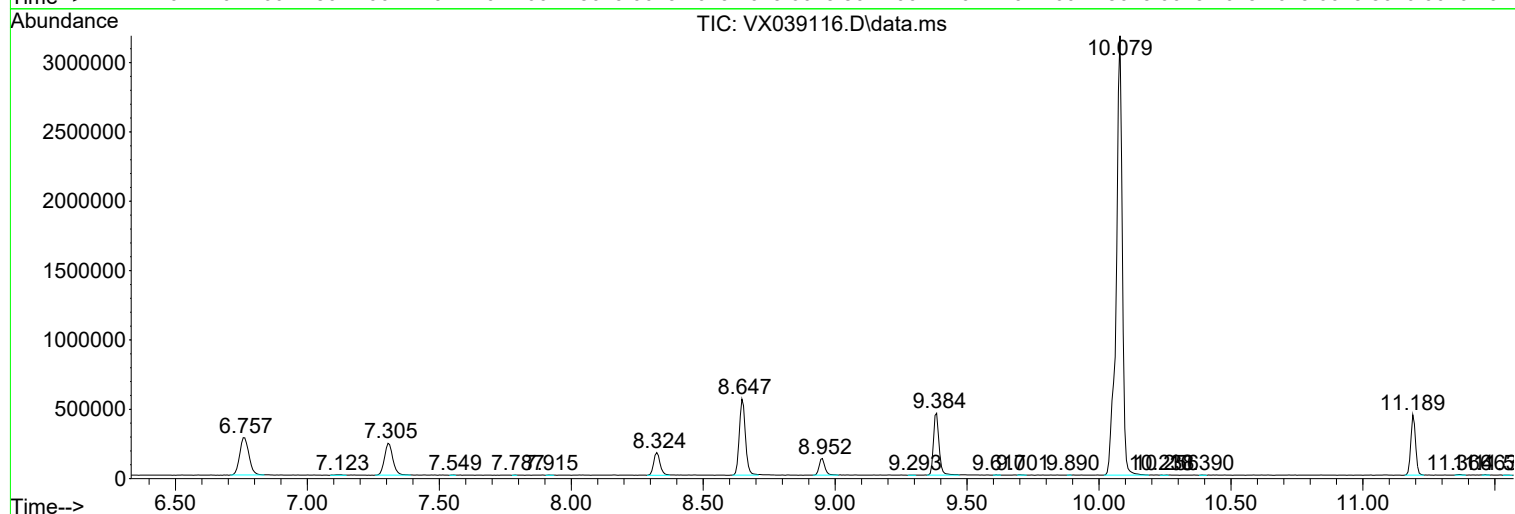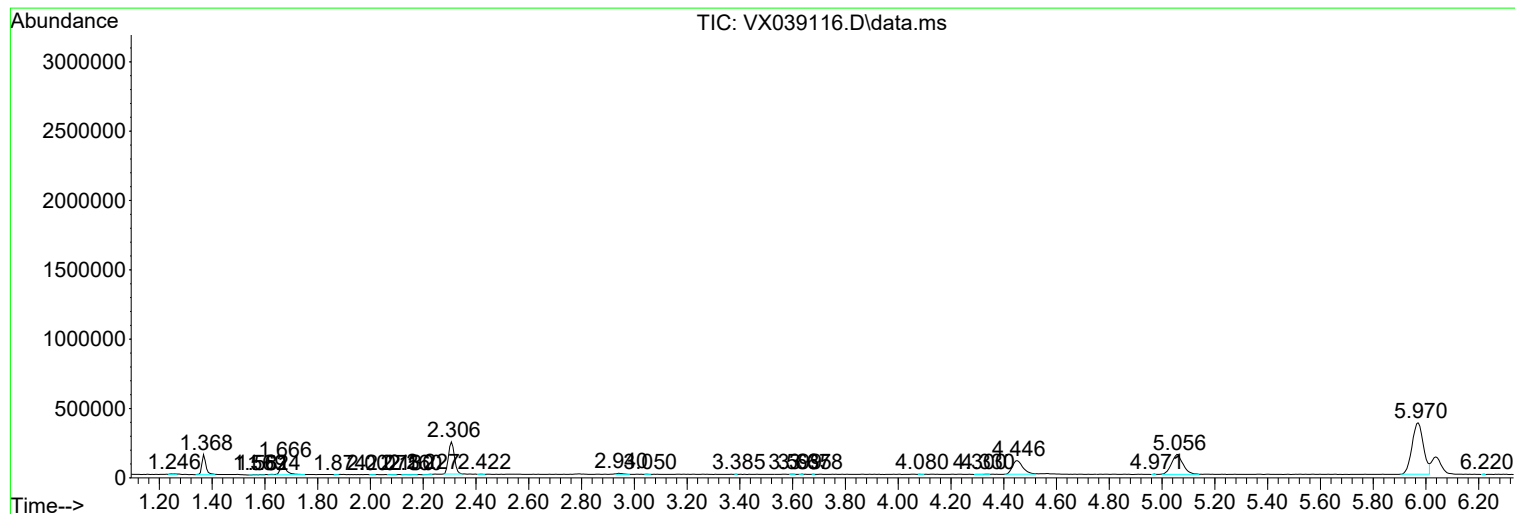

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039116.D
Acq On : 08 Dec 2023 19:36
Operator : JC/MD
Sample : 05646-10 40X
Misc : 3.25g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039116.D
Acq On : 08 Dec 2023 19:36
Operator : JC/MD
Sample : 05646-10 40X
Misc : 3.25g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc