

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039119.D
 Acq On : 08 Dec 2023 20:45
 Operator : JC/MD
 Sample : 05646-15 40X
 Misc : 1.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV2	3347	3254	0.03%	0.010%
2	1.367	42	46	58	rVB	144518	150998	1.18%	0.461%
3	1.569	75	79	80	rBV3	3669	4956	0.04%	0.015%
4	1.581	80	81	82	rVV	1716	978	0.01%	0.003%
5	1.666	91	95	106	rBV	93506	130820	1.03%	0.399%
6	1.989	144	148	152	rBV2	1637	2773	0.02%	0.008%
7	2.227	182	187	188	rBV	4306	6796	0.05%	0.021%
8	2.306	195	200	209	rVB	234732	364060	2.85%	1.110%
9	2.940	301	304	313	rVB2	7876	15455	0.12%	0.047%
10	3.361	371	373	374	rBV	1755	1329	0.01%	0.004%
11	4.446	543	551	564	rBV	103173	294080	2.31%	0.897%
12	5.056	641	651	665	rVB	136687	423804	3.32%	1.293%
13	5.379	700	704	706	rBV	2119	2845	0.02%	0.009%
14	5.647	746	748	750	rBV	2485	1353	0.01%	0.004%
15	5.665	750	751	753	rBV	2039	1279	0.01%	0.004%
16	5.970	789	801	809	rBV2	371658	1132899	8.88%	3.455%
17	6.251	845	847	848	rVB	1680	983	0.01%	0.003%
18	6.324	857	859	860	rBV	1936	1451	0.01%	0.004%
19	6.763	922	931	944	rBV	268205	654849	5.13%	1.997%
20	7.104	985	987	992	rBV2	2650	3903	0.03%	0.012%
21	7.305	1012	1020	1032	rBV	225281	502501	3.94%	1.533%
22	7.696	1082	1084	1086	rBV	2477	2273	0.02%	0.007%
23	7.872	1112	1113	1115	rBV	1601	830	0.01%	0.003%
24	8.141	1155	1157	1160	rBV	2074	1993	0.02%	0.006%
25	8.324	1181	1187	1198	rVB	166959	277477	2.18%	0.846%
26	8.647	1234	1240	1255	rVB	553677	879506	6.90%	2.682%
27	8.951	1285	1290	1299	rBV	119867	186542	1.46%	0.569%
28	9.116	1315	1317	1321	rBV2	1819	1825	0.01%	0.006%
29	9.384	1355	1361	1373	rBV	451319	674527	5.29%	2.057%
30	9.616	1397	1399	1400	rBV	1547	1074	0.01%	0.003%
31	9.695	1410	1412	1421	rVB2	5134	6947	0.05%	0.021%
32	10.055	1465	1471	1472	rBV	597813	776015	6.08%	2.367%
33	10.079	1472	1475	1488	rVB	1011304	1411722	11.07%	4.306%
34	10.671	1571	1572	1574	rBV	1467	905	0.01%	0.003%
35	10.695	1574	1576	1578	rVB	1836	1208	0.01%	0.004%
36	10.719	1578	1580	1583	rVB	1953	1428	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039119.D
 Acq On : 08 Dec 2023 20:45
 Operator : JC/MD
 Sample : 05646-15 40X
 Misc : 1.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	10.750	1583	1585	1586	rBV	1801	1553	0.01%	0.005%
38	11.006	1625	1627	1628	rBV	2354	1687	0.01%	0.005%
39	11.189	1652	1657	1664	rVV	429152	541914	4.25%	1.653%
40	11.268	1668	1670	1671	rBV	1345	736	0.01%	0.002%
41	11.585	1721	1722	1723	rBV	1482	583	0.00%	0.002%
42	11.890	1771	1772	1773	rBV	1994	1082	0.01%	0.003%
43	11.969	1780	1785	1789	rBV	313030	383165	3.00%	1.169%
44	12.042	1789	1797	1805	rVB	9566275	12755048	100.00%	38.902%
45	12.335	1837	1845	1853	rBV2	1840947	2951887	23.14%	9.003%
46	12.707	1903	1906	1908	rBV2	2333	2741	0.02%	0.008%
47	12.920	1939	1941	1945	rVB2	3198	3911	0.03%	0.012%
48	13.054	1959	1963	1970	rVV	39640	73562	0.58%	0.224%
49	13.115	1970	1973	1977	rVB2	7130	8702	0.07%	0.027%
50	13.195	1982	1986	1993	rVB2	15600	20305	0.16%	0.062%
51	13.378	2014	2016	2022	rVB2	8080	11766	0.09%	0.036%
52	13.585	2045	2050	2062	rBV	4693894	5971187	46.81%	18.212%
53	13.957	2106	2111	2118	rBV	1485704	1856097	14.55%	5.661%
54	14.780	2240	2246	2251	rVB3	33123	52900	0.41%	0.161%
55	15.152	2305	2307	2308	rVB	2381	1403	0.01%	0.004%
56	15.176	2308	2311	2313	rBV	1820	1984	0.02%	0.006%
57	15.249	2317	2323	2330	rVB	152869	219624	1.72%	0.670%




Sum of corrected areas: 32787475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039119.D
Acq On : 08 Dec 2023 20:45
Operator : JC/MD
Sample : 05646-15 40X
Misc : 1.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

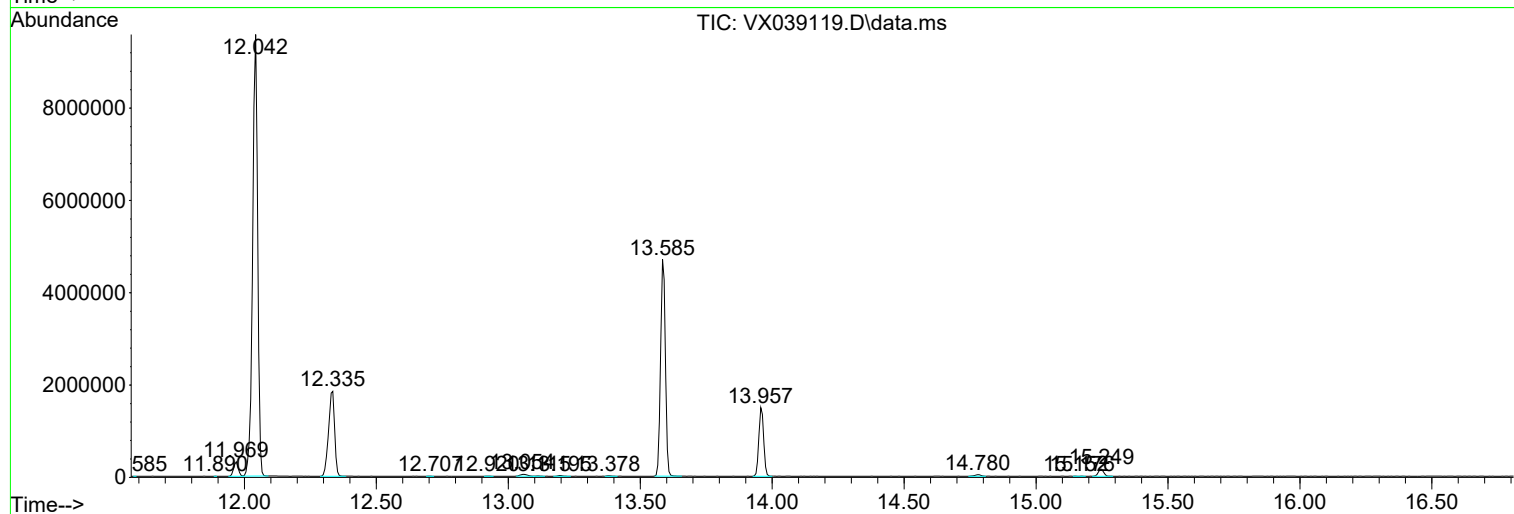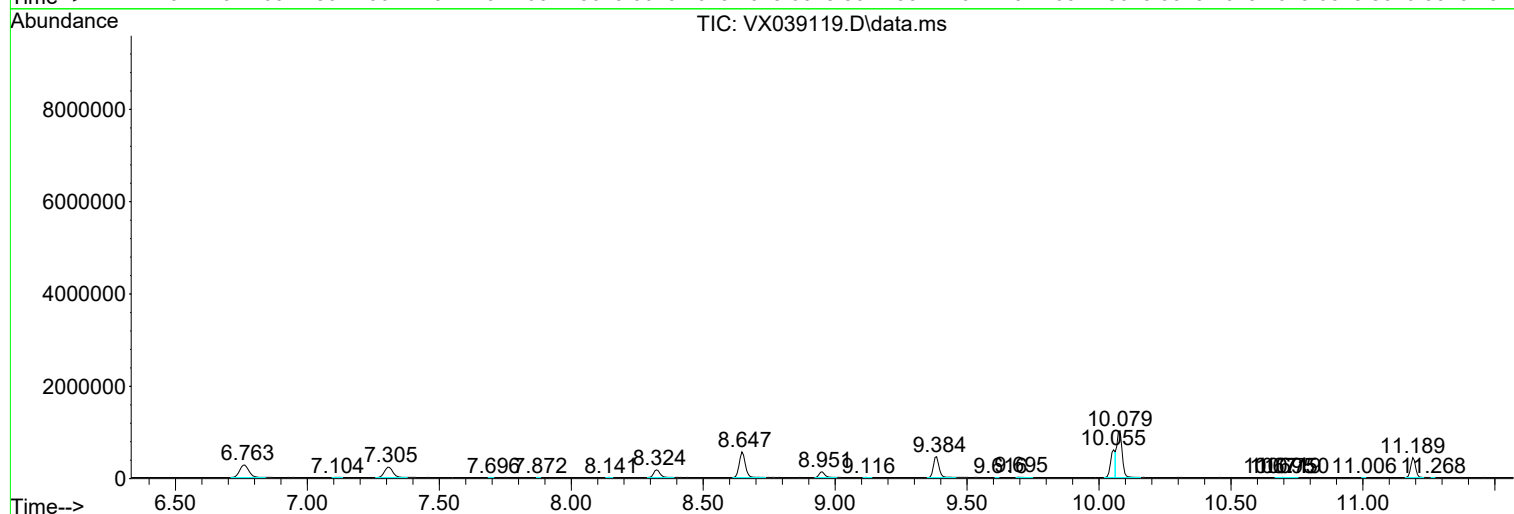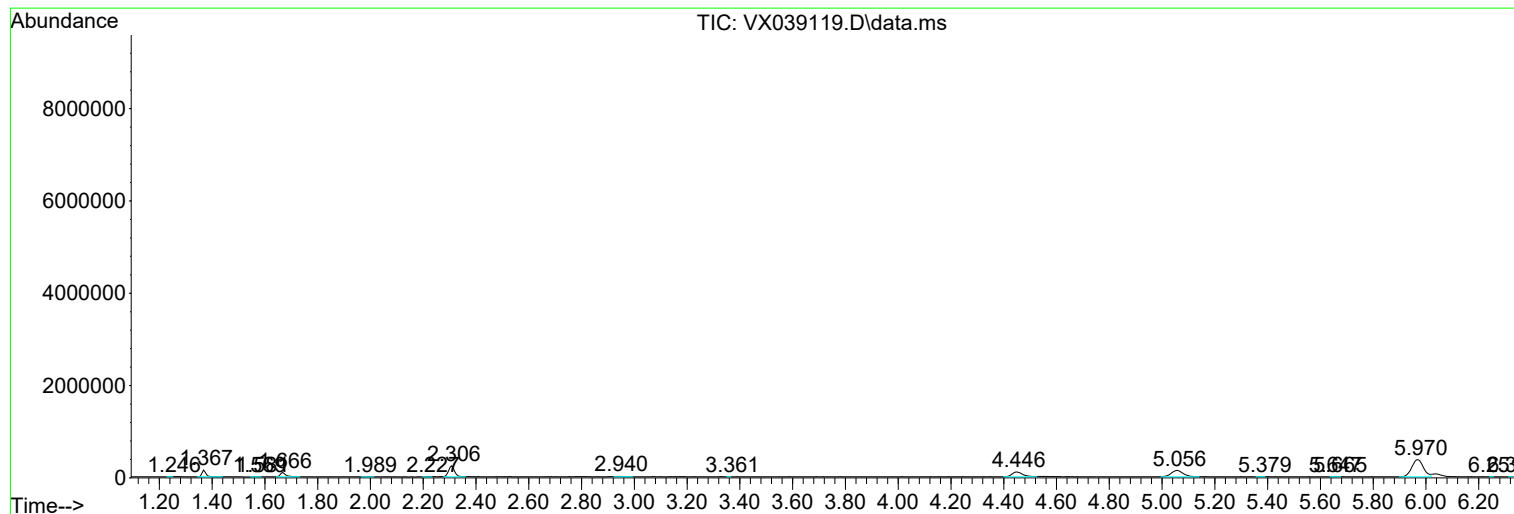

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039119.D
Acq On : 08 Dec 2023 20:45
Operator : JC/MD
Sample : 05646-15 40X
Misc : 1.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039119.D
Acq On : 08 Dec 2023 20:45
Operator : JC/MD
Sample : 05646-15 40X
Misc : 1.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc