

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039120.D
 Acq On : 08 Dec 2023 21:07
 Operator : JC/MD
 Sample : 05646-16 40X
 Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	14	16	18	rVB	1869	1281	0.01%	0.004%
2	1.209	18	20	21	rBV	1606	834	0.01%	0.002%
3	1.246	21	26	27	rBV3	3469	4699	0.04%	0.014%
4	1.368	42	46	58	rVB	140247	150327	1.39%	0.439%
5	1.453	58	60	61	rVV2	1685	1326	0.01%	0.004%
6	1.471	61	63	64	rVV	1480	841	0.01%	0.002%
7	1.489	64	66	68	rVV	1237	1106	0.01%	0.003%
8	1.532	71	73	74	rVB	539	290	0.00%	0.001%
9	1.569	74	79	80	rBV5	2364	2873	0.03%	0.008%
10	1.587	80	82	83	rBV	2744	2386	0.02%	0.007%
11	1.666	91	95	106	rVB	95654	131275	1.21%	0.383%
12	1.776	112	113	114	rVB	2037	746	0.01%	0.002%
13	1.794	114	116	118	rVB	1485	1505	0.01%	0.004%
14	1.825	118	121	124	rBV	1671	2242	0.02%	0.007%
15	1.953	140	142	143	rBV	1018	667	0.01%	0.002%
16	2.026	152	154	155	rVB2	1096	511	0.00%	0.001%
17	2.063	158	160	161	rBV	1492	1208	0.01%	0.004%
18	2.142	171	173	177	rVB2	1936	1995	0.02%	0.006%
19	2.178	177	179	180	rVB	1278	806	0.01%	0.002%
20	2.233	180	188	192	rBV2	4697	13783	0.13%	0.040%
21	2.306	194	200	209	rVB	227933	357007	3.30%	1.043%
22	2.703	264	265	268	rBV	1951	1904	0.02%	0.006%
23	2.940	301	304	309	rBV	6906	11603	0.11%	0.034%
24	3.337	367	369	370	rBV	1994	1693	0.02%	0.005%
25	3.550	402	404	405	rBV	1423	1373	0.01%	0.004%
26	3.641	417	419	423	rBV	1636	2292	0.02%	0.007%
27	3.715	429	431	433	rBV	1223	914	0.01%	0.003%
28	4.452	543	552	563	rBV	100827	283759	2.62%	0.829%
29	5.056	639	651	667	rBV	132973	421451	3.90%	1.231%
30	5.281	686	688	691	rVB	1845	1128	0.01%	0.003%
31	5.970	790	801	822	rBV2	357438	1126367	10.41%	3.289%
32	6.220	839	842	843	rBV	1620	1335	0.01%	0.004%
33	6.257	846	848	851	rBV	1943	2372	0.02%	0.007%
34	6.348	861	863	869	rBV	1603	1691	0.02%	0.005%
35	6.434	875	877	879	rBV	1516	1487	0.01%	0.004%
36	6.757	922	930	942	rBV	270012	651613	6.03%	1.903%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039120.D
 Acq On : 08 Dec 2023 21:07
 Operator : JC/MD
 Sample : 05646-16 40X
 Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.909	953	955	957	rBV	1601	1516	0.01%	0.004%
38	7.305	1012	1020	1038	rVB	222228	494598	4.57%	1.444%
39	7.464	1044	1046	1047	rBV	2016	1376	0.01%	0.004%
40	7.891	1114	1116	1118	rBV	1363	868	0.01%	0.003%
41	7.915	1118	1120	1122	rVV	1635	1270	0.01%	0.004%
42	7.958	1126	1127	1129	rBV	1781	1118	0.01%	0.003%
43	8.025	1136	1138	1140	rBV	2275	2077	0.02%	0.006%
44	8.074	1145	1146	1148	rBV	1820	1266	0.01%	0.004%
45	8.324	1181	1187	1199	rBV	164188	272992	2.52%	0.797%
46	8.647	1234	1240	1255	rBV	540627	857515	7.93%	2.504%
47	8.952	1284	1290	1298	rBV	115384	175990	1.63%	0.514%
48	9.311	1347	1349	1351	rBV	1863	1822	0.02%	0.005%
49	9.384	1355	1361	1370	rBV	456148	663720	6.14%	1.938%
50	9.616	1397	1399	1400	rVB	2367	1194	0.01%	0.003%
51	9.695	1410	1412	1419	rVB2	3611	5350	0.05%	0.016%
52	9.744	1419	1420	1421	rVB	1575	576	0.01%	0.002%
53	10.055	1465	1471	1473	rBV	584142	850455	7.86%	2.484%
54	10.238	1499	1501	1502	rVB	2329	1509	0.01%	0.004%
55	10.256	1502	1504	1505	rBV	1498	1487	0.01%	0.004%
56	10.415	1529	1530	1533	rBV	1653	1963	0.02%	0.006%
57	10.683	1571	1574	1576	rBV	1704	2439	0.02%	0.007%
58	10.939	1614	1616	1617	rVB	2061	953	0.01%	0.003%
59	11.189	1652	1657	1667	rVB	413420	539491	4.99%	1.575%
60	11.293	1673	1674	1676	rBV	2001	1171	0.01%	0.003%
61	11.841	1762	1764	1766	rBV	1663	1246	0.01%	0.004%
62	11.969	1780	1785	1789	rBV	266633	329214	3.04%	0.961%
63	12.042	1789	1797	1806	rVB	7941349	10815084	100.00%	31.583%
64	12.329	1837	1844	1859	rVB2	1681406	2733894	25.28%	7.984%
65	12.829	1924	1926	1929	rBV	1768	1634	0.02%	0.005%
66	12.908	1937	1939	1940	rVB	1810	962	0.01%	0.003%
67	12.926	1940	1942	1943	rBV	1832	1411	0.01%	0.004%
68	13.054	1958	1963	1969	rBV	64384	117197	1.08%	0.342%
69	13.109	1969	1972	1977	rVB2	12240	15691	0.15%	0.046%
70	13.274	1997	1999	2000	rBV	2074	1445	0.01%	0.004%
71	13.384	2013	2017	2021	rVB3	12349	16877	0.16%	0.049%
72	13.591	2045	2051	2067	rVB	7564433	9999739	92.46%	29.202%
73	13.957	2106	2111	2122	rVB	1977256	2546967	23.55%	7.438%
74	14.463	2192	2194	2195	rBV	1421	695	0.01%	0.002%
75	14.542	2204	2207	2212	rBV3	4720	6667	0.06%	0.019%
76	14.627	2217	2221	2224	rBV3	6611	7907	0.07%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039120.D
 Acq On : 08 Dec 2023 21:07
 Operator : JC/MD
 Sample : 05646-16 40X
 Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

77	14.780	2240	2246	2254	rVB	91091	138789	1.28%	0.405%
78	14.957	2273	2275	2277	rBV	1825	1876	0.02%	0.005%
79	15.115	2299	2301	2302	rVV	1879	962	0.01%	0.003%
80	15.133	2302	2304	2307	rVB	2399	2114	0.02%	0.006%
81	15.249	2317	2323	2330	rVB	291995	417191	3.86%	1.218%
82	15.536	2366	2370	2371	rVB	2141	2262	0.02%	0.007%
83	15.560	2371	2374	2375	rBV	1757	1608	0.01%	0.005%
84	16.499	2525	2528	2537	rVB2	6539	10679	0.10%	0.031%




Sum of corrected areas: 34243517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039120.D
Acq On : 08 Dec 2023 21:07
Operator : JC/MD
Sample : 05646-16 40X
Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

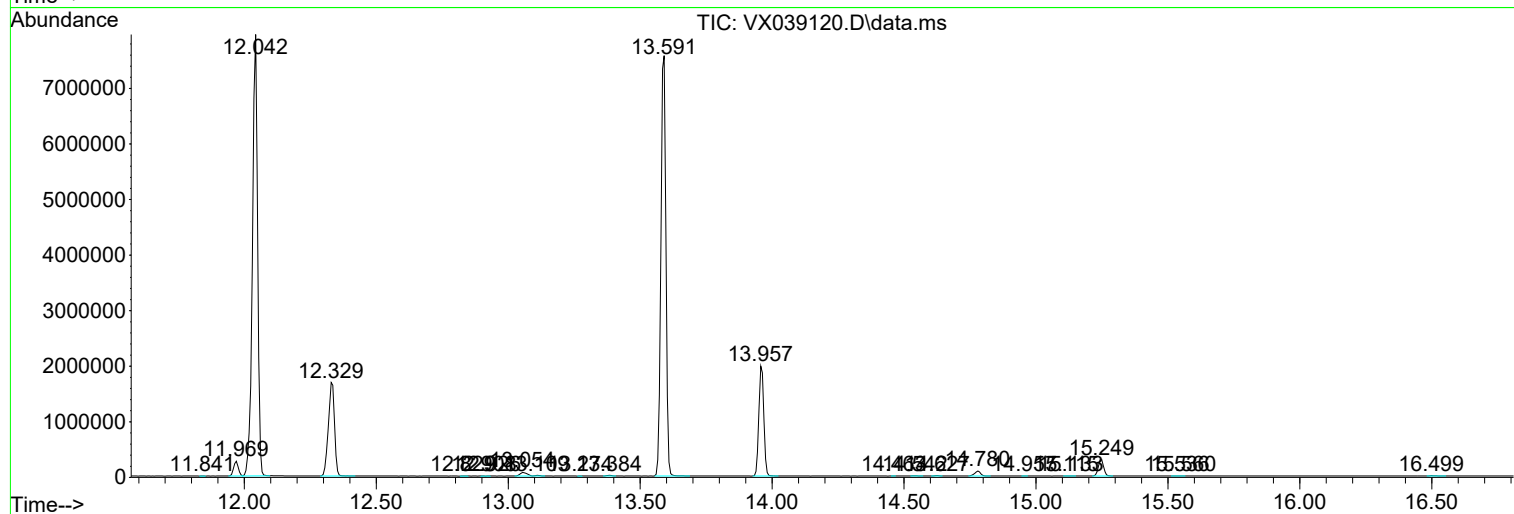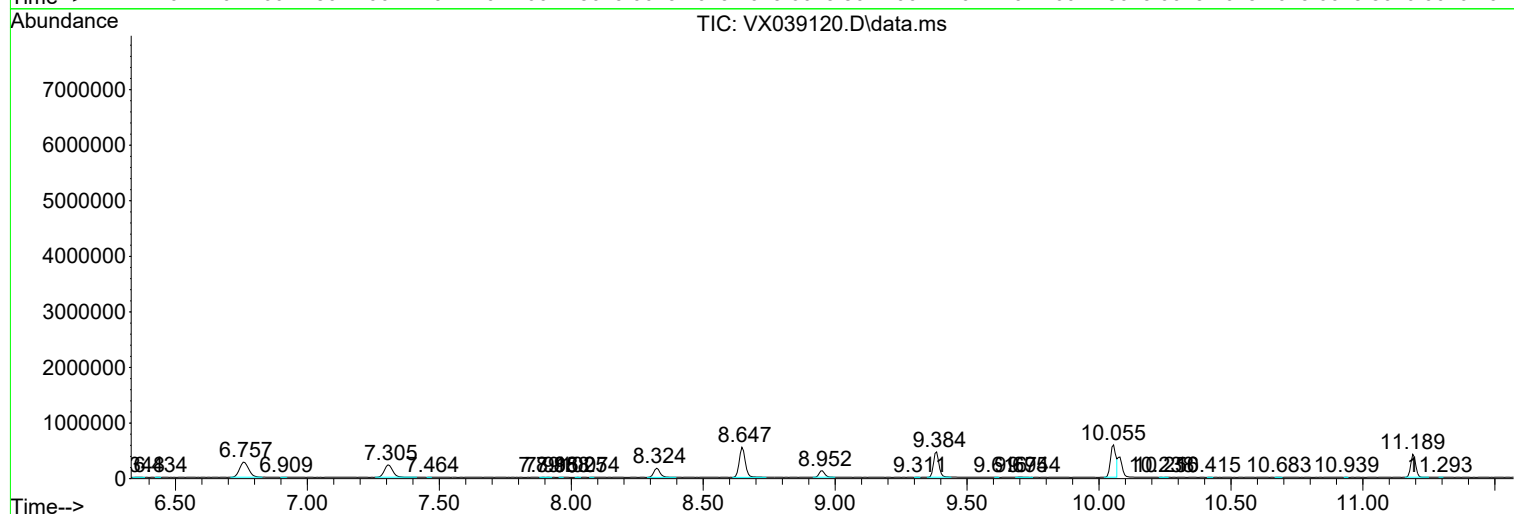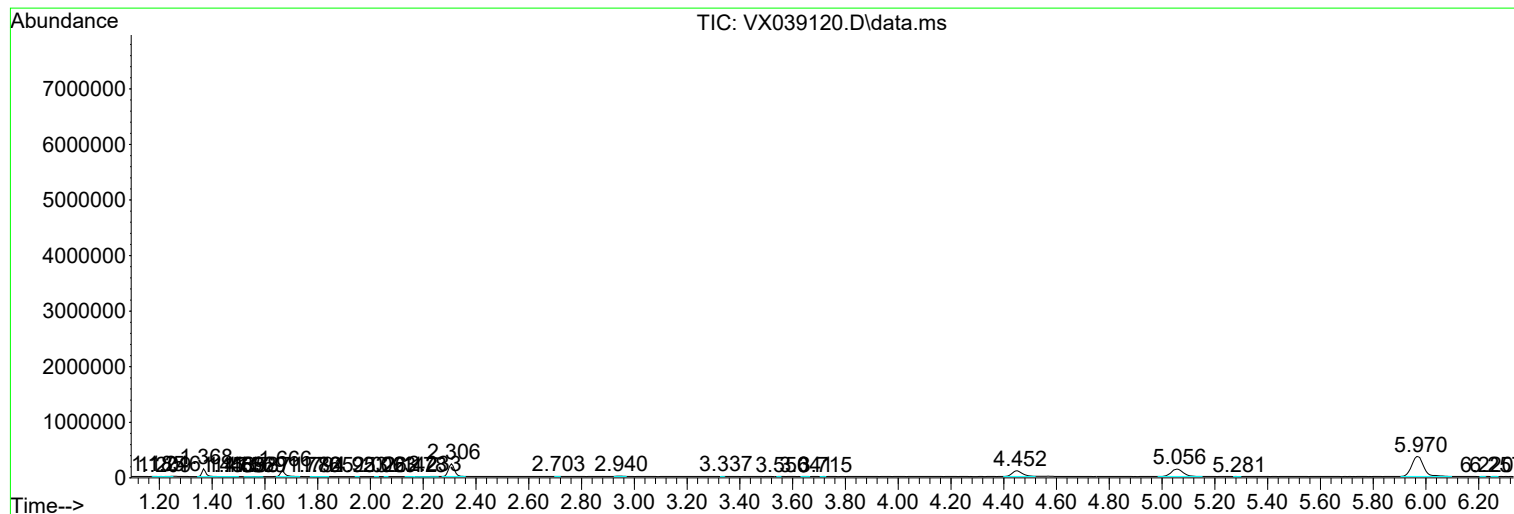

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039120.D
Acq On : 08 Dec 2023 21:07
Operator : JC/MD
Sample : 05646-16 40X
Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039120.D
Acq On : 08 Dec 2023 21:07
Operator : JC/MD
Sample : 05646-16 40X
Misc : 2.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc