

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039123.D
 Acq On : 08 Dec 2023 22:16
 Operator : JC/MD
 Sample : 05646-19 40X
 Misc : 2.18g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.209	18	20	22	rBV	1866	1914	0.04%	0.011%
2	1.367	43	46	58	rVB	142102	148298	2.98%	0.829%
3	1.563	74	78	80	rBV	2821	3186	0.06%	0.018%
4	1.581	80	81	82	rBV	3230	2189	0.04%	0.012%
5	1.666	90	95	106	rBV	90251	135888	2.73%	0.760%
6	1.800	116	117	120	rBV	1363	1576	0.03%	0.009%
7	1.837	122	123	124	rVV	1148	496	0.01%	0.003%
8	2.056	158	159	160	rBV	1754	930	0.02%	0.005%
9	2.233	184	188	189	rBV2	3823	4669	0.09%	0.026%
10	2.306	194	200	209	rVV	241677	374964	7.53%	2.096%
11	2.946	299	305	311	rBV3	9609	20608	0.41%	0.115%
12	3.532	399	401	403	rBV	2004	1588	0.03%	0.009%
13	3.757	436	438	439	rBV	1958	1101	0.02%	0.006%
14	3.989	474	476	477	rVB	1724	944	0.02%	0.005%
15	4.141	498	501	503	rBV	2083	3126	0.06%	0.017%
16	4.452	543	552	563	rBV	100117	286028	5.74%	1.599%
17	5.056	642	651	667	rVB2	141133	418350	8.40%	2.339%
18	5.458	715	717	718	rBV	1505	1015	0.02%	0.006%
19	5.702	756	757	759	rVB	2367	1158	0.02%	0.006%
20	5.720	759	760	763	rBV	2052	2043	0.04%	0.011%
21	5.812	773	775	777	rVB	1816	1413	0.03%	0.008%
22	5.836	777	779	781	rBV	2348	2739	0.06%	0.015%
23	5.970	790	801	811	rBV2	364148	1113945	22.37%	6.228%
24	6.757	922	930	944	rBV	280501	677428	13.60%	3.787%
25	7.080	981	983	985	rBV	1927	1752	0.04%	0.010%
26	7.159	994	996	997	rVB	1854	933	0.02%	0.005%
27	7.190	1000	1001	1002	rBV	1164	521	0.01%	0.003%
28	7.244	1008	1010	1011	rBV	1486	712	0.01%	0.004%
29	7.305	1013	1020	1033	rVV	227578	492831	9.90%	2.755%
30	7.610	1068	1070	1071	rBV	1683	1260	0.03%	0.007%
31	7.799	1099	1101	1103	rVB	2323	2284	0.05%	0.013%
32	8.324	1181	1187	1197	rBV	156380	266285	5.35%	1.489%
33	8.647	1234	1240	1257	rBV	568611	895583	17.99%	5.007%
34	8.860	1273	1275	1277	rBV	1981	2270	0.05%	0.013%
35	8.945	1284	1289	1298	rBV	118832	179729	3.61%	1.005%
36	9.250	1336	1339	1341	rBV	1742	2186	0.04%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039123.D
 Acq On : 08 Dec 2023 22:16
 Operator : JC/MD
 Sample : 05646-19 40X
 Misc : 2.18g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	9.384	1355	1361	1373	rBV	449205	650001	13.05%	3.634%
38	9.579	1391	1393	1397	rBV	2157	2218	0.04%	0.012%
39	9.842	1434	1436	1437	rBV	1574	1341	0.03%	0.007%
40	10.055	1465	1471	1472	rBV	611322	814083	16.35%	4.551%
41	10.079	1472	1475	1486	rVB	881612	1215741	24.42%	6.797%
42	10.232	1498	1500	1502	rBV	1492	1375	0.03%	0.008%
43	10.872	1603	1605	1610	rBV	1603	2392	0.05%	0.013%
44	11.067	1636	1637	1638	rVB	1445	529	0.01%	0.003%
45	11.189	1652	1657	1666	rVB	409997	527227	10.59%	2.948%
46	11.353	1682	1684	1685	rBV	2363	1739	0.03%	0.010%
47	11.463	1700	1702	1703	rBV	1713	1157	0.02%	0.006%
48	11.823	1760	1761	1762	rBV	1617	1170	0.02%	0.007%
49	11.969	1780	1785	1789	rBV	129068	164823	3.31%	0.922%
50	12.042	1789	1797	1807	rVB2	3334287	4979306	100.00%	27.839%
51	12.323	1837	1843	1854	rBV2	753433	1354917	27.21%	7.575%
52	13.054	1958	1963	1970	rBV3	24174	50626	1.02%	0.283%
53	13.109	1970	1972	1976	rVB2	6087	8325	0.17%	0.047%
54	13.146	1976	1978	1981	rBV	1377	1423	0.03%	0.008%
55	13.384	2014	2017	2024	rVB5	4044	5916	0.12%	0.033%
56	13.585	2045	2050	2060	rBV	1713567	2076846	41.71%	11.611%
57	13.749	2075	2077	2078	rBV	1623	827	0.02%	0.005%
58	13.957	2106	2111	2118	rBV	626348	796910	16.00%	4.455%
59	14.127	2137	2139	2140	rBV	1513	722	0.01%	0.004%
60	14.780	2240	2246	2251	rVB3	25437	40567	0.81%	0.227%
61	15.249	2317	2323	2329	rBV	91461	130828	2.63%	0.731%
62	16.072	2456	2458	2461	rBV	1745	2236	0.04%	0.013%
63	16.127	2465	2467	2468	rVB	1824	1012	0.02%	0.006%




Sum of corrected areas: 17886199

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039123.D
Acq On : 08 Dec 2023 22:16
Operator : JC/MD
Sample : 05646-19 40X
Misc : 2.18g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

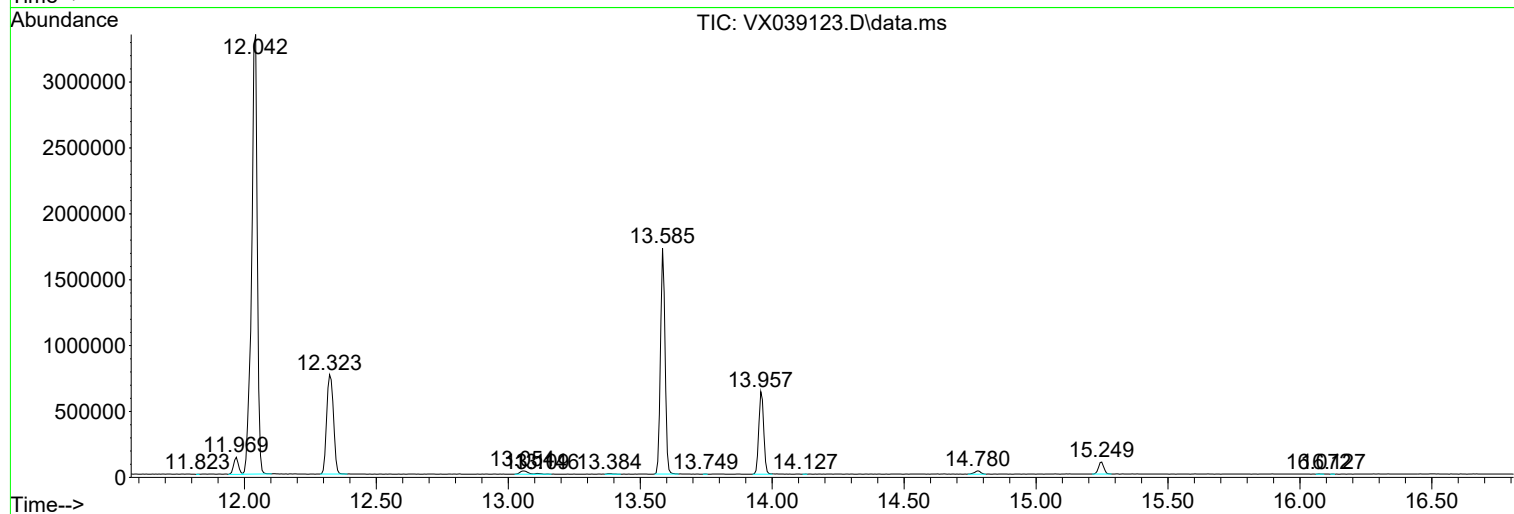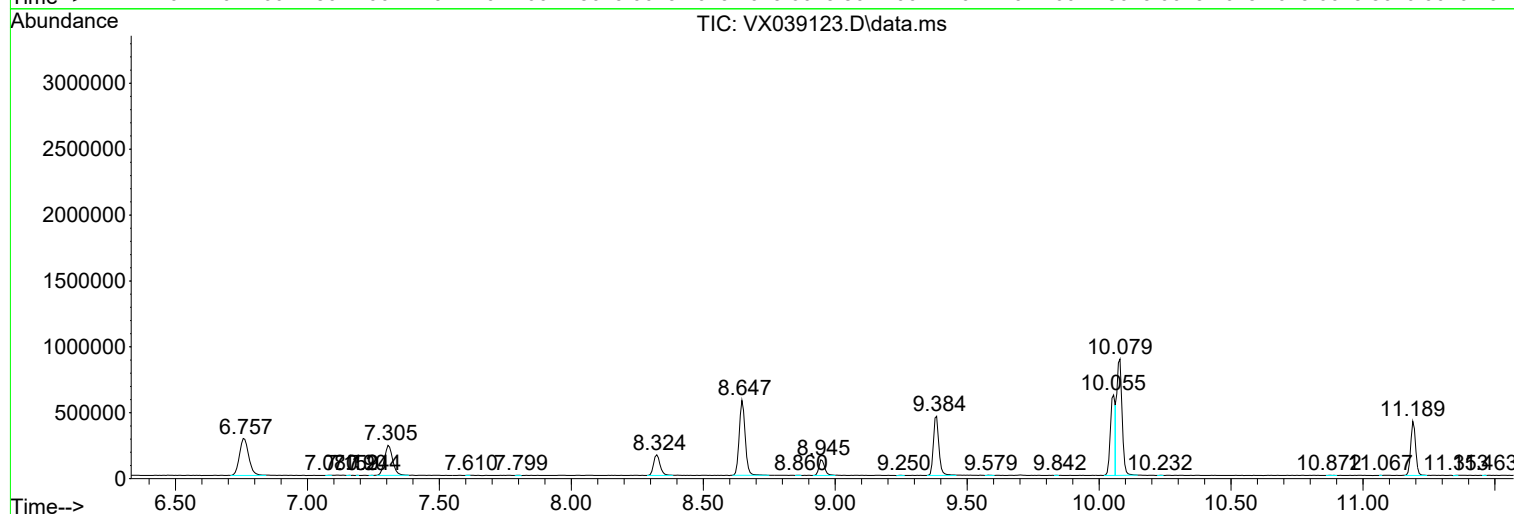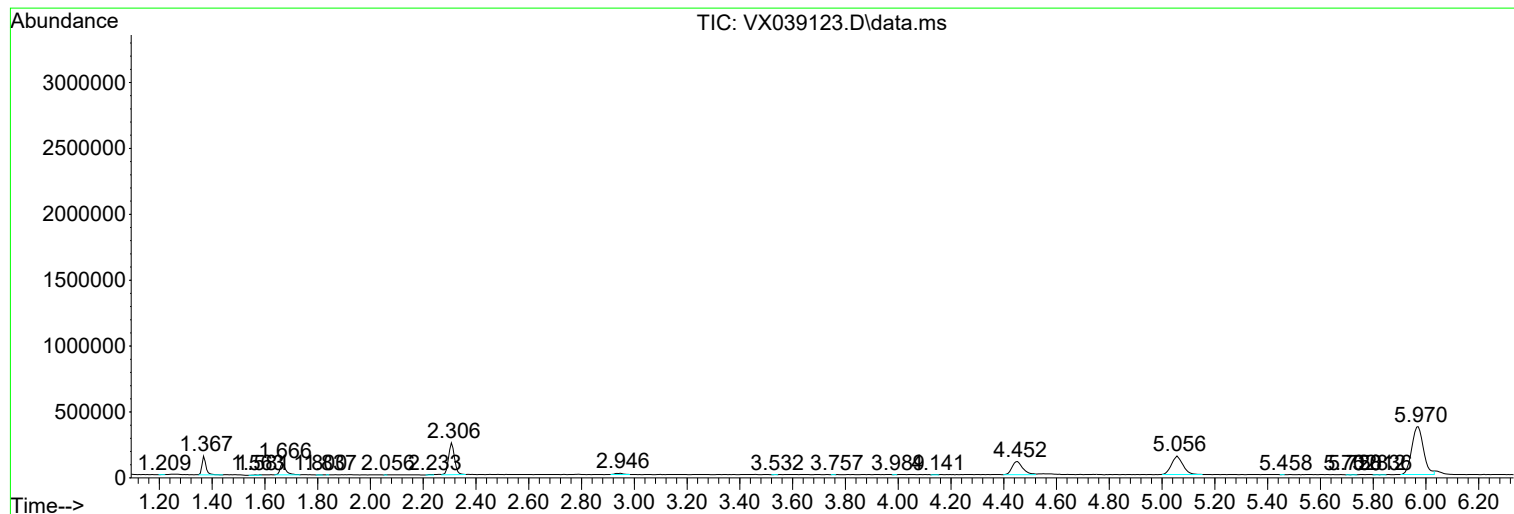

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039123.D
Acq On : 08 Dec 2023 22:16
Operator : JC/MD
Sample : 05646-19 40X
Misc : 2.18g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039123.D
Acq On : 08 Dec 2023 22:16
Operator : JC/MD
Sample : 05646-19 40X
Misc : 2.18g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc