

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039125.D
 Acq On : 08 Dec 2023 23:02
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV2	3310	3968	0.37%	0.046%
2	1.368	42	46	55	rBV	137844	143624	13.39%	1.671%
3	1.453	57	60	62	rBV2	2066	2223	0.21%	0.026%
4	1.477	62	64	74	rVB	5261	13676	1.28%	0.159%
5	1.575	74	80	81	rBV2	4687	5511	0.51%	0.064%
6	1.672	91	96	106	rVB	93631	131128	12.23%	1.526%
7	1.947	137	141	142	rBV2	1369	1433	0.13%	0.017%
8	2.233	184	188	190	rBV2	3770	5825	0.54%	0.068%
9	2.306	194	200	210	rVV	229958	360839	33.65%	4.199%
10	2.563	240	242	245	rVB	1794	1894	0.18%	0.022%
11	2.599	245	248	251	rBV	1503	1873	0.17%	0.022%
12	2.630	251	253	256	rVB	1326	1404	0.13%	0.016%
13	2.788	277	279	282	rVV2	1727	1864	0.17%	0.022%
14	2.941	298	304	308	rBV3	4058	9616	0.90%	0.112%
15	3.495	394	395	401	rVB	2481	2835	0.26%	0.033%
16	3.587	409	410	412	rBV	1958	1620	0.15%	0.019%
17	3.812	445	447	449	rBV	1623	1415	0.13%	0.016%
18	3.873	456	457	460	rBV	1372	1358	0.13%	0.016%
19	4.135	498	500	503	rBV	1757	1803	0.17%	0.021%
20	4.361	535	537	540	rBV2	1915	2293	0.21%	0.027%
21	4.446	543	551	566	rBV	103448	294469	27.46%	3.426%
22	4.800	606	609	611	rBV	1702	2415	0.23%	0.028%
23	4.855	616	618	622	rVB	1449	1405	0.13%	0.016%
24	4.910	624	627	629	rBV	1915	2123	0.20%	0.025%
25	5.056	640	651	664	rBV	132024	415901	38.79%	4.839%
26	5.367	701	702	705	rBV	1793	2329	0.22%	0.027%
27	5.477	718	720	721	rBV	1552	1504	0.14%	0.018%
28	5.708	756	758	761	rBV	1787	1972	0.18%	0.023%
29	5.970	789	801	814	rBV2	354341	1072257	100.00%	12.477%
30	6.306	853	856	859	rBV	1554	1985	0.19%	0.023%
31	6.373	864	867	870	rBV	1318	1939	0.18%	0.023%
32	6.403	870	872	875	rVV	1501	1598	0.15%	0.019%
33	6.531	890	893	894	rBV	1410	1533	0.14%	0.018%
34	6.757	922	930	944	rBV	256883	626011	58.38%	7.284%
35	7.019	971	973	975	rBV	1479	1478	0.14%	0.017%
36	7.111	983	988	990	rBV3	2812	3879	0.36%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039125.D
 Acq On : 08 Dec 2023 23:02
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.129	990	991	994	rVV	2973	2084	0.19%	0.024%
38	7.184	998	1000	1003	rBV	1653	1619	0.15%	0.019%
39	7.306	1011	1020	1033	rBV	221977	492683	45.95%	5.733%
40	7.482	1048	1049	1053	rBV2	1410	2039	0.19%	0.024%
41	7.623	1071	1072	1074	rBV	1952	1458	0.14%	0.017%
42	7.647	1074	1076	1079	rVB	1770	1741	0.16%	0.020%
43	7.720	1087	1088	1092	rVB	2029	1903	0.18%	0.022%
44	7.842	1104	1108	1113	rBV	1521	2455	0.23%	0.029%
45	8.092	1147	1149	1152	rVB	2073	1532	0.14%	0.018%
46	8.116	1152	1153	1158	rVB2	1601	1989	0.19%	0.023%
47	8.159	1158	1160	1162	rBV	2641	2476	0.23%	0.029%
48	8.324	1181	1187	1196	rBV	155622	261640	24.40%	3.044%
49	8.433	1202	1205	1208	rBV	1781	2574	0.24%	0.030%
50	8.647	1234	1240	1254	rBV	529595	843269	78.64%	9.812%
51	8.818	1267	1268	1270	rVB	2143	1377	0.13%	0.016%
52	8.842	1270	1272	1274	rBV	2018	2059	0.19%	0.024%
53	8.891	1278	1280	1283	rVB	1719	1909	0.18%	0.022%
54	8.952	1283	1290	1301	rBV	113649	180586	16.84%	2.101%
55	9.122	1316	1318	1321	rVB	2427	1731	0.16%	0.020%
56	9.384	1355	1361	1371	rBV	458170	694203	64.74%	8.078%
57	9.695	1410	1412	1413	rBV	2141	1770	0.17%	0.021%
58	9.726	1415	1417	1419	rVB	2046	1757	0.16%	0.020%
59	9.750	1419	1421	1422	rBV	1627	1603	0.15%	0.019%
60	9.884	1441	1443	1446	rBV2	1651	1701	0.16%	0.020%
61	10.055	1465	1471	1483	rBV	545180	778683	72.62%	9.061%
62	10.171	1488	1490	1492	rBV	1417	1868	0.17%	0.022%
63	10.500	1543	1544	1548	rVB	1719	1521	0.14%	0.018%
64	10.537	1548	1550	1553	rBV	2285	1707	0.16%	0.020%
65	10.866	1602	1604	1606	rBV	1612	1805	0.17%	0.021%
66	10.976	1621	1622	1623	rBV	3176	1816	0.17%	0.021%
67	11.189	1652	1657	1664	rBV	417189	534121	49.81%	6.215%
68	11.305	1674	1676	1679	rVV	1762	1931	0.18%	0.022%
69	11.384	1687	1689	1691	rVB	1841	1571	0.15%	0.018%
70	11.494	1704	1707	1709	rVB	1616	1568	0.15%	0.018%
71	11.951	1780	1782	1783	rBV	1409	1426	0.13%	0.017%
72	12.018	1788	1793	1802	rBV	588848	808798	75.43%	9.411%
73	12.317	1837	1842	1848	rBV	570611	728813	67.97%	8.480%
74	12.829	1925	1926	1931	rVB	2273	2034	0.19%	0.024%
75	12.939	1941	1944	1946	rBV	1755	1610	0.15%	0.019%
76	12.957	1946	1947	1950	rBV	1460	1448	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
 Data File : VX039125.D
 Acq On : 08 Dec 2023 23:02
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.994	1950	1953	1955	rBV	1327	1353	0.13%	0.016%
78	13.146	1976	1978	1982	rVB	1522	1504	0.14%	0.018%
79	13.305	2001	2004	2005	rBV	1354	1610	0.15%	0.019%
80	13.317	2005	2006	2009	rVB	2272	1473	0.14%	0.017%
81	13.353	2009	2012	2013	rBV	1407	1413	0.13%	0.016%
82	13.585	2046	2050	2055	rVV2	22025	30190	2.82%	0.351%
83	13.774	2079	2081	2084	rVV	2418	1667	0.16%	0.019%
84	13.963	2109	2112	2118	rVB3	7900	10565	0.99%	0.123%
85	14.304	2167	2168	2171	rVB	2290	1532	0.14%	0.018%
86	14.329	2171	2172	2176	rBV	1791	1927	0.18%	0.022%
87	14.414	2181	2186	2189	rBV	2095	4403	0.41%	0.051%
88	14.463	2192	2194	2195	rBV	1763	1381	0.13%	0.016%
89	14.634	2220	2222	2226	rBV	1535	2070	0.19%	0.024%
90	14.829	2251	2254	2256	rBV	2069	2842	0.27%	0.033%
91	14.908	2265	2267	2269	rVB	1853	1481	0.14%	0.017%
92	14.938	2269	2272	2274	rBV	2148	2369	0.22%	0.028%
93	15.249	2319	2323	2327	rBV3	2724	4823	0.45%	0.056%
94	15.371	2341	2343	2345	rBV	1547	1504	0.14%	0.018%
95	15.469	2357	2359	2362	rBV	1578	1958	0.18%	0.023%
96	15.755	2404	2406	2410	rVB	2165	2497	0.23%	0.029%
97	16.133	2466	2468	2471	rVB	2110	2408	0.22%	0.028%
98	16.395	2510	2511	2514	rBV	1982	1808	0.17%	0.021%
99	16.505	2527	2529	2533	rVB	1247	1381	0.13%	0.016%
100	16.761	2569	2571	2575	rBV	1481	2095	0.20%	0.024%




Sum of corrected areas: 8594132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039125.D
Acq On : 08 Dec 2023 23:02
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

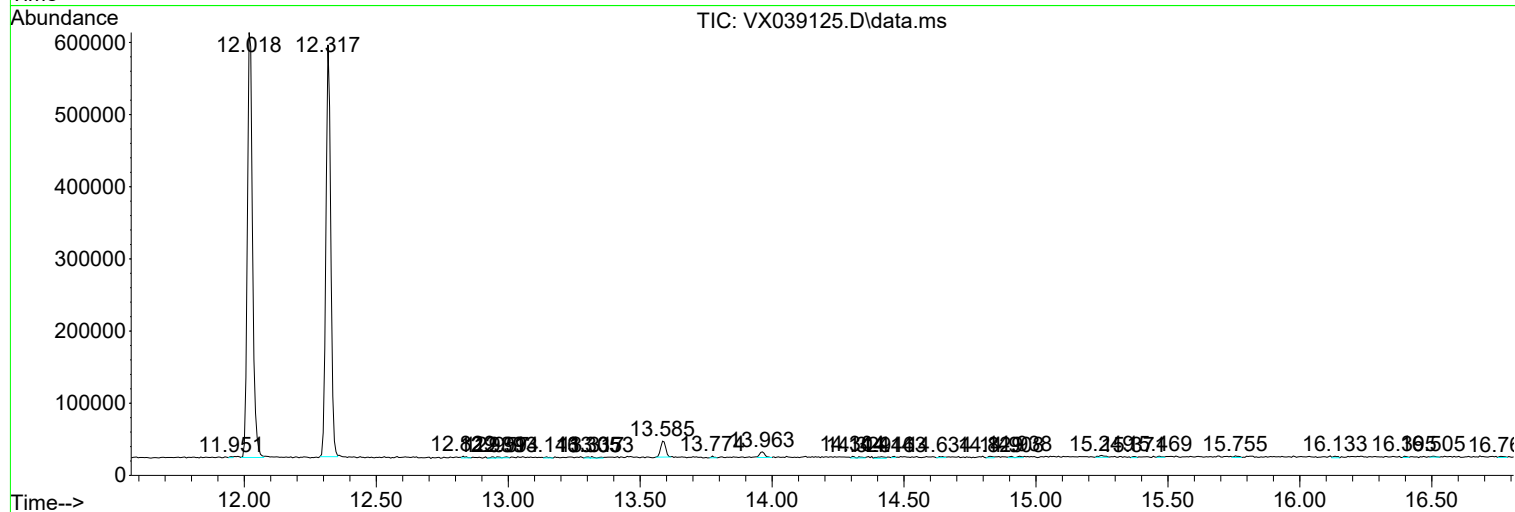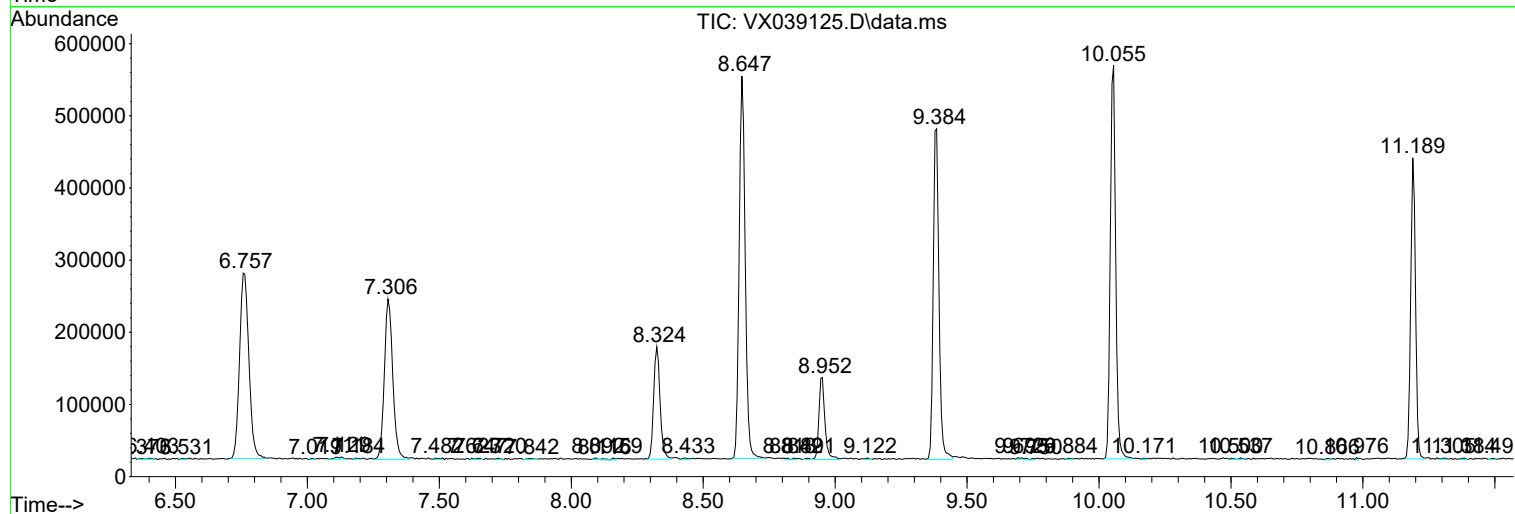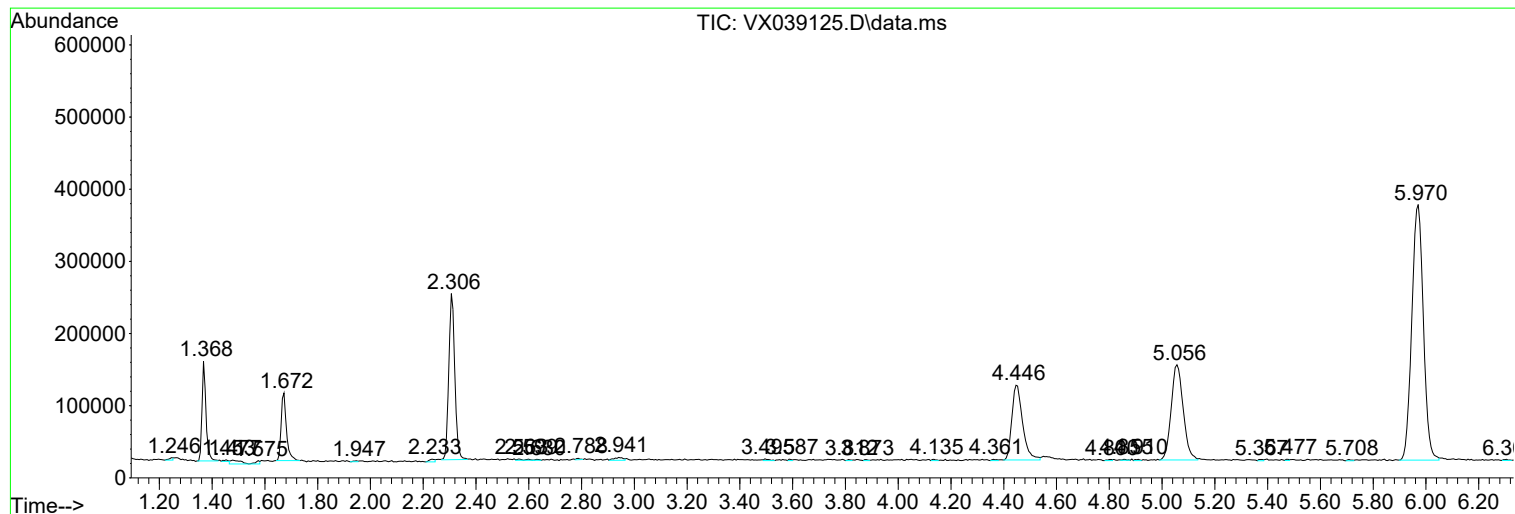

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039125.D
Acq On : 08 Dec 2023 23:02
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120923\
Data File : VX039125.D
Acq On : 08 Dec 2023 23:02
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc