

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
 Data File : VX048786.D
 Acq On : 09 Dec 2025 15:49
 Operator : JC/MD
 Sample : Q3803-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 10 00:26:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	207524	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	423652	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	448489	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	242407	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	148729	53.397	ug/l	0.00
Spiked Amount 50.000	Range	78 - 117	Recovery	=	106.800%	
35) Dibromofluoromethane	5.373	113	135240	46.363	ug/l	0.00
Spiked Amount 50.000	Range	75 - 124	Recovery	=	92.720%	
50) Toluene-d8	8.635	98	484910	47.424	ug/l	0.00
Spiked Amount 50.000	Range	92 - 112	Recovery	=	94.840%	
62) 4-Bromofluorobenzene	11.061	95	216901	61.516	ug/l	0.00
Spiked Amount 50.000	Range	83 - 123	Recovery	=	123.040%#	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.941	59	5315	11.819	ug/l	99
13) Acrolein	2.240	56	722	41.573	ug/l #	1
15) Acrylonitrile	3.075	53	606	0.432	ug/l #	77
16) Acetone	2.374	43	98769	92.629	ug/l	100
18) Methyl Acetate	2.703	43	5534	1.845	ug/l	95
20) Methylene Chloride	2.794	84	124447	46.693	ug/l	96
25) 2-Butanone	4.544	43	18421	11.705	ug/l	99
29) Tetrahydrofuran	5.026	42	514	0.428	ug/l #	40
31) Cyclohexane	5.471	56	1558	0.414	ug/l #	78
36) 1,1-Dichloropropene	5.538	75	15774	3.948	ug/l #	49
37) Ethyl Acetate	4.544	43	18421	3.859	ug/l #	71
38) Carbon Tetrachloride	5.538	117	21053	4.652	ug/l #	13
39) Methylcyclohexane	7.361	83	1365	0.289	ug/l #	88
40) Benzene	6.025	78	1396428	117.904	ug/l	99
42) 1,2-Dichloroethane	6.025	62	11427	2.726	ug/l #	73
43) Isopropyl Acetate	6.324	43	14503	2.006	ug/l	96
48) Methyl methacrylate	7.781	41	54326	14.940	ug/l #	41
51) 4-Methyl-2-Pentanone	8.555	43	341291	76.064	ug/l	91
52) Toluene	8.702	92	536815	75.164	ug/l	100
54) cis-1,3-Dichloropropene	8.531	75	21626	4.519	ug/l #	64
55) 1,1,2-Trichloroethane	9.000	97	3145	1.094	ug/l #	19
57) 1,3-Dichloropropane	9.464	76	1820	0.381	ug/l #	42
59) 2-Hexanone	9.421	43	2397	0.761	ug/l	95
67) Ethyl Benzene	10.177	91	55086	3.439	ug/l	98
68) m/p-Xylenes	10.281	106	106549	17.075	ug/l	98
69) o-Xylene	10.622	106	73291	12.534	ug/l	96
70) Styrene	10.640	104	24268	2.418	ug/l #	63
74) N-amyl acetate	10.842	43	1605	0.226	ug/l #	26
76) 1,2,3-Trichloropropane	11.061	75	107880	23.894	ug/l #	30
78) n-propylbenzene	11.287	91	4326	0.229	ug/l	90
79) 2-Chlorotoluene	11.360	91	2832	0.245	ug/l #	50
80) 1,3,5-Trimethylbenzene	11.433	105	11899	0.886	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.061	75	107880	56.758	ug/l #	3
84) 1,2,4-Trimethylbenzene	11.732	105	63103	4.659	ug/l	70
85) sec-Butylbenzene	11.732	105	63103	3.732	ug/l #	57
95) Naphthalene	13.756	128	361957	26.695	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
Data File : VX048786.D
Acq On : 09 Dec 2025 15:49
Operator : JC/MD
Sample : Q3803-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 10 00:26:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
Data File : VX048786.D
Acq On : 09 Dec 2025 15:49
Operator : JC/MD
Sample : Q3803-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 10 00:26:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration




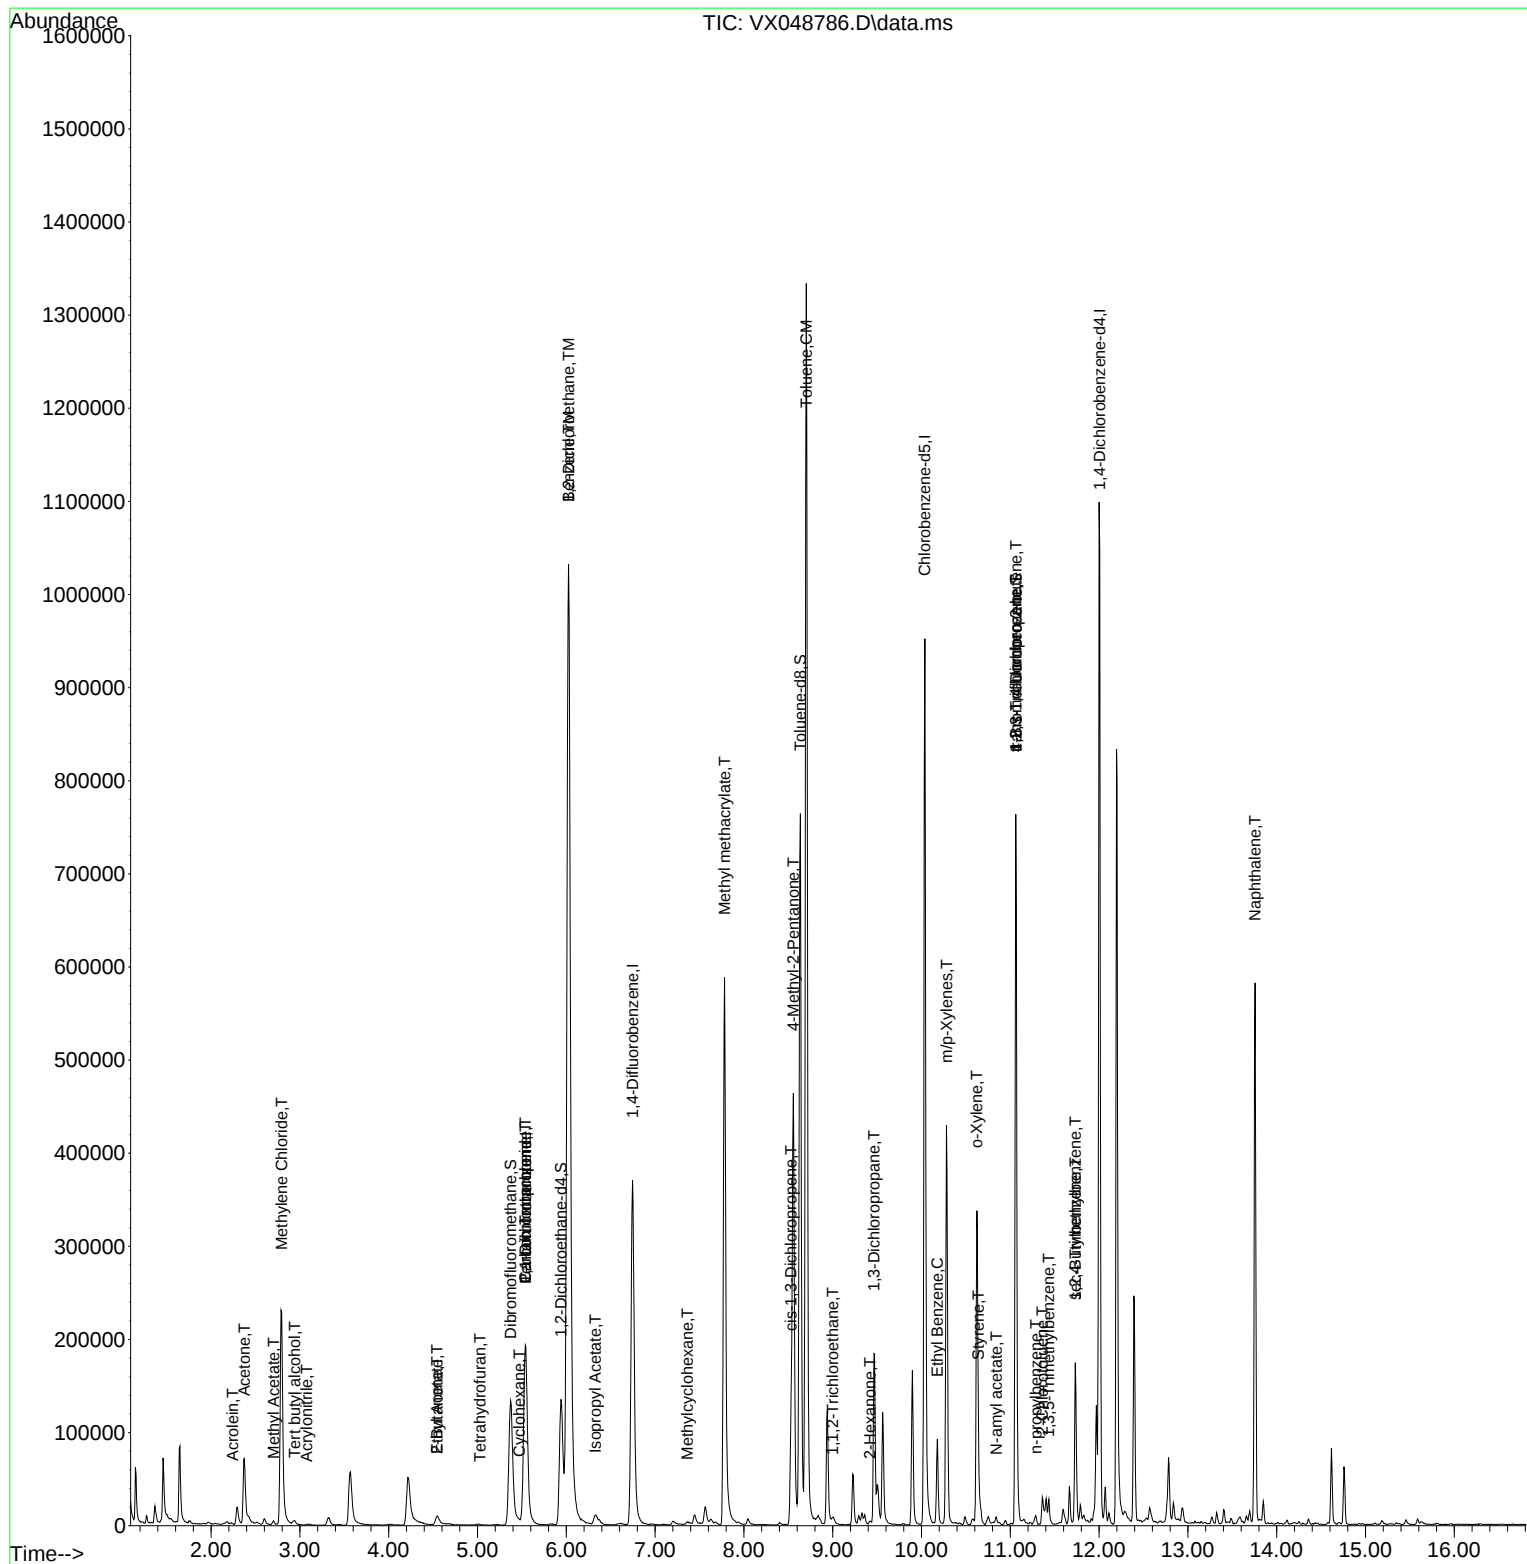




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 207524
Ion Ratio Lower Upper
168 100
99 55.0 44.2 66.4



#11
Tert butyl alcohol
Concen: 11.819 ug/l
RT: 2.941 min Scan# 304
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49


Tgt Ion: 59 Resp: 5315
Ion Ratio Lower Upper
59 100
57 9.7 8.1 12.1








#13
Acrolein
Concen: 41.573 ug/l
RT: 2.240 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 722
Ion Ratio Lower Upper
56 100
55 155.3 55.8 83.6#

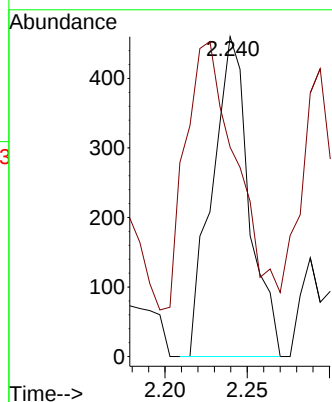

#15
Acrylonitrile
Concen: 0.432 ug/l
RT: 3.075 min Scan# 326
Delta R.T. 0.018 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 53 Resp: 606
Ion Ratio Lower Upper
53 100
52 76.9 66.3 99.5
51 0.0 28.7 43.1#









#16
Acetone
Concen: 92.629 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 98769
Ion Ratio Lower Upper
43 100
58 31.1 25.0 37.4

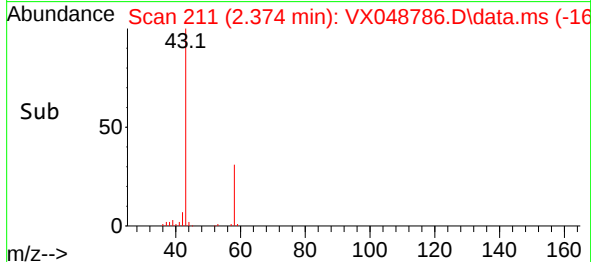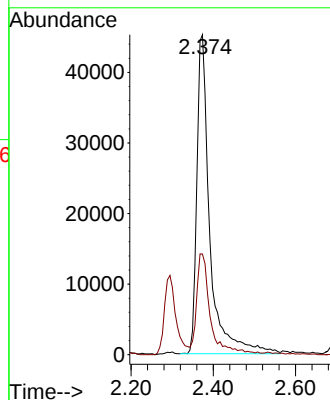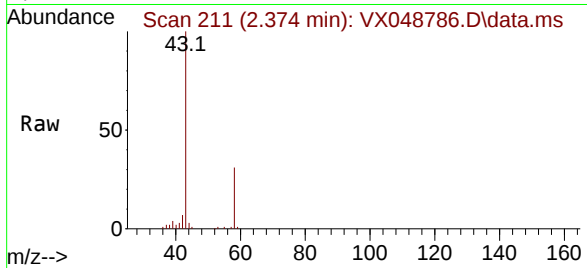

#18
Methyl Acetate
Concen: 1.845 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49


Tgt Ion: 43 Resp: 5534
Ion Ratio Lower Upper
43 100
74 26.7 19.2 28.8

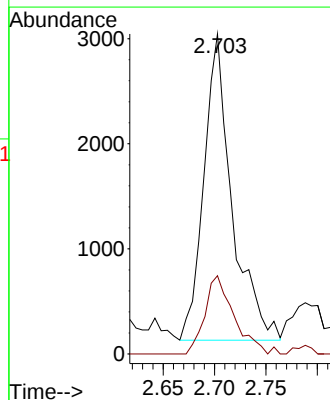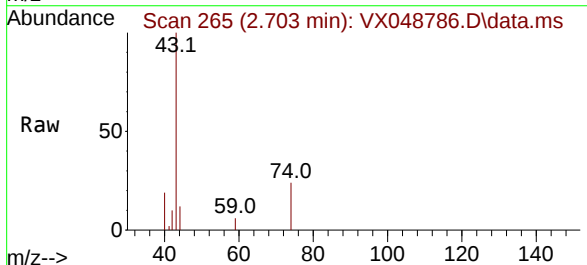





#20
Methylene Chloride
Concen: 46.693 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84	Resp: 124447		
Ion	Ratio	Lower	Upper
84	100		
49	116.7	98.7	148.1
51	36.1	29.4	44.2
86	64.2	52.5	78.7



#25
2-Butanone
Concen: 11.705 ug/l
RT: 4.544 min Scan# 567
Delta R.T. 0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 43	Resp: 18421
Ion Ratio	Lower Upper
43 100	
72 28.9	22.6 34.0





#29

Tetrahydrofuran

Concen: 0.428 ug/l

RT: 5.026 min Scan# 64

Delta R.T. 0.043 min

Lab File: VX048786.D





Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	42	Resp:	514
Ion	Ratio	Lower	Upper
42	100		
72	10.1	39.4	59.2#
71	3.9	35.8	53.6#

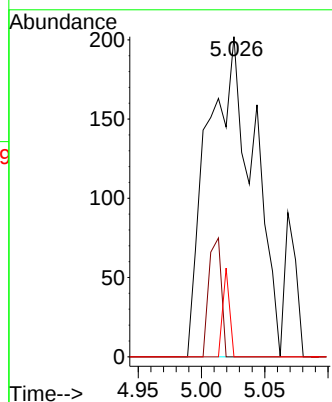

#31

Cyclohexane

Concen: 0.414 ug/l




RT: 5.471 min Scan# 719


Delta R.T. 0.006 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Tgt Ion:	56	Resp:	1558
Ion	Ratio	Lower	Upper
56	100		
69	38.8	24.2	36.2#
84	67.6	72.1	108.1#





#33

1,2-Dichloroethane-d4

Concen: 53.397 ug/l

RT: 5.940 min Scan# 796

Delta R.T. 0.000 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 148729

Ion Ratio Lower Upper

65 100

67 52.9 0.0 107.4



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.745 min Scan# 928

Delta R.T. 0.000 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49




Tgt Ion: 114 Resp: 423652


Ion Ratio Lower Upper

114 100

63 20.8 0.0 39.0

88 16.1 0.0 31.8



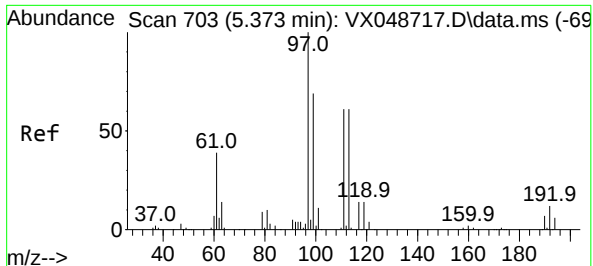

#35

Dibromofluoromethane

Concen: 46.363 ug/l

RT: 5.373 min Scan# 703

Delta R.T. 0.000 min


Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X

ClientSampleId :

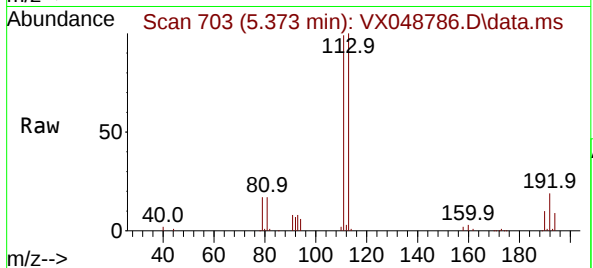




Tgt Ion:113 Resp: 135240

Ion Ratio Lower Upper

113 100

111 101.6 79.5 119.3

192 19.7 16.1 24.1

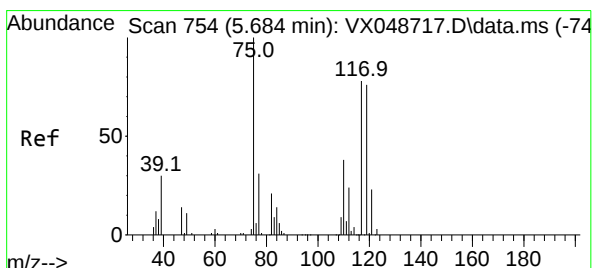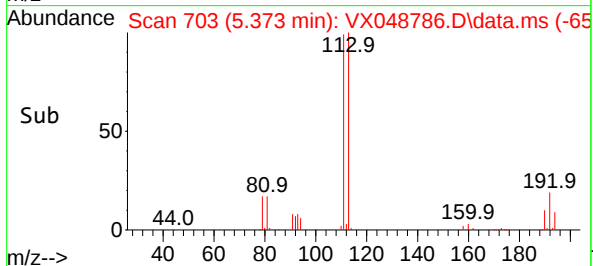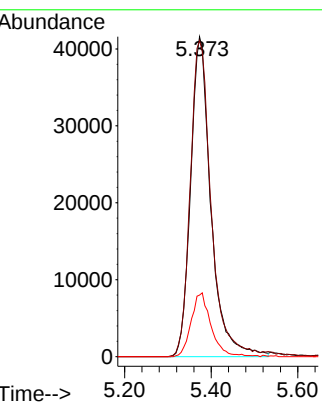

#36

1,1-Dichloropropene

Concen: 3.948 ug/l

RT: 5.538 min Scan# 730

Delta R.T. -0.146 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49




Tgt Ion: 75 Resp: 15774


Ion Ratio Lower Upper

75 100

110 9.3 18.6 55.8#

77 0.0 25.3 37.9#

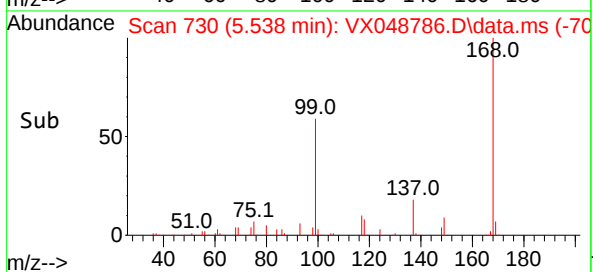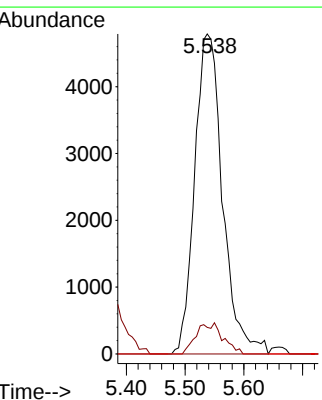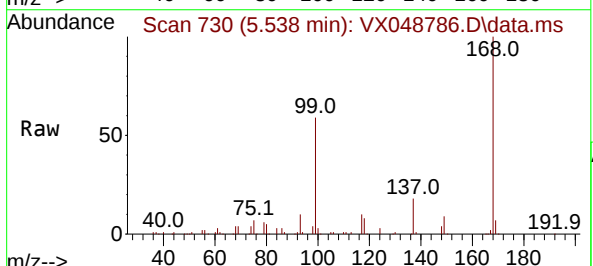



#37

Ethyl Acetate

Concen: 3.859 ug/l

RT: 4.544 min Scan# 5

Delta R.T. -0.152 min


Lab File: VX048786.D

Acq: 09 Dec 2025 15:49




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:	43	Resp:	18421
Ion Ratio	100	Lower	Upper
61	0.0	9.7	14.5#
70	0.0	8.2	12.4#



#38

Carbon Tetrachloride

Concen: 4.652 ug/l




RT: 5.538 min Scan# 730


Delta R.T. -0.128 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Tgt Ion:	117	Resp:	21053
Ion Ratio	100	Lower	Upper
119	4.4	80.5	120.7#
121	0.0	25.4	38.0#


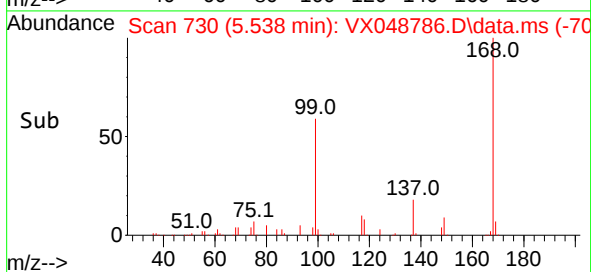




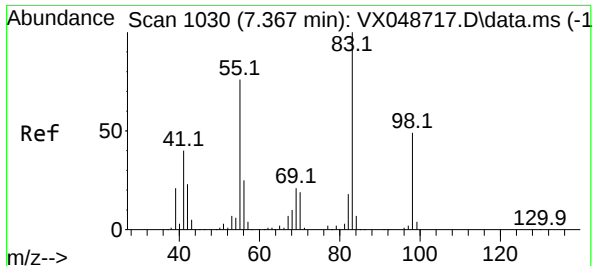

#39
Methylcyclohexane
Concen: 0.289 ug/l
RT: 7.361 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 1365
Ion Ratio Lower Upper
83 100
55 92.9 60.6 90.8#
98 49.4 39.3 58.9

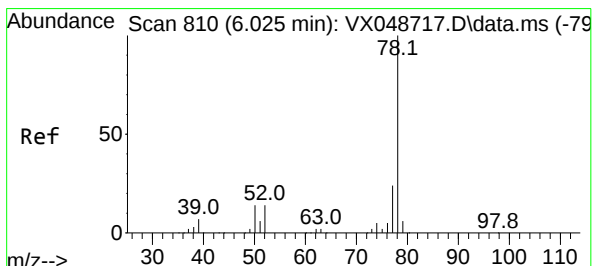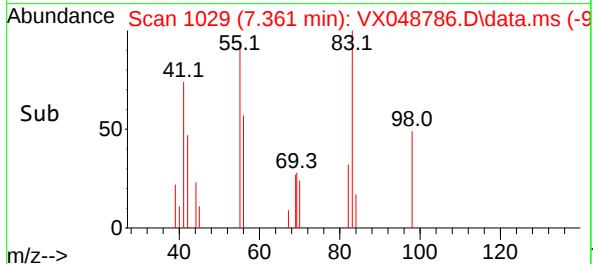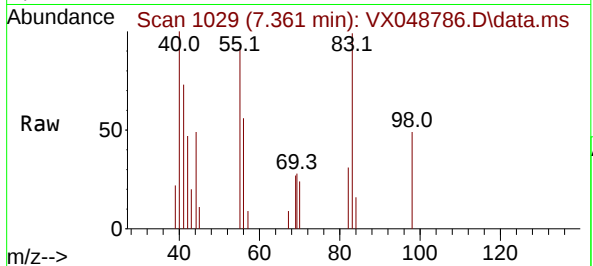

#40
Benzene
Concen: 117.904 ug/l
RT: 6.025 min Scan# 810
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 78 Resp: 1396428
Ion Ratio Lower Upper
78 100
77 23.9 18.8 28.2

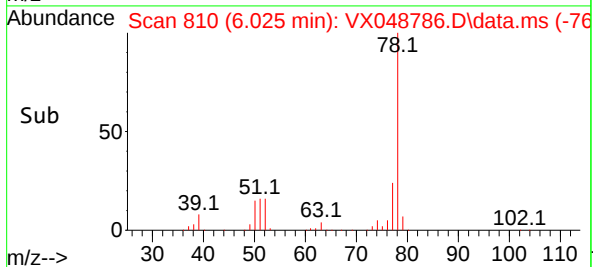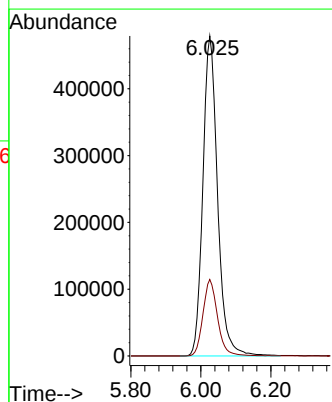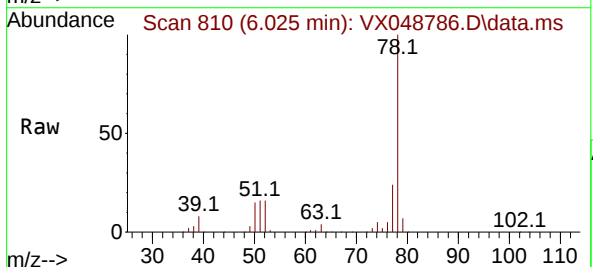



#42

1,2-Dichloroethane

Concen: 2.726 ug/l

RT: 6.025 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 11427

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2

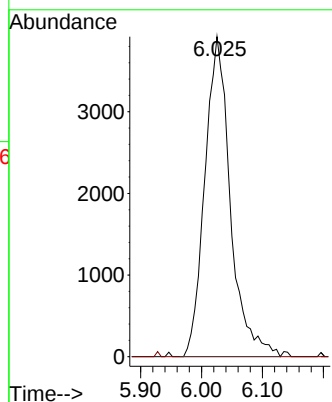

#43

Isopropyl Acetate

Concen: 2.006 ug/l

RT: 6.324 min Scan# 859

Delta R.T. 0.000 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49




Tgt Ion: 43 Resp: 14503


Ion Ratio Lower Upper

43 100

61 19.6 16.8 25.2

87 12.3 11.8 17.6









#48
Methyl methacrylate
Concen: 14.940 ug/l
RT: 7.781 min Scan# 1098
Delta R.T. 0.104 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 41 Resp: 54326
Ion Ratio Lower Upper
41 100
69 0.0 68.5 102.7#
39 51.1 43.5 65.3

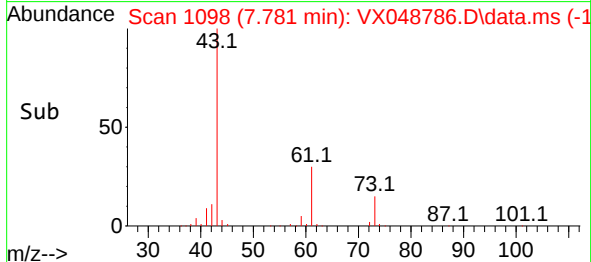

#50
Toluene-d8
Concen: 47.424 ug/l
RT: 8.635 min Scan# 1238
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 98 Resp: 484910
Ion Ratio Lower Upper
98 100
100 65.5 53.4 80.0


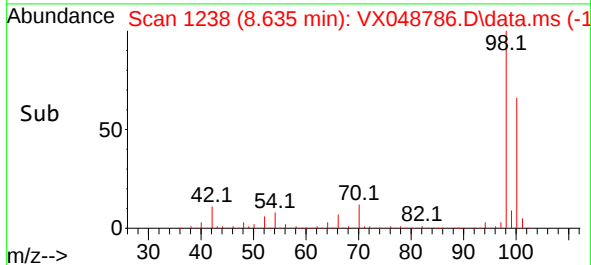






#51
4-Methyl-2-Pentanone
Concen: 76.064 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 341291
Ion Ratio Lower Upper
43 100
58 34.5 32.2 48.4

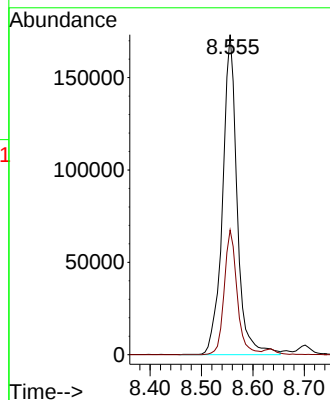

#52
Toluene
Concen: 75.164 ug/l
RT: 8.702 min Scan# 1249
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 92 Resp: 536815
Ion Ratio Lower Upper
92 100
91 170.8 136.3 204.5



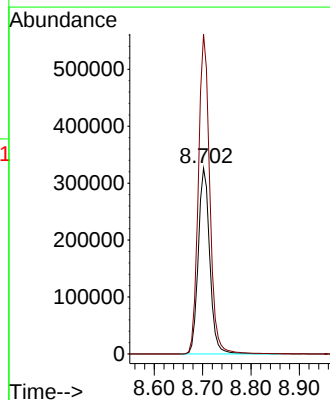





#54
 cis-1,3-Dichloropropene
 Concen: 4.519 ug/l
 RT: 8.531 min Scan# 1191
 Delta R.T. 0.183 min
 Lab File: VX048786.D
 Acq: 09 Dec 2025 15:49




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 21626
 Ion Ratio Lower Upper
 75 100
 77 0.8 26.1 39.1#
 39 33.3 38.2 57.4#



#55
 1,1,2-Trichloroethane
 Concen: 1.094 ug/l
 RT: 9.000 min Scan# 1298
 Delta R.T. -0.134 min
 Lab File: VX048786.D
 Acq: 09 Dec 2025 15:49

Tgt Ion: 97 Resp: 3145
 Ion Ratio Lower Upper
 97 100
 83 0.0 66.0 99.0#
 85 0.0 43.2 64.8#
 99 7.1 50.0 75.0#

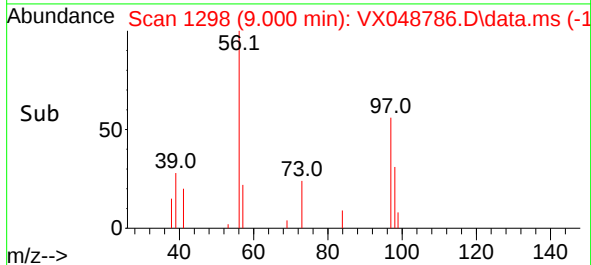

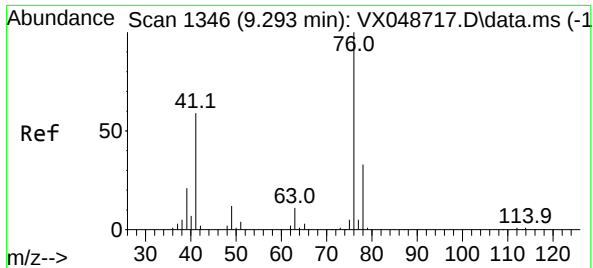

#57

1,3-Dichloropropane

Concen: 0.381 ug/l

RT: 9.464 min Scan# 1374

Delta R.T. 0.171 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 1820

Ion Ratio Lower Upper

76 100

78 0.0 26.0 39.0#

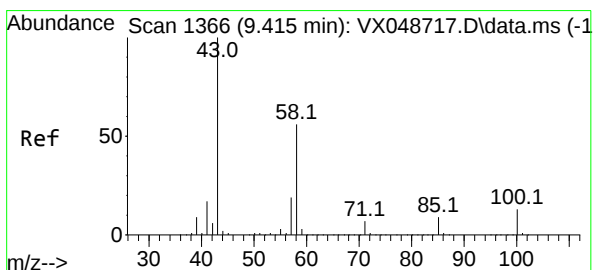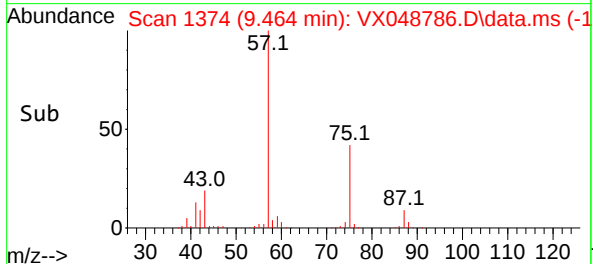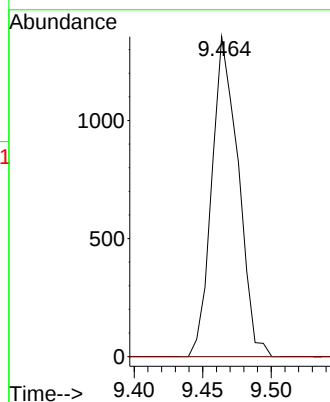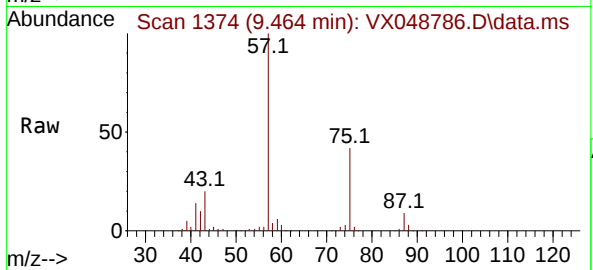

#59

2-Hexanone

Concen: 0.761 ug/l

RT: 9.421 min Scan# 1367

Delta R.T. 0.006 min

Lab File: VX048786.D




Acq: 09 Dec 2025 15:49


Tgt Ion: 43 Resp: 2397

Ion Ratio Lower Upper

43 100

58 51.6 27.8 83.4


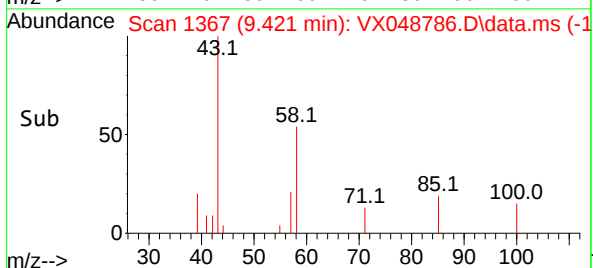
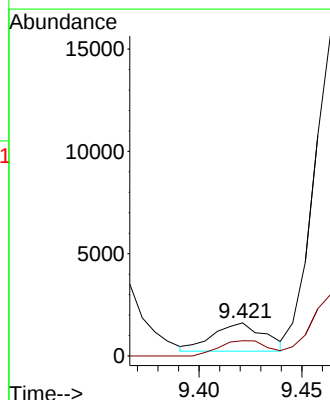
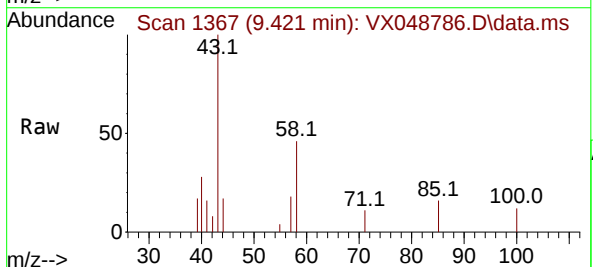




#62
4-Bromofluorobenzene
Concen: 61.516 ug/l
RT: 11.061 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 216901
Ion Ratio Lower Upper
95 100
174 78.6 0.0 157.8
176 76.9 0.0 154.0

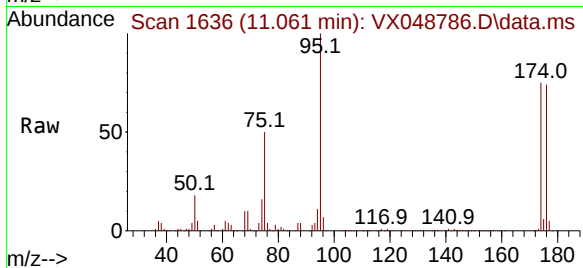

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 117 Resp: 448489
Ion Ratio Lower Upper
117 100
82 54.9 44.1 66.1
119 32.3 25.2 37.8

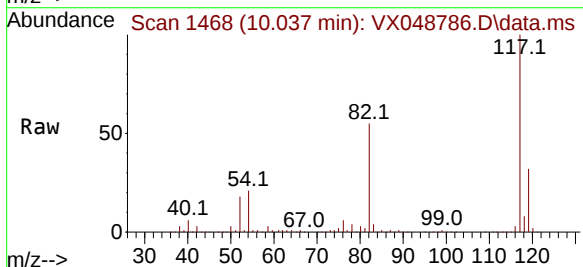



#67

Ethyl Benzene

Concen: 3.439 ug/l

RT: 10.177 min Scan# 1491

Delta R.T. 0.000 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 55086

Ion Ratio Lower Upper

91 100

106 30.2 25.3 37.9

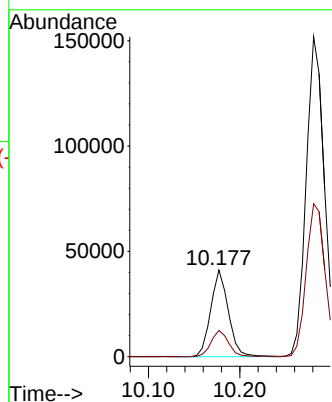

#68

m/p-Xylenes

Concen: 17.075 ug/l

RT: 10.281 min Scan# 1508

Delta R.T. 0.000 min

Lab File: VX048786.D




Acq: 09 Dec 2025 15:49


Tgt Ion: 106 Resp: 106549

Ion Ratio Lower Upper

106 100

91 202.4 164.2 246.4









#69
o-Xylene
Concen: 12.534 ug/l
RT: 10.622 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 73291
Ion Ratio Lower Upper
106 100
91 210.6 108.1 324.3

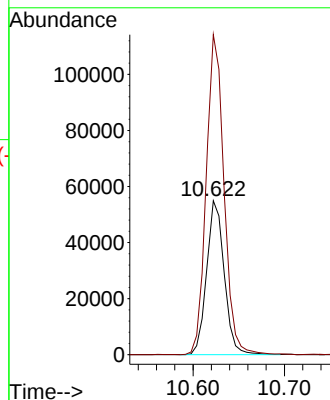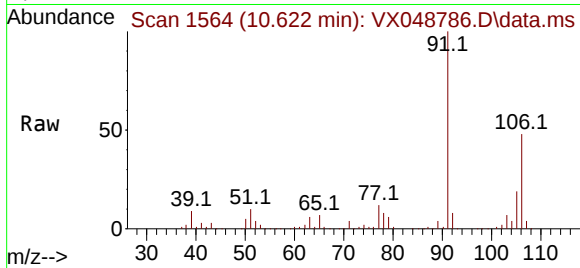

#70
Styrene
Concen: 2.418 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49


Tgt Ion:104 Resp: 24268
Ion Ratio Lower Upper
104 100
78 78.9 40.6 60.8#
103 79.1 43.4 65.2#

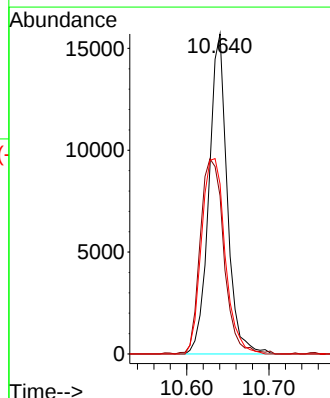






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49


Instrument :
MSVOA_X
ClientSampleId :

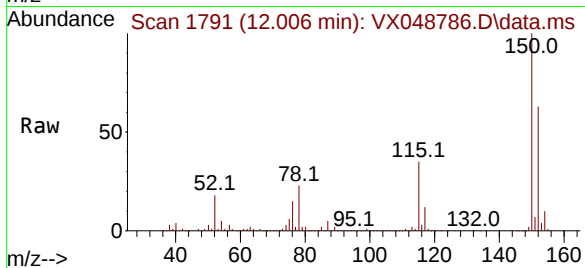



Tgt Ion:152 Resp: 242407
Ion Ratio Lower Upper
152 100
115 57.9 42.1 126.4
150 157.6 0.0 347.8

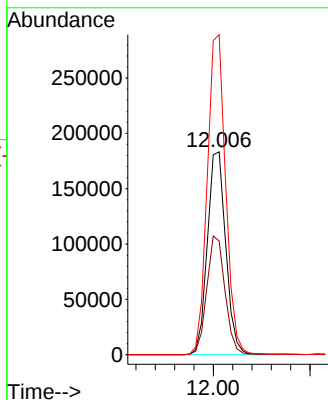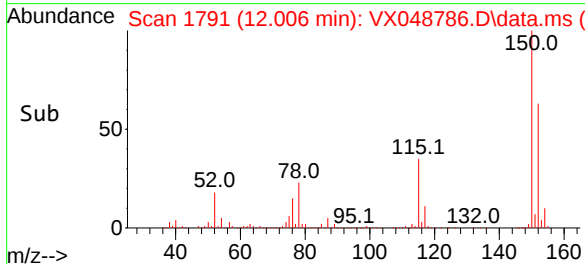


#74
N-ethyl acetate
Concen: 0.226 ug/l
RT: 10.842 min Scan# 1600
Delta R.T. 0.018 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

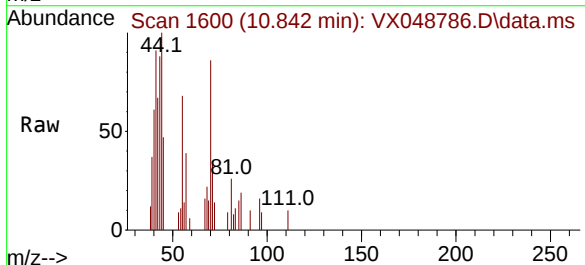

Tgt Ion: 43 Resp: 1605
Ion Ratio Lower Upper
43 100
70 102.6 33.9 50.9#
55 54.6 19.1 28.7#
61 0.0 19.0 28.6#



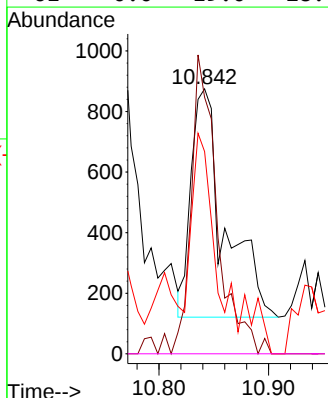
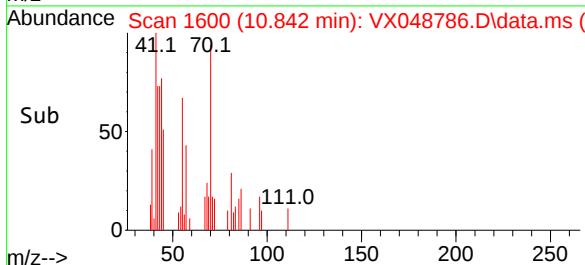




#76
1,2,3-Trichloropropane
Concen: 23.894 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.158 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 107880
Ion Ratio Lower Upper
75 100
77 1.1 24.3 73.0#

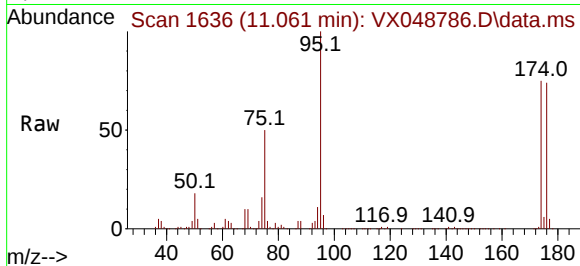

#78
n-propylbenzene
Concen: 0.229 ug/l
RT: 11.287 min Scan# 1673
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 91 Resp: 4326
Ion Ratio Lower Upper
91 100
120 18.0 11.4 34.2

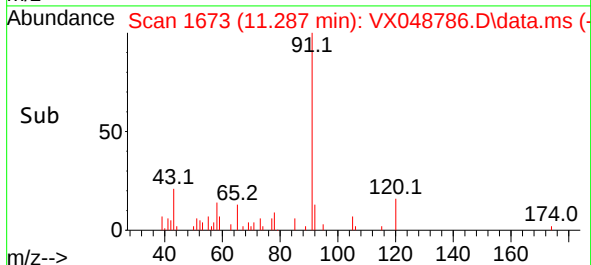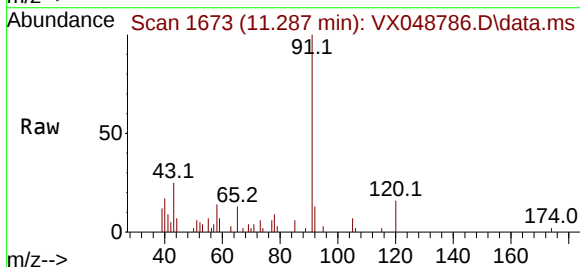



#79

2-Chlorotoluene

Concen: 0.245 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX048786.D

Acq: 09 Dec 2025 15:49

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 2832

Ion Ratio Lower Upper

91 100

126 5.3 16.8 50.3#

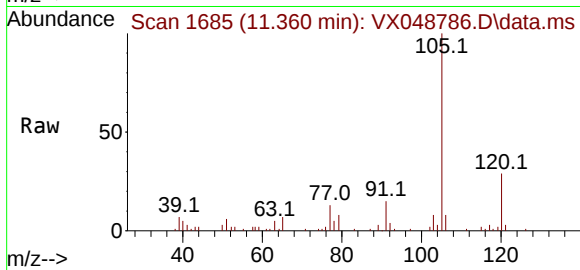

#80

1,3,5-Trimethylbenzene

Concen: 0.886 ug/l

RT: 11.433 min Scan# 1697

Delta R.T. 0.000 min

Lab File: VX048786.D




Acq: 09 Dec 2025 15:49


Tgt Ion:105 Resp: 11899

Ion Ratio Lower Upper

105 100

120 47.3 24.4 73.2


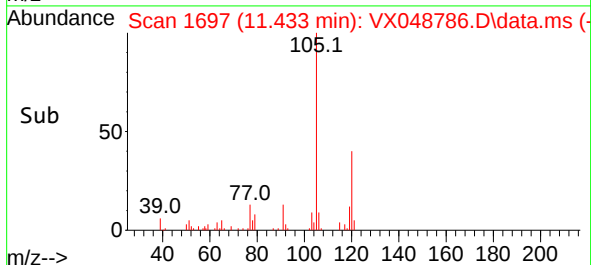

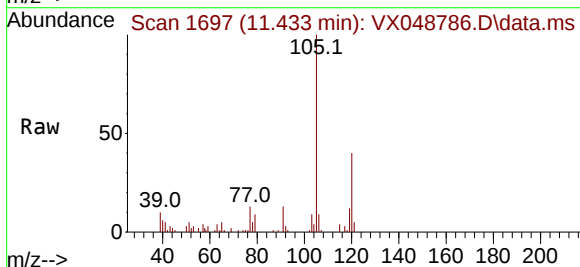




#81
trans-1,4-Dichloro-2-butene
Concen: 56.758 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 107880
Ion Ratio Lower Upper
75 100
53 0.0 79.9 119.9#
89 0.0 67.1 100.7#

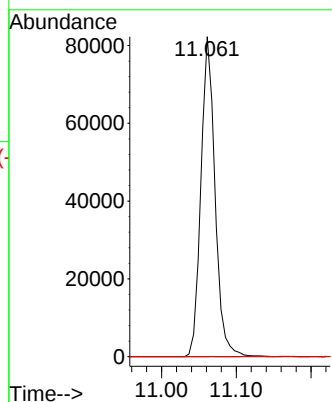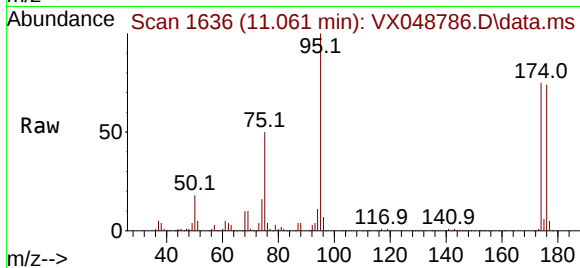

#84
1,2,4-Trimethylbenzene
Concen: 4.659 ug/l
RT: 11.732 min Scan# 1746
Delta R.T. 0.000 min
Lab File: VX048786.D
Acq: 09 Dec 2025 15:49

Tgt Ion: 105 Resp: 63103
Ion Ratio Lower Upper
105 100
120 25.0 22.3 66.8


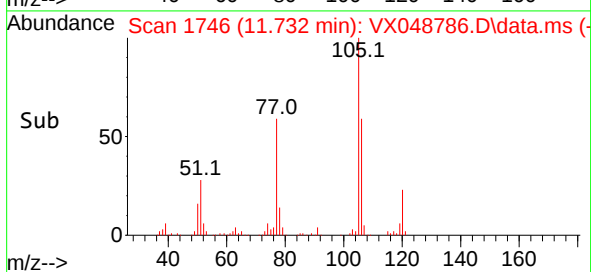
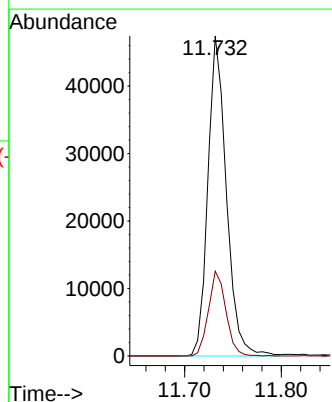
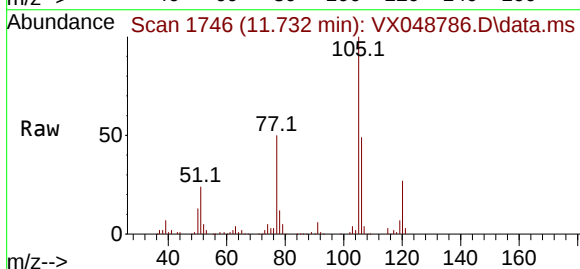




#85
 sec-Butylbenzene
 Concen: 3.732 ug/l
 RT: 11.732 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX048786.D
 Acq: 09 Dec 2025 15:49

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion:105 Resp: 63103
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.5#

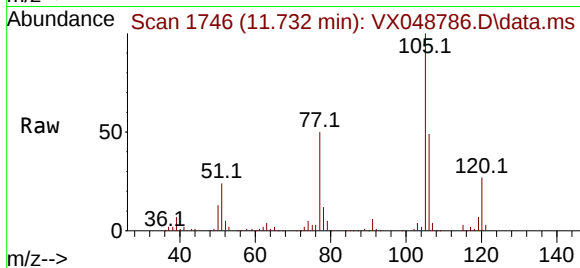

#95
 Naphthalene
 Concen: 26.695 ug/l
 RT: 13.756 min Scan# 2078
 Delta R.T. 0.000 min
 Lab File: VX048786.D
 Acq: 09 Dec 2025 15:49

Tgt Ion:128 Resp: 361957
 Ion Ratio Lower Upper
 128 100
 127 12.6 10.2 15.2
 129 10.7 8.6 13.0

