

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
 Data File : VX048790.D
 Acq On : 09 Dec 2025 17:11
 Operator : JC/MD
 Sample : Q3803-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 10 00:28:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	165845	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	334402	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	356325	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	195561	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	116404	52.294	ug/l	0.00
Spiked Amount 50.000	Range	78 - 117	Recovery	=	104.580%	
35) Dibromofluoromethane	5.373	113	103439	44.925	ug/l	0.00
Spiked Amount 50.000	Range	75 - 124	Recovery	=	89.840%	
50) Toluene-d8	8.635	98	373157	46.235	ug/l	0.00
Spiked Amount 50.000	Range	92 - 112	Recovery	=	92.460%	
62) 4-Bromofluorobenzene	11.061	95	168849	60.669	ug/l	0.00
Spiked Amount 50.000	Range	83 - 123	Recovery	=	121.340%	
Target Compounds						Qvalue
11) Tert butyl alcohol	2.928	59	5175	14.400	ug/l	99
13) Acrolein	2.233	56	918	42.398	ug/l #	61
14) Allyl chloride	2.642	41	842	0.260	ug/l #	27
15) Acrylonitrile	3.081	53	1218	1.088	ug/l #	43
16) Acetone	2.374	43	84793	99.506	ug/l	100
18) Methyl Acetate	2.703	43	9183	3.830	ug/l	98
20) Methylene Chloride	2.788	84	131079	61.541	ug/l	97
25) 2-Butanone	4.550	43	14160	11.259	ug/l	98
29) Tetrahydrofuran	5.001	42	290	0.302	ug/l #	71
31) Cyclohexane	5.452	56	1741	0.579	ug/l #	68
36) 1,1-Dichloropropene	5.544	75	12359	3.919	ug/l #	45
38) Carbon Tetrachloride	5.544	117	16244	4.547	ug/l #	14
39) Methylcyclohexane	7.361	83	1702	0.456	ug/l #	70
40) Benzene	6.025	78	934094	99.917	ug/l	100
42) 1,2-Dichloroethane	6.025	62	7623	2.304	ug/l #	73
43) Isopropyl Acetate	6.324	43	15769	2.764	ug/l	94
48) Methyl methacrylate	7.781	41	57650	20.085	ug/l #	40
51) 4-Methyl-2-Pentanone	8.531	43	56540	15.964	ug/l #	35
52) Toluene	8.702	92	351856	62.415	ug/l	100
54) cis-1,3-Dichloropropene	8.531	75	21967	5.816	ug/l #	56
55) 1,1,2-Trichloroethane	9.000	97	2444	1.077	ug/l #	18
57) 1,3-Dichloropropane	9.464	76	1832	0.486	ug/l #	42
59) 2-Hexanone	9.464	43	24964	10.041	ug/l #	46
67) Ethyl Benzene	10.177	91	40078	3.149	ug/l	97
68) m/p-Xylenes	10.281	106	76681	15.467	ug/l	99
69) o-Xylene	10.622	106	46986	10.114	ug/l	99
70) Styrene	10.640	104	16395	2.056	ug/l #	67
74) N-amyl acetate	10.842	43	1507	0.263	ug/l #	1
76) 1,2,3-Trichloropropane	11.061	75	84158	23.105	ug/l #	30
78) n-propylbenzene	11.287	91	4197	0.275	ug/l	98
79) 2-Chlorotoluene	11.360	91	2458	0.264	ug/l #	63
80) 1,3,5-Trimethylbenzene	11.433	105	11734	1.083	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.061	75	84158	54.884	ug/l #	3
84) 1,2,4-Trimethylbenzene	11.732	105	44016	4.028	ug/l	78
85) sec-Butylbenzene	11.732	105	44016	3.227	ug/l #	57
95) Naphthalene	13.756	128	295930	27.036	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
Data File : VX048790.D
Acq On : 09 Dec 2025 17:11
Operator : JC/MD
Sample : Q3803-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 10 00:28:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120925\
Data File : VX048790.D
Acq On : 09 Dec 2025 17:11
Operator : JC/MD
Sample : Q3803-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 10 00:28:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration

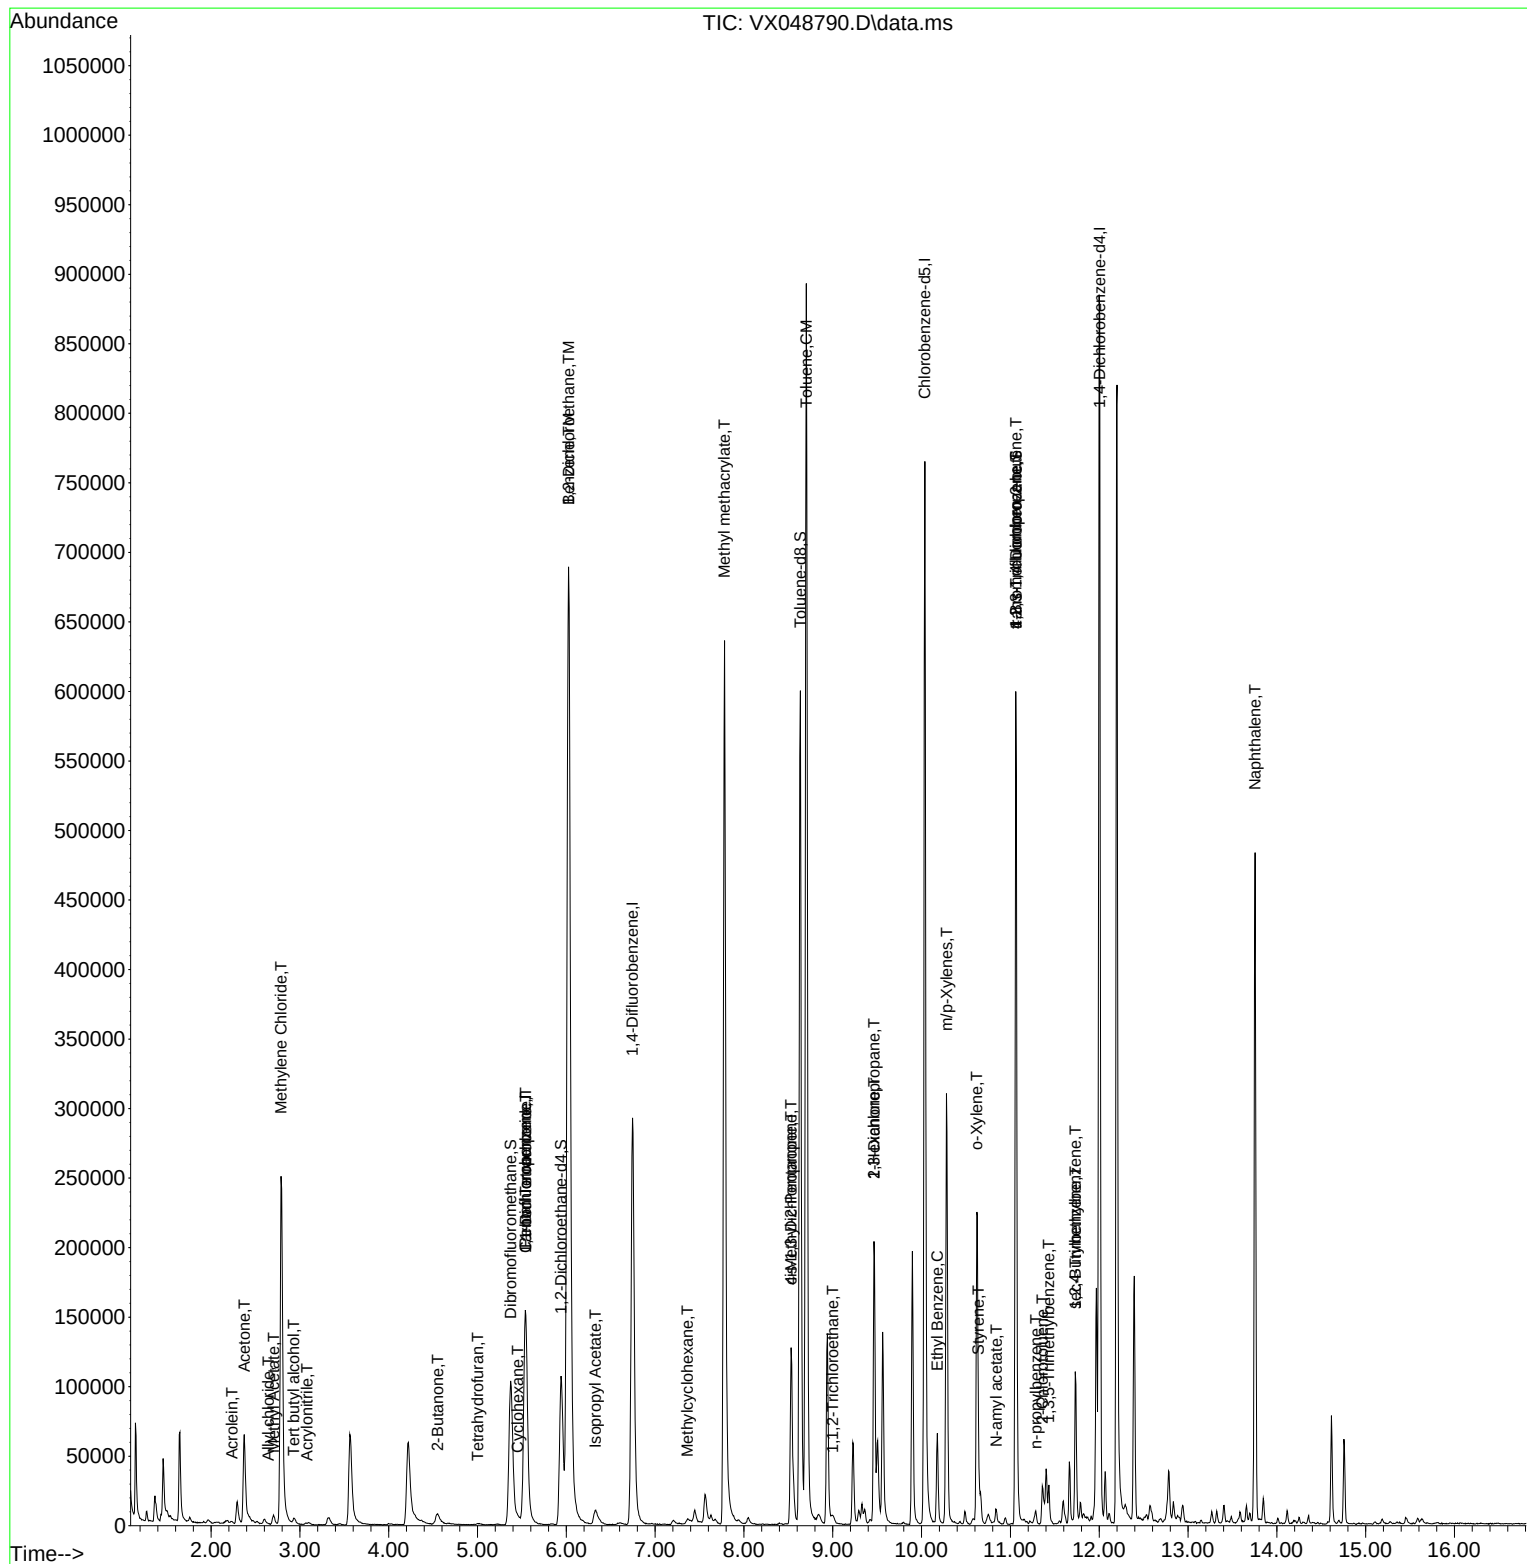



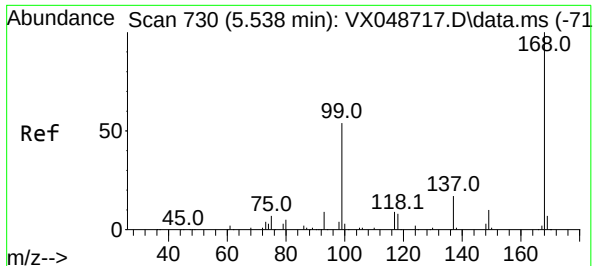


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Instrument :
MSVOA_X
ClientSampleId :



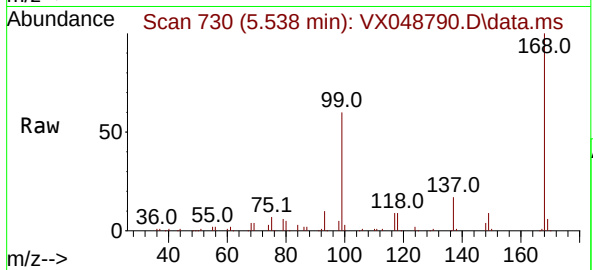



Tgt Ion:168 Resp: 165845
Ion Ratio Lower Upper
168 100
99 59.9 44.2 66.4

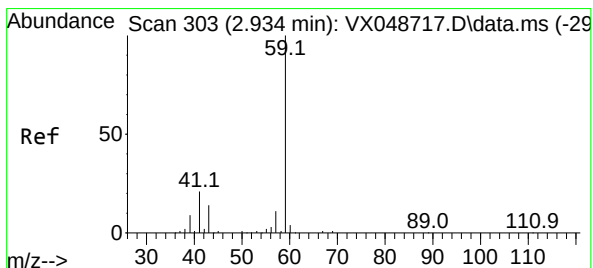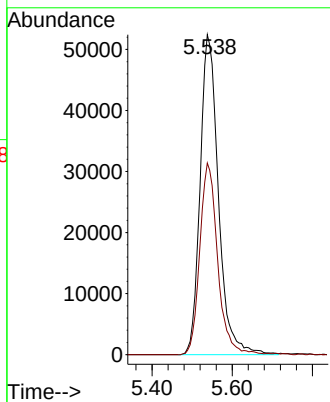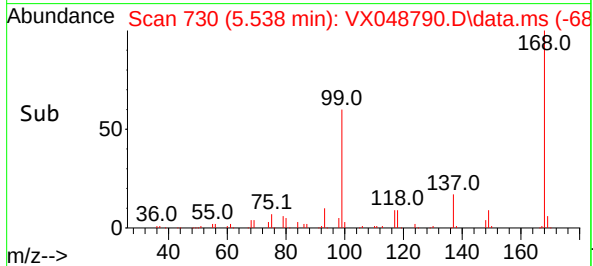

#11
Tert butyl alcohol
Concen: 14.400 ug/l
RT: 2.928 min Scan# 302
Delta R.T. -0.006 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11


Tgt Ion: 59 Resp: 5175
Ion Ratio Lower Upper
59 100
57 9.8 8.1 12.1

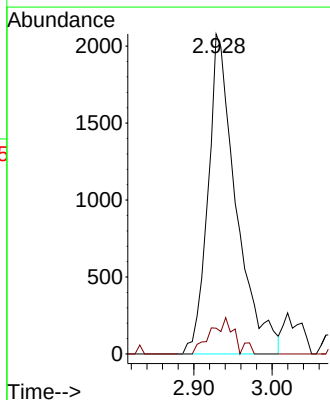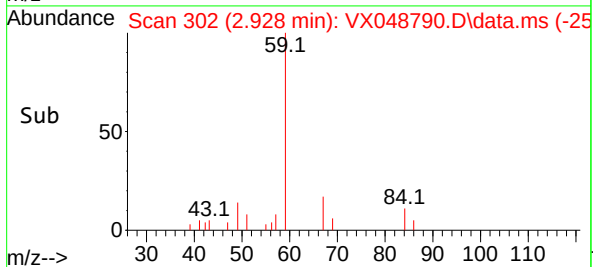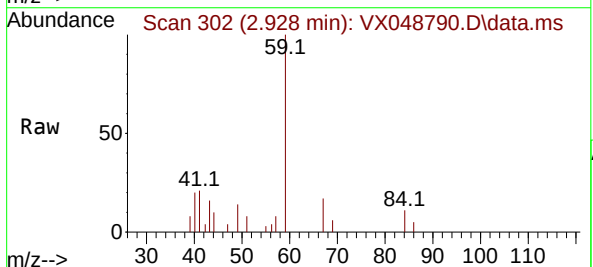






#13
Acrolein
Concen: 42.398 ug/l
RT: 2.233 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 56 Resp: 918
Ion Ratio Lower Upper
56 100
55 101.3 55.8 83.6#

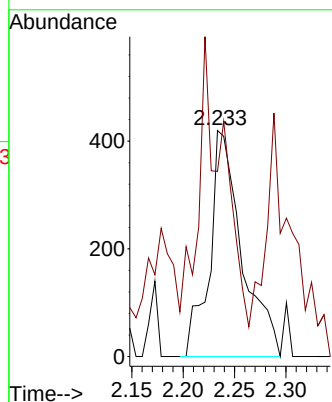


#14
Allyl chloride
Concen: 0.260 ug/l
RT: 2.642 min Scan# 255
Delta R.T. -0.024 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11



Tgt Ion: 41 Resp: 842
Ion Ratio Lower Upper
41 100
39 0.0 49.8 74.6#
76 0.0 27.3 40.9#





#15

Acrylonitrile

Concen: 1.088 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.024 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 53 Resp: 1218

Ion Ratio Lower Upper

53 100

52 33.2 66.3 99.5#

51 0.0 28.7 43.1#

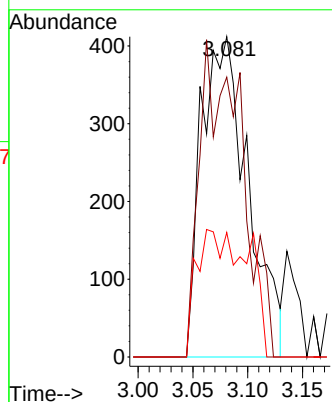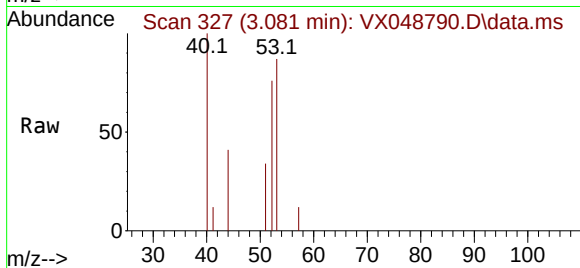

#16

Acetone

Concen: 99.506 ug/l

RT: 2.374 min Scan# 211

Delta R.T. 0.000 min

Lab File: VX048790.D




Acq: 09 Dec 2025 17:11


Tgt Ion: 43 Resp: 84793

Ion Ratio Lower Upper

43 100

58 31.3 25.0 37.4


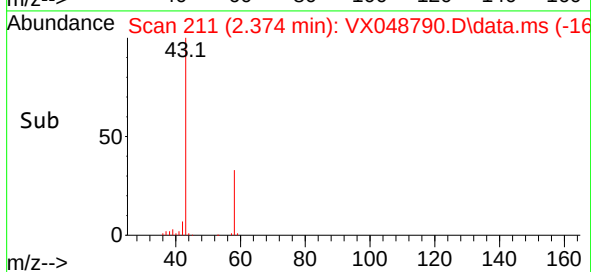
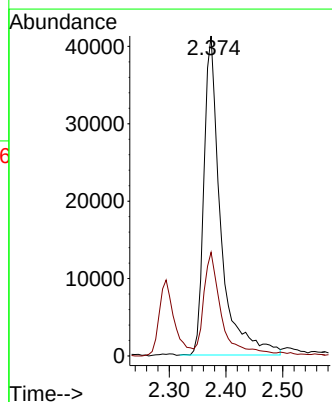
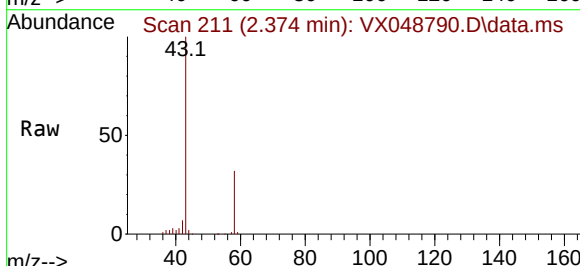




#18
Methyl Acetate
Concen: 3.830 ug/l
RT: 2.703 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 9183
Ion Ratio Lower Upper
43 100
74 24.7 19.2 28.8

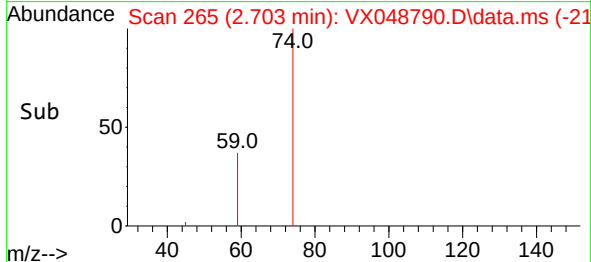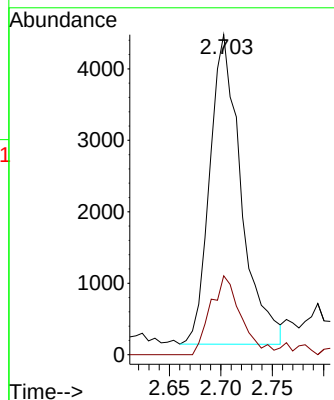

#20
Methylene Chloride
Concen: 61.541 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 84 Resp: 131079
Ion Ratio Lower Upper
84 100
49 120.8 98.7 148.1
51 36.3 29.4 44.2
86 62.0 52.5 78.7



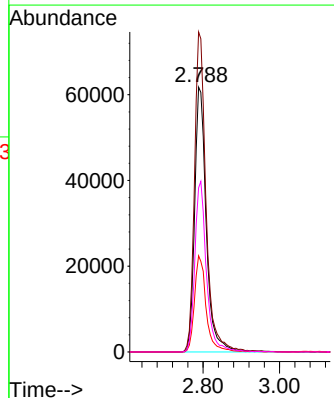
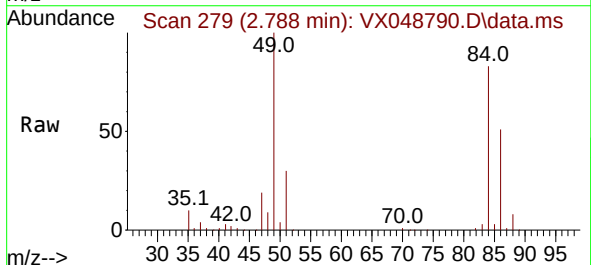




#25
2-Butanone
Concen: 11.259 ug/l
RT: 4.550 min Scan# 50
Delta R.T. 0.012 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 14160
Ion Ratio Lower Upper
43 100
72 27.0 22.6 34.0



#29
Tetrahydrofuran
Concen: 0.302 ug/l
RT: 5.001 min Scan# 642
Delta R.T. 0.018 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11


Tgt Ion: 42 Resp: 290
Ion Ratio Lower Upper
42 100
72 11.7 39.4 59.2#
71 45.2 35.8 53.6

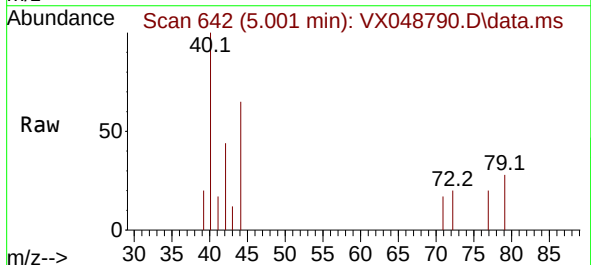






#31
Cyclohexane
Concen: 0.579 ug/l
RT: 5.452 min Scan# 716
Delta R.T. -0.012 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 1741
Ion Ratio Lower Upper
56 100
69 22.1 24.2 36.2#
84 54.9 72.1 108.1#

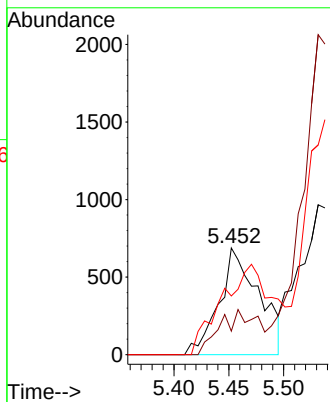

#33
1,2-Dichloroethane-d4
Concen: 52.294 ug/l
RT: 5.940 min Scan# 796
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 65 Resp: 116404
Ion Ratio Lower Upper
65 100
67 52.5 0.0 107.4


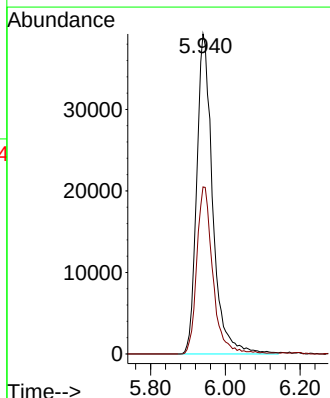






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 334402
Ion Ratio Lower Upper
114 100
63 19.8 0.0 39.0
88 15.9 0.0 31.8



#35
Dibromofluoromethane
Concen: 44.925 ug/l
RT: 5.373 min Scan# 703
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion:113 Resp: 103439
Ion Ratio Lower Upper
113 100
111 102.3 79.5 119.3
192 20.3 16.1 24.1





#36

1,1-Dichloropropene

Concen: 3.919 ug/l

RT: 5.544 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 75 Resp: 12359

Ion Ratio Lower Upper

75 100

110 5.4 18.6 55.8#

77 0.0 25.3 37.9#



#38

Carbon Tetrachloride

Concen: 4.547 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.122 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11




Tgt Ion: 117 Resp: 16244


Ion Ratio Lower Upper

117 100

119 5.2 80.5 120.7#

121 0.0 25.4 38.0#



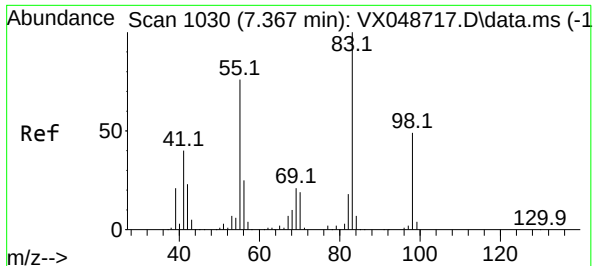

#39

Methylcyclohexane

Concen: 0.456 ug/l

RT: 7.361 min Scan# 1030

Delta R.T. -0.006 min

Lab File: VX048790.D





Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 83	Resp: 1702
Ion Ratio	Lower Upper
83 100	
55 53.6	60.6 90.8#
98 25.1	39.3 58.9#

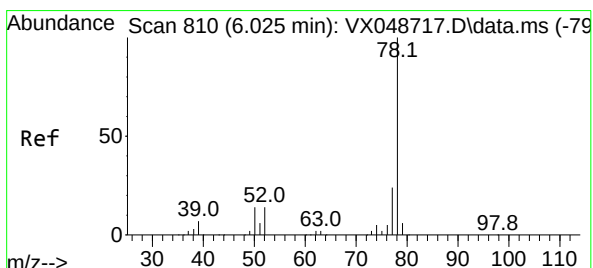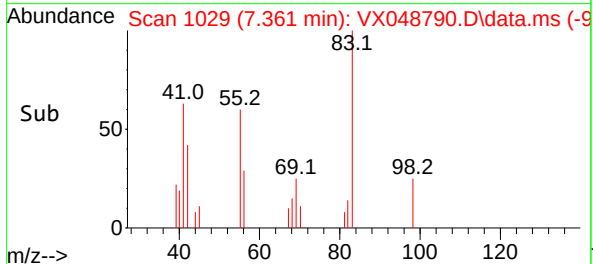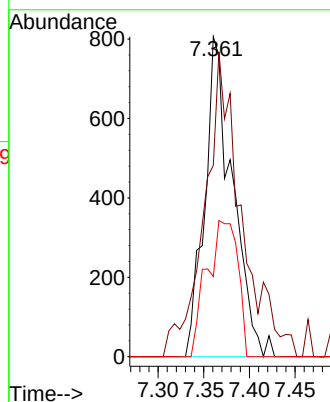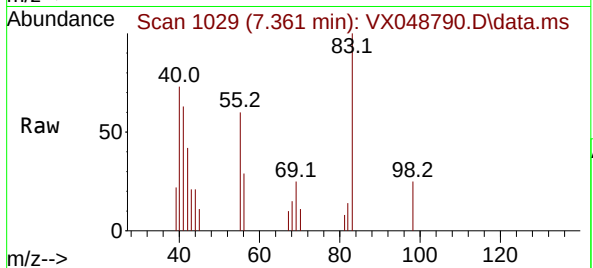

#40

Benzene

Concen: 99.917 ug/l




RT: 6.025 min Scan# 810


Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Tgt Ion: 78	Resp: 934094
Ion Ratio	Lower Upper
78 100	
77 23.3	18.8 28.2

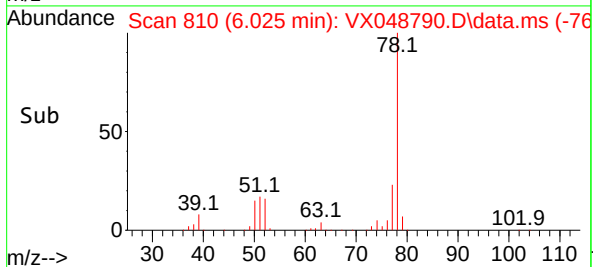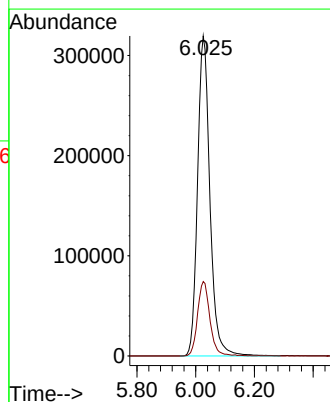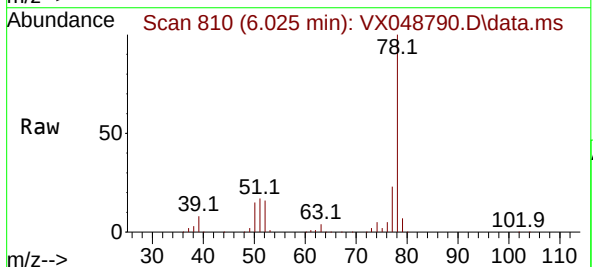



#42

1,2-Dichloroethane

Concen: 2.304 ug/l

RT: 6.025 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 7623

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2



#43

Isopropyl Acetate

Concen: 2.764 ug/l

RT: 6.324 min Scan# 859

Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11




Tgt Ion: 43 Resp: 15769


Ion Ratio Lower Upper

43 100

61 18.5 16.8 25.2

87 12.1 11.8 17.6





#48

Methyl methacrylate

Concen: 20.085 ug/l

RT: 7.781 min Scan# 1098

Delta R.T. 0.104 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 41 Resp: 57650

Ion Ratio Lower Upper

41 100

69 0.1 68.5 102.7#

39 49.3 43.5 65.3



#50

Toluene-d8

Concen: 46.235 ug/l

RT: 8.635 min Scan# 1238

Delta R.T. 0.000 min

Lab File: VX048790.D




Acq: 09 Dec 2025 17:11


Tgt Ion: 98 Resp: 373157

Ion Ratio Lower Upper

98 100

100 66.1 53.4 80.0




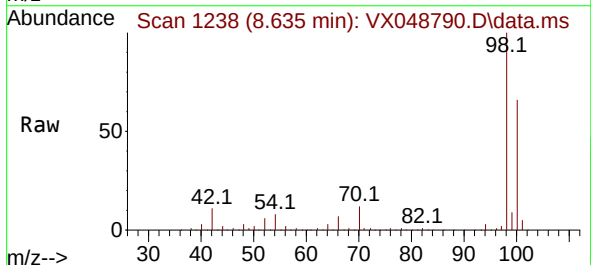




#51
4-Methyl-2-Pentanone
Concen: 15.964 ug/l
RT: 8.531 min Scan# 1221
Delta R.T. -0.024 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 56540
Ion Ratio Lower Upper
43 100
58 0.0 32.2 48.4#



#52
Toluene
Concen: 62.415 ug/l
RT: 8.702 min Scan# 1249
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 92 Resp: 351856
Ion Ratio Lower Upper
92 100
91 170.8 136.3 204.5







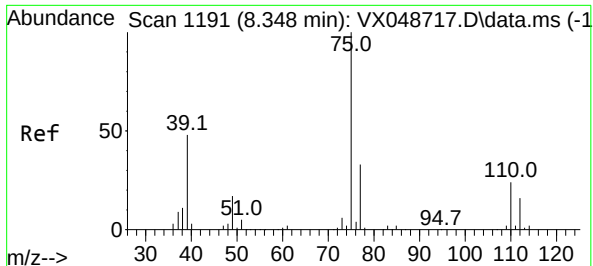

#54
 cis-1,3-Dichloropropene
 Concen: 5.816 ug/l
 RT: 8.531 min Scan# 1191
 Delta R.T. 0.183 min
 Lab File: VX048790.D
 Acq: 09 Dec 2025 17:11




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 21967
 Ion Ratio Lower Upper
 75 100
 77 0.5 26.1 39.1#
 39 23.9 38.2 57.4#

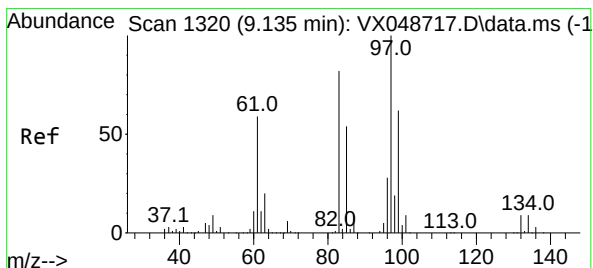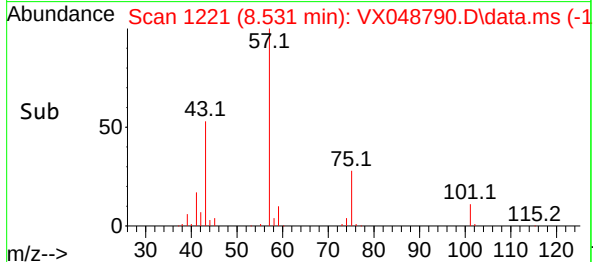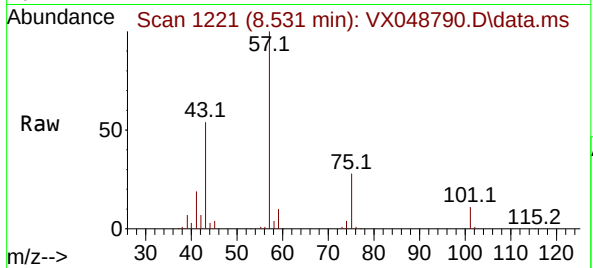

#55
 1,1,2-Trichloroethane
 Concen: 1.077 ug/l
 RT: 9.000 min Scan# 1298
 Delta R.T. -0.134 min
 Lab File: VX048790.D
 Acq: 09 Dec 2025 17:11

Tgt Ion: 97 Resp: 2444
 Ion Ratio Lower Upper
 97 100
 83 0.0 66.0 99.0#
 85 0.0 43.2 64.8#
 99 3.8 50.0 75.0#

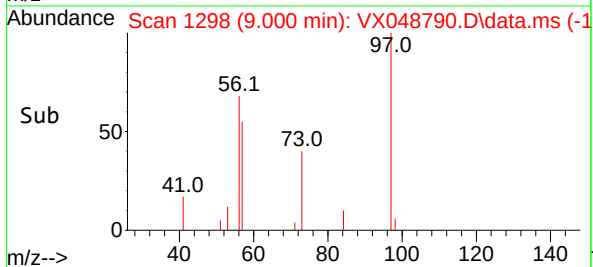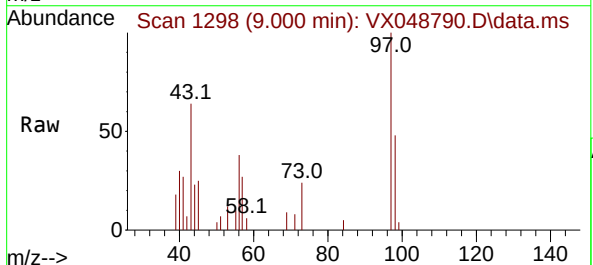



#57

1,3-Dichloropropane

Concen: 0.486 ug/l

RT: 9.464 min Scan# 1374

Delta R.T. 0.171 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 1832

Ion Ratio Lower Upper

76 100

78 0.0 26.0 39.0#

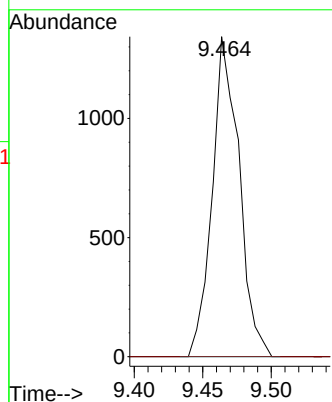

#59

2-Hexanone

Concen: 10.041 ug/l

RT: 9.464 min Scan# 1374

Delta R.T. 0.049 min

Lab File: VX048790.D




Acq: 09 Dec 2025 17:11


Tgt Ion: 43 Resp: 24964

Ion Ratio Lower Upper

43 100

58 16.3 27.8 83.4#



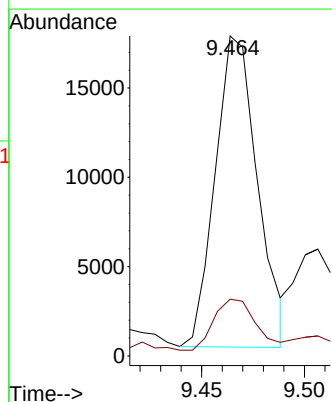





#62
4-Bromofluorobenzene
Concen: 60.669 ug/l
RT: 11.061 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 168849
Ion Ratio Lower Upper
95 100
174 79.9 0.0 157.8
176 77.9 0.0 154.0

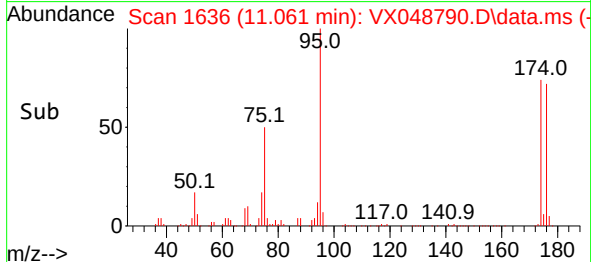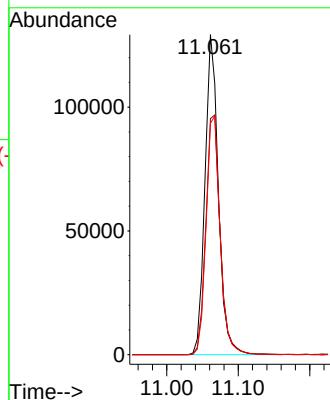

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 117 Resp: 356325
Ion Ratio Lower Upper
117 100
82 55.4 44.1 66.1
119 31.8 25.2 37.8

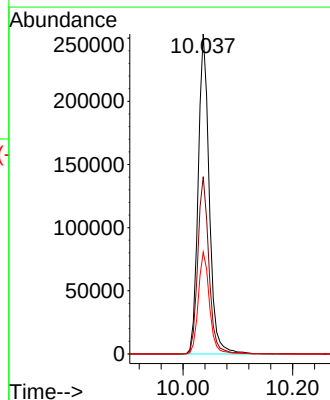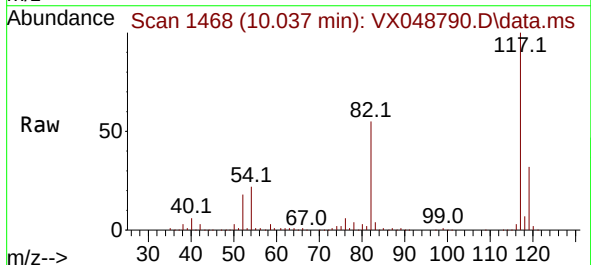



#67

Ethyl Benzene

Concen: 3.149 ug/l

RT: 10.177 min Scan# 1491

Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 40078

Ion Ratio Lower Upper

91 100

106 30.1 25.3 37.9



#68

m/p-Xylenes

Concen: 15.467 ug/l

RT: 10.281 min Scan# 1508

Delta R.T. 0.000 min

Lab File: VX048790.D




Acq: 09 Dec 2025 17:11


Tgt Ion:106 Resp: 76681

Ion Ratio Lower Upper

106 100

91 203.3 164.2 246.4





#69

o-Xylene

Concen: 10.114 ug/l

RT: 10.622 min Scan# 1564

Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 46986

Ion Ratio Lower Upper

106 100

91 215.4 108.1 324.3

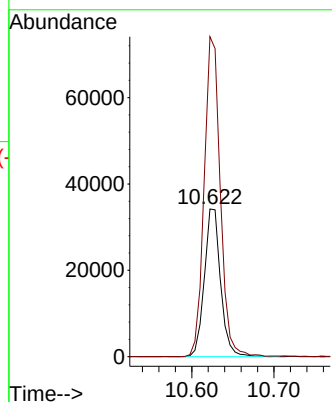

#70

Styrene

Concen: 2.056 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11




Tgt Ion:104 Resp: 16395


Ion Ratio Lower Upper

104 100

78 75.6 40.6 60.8#


103 75.7 43.4 65.2#

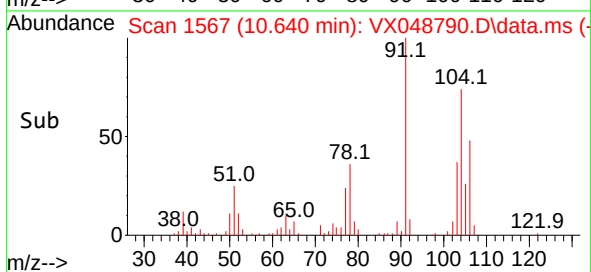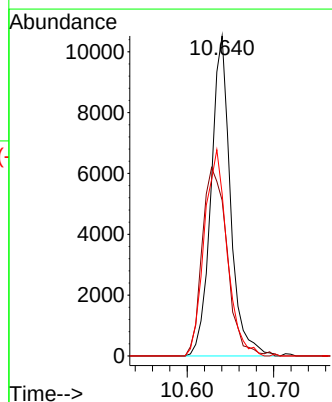






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.006 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX048790.D
 Acq: 09 Dec 2025 17:11


Instrument :
 MSVOA_X
 ClientSampleId :

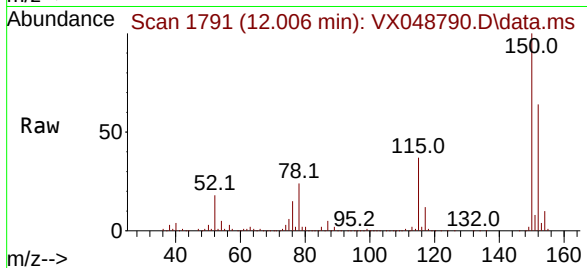



Tgt Ion:152 Resp: 195561
 Ion Ratio Lower Upper
 152 100
 115 59.0 42.1 126.4
 150 157.4 0.0 347.8

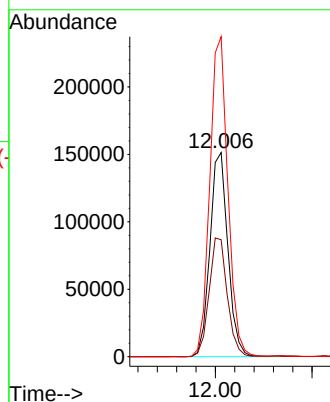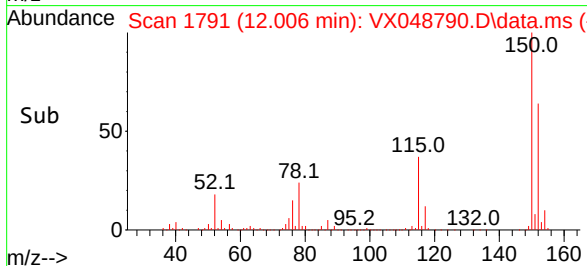


#74
 N-ethyl acetate
 Concen: 0.263 ug/l
 RT: 10.842 min Scan# 1600
 Delta R.T. 0.018 min
 Lab File: VX048790.D
 Acq: 09 Dec 2025 17:11

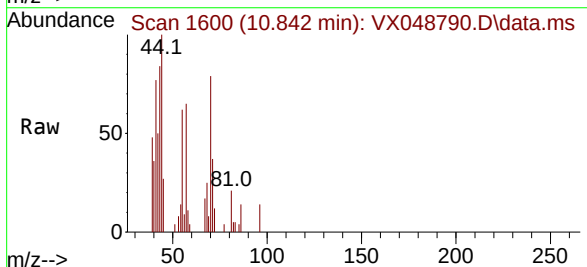

Tgt Ion: 43 Resp: 1507
 Ion Ratio Lower Upper
 43 100
 70 129.1 33.9 50.9#
 55 97.1 19.1 28.7#
 61 0.0 19.0 28.6#



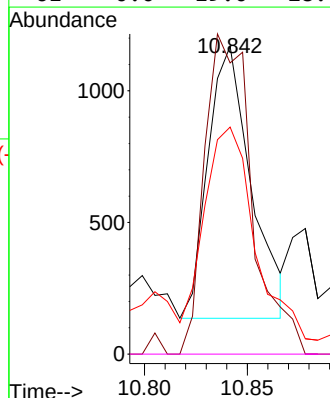
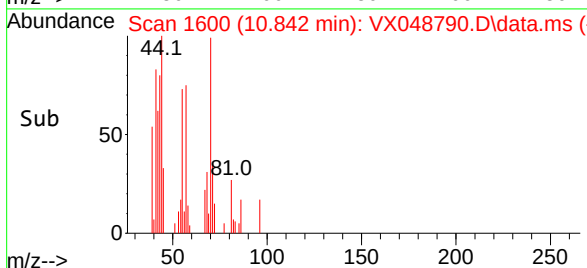




#76
1,2,3-Trichloropropane
Concen: 23.105 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.158 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 84158
Ion Ratio Lower Upper
75 100
77 1.4 24.3 73.0#

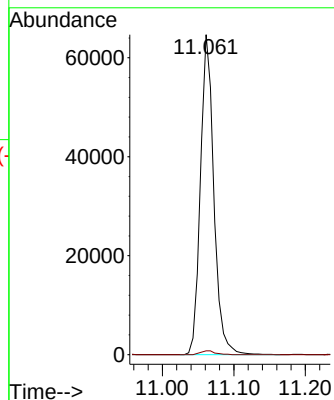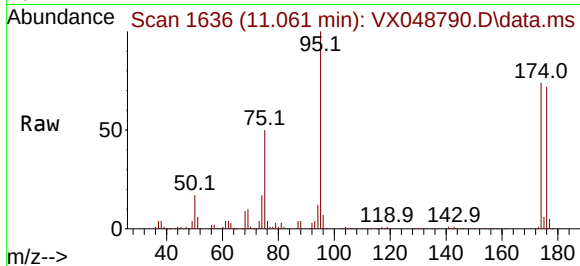

#78
n-propylbenzene
Concen: 0.275 ug/l
RT: 11.287 min Scan# 1673
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 91 Resp: 4197
Ion Ratio Lower Upper
91 100
120 23.8 11.4 34.2



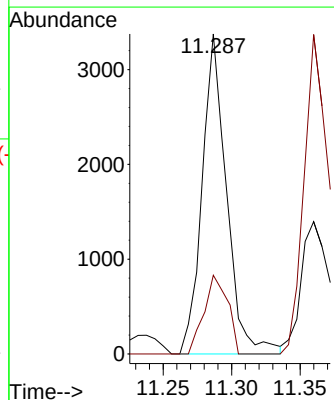
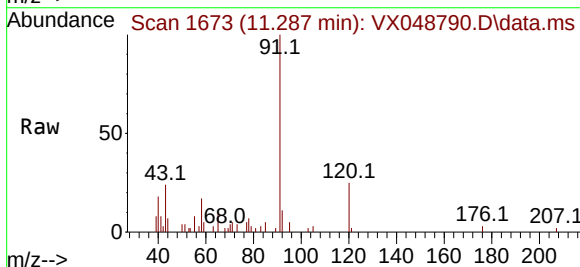




#79
2-Chlorotoluene
Concen: 0.264 ug/l
RT: 11.360 min Scan# 1685
Delta R.T. 0.012 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 2458
Ion Ratio Lower Upper
91 100
126 12.7 16.8 50.3#



#80
1,3,5-Trimethylbenzene
Concen: 1.083 ug/l
RT: 11.433 min Scan# 1697
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion:105 Resp: 11734
Ion Ratio Lower Upper
105 100
120 49.1 24.4 73.2









#81
trans-1,4-Dichloro-2-butene
Concen: 54.884 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 84158
Ion Ratio Lower Upper
75 100
53 0.0 79.9 119.9#
89 0.0 67.1 100.7#

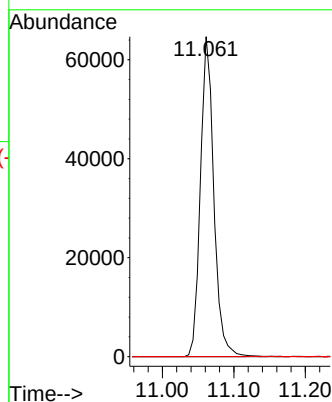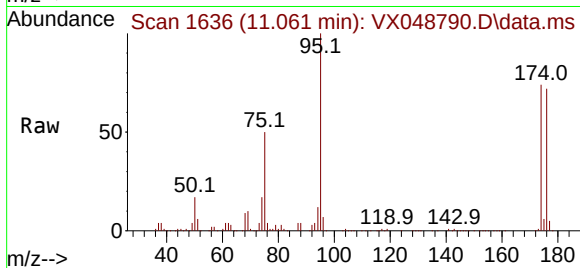

#84
1,2,4-Trimethylbenzene
Concen: 4.028 ug/l
RT: 11.732 min Scan# 1746
Delta R.T. 0.000 min
Lab File: VX048790.D
Acq: 09 Dec 2025 17:11

Tgt Ion: 105 Resp: 44016
Ion Ratio Lower Upper
105 100
120 30.2 22.3 66.8

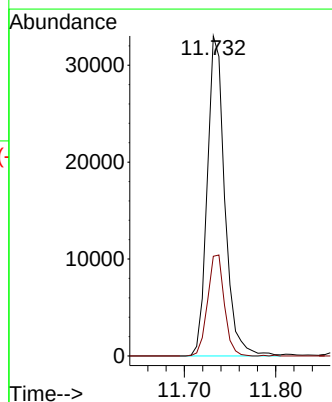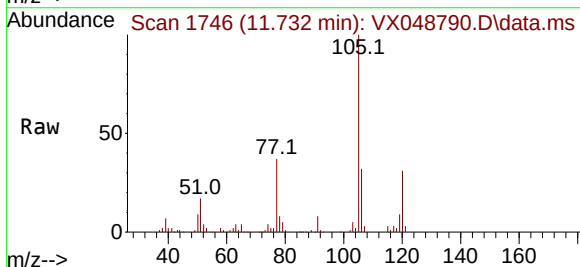



#85

sec-Butylbenzene

Concen: 3.227 ug/l

RT: 11.732 min Scan# 1

Delta R.T. -0.140 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 44016

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.5#



#95

Naphthalene

Concen: 27.036 ug/l

RT: 13.756 min Scan# 2078

Delta R.T. 0.000 min

Lab File: VX048790.D

Acq: 09 Dec 2025 17:11

Tgt Ion:128 Resp: 295930

Ion Ratio Lower Upper

128 100

127 12.7 10.2 15.2

129 10.9 8.6 13.0

