

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121018\
 Data File : VX006403.D
 Acq On : 11 Dec 2018 06:52
 Operator : JC/MD
 Sample : J6314-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPS1-TT-MW313S-20181206

Quant Time: Dec 11 07:56:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	687458	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1095651	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	1002269	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	471134	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	366651	52.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.50%	
35) Dibromofluoromethane	5.51	113	337713	47.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.22%	
50) Toluene-d8	8.71	98	1288460	49.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.86%	
62) 4-Bromofluorobenzene	11.13	95	480539	49.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.84%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121018\
Data File : VX006403.D
Acq On : 11 Dec 2018 06:52
Operator : JC/MD
Sample : J6314-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW313S-20181206

Quant Time: Dec 11 07:56:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

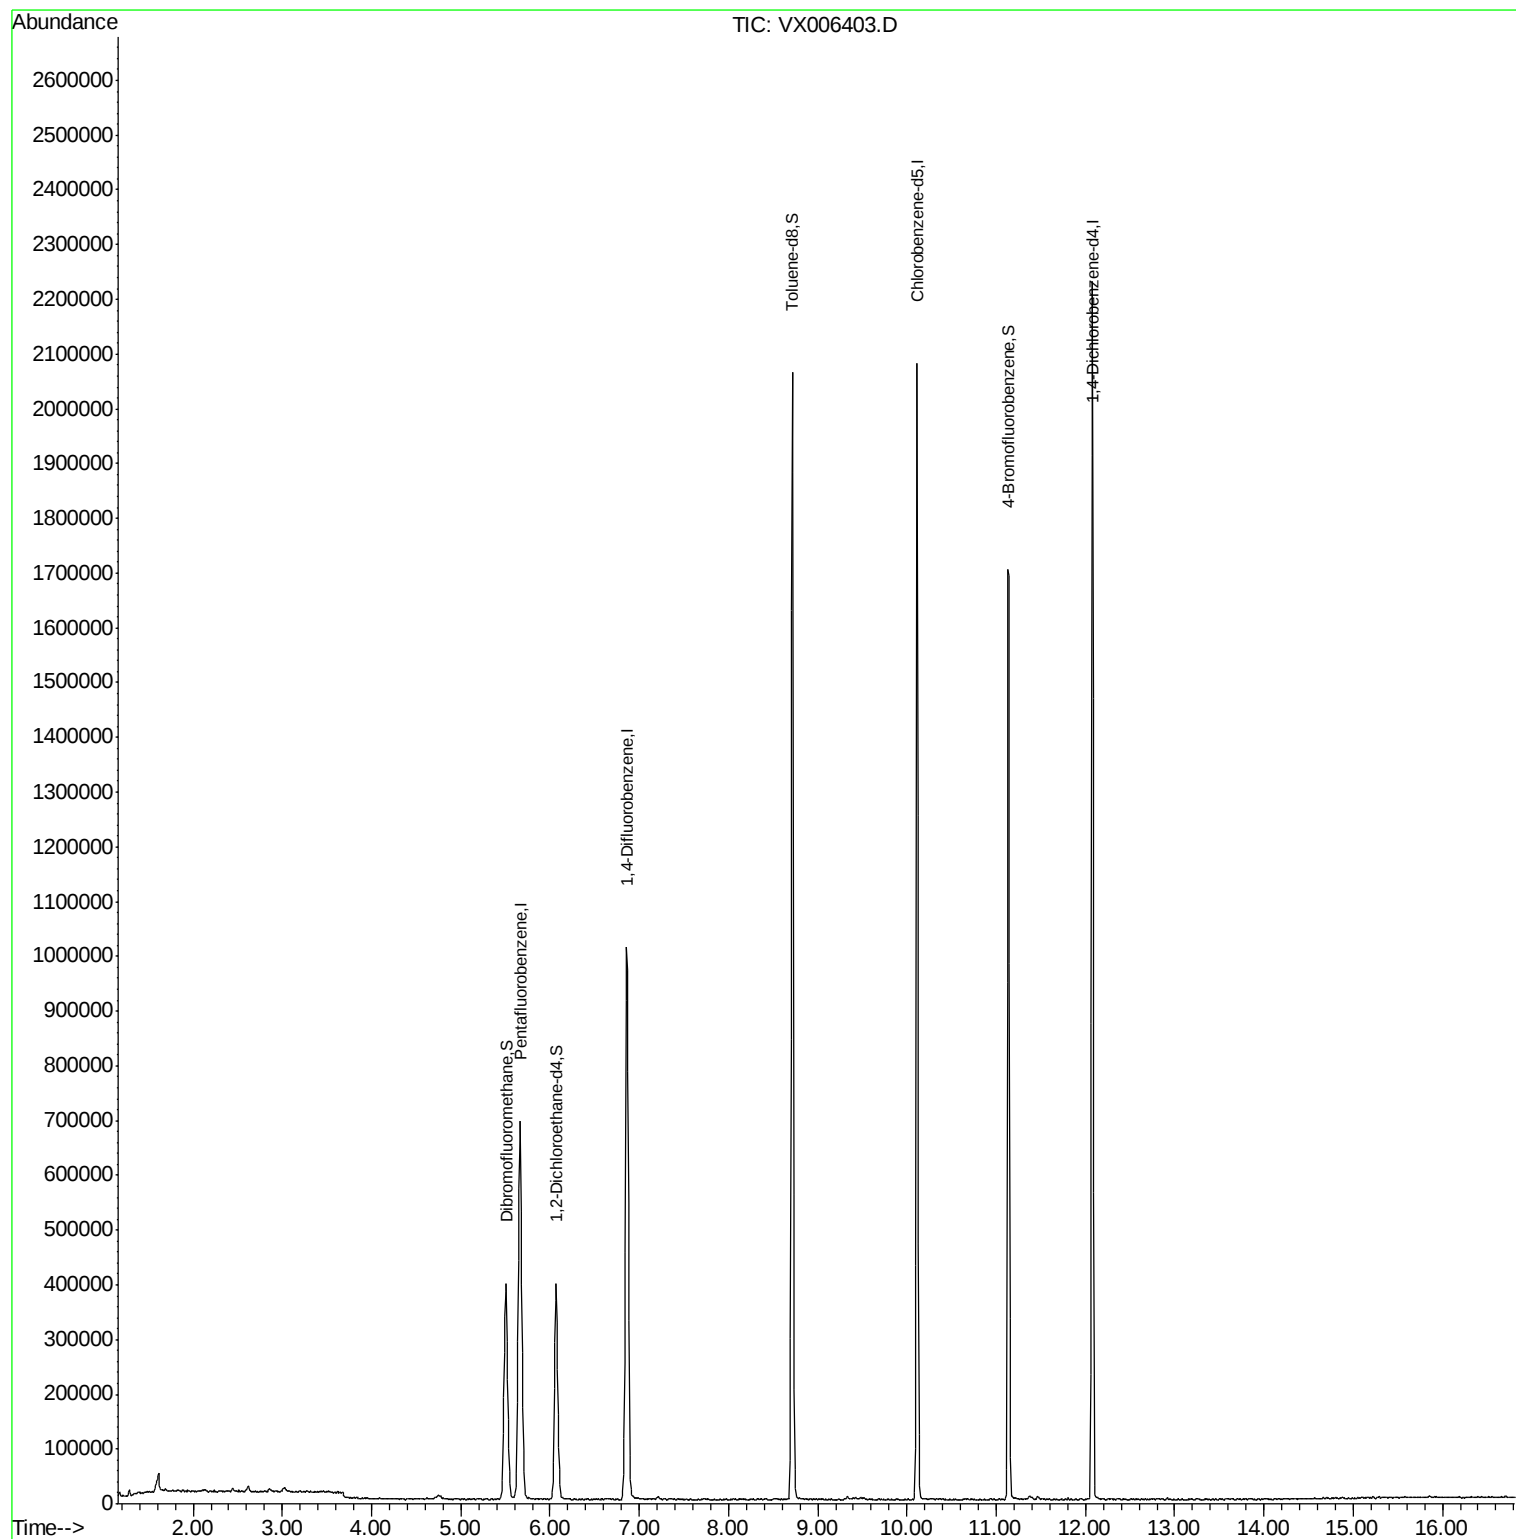

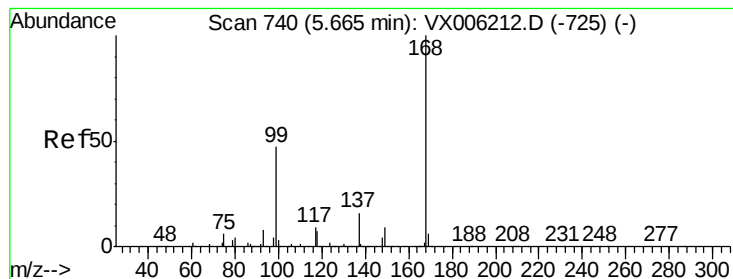

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52

Instrument :

MSVOA_X

ClientSampleId :


BPS1-TT-MW313S-20181206

Tot Ion:168 Resp: 687458

Ion Ratio Lower Upper

168 100

99 55.3 37.8 56.8

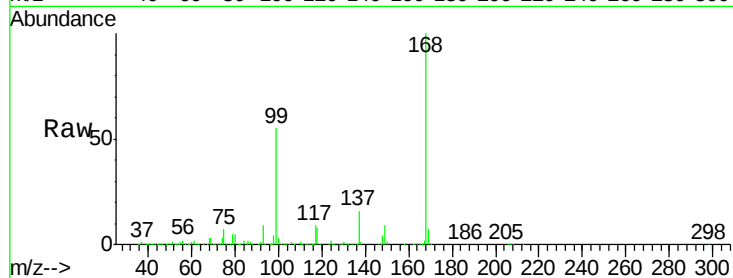

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

250000

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

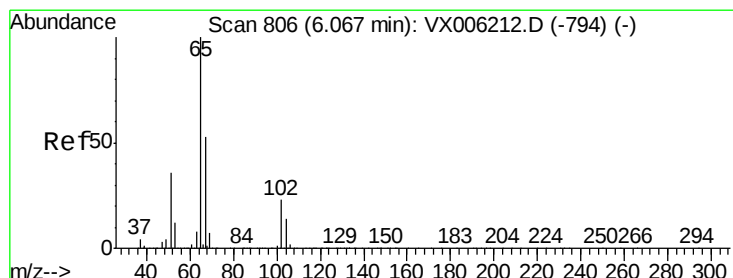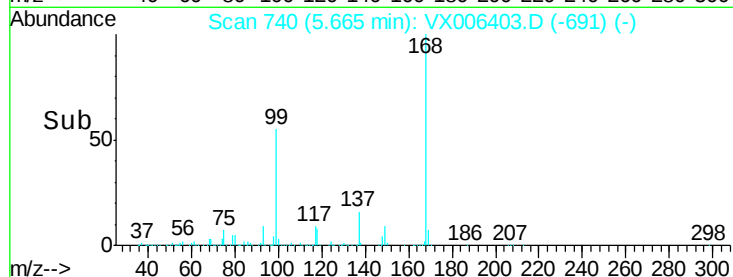

#33

1,2-Dichloroethane-d4

Concen: 52.246 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006403.D


Acq: 11 Dec 2018 06:52

Tgt Ion: 65 Resp: 366651

Ion Ratio Lower Upper

65 100

67 54.1 0.0 107.2

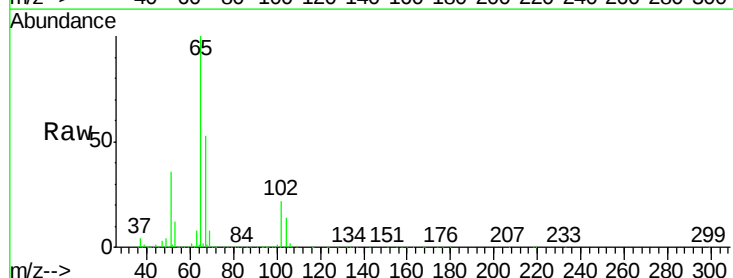

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

150000


100000


50000

0

Time-->

6.00 6.10

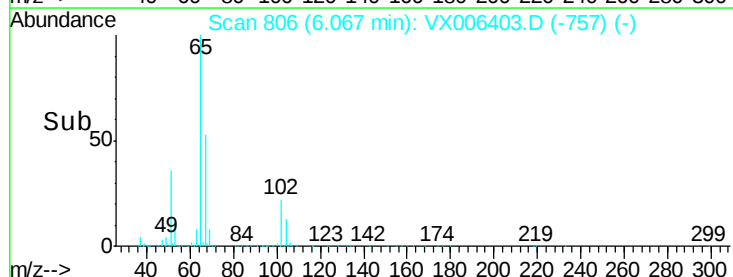

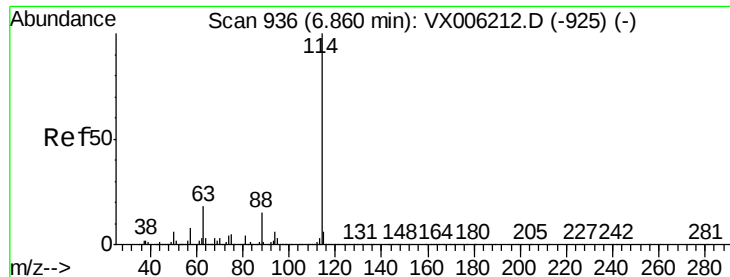

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52

Instrument :

MSVOA_X

ClientSampleId :

BPS1-TT-MW313S-20181206


Tot Ion:114 Resp: 1095651

Ion Ratio Lower Upper

114 100

63 17.6 0.0 36.6




88 15.4 0.0 29.0

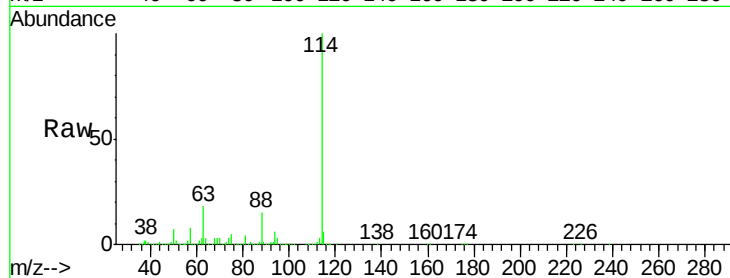

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

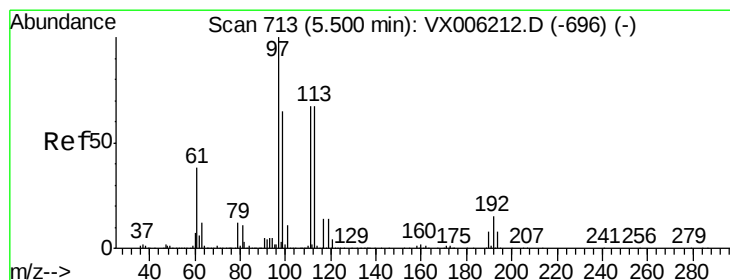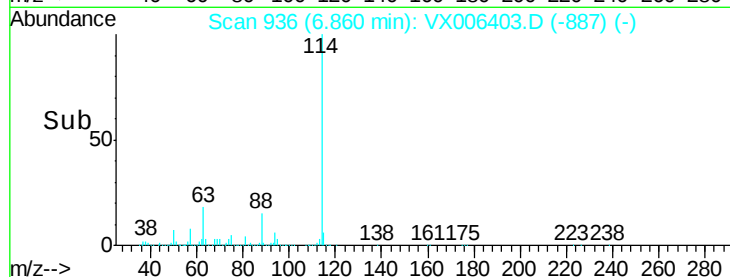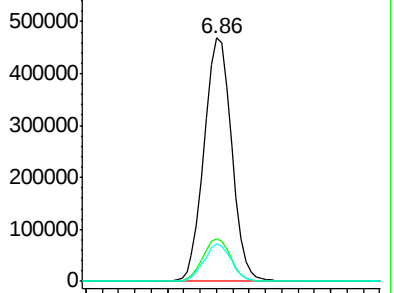

#35

Dibromofluoromethane

Concen: 47.606 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52


Tgt Ion:113 Resp: 337713

Ion Ratio Lower Upper

113 100

111 101.6 81.1 121.7



192 20.5 18.2 27.2

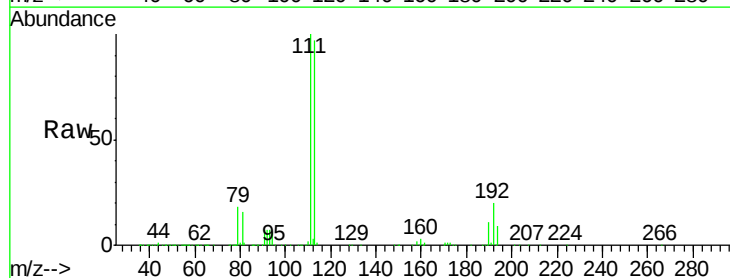


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

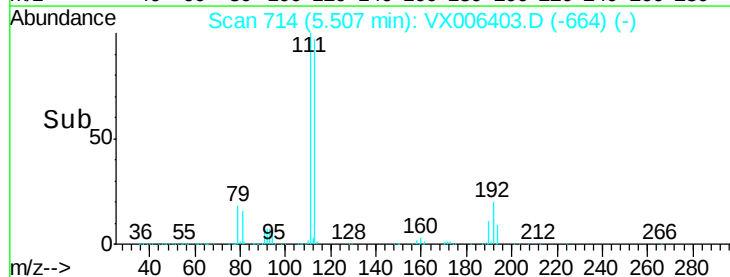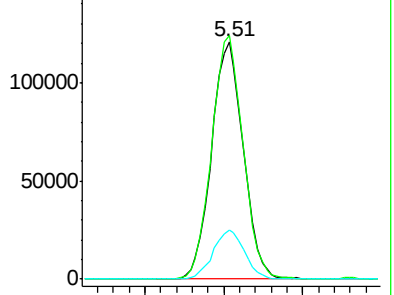

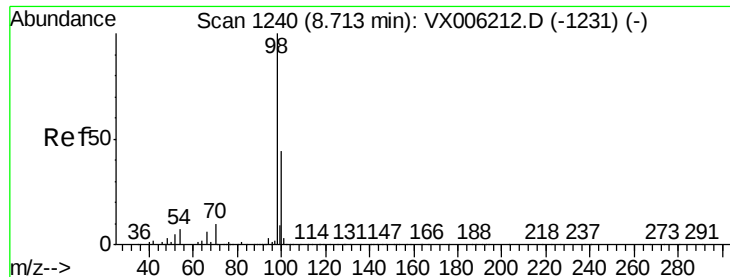

#50

Toluene-d8

Concen: 49.933 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52

Instrument :

MSVOA_X

ClientSampleId :





BPS1-TT-MW313S-20181206

Tot Ion: 98 Resp: 1288460

Ion Ratio Lower Upper

98 100

100 64.5 52.2 78.2

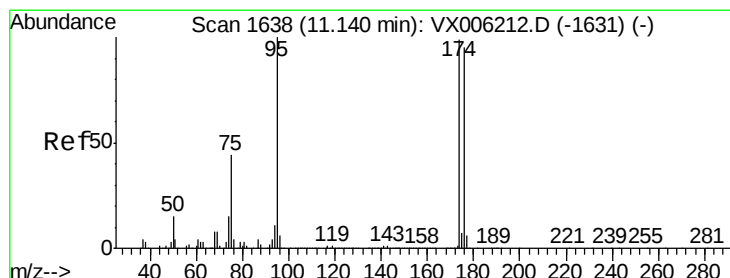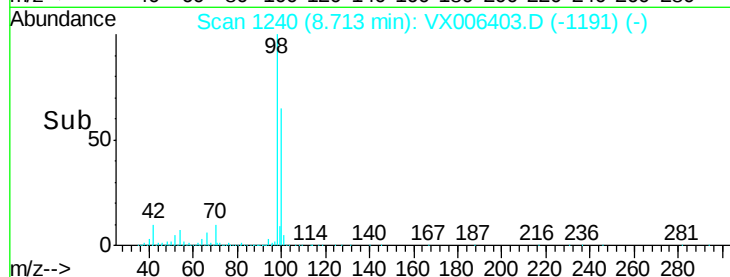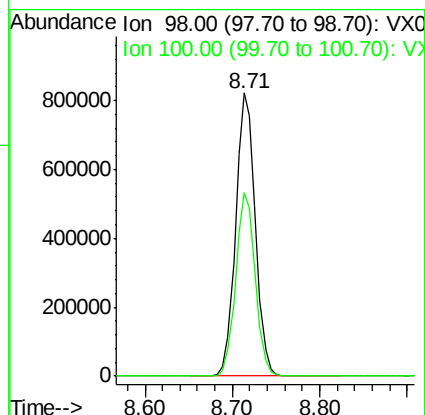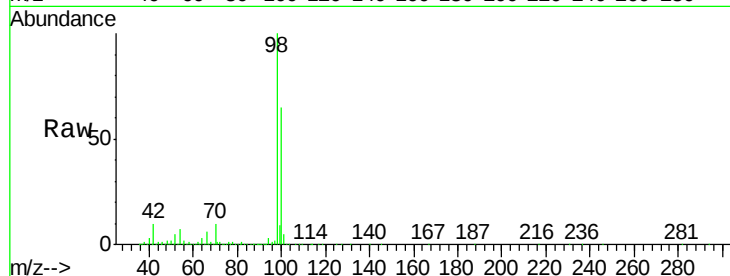

#62

4-Bromofluorobenzene

Concen: 49.420 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52




Tgt Ion: 95 Resp: 480539


Ion Ratio Lower Upper

95 100

174 83.6 0.0 187.0

176 81.4 0.0 181.8

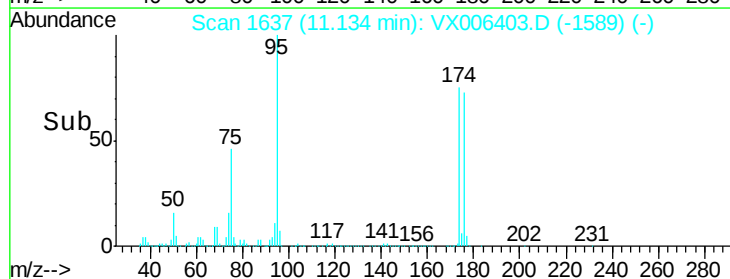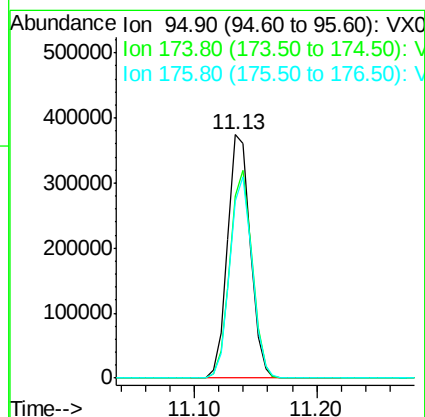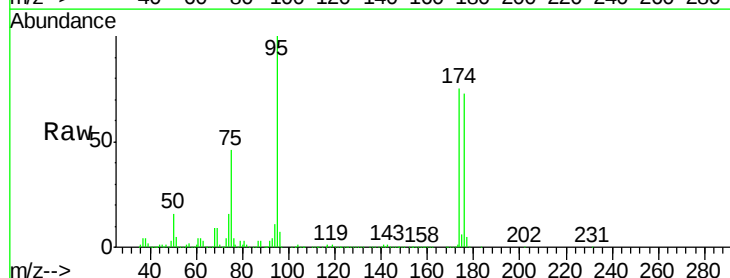

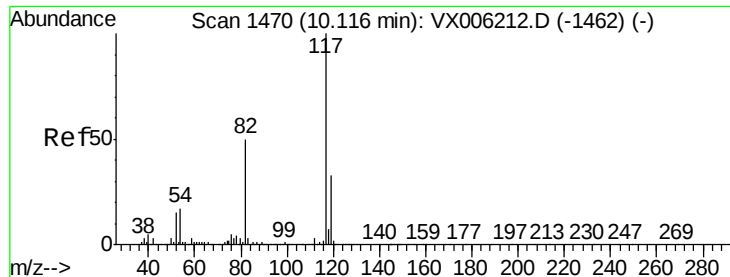

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52

Instrument :

MSVOA_X

ClientSampleId :

BPS1-TT-MW313S-20181206


Tot Ion:117 Resp: 1002269

Ion Ratio Lower Upper

117 100

82 51.5 39.6 59.4




119 32.2 26.3 39.5

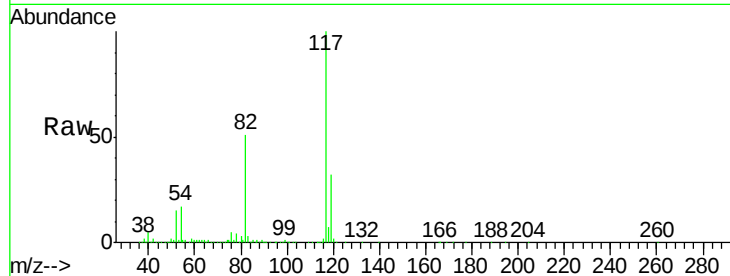

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

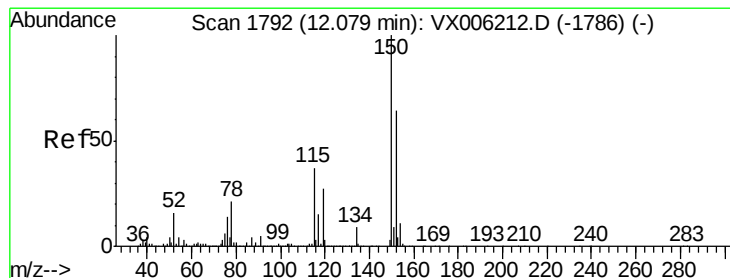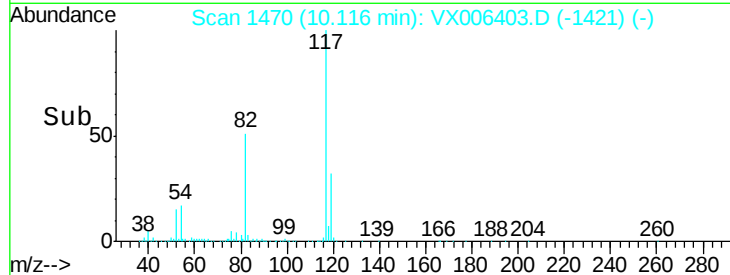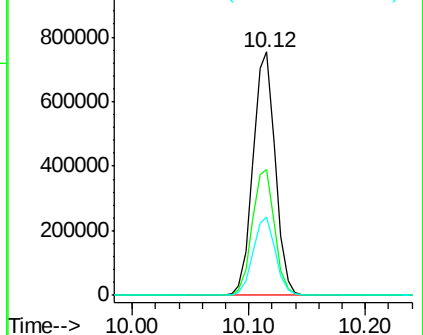

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX006403.D

Acq: 11 Dec 2018 06:52


Tgt Ion:152 Resp: 471134

Ion Ratio Lower Upper

152 100

115 57.5 39.0 116.9

150 157.8 0.0 345.8

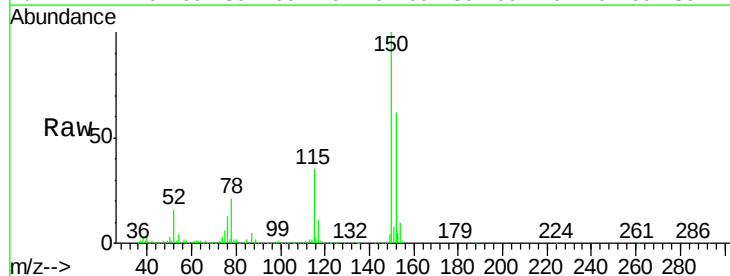

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

