


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121018\
Data File : VX006385.D
Acq On : 10 Dec 2018 22:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

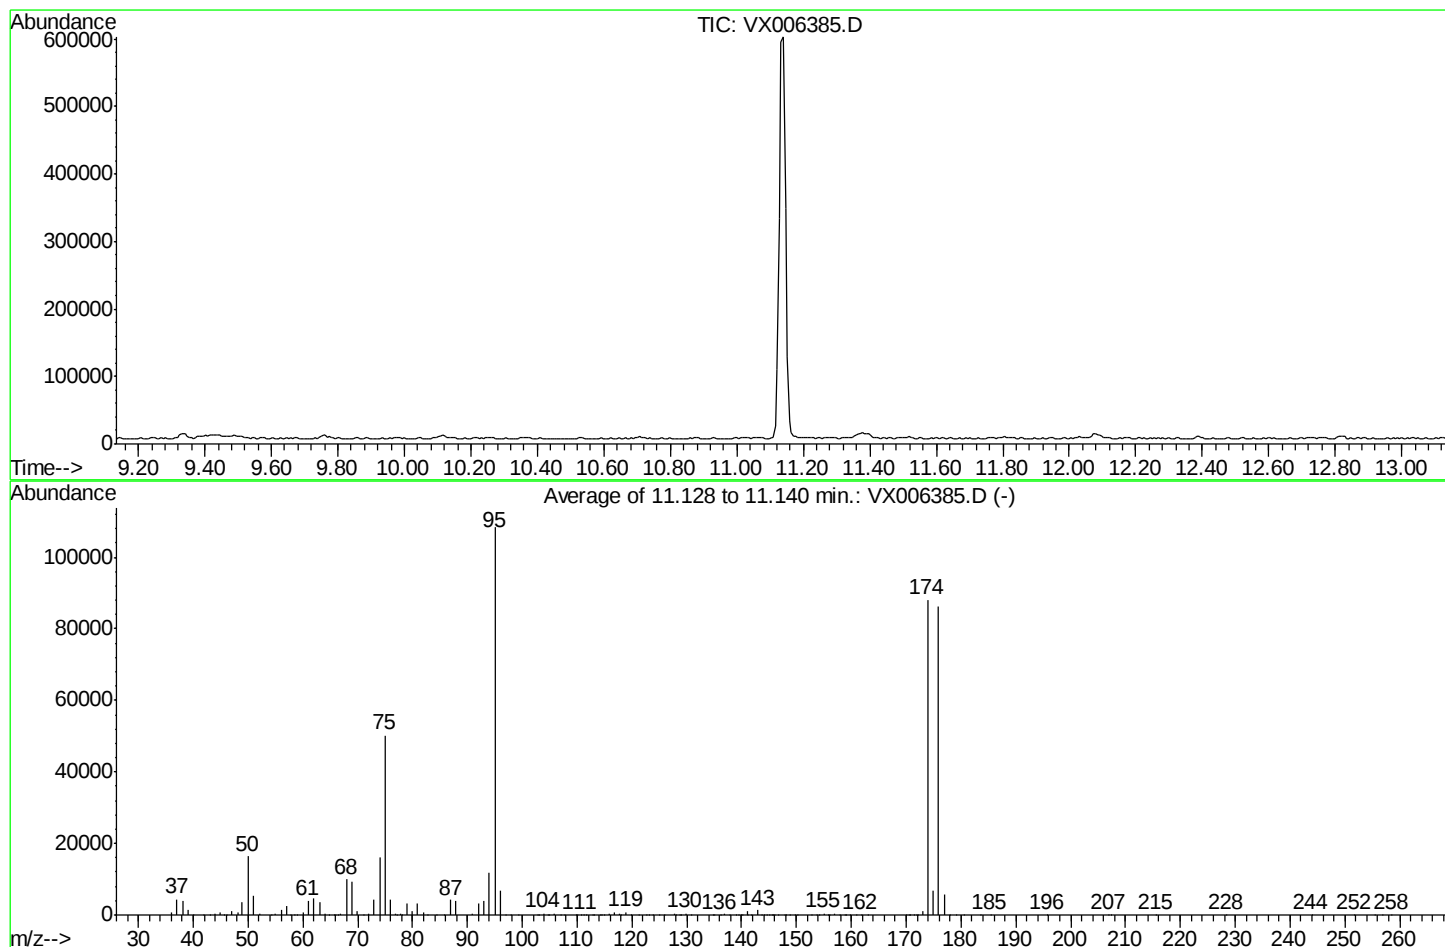

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	16381	PASS
75	95	30	60	46.3	50131	PASS
95	95	100	100	100.0	108360	PASS
96	95	5	9	6.4	6943	PASS
173	174	0.00	2	1.1	965	PASS
174	95	50	100	81.3	88112	PASS
175	174	5	9	7.8	6881	PASS
176	174	95	101	97.9	86277	PASS
177	176	5	9	6.8	5849	PASS