

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121020\
 Data File : VX019839.D
 Acq On : 10 Dec 2020 20:55
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Quant Time: Dec 11 02:45:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	258251	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	423846	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	399087	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	198154	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	164777	48.55	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.10%	
35) Dibromofluoromethane		5.46	113	133035	48.57	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.14%	
50) Toluene-d8		8.70	98	508905	48.66	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.32%	
62) 4-Bromofluorobenzene		11.12	95	193442	48.60	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.20%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.18	85	121423	51.355	ug/l	99
3) Chloromethane	1.31	50	135630	48.776	ug/l	100
4) Vinyl Chloride	1.39	62	153195	52.250	ug/l	99
5) Bromomethane	1.62	94	47305	48.591	ug/l	98
6) Chloroethane	1.70	64	101372	57.556	ug/l	98
7) Trichlorofluoromethane	1.91	101	217036	53.153	ug/l	98
8) Diethyl Ether	2.17	74	91637	52.959	ug/l	98
9) 1,1,2-Trichlorotrifluoroet	2.36	101	130514	55.765	ug/l	99
10) Methyl Iodide	2.49	142	161144	46.711	ug/l	100
11) Tert butyl alcohol	3.02	59	188061	269.715	ug/l	99
12) 1,1-Dichloroethene	2.36	96	127662	53.954	ug/l	99
13) Acrolein	2.27	56	85348	227.806	ug/l	98
14) Allyl chloride	2.70	41	209224	52.356	ug/l	99
15) Acrylonitrile	3.11	53	429188	279.708	ug/l	99
16) Acetone	2.42	43	333641	261.518	ug/l	98
17) Carbon Disulfide	2.55	76	317595	46.779	ug/l	100
18) Methyl Acetate	2.75	43	182052	58.313	ug/l	100
19) Methyl tert-butyl Ether	3.17	73	472716	54.858	ug/l	99
20) Methylene Chloride	2.83	84	158545	54.564	ug/l	99
21) trans-1,2-Dichloroethene	3.14	96	145702	52.818	ug/l	98
22) Diisopropyl ether	3.82	45	454339	56.232	ug/l	94
23) Vinyl Acetate	3.78	43	1933298	280.857	ug/l	100
24) 1,1-Dichloroethane	3.67	63	265007	54.390	ug/l	100
25) 2-Butanone	4.63	43	541122	276.030	ug/l	99
26) 2,2-Dichloropropane	4.55	77	202314	48.217	ug/l	100
27) cis-1,2-Dichloroethene	4.56	96	173081	53.615	ug/l	98
28) Bromochloromethane	4.98	49	119033	51.248	ug/l	100
29) Tetrahydrofuran	5.09	42	350968	277.875	ug/l	100
30) Chloroform	5.17	83	275499	54.991	ug/l	99
31) Cyclohexane	5.55	56	222072	52.598	ug/l	100
32) 1,1,1-Trichloroethane	5.46	97	232995	54.004	ug/l	100
36) 1,1-Dichloropropene	5.77	75	195617	51.075	ug/l	100
37) Ethyl Acetate	4.79	43	209632	54.210	ug/l	99
38) Carbon Tetrachloride	5.75	117	196187	52.309	ug/l	99

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121020\
 Data File : VX019839.D
 Acq On : 10 Dec 2020 20:55
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Quant Time: Dec 11 02:45:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) Methylcyclohexane	7.44	83	231176	51.375	ug/l	98
40) Benzene	6.11	78	619715	52.969	ug/l	100
41) Methacrylonitrile	5.00	41	116864	55.042	ug/l	99
42) 1,2-Dichloroethane	6.16	62	214331	53.618	ug/l	100
43) Isopropyl Acetate	6.41	43	335683	53.393	ug/l	100
44) Trichloroethene	7.19	130	156837	51.092	ug/l	99
45) 1,2-Dichloropropane	7.49	63	158091	54.066	ug/l	99
46) Dibromomethane	7.63	93	106473	53.920	ug/l	99
47) Bromodichloromethane	7.87	83	210433	53.705	ug/l	100
48) Methyl methacrylate	7.74	41	167958	54.320	ug/l	99
49) 1,4-Dioxane	7.71	88	80023	1068.352	ug/l	99
51) 4-Methyl-2-Pentanone	8.62	43	1074771	280.003	ug/l	100
52) Toluene	8.76	92	386086	52.763	ug/l	99
53) t-1,3-Dichloropropene	9.02	75	228992	52.664	ug/l	100
54) cis-1,3-Dichloropropene	8.41	75	250785	53.089	ug/l	98
55) 1,1,2-Trichloroethane	9.20	97	161813	54.874	ug/l	98
56) Ethyl methacrylate	9.16	69	246385	55.226	ug/l	99
57) 1,3-Dichloropropane	9.35	76	270608	53.744	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.29	63	663015	280.524	ug/l	100
59) 2-Hexanone	9.47	43	823000	276.612	ug/l	100
60) Dibromochloromethane	9.56	129	164859	55.027	ug/l	100
61) 1,2-Dibromoethane	9.65	107	167396	53.460	ug/l	100
64) Tetrachloroethene	9.32	164	138501	51.750	ug/l	97
65) Chlorobenzene	10.12	112	403208	50.712	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.20	131	154861	54.114	ug/l	99
67) Ethyl Benzene	10.23	91	734245	52.025	ug/l	100
68) m/p-Xylenes	10.34	106	551890	103.776	ug/l	100
69) o-Xylene	10.68	106	266740	52.141	ug/l	100
70) Styrene	10.70	104	463074	53.629	ug/l	100
71) Bromoform	10.84	173	117813	52.332	ug/l	97
73) Isopropylbenzene	11.00	105	712679	52.644	ug/l	100
74) N-amyl acetate	10.88	43	287980	53.082	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.25	83	258746	54.212	ug/l	99
76) 1,2,3-Trichloropropane	11.28	75	290529	65.372	ug/l	89
77) Bromobenzene	11.24	156	179277	51.747	ug/l	99
78) n-propylbenzene	11.34	91	819185	52.980	ug/l	99
79) 2-Chlorotoluene	11.40	91	495633	52.052	ug/l	100
80) 1,3,5-Trimethylbenzene	11.49	105	602363	52.721	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.05	75	80609	52.433	ug/l	98
82) 4-Chlorotoluene	11.49	91	584956	52.454	ug/l	99
83) tert-Butylbenzene	11.76	119	601795	53.705	ug/l	99
84) 1,2,4-Trimethylbenzene	11.79	105	618713	53.758	ug/l	99
85) sec-Butylbenzene	11.93	105	695283	54.346	ug/l	100
86) p-Isopropyltoluene	12.05	119	633554	54.034	ug/l	100
87) 1,3-Dichlorobenzene	12.01	146	322264	50.682	ug/l	99
88) 1,4-Dichlorobenzene	12.08	146	326598	50.429	ug/l	99
89) n-Butylbenzene	12.37	91	552064	53.144	ug/l	99
90) Hexachloroethane	12.58	117	107213	52.963	ug/l	98
91) 1,2-Dichlorobenzene	12.37	146	324519	52.354	ug/l	99
92) 1,2-Dibromo-3-Chloropropan	12.98	75	56308	54.878	ug/l	97


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121020\
Data File : VX019839.D
Acq On : 10 Dec 2020 20:55
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Quant Time: Dec 11 02:45:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 04 15:32:53 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	13.63	180	213027	52.795	ug/l	99
94) Hexachlorobutadiene	13.76	225	92684	51.393	ug/l	99
95) Naphthalene	13.82	128	724862	55.412	ug/l	100
96) 1,2,3-Trichlorobenzene	14.00	180	215920	54.756	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :


VSTDCCC050

Tgt Ion:168 Resp: 258251




Ion Ratio Lower Upper

168 100

99 57.0 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V



#2

Dichlorodifluoromethane

Concen: 51.355 ug/l

RT: 1.18 min Scan# 16

Delta R.T. -0.00 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 85 Resp: 121423



Ion Ratio Lower Upper


85 100

87 32.4 16.4 49.2



Abundance Ion 84.90 (84.60 to 85.60): VX0





#3

Chloromethane

Concen: 48.776 ug/l

RT: 1.31 min Scan# 37

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :





VSTDCCC050

Tgt Ion: 50 Resp: 135630

Ion Ratio Lower Upper

50 100

52 32.7 26.4 39.6



#4

Vinyl Chloride

Concen: 52.250 ug/l

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX019839.D




Acq: 10 Dec 2020 20:55


Tgt Ion: 62 Resp: 153195

Ion Ratio Lower Upper

62 100

64 32.5 25.7 38.5





#5

Bromomethane

Concen: 48.591 ug/l

RT: 1.62 min Scan# 88

Delta R.T. 0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :


VSTDCCC050

Tgt Ion: 94 Resp: 47305

Ion Ratio Lower Upper




94 100

96 93.2 76.4 114.6



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0



#6

Chloroethane

Concen: 57.556 ug/l

RT: 1.70 min Scan# 101

Delta R.T. -0.00 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 64 Resp: 101372

Ion Ratio Lower Upper



64 100


66 33.0 25.4 38.0



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0









#7

Trichlorofluoromethane
 Concen: 53.153 ug/l
 RT: 1.91 min Scan# 135
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050




Tgt Ion:101 Resp: 217036
 Ion Ratio Lower Upper
 101 100
 103 65.0 53.2 79.8




#8

Diethyl Ether
 Concen: 52.959 ug/l
 RT: 2.17 min Scan# 177
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 74 Resp: 91637
 Ion Ratio Lower Upper
 74 100
 45 90.6 44.5 133.5





#9

1,1,2-Trichlorotrifluoroethane

Concen: 55.765 ug/l

RT: 2.36 min Scan# 209

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:101 Resp: 130514

Ion Ratio Lower Upper

101 100

85 42.6 34.9 52.3




151 76.7 61.4 92.2



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V



#10

Methyl Iodide

Concen: 46.711 ug/l

RT: 2.49 min Scan# 230

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion:142 Resp: 161144

Ion Ratio Lower Upper

142 100

127 41.8 33.3 49.9



141 13.9 11.4 17.0




Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V









#11

Tert butyl alcohol
Concen: 269.715 ug/l
RT: 3.02 min Scan# 317
Delta R.T. 0.01 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050




Tgt Ion: 59 Resp: 188061
Ion Ratio Lower Upper
59 100
57 9.5 7.8 11.8




#12

1,1-Dichloroethene
Concen: 53.954 ug/l
RT: 2.36 min Scan# 208
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 96 Resp: 127662
Ion Ratio Lower Upper
96 100
61 155.4 124.6 187.0
98 64.2 50.6 76.0





#13

Acrolein

Concen: 227.806 ug/l

RT: 2.27 min Scan# 194

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :





VSTDCCC050

Tgt Ion: 56 Resp: 85348

Ion Ratio Lower Upper

56 100

55 69.3 56.4 84.6



#14

Allyl chloride

Concen: 52.356 ug/l

RT: 2.70 min Scan# 265

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55




Tgt Ion: 41 Resp: 209224


Ion Ratio Lower Upper

41 100

39 63.5 51.6 77.4

76 37.5 30.5 45.7





#15

Acrylonitrile

Concen: 279.708 ug/l

RT: 3.11 min Scan# 332

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050





Tgt Ion: 53 Resp: 429188

Ion Ratio Lower Upper

53 100

52 82.1 65.3 97.9

51 34.9 28.2 42.2



#16

Acetone

Concen: 261.518 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX019839.D




Acq: 10 Dec 2020 20:55


Tgt Ion: 43 Resp: 333641

Ion Ratio Lower Upper

43 100

58 33.9 27.8 41.8









#17
Carbon Disulfide
Concen: 46.779 ug/l
RT: 2.55 min Scan# 240
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 76 Resp: 317595
Ion Ratio Lower Upper
76 100
78 9.1 7.2 10.8



#18
Methyl Acetate
Concen: 58.313 ug/l
RT: 2.75 min Scan# 272
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 43 Resp: 182052
Ion Ratio Lower Upper
43 100
74 27.2 21.9 32.9









#19
Methyl tert-butyl Ether
Concen: 54.858 ug/l
RT: 3.17 min Scan# 341
Delta R.T. 0.01 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 73 Resp: 472716
Ion Ratio Lower Upper
73 100
57 21.7 17.1 25.7



#20
Methylene Chloride
Concen: 54.564 ug/l
RT: 2.83 min Scan# 286
Delta R.T. 0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 84 Resp: 158545
Ion Ratio Lower Upper
84 100
49 112.3 88.6 132.8
51 35.3 27.0 40.6
86 62.8 50.3 75.5





#21

trans-1,2-Dichloroethene

Concen: 52.818 ug/l

RT: 3.14 min Scan# 337

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 96 Resp: 145702

Ion Ratio Lower Upper

96 100

61 133.2 107.7 161.5




98 64.7 50.4 75.6



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0



#22

Diisopropyl ether

Concen: 56.232 ug/l

RT: 3.82 min Scan# 449

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Tgt Ion: 45 Resp: 454339


Ion Ratio Lower Upper

45 100

43 65.5 58.0 87.0

87 31.0 25.4 38.0

59 12.6 10.2 15.2






Abundance Ion 45.00 (44.70 to 45.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

Ion 59.00 (58.70 to 59.70): VX0





#23

Vinyl Acetate

Concen: 280.857 ug/l

RT: 3.78 min Scan# 442

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :


VSTDCCC050

Tgt Ion: 43 Resp: 1933298

Ion Ratio Lower Upper




43 100

86 12.3 9.9 14.9



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 86.00 (85.70 to 86.70): VX0



#24

1,1-Dichloroethane

Concen: 54.390 ug/l

RT: 3.67 min Scan# 423

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion: 63 Resp: 265007

Ion Ratio Lower Upper

63 100

98 7.5 3.8 11.2



100 4.8 2.5 7.5




Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

Ion 99.90 (99.60 to 100.60): VX0





#25

2-Butanone

Concen: 276.030 ug/l

RT: 4.63 min Scan# 581

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :


VSTDCCC050

Tgt Ion: 43 Resp: 541122

Ion Ratio Lower Upper




43 100

72 30.1 23.7 35.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0



#26

2,2-Dichloropropane

Concen: 48.217 ug/l

RT: 4.55 min Scan# 568

Delta R.T. 0.01 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 77 Resp: 202314

Ion Ratio Lower Upper



77 100


97 23.5 11.7 35.1



Abundance Ion 76.90 (76.60 to 77.60): VX0

Ion 96.90 (96.60 to 97.60): VX0









#27

cis-1,2-Dichloroethene
 Concen: 53.615 ug/l
 RT: 4.56 min Scan# 570
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050




Tgt Ion: 96 Resp: 173081
 Ion Ratio Lower Upper
 96 100
 61 140.1 0.0 285.6
 98 63.6 0.0 129.6




#28

Bromochloromethane
 Concen: 51.248 ug/l
 RT: 4.98 min Scan# 638
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 49 Resp: 119033
 Ion Ratio Lower Upper
 49 100
 129 1.1 0.0 4.0
 130 85.1 68.2 102.2





#29

Tetrahydrofuran

Concen: 277.875 ug/l

RT: 5.09 min Scan# 656

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 42 Resp: 350968

Ion Ratio Lower Upper

42 100

72 51.6 41.7 62.5




71 47.9 38.4 57.6



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0



#30

Chloroform

Concen: 54.991 ug/l

RT: 5.17 min Scan# 670

Delta R.T. -0.00 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 83 Resp: 275499

Ion Ratio Lower Upper



83 100


85 64.6 52.0 78.0



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0









#31
Cyclohexane
Concen: 52.598 ug/l
RT: 5.55 min Scan# 732
Delta R.T. 0.01 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 56 Resp: 222072
Ion Ratio Lower Upper
56 100
69 31.8 25.3 37.9
84 88.7 71.4 107.0



#32
1,1,1-Trichloroethane
Concen: 54.004 ug/l
RT: 5.46 min Scan# 717
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 97 Resp: 232995
Ion Ratio Lower Upper
97 100
99 64.6 51.5 77.3
61 42.7 34.2 51.4









#33
 1,2-Dichloroethane-d4
 Concen: 48.547 ug/l
 RT: 6.03 min Scan# 810
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion: 65 Resp: 164777
 Ion Ratio Lower Upper
 65 100
 67 53.0 0.0 105.4



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 114 Resp: 423846
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 40.8
 88 16.4 0.0 32.8





#35

Dibromofluoromethane

Concen: 48.566 ug/l

RT: 5.46 min Scan# 718

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:113 Resp: 133035

Ion Ratio Lower Upper

113 100

111 102.5 81.9 122.9




192 20.8 16.7 25.1



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



#36

1,1-Dichloropropene

Concen: 51.075 ug/l

RT: 5.77 min Scan# 768

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion: 75 Resp: 195617

Ion Ratio Lower Upper

75 100

110 36.1 18.1 54.4



77 31.4 25.3 37.9




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0









#37
 Ethyl Acetate
 Concen: 54.210 ug/l
 RT: 4.79 min Scan# 608
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Tgt Ion: 43 Resp: 209632
 Ion Ratio Lower Upper
 43 100
 61 15.3 12.8 19.2
 70 12.8 10.5 15.7




Abundance Ion 43.00 (42.70 to 43.70): VX0
 Ion 60.90 (60.60 to 61.60): VX0
 Ion 70.00 (69.70 to 70.70): VX0






#38
 Carbon Tetrachloride
 Concen: 52.309 ug/l
 RT: 5.75 min Scan# 765
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 117 Resp: 196187
 Ion Ratio Lower Upper
 117 100
 119 96.7 76.2 114.2
 121 31.6 24.8 37.2



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V





#39

Methylcyclohexane

Concen: 51.375 ug/l

RT: 7.44 min Scan# 1042

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 83 Resp: 231176

Ion Ratio Lower Upper

83 100

55 75.8 58.9 88.3




98 47.9 38.1 57.1



Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0



#40

Benzene

Concen: 52.969 ug/l

RT: 6.11 min Scan# 824

Delta R.T. 0.01 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 78 Resp: 619715

Ion Ratio Lower Upper



78 100


77 23.8 18.9 28.3



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0





#41

Methacrylonitrile

Concen: 55.042 ug/l

RT: 5.00 min Scan# 642

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 41 Resp: 116864


Ion Ratio Lower Upper

41 100

39 52.8 42.5 63.7

67 81.3 65.0 97.6

52 30.4 25.3 37.9






Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

Ion 67.00 (66.70 to 67.70): VX0

Ion 52.00 (51.70 to 52.70): VX0



#42

1,2-Dichloroethane

Concen: 53.618 ug/l

RT: 6.16 min Scan# 832

Delta R.T. 0.01 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 62 Resp: 214331

Ion Ratio Lower Upper



62 100


98 10.3 0.0 20.2



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 97.90 (97.60 to 98.60): VX0





#43

Isopropyl Acetate

Concen: 53.393 ug/l

RT: 6.41 min Scan# 873

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 43 Resp: 335683

Ion Ratio Lower Upper

43 100

61 22.8 18.2 27.4




87 15.3 12.5 18.7



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0



#44

Trichloroethene

Concen: 51.092 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. 0.01 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 130 Resp: 156837

Ion Ratio Lower Upper



130 100


95 97.6 0.0 198.0



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0





#45

1,2-Dichloropropane

Concen: 54.066 ug/l

RT: 7.49 min Scan# 1050

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :





VSTDCCC050

Tgt Ion: 63 Resp: 158091

Ion Ratio Lower Upper

63 100

65 31.3 25.7 38.5



#46

Dibromomethane

Concen: 53.920 ug/l

RT: 7.63 min Scan# 1074

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55




Tgt Ion: 93 Resp: 106473


Ion Ratio Lower Upper

93 100

95 83.1 66.8 100.2

174 103.1 83.1 124.7





#47

Bromodichloromethane

Concen: 53.705 ug/l

RT: 7.87 min Scan# 1113

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 83 Resp: 210433

Ion Ratio Lower Upper




83 100

85 64.2 51.4 77.0

127 8.7 6.8 10.2



Abundance Ion 82.90 (82.60 to 83.60): VX0
Ion 84.90 (84.60 to 85.60): VX0
Ion 126.80 (126.50 to 127.50): V



#48

Methyl methacrylate

Concen: 54.320 ug/l

RT: 7.74 min Scan# 1092

Delta R.T. 0.01 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion: 41 Resp: 167958

Ion Ratio Lower Upper



41 100


69 94.1 76.0 114.0

39 54.4 44.6 67.0



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0









#49
 1,4-Dioxane
 Concen: 1068.352 ug/l
 RT: 7.71 min Scan# 1087
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion: 88 Resp: 80023
 Ion Ratio Lower Upper
 88 100
 43 28.4 23.2 34.8
 58 69.2 55.0 82.4



#50
 Toluene-d8
 Concen: 48.663 ug/l
 RT: 8.70 min Scan# 1248
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 98 Resp: 508905
 Ion Ratio Lower Upper
 98 100
 100 66.3 51.9 77.9









#51
4-Methyl-2-Pentanone
Concen: 280.003 ug/l
RT: 8.62 min Scan# 1235
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 43 Resp: 1074771
Ion Ratio Lower Upper
43 100
58 44.1 35.4 53.0



#52
Toluene
Concen: 52.763 ug/l
RT: 8.76 min Scan# 1259
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 92 Resp: 386086
Ion Ratio Lower Upper
92 100
91 172.1 137.1 205.7









#53
 t-1,3-Dichloropropene
 Concen: 52.664 ug/l
 RT: 9.02 min Scan# 1301
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion: 75 Resp: 228992
 Ion Ratio Lower Upper
 75 100
 77 31.0 24.9 37.3



#54
 cis-1,3-Dichloropropene
 Concen: 53.089 ug/l
 RT: 8.41 min Scan# 1202
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 75 Resp: 250785
 Ion Ratio Lower Upper
 75 100
 77 31.8 25.7 38.5
 39 42.2 35.1 52.7









#55
 1,1,2-Trichloroethane
 Concen: 54.874 ug/l
 RT: 9.20 min Scan# 1330
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion:	97	Resp:	161813
Ion	Ratio	Lower	Upper
97	100		
83	84.5	69.3	103.9
85	54.1	44.3	66.5
99	63.9	50.3	75.5



#56
 Ethyl methacrylate
 Concen: 55.226 ug/l
 RT: 9.16 min Scan# 1324
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion:	69	Resp:	246385
Ion	Ratio	Lower	Upper
69	100		
41	58.0	46.8	70.2
39	30.3	24.7	37.1









#57
 1,3-Dichloropropane
 Concen: 53.744 ug/l
 RT: 9.35 min Scan# 1356
 Delta R.T. 0.01 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion: 76 Resp: 270608
 Ion Ratio Lower Upper
 76 100
 78 32.3 26.2 39.2



#58
 2-Chloroethyl Vinyl ether
 Concen: 280.524 ug/l
 RT: 8.29 min Scan# 1181
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion: 63 Resp: 663015
 Ion Ratio Lower Upper
 63 100
 106 29.5 23.5 35.3









#59
2-Hexanone
Concen: 276.612 ug/l
RT: 9.47 min Scan# 1375
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 43 Resp: 823000
Ion Ratio Lower Upper
43 100
58 61.5 30.9 92.8



#60
Dibromochloromethane
Concen: 55.027 ug/l
RT: 9.56 min Scan# 1390
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 129 Resp: 164859
Ion Ratio Lower Upper
129 100
127 76.6 38.4 115.2





#61

1,2-Dibromoethane

Concen: 53.460 ug/l

RT: 9.65 min Scan# 1405

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :


VSTDCCC050

Tgt Ion: 107 Resp: 167396

Ion Ratio Lower Upper




107 100

109 94.2 75.8 113.6



Abundance Ion 106.90 (106.60 to 107.60): V

Ion 108.80 (108.50 to 109.50): V



#62

4-Bromofluorobenzene

Concen: 48.599 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion: 95 Resp: 193442

Ion Ratio Lower Upper

95 100

174 78.0 0.0 154.6



176 77.1 0.0 155.8




Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.01 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion	Ratio	Lower	Upper
117	100		
82	53.2	47.4	71.2
119	31.5	26.6	39.8



#64
Tetrachloroethene
Concen: 51.750 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion	Ratio	Lower	Upper
164	100		
166	131.2	103.4	155.2
129	95.9	70.8	106.2
131	91.1	72.5	108.7









#65
Chlorobenzene
Concen: 50.712 ug/l
RT: 10.12 min Scan# 1482
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion:112 Resp: 403208
Ion Ratio Lower Upper
112 100
114 31.2 25.8 38.6



#66
1,1,1,2-Tetrachloroethane
Concen: 54.114 ug/l
RT: 10.20 min Scan# 1495
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion:131 Resp: 154861
Ion Ratio Lower Upper
131 100
133 93.7 47.7 143.1
119 64.5 32.1 96.5









#67
Ethyl Benzene
Concen: 52.025 ug/l
RT: 10.23 min Scan# 1500
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 91 Resp: 734245
Ion Ratio Lower Upper
91 100
106 30.6 24.6 37.0



#68
m/p-Xylenes
Concen: 103.776 ug/l
RT: 10.34 min Scan# 1518
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 106 Resp: 551890
Ion Ratio Lower Upper
106 100
91 203.3 162.8 244.2









#69
o-Xylene
Concen: 52.141 ug/l
RT: 10.68 min Scan# 1574
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion:106 Resp: 266740
Ion Ratio Lower Upper
106 100
91 216.3 108.1 324.2



#70
Styrene
Concen: 53.629 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion:104 Resp: 463074
Ion Ratio Lower Upper
104 100
78 49.7 40.0 60.0
103 54.1 43.4 65.0





#71

Bromoform

Concen: 52.332 ug/l

RT: 10.84 min Scan# 1600

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:173 Resp: 117813

Ion Ratio Lower Upper




173 100

175 49.7 23.9 71.8

254 0.1 0.1 0.1



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion:152 Resp: 198154

Ion Ratio Lower Upper



152 100


115 83.4 41.1 123.3

150 171.9 0.0 349.0



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V





#73

Isopropylbenzene

Concen: 52.644 ug/l

RT: 11.00 min Scan# 1626

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :





VSTDCCC050

Tgt Ion: 105 Resp: 712679

Ion Ratio Lower Upper

105 100

120 26.3 13.2 39.6



#74

N-ethyl acetate

Concen: 53.082 ug/l

RT: 10.88 min Scan# 1606

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Tgt Ion: 43 Resp: 287980




Ion Ratio Lower Upper


43 100

70 49.5 39.0 58.6

55 28.1 21.5 32.3

61 27.7 22.1 33.1





#75

1,1,2,2-Tetrachloroethane

Concen: 54.212 ug/l

RT: 11.25 min Scan# 1667

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion: 83 Resp: 258746

Ion Ratio Lower Upper

83 100

131 9.9 5.1 15.2




85 64.4 31.8 95.4



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 130.80 (130.50 to 131.50): VX0

Ion 84.90 (84.60 to 85.60): VX0



#76

1,2,3-Trichloropropane

Concen: 65.372 ug/l

RT: 11.28 min Scan# 1672

Delta R.T. -0.00 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 75 Resp: 290529

Ion Ratio Lower Upper



75 100


77 31.5 19.1 57.5



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0





#77

Bromobenzene

Concen: 51.747 ug/l

RT: 11.24 min Scan# 1665

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:156 Resp: 179277

Ion Ratio Lower Upper

156 100

77 166.7 82.8 248.6




158 97.0 49.1 147.4



Abundance Ion 155.80 (155.50 to 156.50): V

Ion 77.00 (76.70 to 77.70): VX0

Ion 157.80 (157.50 to 158.50): V



#78

n-propylbenzene

Concen: 52.980 ug/l

RT: 11.34 min Scan# 1682

Delta R.T. -0.00 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion: 91 Resp: 819185

Ion Ratio Lower Upper



91 100


120 22.6 11.5 34.5



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 120.00 (119.70 to 120.70): V









#79
2-Chlorotoluene
Concen: 52.052 ug/l
RT: 11.40 min Scan# 1692
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 91 Resp: 495633
Ion Ratio Lower Upper
91 100
126 33.2 16.6 49.8



#80
1,3,5-Trimethylbenzene
Concen: 52.721 ug/l
RT: 11.49 min Scan# 1706
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 105 Resp: 602363
Ion Ratio Lower Upper
105 100
120 49.9 23.8 71.5





#81

trans-1,4-Dichloro-2-butene

Concen: 52.433 ug/l

RT: 11.05 min Scan# 1635

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050





Tgt Ion: 75 Resp: 80609

Ion Ratio Lower Upper

75 100

53 92.5 74.5 111.7

89 44.7 37.9 56.9



#82

4-Chlorotoluene

Concen: 52.454 ug/l

RT: 11.49 min Scan# 1707

Delta R.T. -0.00 min

Lab File: VX019839.D




Acq: 10 Dec 2020 20:55


Tgt Ion: 91 Resp: 584956

Ion Ratio Lower Upper

91 100

126 29.2 14.9 44.5





#83

tert-Butylbenzene

Concen: 53.705 ug/l

RT: 11.76 min Scan# 1750

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:119 Resp: 601795

Ion Ratio Lower Upper

119 100

91 57.2 27.9 83.7




134 22.7 11.3 33.9



Abundance Ion 119.00 (118.70 to 119.70): V

Ion 91.00 (90.70 to 91.70): VX0

Ion 134.00 (133.70 to 134.70): V



#84

1,2,4-Trimethylbenzene

Concen: 53.758 ug/l

RT: 11.79 min Scan# 1755

Delta R.T. -0.01 min

Lab File: VX019839.D


Acq: 10 Dec 2020 20:55

Tgt Ion:105 Resp: 618713

Ion Ratio Lower Upper



105 100


120 44.4 22.4 67.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V









#85
 sec-Butylbenzene
 Concen: 54.346 ug/l
 RT: 11.93 min Scan# 1778
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion:105 Resp: 695283
 Ion Ratio Lower Upper
 105 100
 134 19.7 10.0 29.8



#86
 p-Isopropyltoluene
 Concen: 54.034 ug/l
 RT: 12.05 min Scan# 1798
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion:119 Resp: 633554
 Ion Ratio Lower Upper
 119 100
 134 26.0 12.9 38.7
 91 23.5 11.7 35.0





#87

1,3-Dichlorobenzene

Concen: 50.682 ug/l

RT: 12.01 min Scan# 1791

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:146 Resp: 322264

Ion Ratio Lower Upper

146 100

111 41.2 20.2 60.5




148 64.5 31.9 95.7



Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V



#88

1,4-Dichlorobenzene

Concen: 50.429 ug/l

RT: 12.08 min Scan# 1803

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion:146 Resp: 326598

Ion Ratio Lower Upper

146 100

111 39.8 19.6 58.8



148 64.4 31.6 95.0




Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V









#89
n-Butylbenzene
Concen: 53.144 ug/l
RT: 12.37 min Scan# 1851
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050


Tgt Ion: 91 Resp: 552064
Ion Ratio Lower Upper
91 100
92 54.3 27.4 82.0
134 25.8 13.2 39.5



#90
Hexachloroethane
Concen: 52.963 ug/l
RT: 12.58 min Scan# 1885
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion: 117 Resp: 107213
Ion Ratio Lower Upper
117 100
201 82.4 40.4 121.2





#91

1,2-Dichlorobenzene

Concen: 52.354 ug/l

RT: 12.37 min Scan# 1851

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55

Instrument :

MSVOA_X

ClientSampleId :

VSTDCCC050


Tgt Ion:146 Resp: 324519

Ion Ratio Lower Upper

146 100

111 41.8 20.8 62.2




148 64.2 31.9 95.5



Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V



#92

1,2-Dibromo-3-Chloropropane

Concen: 54.878 ug/l

RT: 12.98 min Scan# 1951

Delta R.T. -0.00 min

Lab File: VX019839.D

Acq: 10 Dec 2020 20:55


Tgt Ion: 75 Resp: 56308

Ion Ratio Lower Upper

75 100

155 88.7 45.3 135.9



157 111.0 57.7 173.1




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V









#93
 1,2,4-Trichlorobenzene
 Concen: 52.795 ug/l
 RT: 13.63 min Scan# 2057
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050


Tgt Ion:180 Resp: 213027
 Ion Ratio Lower Upper
 180 100
 182 95.9 47.7 143.1
 145 30.4 15.0 45.0



#94
 Hexachlorobutadiene
 Concen: 51.393 ug/l
 RT: 13.76 min Scan# 2079
 Delta R.T. -0.00 min
 Lab File: VX019839.D
 Acq: 10 Dec 2020 20:55

Tgt Ion:225 Resp: 92684
 Ion Ratio Lower Upper
 225 100
 223 62.0 31.1 93.2
 227 64.9 31.6 95.0









#95
Naphthalene
Concen: 55.412 ug/l
RT: 13.82 min Scan# 2088
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Tgt Ion:128 Resp: 724862
Ion Ratio Lower Upper
128 100
127 13.0 10.3 15.5
129 11.1 8.8 13.2

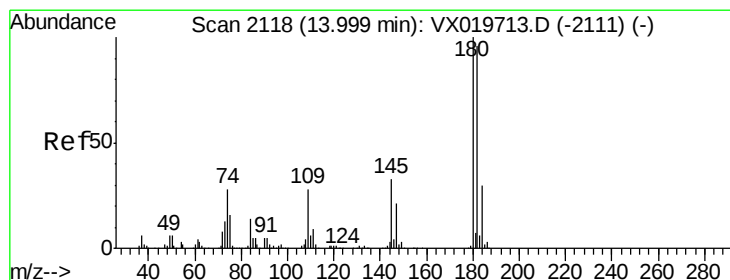

#96
1,2,3-Trichlorobenzene
Concen: 54.756 ug/l
RT: 14.00 min Scan# 2118
Delta R.T. -0.00 min
Lab File: VX019839.D
Acq: 10 Dec 2020 20:55

Tgt Ion:180 Resp: 215920
Ion Ratio Lower Upper
180 100
182 94.7 47.6 142.9
145 32.8 16.1 48.3

