

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121020\  
 Data File : VX019820.D  
 Acq On : 10 Dec 2020 13:11  
 Operator : JC/MD  
 Sample : L4996-26  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB01-20201208

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X120420W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.575       | 237           | 244         | 256          | rVB      | 25047          | 47407         | 2.91%           | 0.552%        |
| 2         | 2.831       | 280           | 286         | 294          | rVB      | 10549          | 19937         | 1.22%           | 0.232%        |
| 3         | 5.464       | 705           | 718         | 732          | rBV      | 186368         | 526329        | 32.32%          | 6.130%        |
| 4         | 5.629       | 732           | 745         | 760          | rVB      | 318627         | 899996        | 55.27%          | 10.482%       |
| 5         | 6.031       | 798           | 811         | 829          | rBV      | 206726         | 547493        | 33.62%          | 6.377%        |
| 6         | 6.830       | 931           | 942         | 955          | rBV      | 501773         | 1186731       | 72.87%          | 13.822%       |
| 7         | 8.695       | 1241          | 1248        | 1255         | rBV      | 1083799        | 1628485       | 100.00%         | 18.967%       |
| 8         | 8.763       | 1255          | 1259        | 1267         | rVB      | 66019          | 99832         | 6.13%           | 1.163%        |
| 9         | 10.092      | 1471          | 1477        | 1492         | rBV      | 1008926        | 1391183       | 85.43%          | 16.203%       |
| 10        | 11.122      | 1640          | 1646        | 1659         | rBV      | 803787         | 1020265       | 62.65%          | 11.883%       |
| 11        | 12.061      | 1794          | 1800        | 1812         | rBV      | 1026038        | 1218055       | 74.80%          | 14.187%       |


Sum of corrected areas: 8585713

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121020\  
Data File : VX019820.D  
Acq On : 10 Dec 2020 13:11  
Operator : JC/MD  
Sample : L4996-26  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-20201208

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X120420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

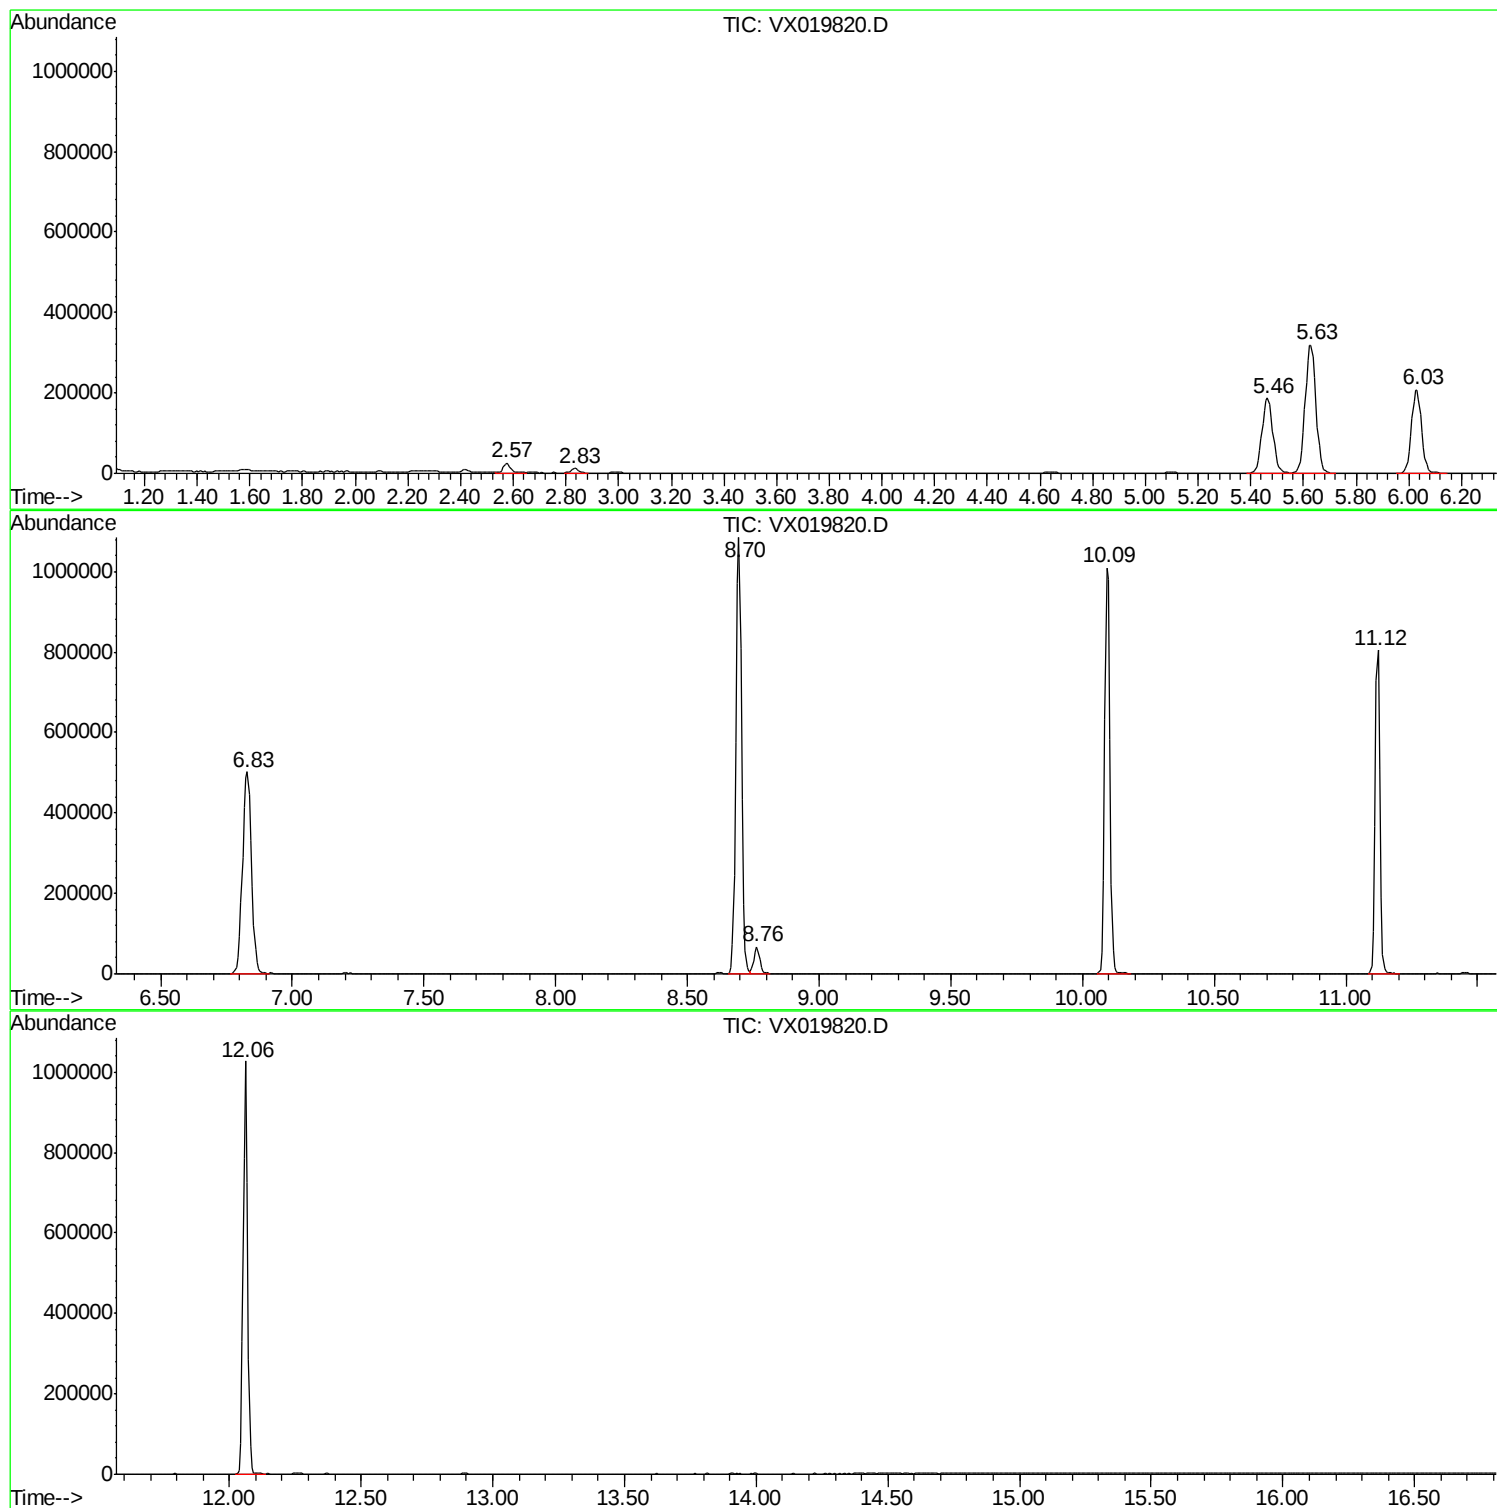

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX121020\  
Data File : VX019820.D  
Acq On : 10 Dec 2020 13:11  
Operator : JC/MD  
Sample : L4996-26  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-20201208

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X120420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX121020\  
Data File : VX019820.D  
Acq On : 10 Dec 2020 13:11  
Operator : JC/MD  
Sample : L4996-26  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-20201208

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X120420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |