


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121020\
 Data File : VX019838.D
 Acq On : 10 Dec 2020 20:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Title : SW846 8260
 Last Update : Fri Dec 04 15:32:53 2020

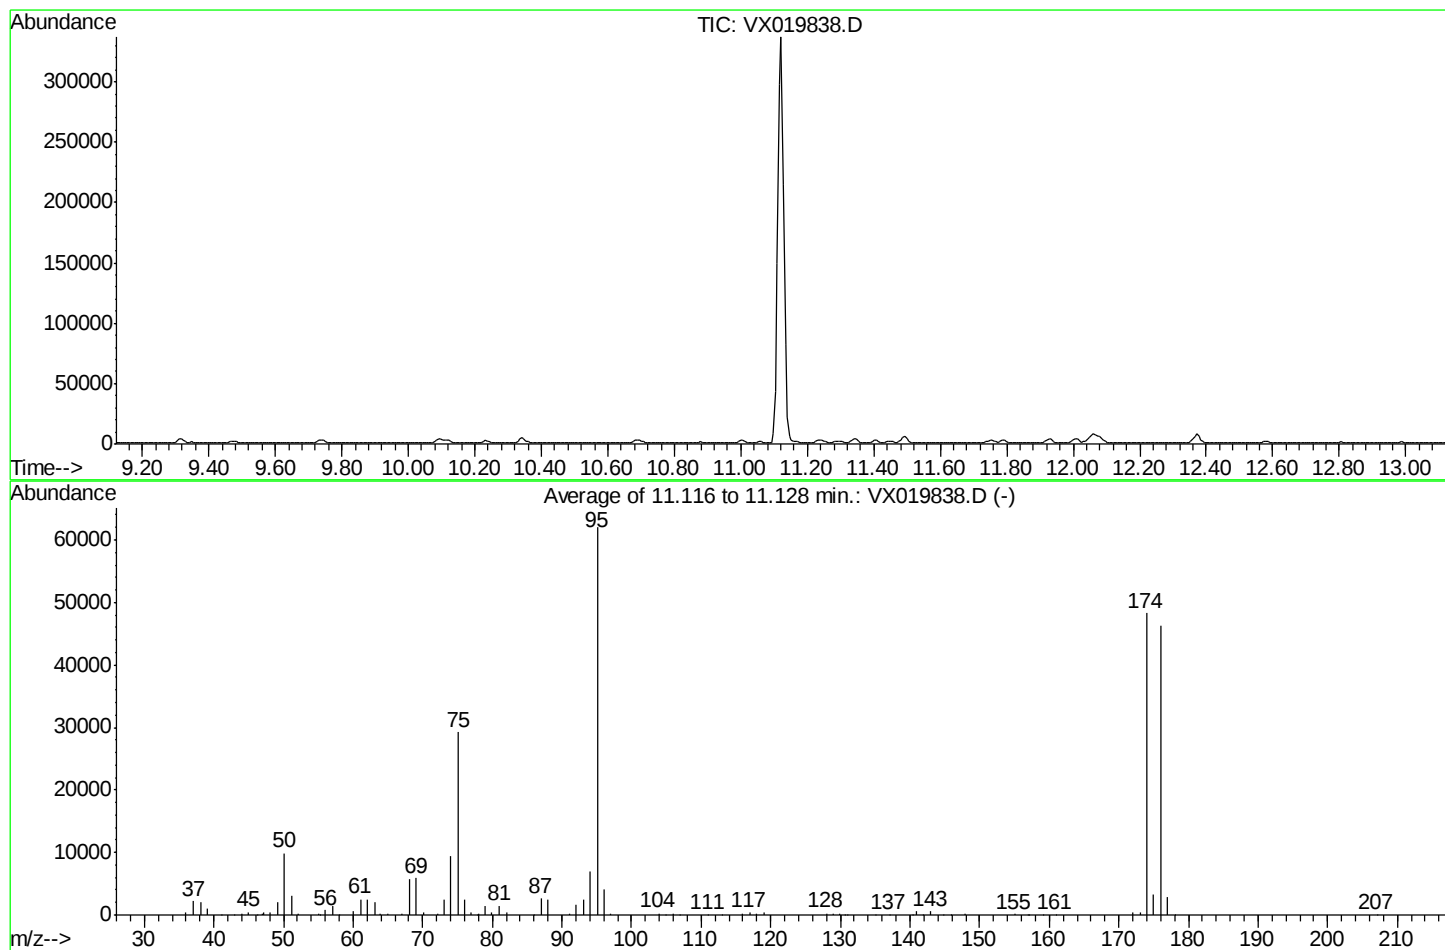

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9850	PASS
75	95	30	60	47.1	29216	PASS
95	95	100	100	100.0	62008	PASS
96	95	5	9	6.6	4104	PASS
173	174	0.00	2	0.8	405	PASS
174	95	50	100	77.9	48274	PASS
175	174	5	9	6.7	3253	PASS
176	174	95	101	95.8	46253	PASS
177	176	5	9	6.4	2948	PASS