




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025725.D
Acq On : 11 Dec 2021 00:37
Operator : JC/MD
Sample : M4981-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CQ0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/11/2021
Supervised By :Mahesh Dadoda 12/11/2021

Quant Time: Dec 11 01:06:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 11 00:48:07 2021
Response via : Initial Calibration

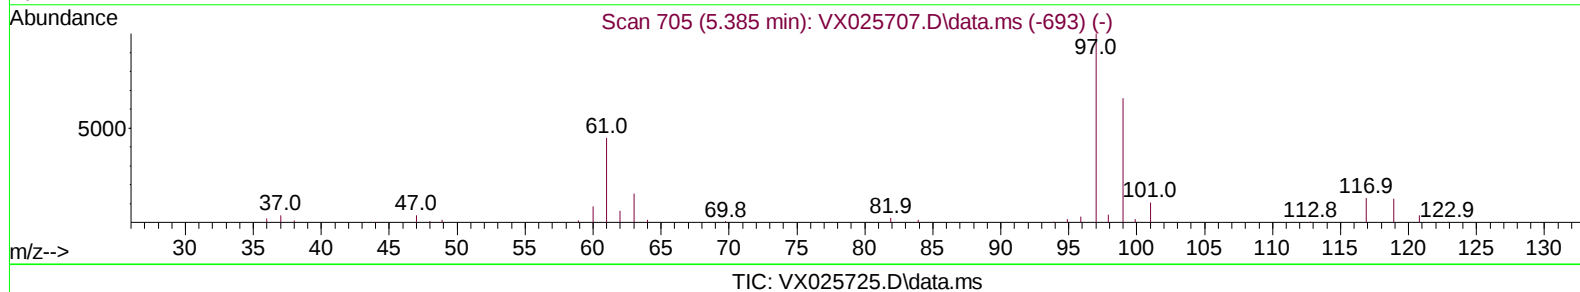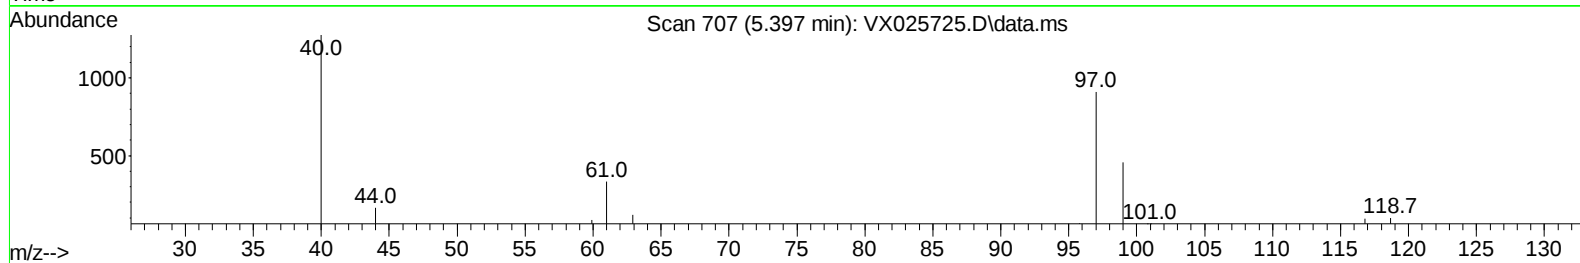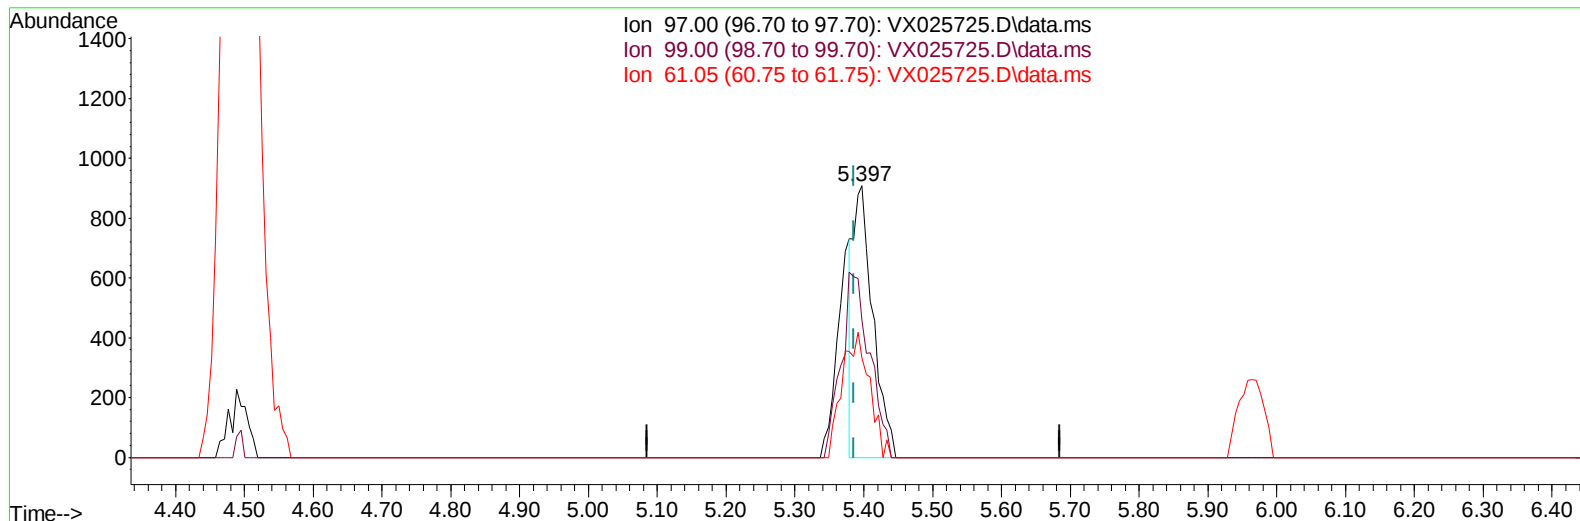

(30) 1,1,1-Trichloroethane (T)

5.397min (+ 0.012) 1.79 ug/L

response 1783

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.40	0.00#
61.05	41.40	31.91#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025725.D
Acq On : 11 Dec 2021 00:37
Operator : JC/MD
Sample : M4981-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CQ0

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:06:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 11 00:48:07 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/11/2021
Supervised By :Mahesh Dadoda 12/11/2021

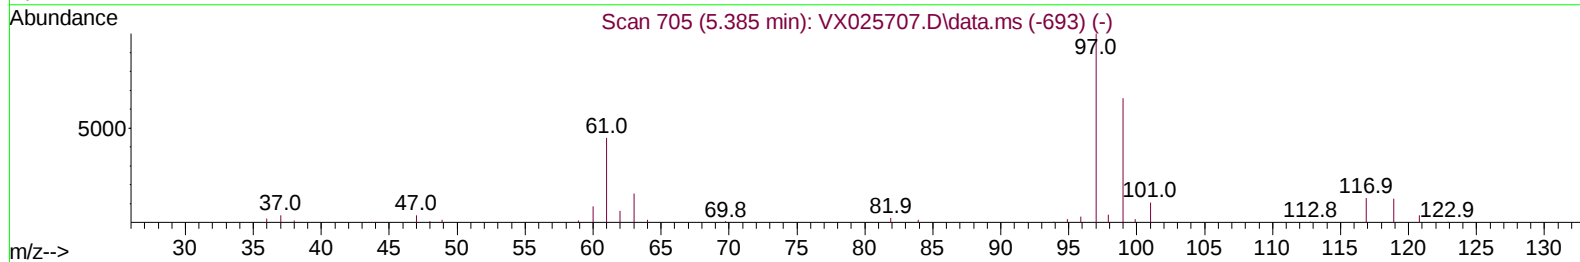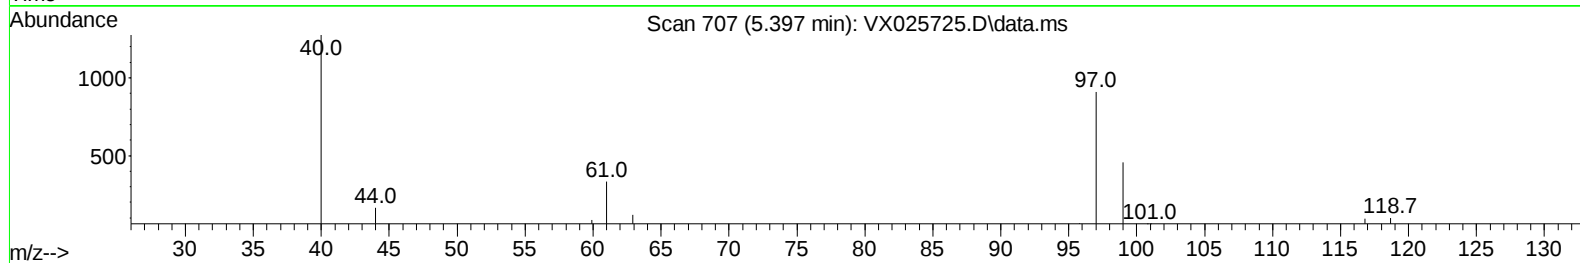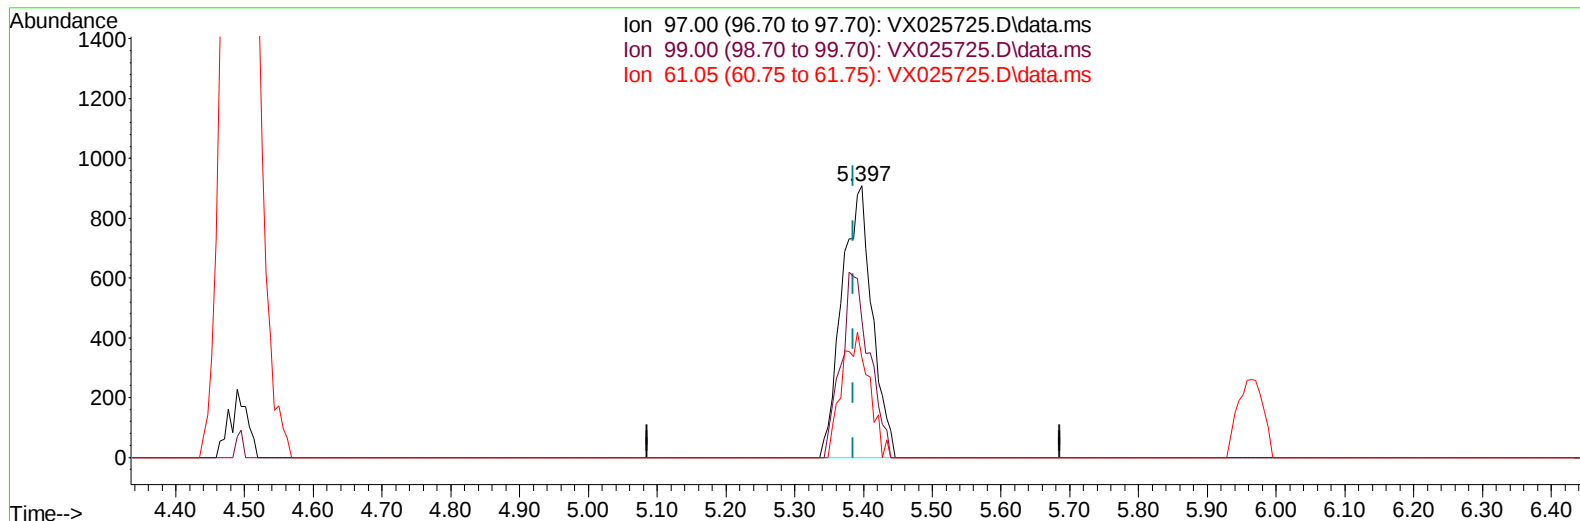

TIC: VX025725.D\data.ms

(30) 1,1,1-Trichloroethane (T)

5.397min (+ 0.012) 2.77 ug/L m

response 2768

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.40	0.00#
61.05	41.40	20.56#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025725.D
 Acq On : 11 Dec 2021 00:37
 Operator : JC/MD
 Sample : M4981-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CQ0

Manual IntegrationsAPPROVED

Quant Time: Dec 11 01:06:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 11 00:48:07 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 12/11/2021
 Supervised By :Mahesh Dadoda 12/11/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	95660	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	90390	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	38876	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	26862	41.147	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	82.300%	
7) Chloroethane-d5	1.666	69	23302	43.247	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	86.500%	
11) 1,1-Dichloroethene-d2	2.306	63	42195	40.536	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.080%	
21) 2-Butanone-d5	4.458	46	45136	92.878	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	92.880%	
24) Chloroform-d	5.068	84	54641	47.890	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.780%	
26) 1,2-Dichloroethane-d4	5.958	65	36568	51.419	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.840%	
32) Benzene-d6	5.976	84	109780	45.825	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.660%	
36) 1,2-Dichloropropane-d6	7.312	67	33466	45.120	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.240%	
41) Toluene-d8	8.653	98	100996	44.665	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.320%	
43) trans-1,3-Dichloroprop...	8.952	79	15265	40.936	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.880%	
47) 2-Hexanone-d5	9.384	63	31669	82.025	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	82.020%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	47554	45.365	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	90.740%	
66) 1,2-Dichlorobenzene-d4	12.323	152	36019	47.239	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.480%	
Target Compounds						
12) 1,1-Dichloroethene	2.319	96	5904	11.493	ug/L #	1
19) 1,1-Dichloroethane	3.617	63	1023	1.033	ug/L	88
20) cis-1,2-Dichloroethene	4.495	96	10836	16.627	ug/L	95
30) 1,1,1-Trichloroethane	5.397	97	2768m	2.774	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025725.D
Acq On : 11 Dec 2021 00:37
Operator : JC/MD
Sample : M4981-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CQ0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/11/2021
Supervised By :Mahesh Dadoda 12/11/2021

Quant Time: Dec 11 01:06:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 11 00:48:07 2021
Response via : Initial Calibration

