

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025723.D
 Acq On : 10 Dec 2021 23:51
 Operator : JC/MD
 Sample : M4981-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CP7

Quant Time: Dec 11 01:05:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 11 00:48:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	94951	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	89348	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	37966	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	26734	41.256	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.520%
7) Chloroethane-d5	1.666	69	22895	42.809	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.620%
11) 1,1-Dichloroethene-d2	2.307	63	39309	38.046	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.100%
21) 2-Butanone-d5	4.459	46	45934	95.226	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.230%
24) Chloroform-d	5.062	84	54511	48.133	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.260%
26) 1,2-Dichloroethane-d4	5.964	65	36444	51.627	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.260%
32) Benzene-d6	5.977	84	110227	46.549	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.100%
36) 1,2-Dichloropropane-d6	7.312	67	33264	45.371	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.740%
41) Toluene-d8	8.653	98	101844	45.565	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.140%
43) trans-1,3-Dichloroprop...	8.952	79	15512	42.083	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.160%
47) 2-Hexanone-d5	9.384	63	31651	82.934	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.930%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	47724	46.058	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.120%
66) 1,2-Dichlorobenzene-d4	12.323	152	35741	47.997	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.000%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.135	95	1896	3.020	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025723.D
Acq On : 10 Dec 2021 23:51
Operator : JC/MD
Sample : M4981-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CP7


Quant Time: Dec 11 01:05:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 11 00:48:07 2021
Response via : Initial Calibration

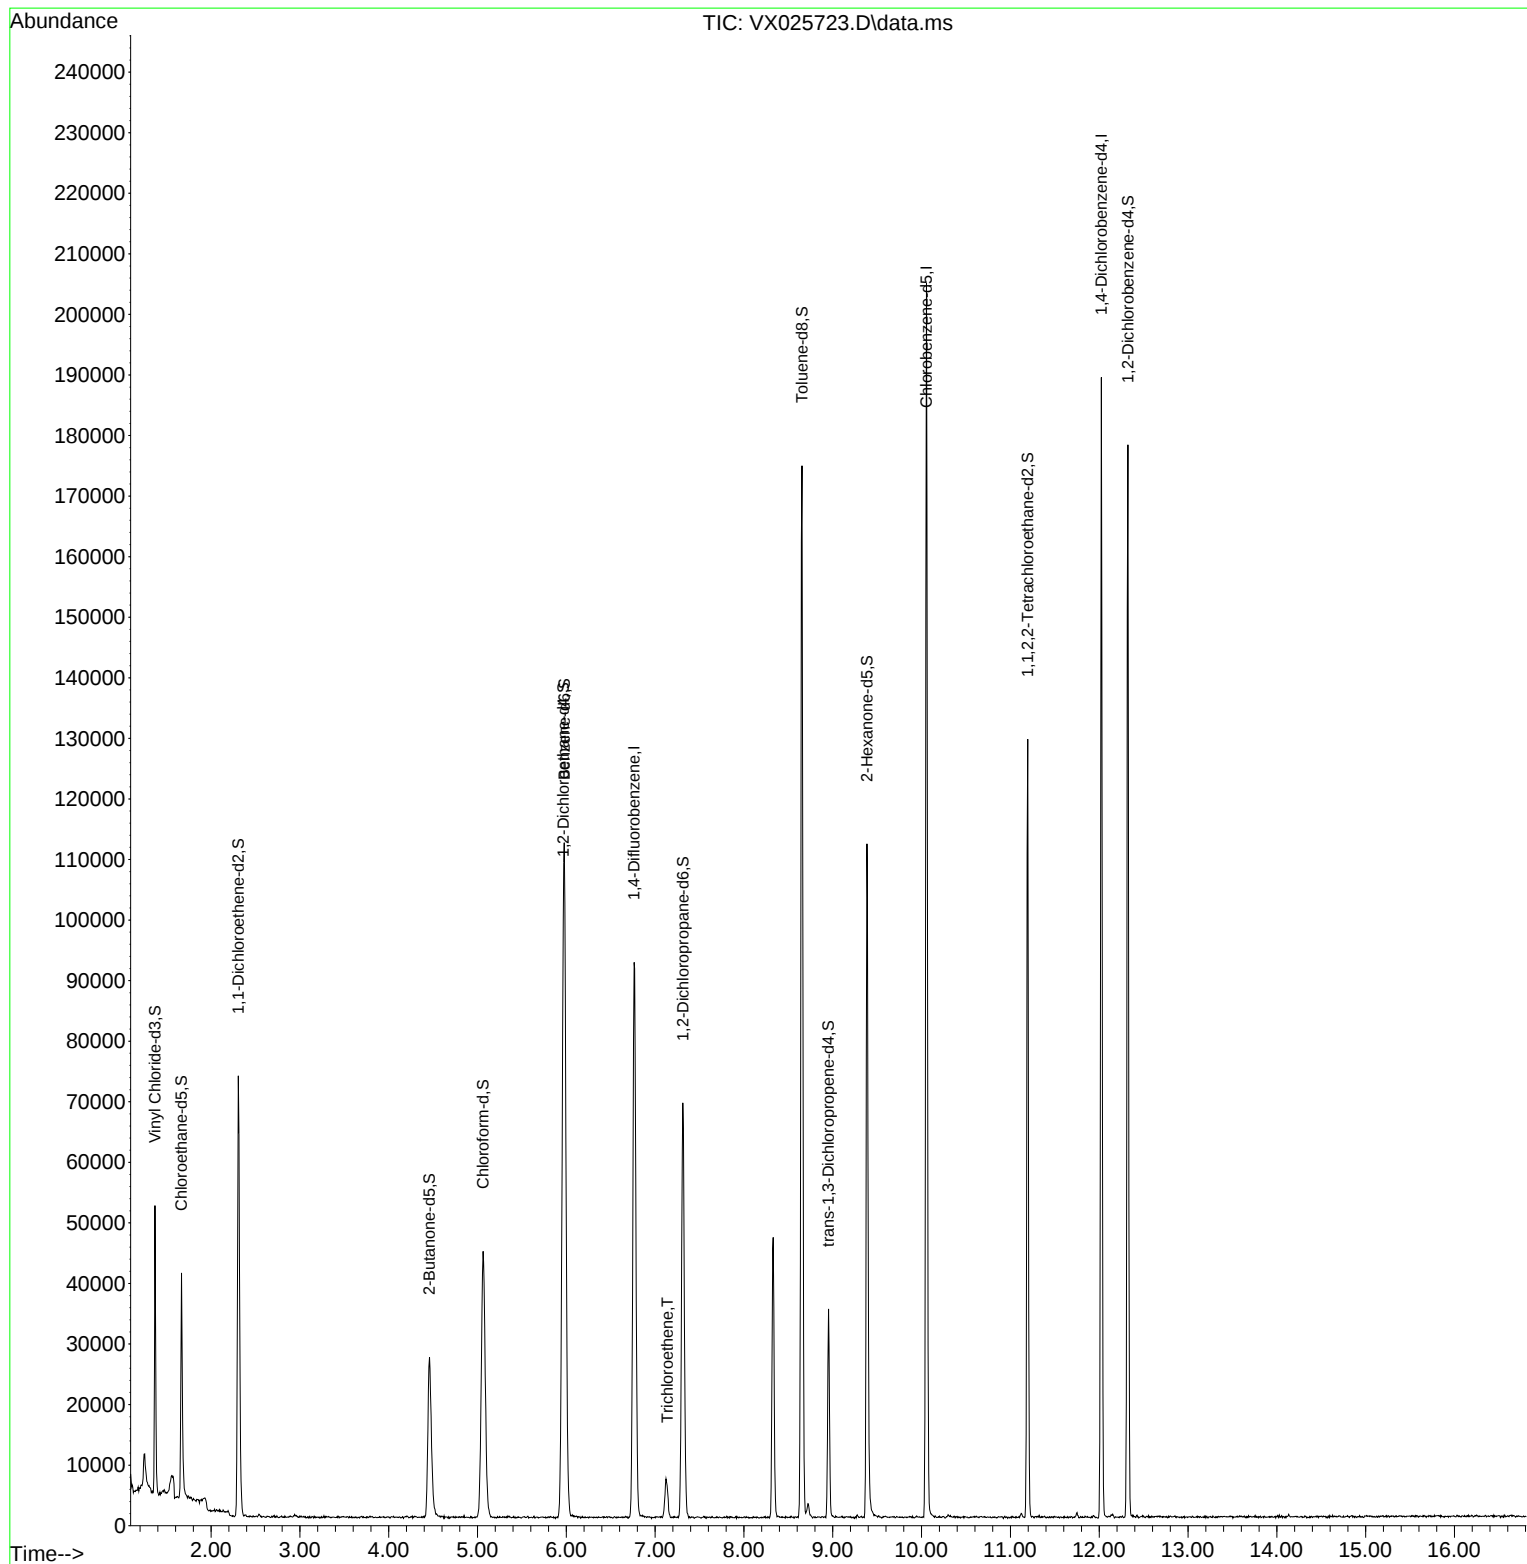

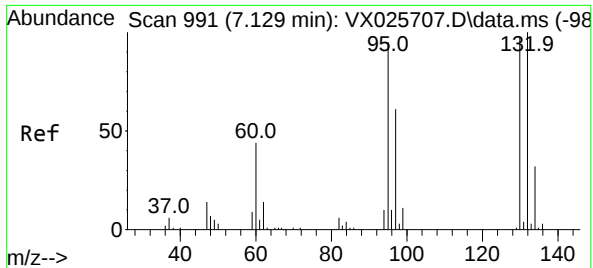

#34
 Trichloroethene
 Concen: 3.020 ug/L
 RT: 7.135 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX025723.D
 Acq: 10 Dec 2021 23:51

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CP7

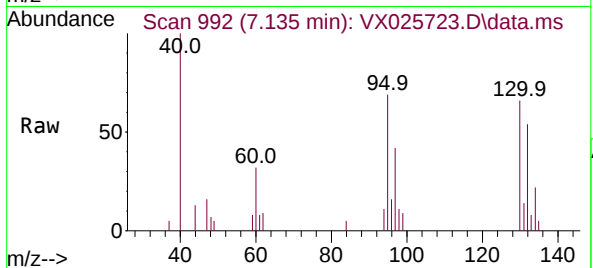

Tgt Ion: 95 Resp: 1896

Ion	Ratio	Lower	Upper
95	100		
97	61.0	46.0	85.4
132	78.8	75.0	139.2
130	96.0	77.9	144.7

