

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025700.D
 Acq On : 10 Dec 2021 14:41
 Operator : JC/MD
 Sample : M4888-02ME
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX8A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	45363	55195	13.44%	1.684%
2	1.648	89	92	100	rVB	31978	38454	9.36%	1.173%
3	2.282	189	196	207	rBV	86581	151828	36.97%	4.633%
4	2.953	300	306	324	rVB	3905	11361	2.77%	0.347%
5	3.196	344	346	348	rBV2	330	248	0.06%	0.008%
6	3.251	353	355	357	rBV	354	410	0.10%	0.013%
7	3.617	414	415	417	rBV	279	173	0.04%	0.005%
8	4.056	485	487	490	rVB	386	256	0.06%	0.008%
9	4.233	514	516	518	rBV	353	273	0.07%	0.008%
10	4.495	551	559	583	rBV	16428	75436	18.37%	2.302%
11	4.830	612	614	615	rBV2	175	189	0.05%	0.006%
12	4.861	617	619	621	rBV2	318	343	0.08%	0.010%
13	5.068	641	653	671	rVB2	47642	164536	40.06%	5.021%
14	5.281	686	688	689	rBV	213	139	0.03%	0.004%
15	5.324	693	695	697	rBV	217	249	0.06%	0.008%
16	5.489	720	722	724	rBV	211	190	0.05%	0.006%
17	5.708	756	758	762	rBV	267	214	0.05%	0.007%
18	5.970	790	801	819	rVB2	142098	410712	100.00%	12.532%
19	6.220	840	842	844	rBV2	288	325	0.08%	0.010%
20	6.373	860	867	868	rBV3	1386	2740	0.67%	0.084%
21	6.470	881	883	888	rVB2	259	247	0.06%	0.008%
22	6.690	917	919	921	rBV	235	109	0.03%	0.003%
23	6.769	922	932	944	rBV	104115	265903	64.74%	8.114%
24	7.007	969	971	972	rVB	243	150	0.04%	0.005%
25	7.129	983	991	1000	rVB3	10975	25692	6.26%	0.784%
26	7.318	1013	1022	1037	rVB	76404	180870	44.04%	5.519%
27	7.446	1042	1043	1045	rBV	287	221	0.05%	0.007%
28	7.531	1055	1057	1061	rVB2	263	253	0.06%	0.008%
29	7.604	1067	1069	1070	rVB	364	151	0.04%	0.005%
30	7.690	1081	1083	1085	rVB	268	179	0.04%	0.005%
31	7.763	1094	1095	1098	rBV	309	370	0.09%	0.011%
32	7.793	1098	1100	1101	rVV	217	132	0.03%	0.004%
33	7.946	1123	1125	1127	rBV2	180	172	0.04%	0.005%
34	7.970	1127	1129	1132	rVV2	350	355	0.09%	0.011%
35	8.110	1151	1152	1155	rVB	243	132	0.03%	0.004%
36	8.226	1168	1171	1172	rBV2	248	290	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025700.D
 Acq On : 10 Dec 2021 14:41
 Operator : JC/MD
 Sample : M4888-02ME
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX8A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.330	1182	1188	1197	rVB	52624	91076	22.18%	2.779%
38	8.476	1210	1212	1213	rBV	199	108	0.03%	0.003%
39	8.494	1213	1215	1217	rVB	256	173	0.04%	0.005%
40	8.653	1234	1241	1249	rBV	210468	340159	82.82%	10.379%
41	8.720	1249	1252	1257	rVB	2508	3466	0.84%	0.106%
42	8.958	1285	1291	1299	rBV	33045	55774	13.58%	1.702%
43	9.037	1303	1304	1305	rBV	423	244	0.06%	0.007%
44	9.073	1308	1310	1312	rVB2	237	129	0.03%	0.004%
45	9.165	1320	1325	1330	rBV	2640	4209	1.02%	0.128%
46	9.201	1330	1331	1333	rVV	213	106	0.03%	0.003%
47	9.275	1337	1343	1352	rVB	66152	98212	23.91%	2.997%
48	9.403	1357	1364	1374	rBV	101124	169059	41.16%	5.159%
49	9.579	1390	1393	1395	rBV2	240	267	0.07%	0.008%
50	9.683	1406	1410	1411	rBV	302	396	0.10%	0.012%
51	9.707	1412	1414	1417	rVB2	386	429	0.10%	0.013%
52	9.842	1434	1436	1437	rVB	288	130	0.03%	0.004%
53	9.854	1437	1438	1441	rBV	290	345	0.08%	0.011%
54	10.061	1466	1472	1482	rBV	206029	311841	75.93%	9.515%
55	10.201	1492	1495	1498	rBV2	432	613	0.15%	0.019%
56	10.262	1503	1505	1508	rBV2	182	201	0.05%	0.006%
57	10.305	1510	1512	1516	rVV3	570	690	0.17%	0.021%
58	10.342	1516	1518	1521	rVV	231	179	0.04%	0.005%
59	10.518	1545	1547	1548	rVB	241	153	0.04%	0.005%
60	10.537	1548	1550	1552	rBV2	191	177	0.04%	0.005%
61	10.555	1552	1553	1555	rVV	192	143	0.03%	0.004%
62	10.622	1563	1564	1566	rVB	215	104	0.03%	0.003%
63	10.652	1566	1569	1571	rBV2	287	363	0.09%	0.011%
64	10.701	1574	1577	1578	rBV	471	449	0.11%	0.014%
65	10.787	1589	1591	1593	rBV	314	247	0.06%	0.008%
66	10.823	1596	1597	1599	rBV	277	245	0.06%	0.007%
67	10.878	1605	1606	1608	rVB	378	234	0.06%	0.007%
68	10.902	1608	1610	1611	rBV	257	196	0.05%	0.006%
69	10.976	1619	1622	1624	rBV	359	476	0.12%	0.015%
70	11.122	1643	1646	1650	rVB2	1983	2414	0.59%	0.074%
71	11.195	1653	1658	1668	rVV	137693	188529	45.90%	5.753%
72	11.408	1691	1693	1694	rBV	289	194	0.05%	0.006%
73	11.750	1746	1749	1754	rVB4	2055	2952	0.72%	0.090%
74	11.792	1754	1756	1758	rBV2	288	329	0.08%	0.010%
75	11.847	1763	1765	1767	rVV2	428	341	0.08%	0.010%
76	11.908	1773	1775	1776	rBV	280	246	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025700.D
 Acq On : 10 Dec 2021 14:41
 Operator : JC/MD
 Sample : M4888-02ME
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX8A9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	11.939	1776	1780	1783	rVB3	1008	1317	0.32%	0.040%
78	12.024	1789	1794	1800	rBV	242462	307503	74.87%	9.383%
79	12.128	1807	1811	1813	rBV5	1023	1680	0.41%	0.051%
80	12.256	1830	1832	1833	rVB	306	154	0.04%	0.005%
81	12.274	1833	1835	1836	rBV	221	182	0.04%	0.006%
82	12.323	1836	1843	1853	rVV	242760	297410	72.41%	9.075%
83	12.426	1858	1860	1863	rVB	982	889	0.22%	0.027%
84	12.542	1877	1879	1883	rBV	244	291	0.07%	0.009%
85	12.658	1896	1898	1903	rVB3	627	774	0.19%	0.024%
86	12.804	1920	1922	1924	rBV	252	274	0.07%	0.008%
87	13.018	1955	1957	1960	rVB	439	329	0.08%	0.010%
88	13.042	1960	1961	1966	rBB2	428	414	0.10%	0.013%
89	13.079	1966	1967	1968	rVB	257	94	0.02%	0.003%
90	13.103	1968	1971	1973	rBV	273	367	0.09%	0.011%
91	13.420	2022	2023	2025	rBV	288	185	0.05%	0.006%
92	13.871	2096	2097	2099	rBV	266	115	0.03%	0.004%
93	13.890	2099	2100	2102	rVB	354	209	0.05%	0.006%
94	14.134	2137	2140	2143	rVB	689	872	0.21%	0.027%
95	15.956	2437	2439	2440	rBB	301	113	0.03%	0.003%




Sum of corrected areas: 3277267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025700.D
Acq On : 10 Dec 2021 14:41
Operator : JC/MD
Sample : M4888-02ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX8A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

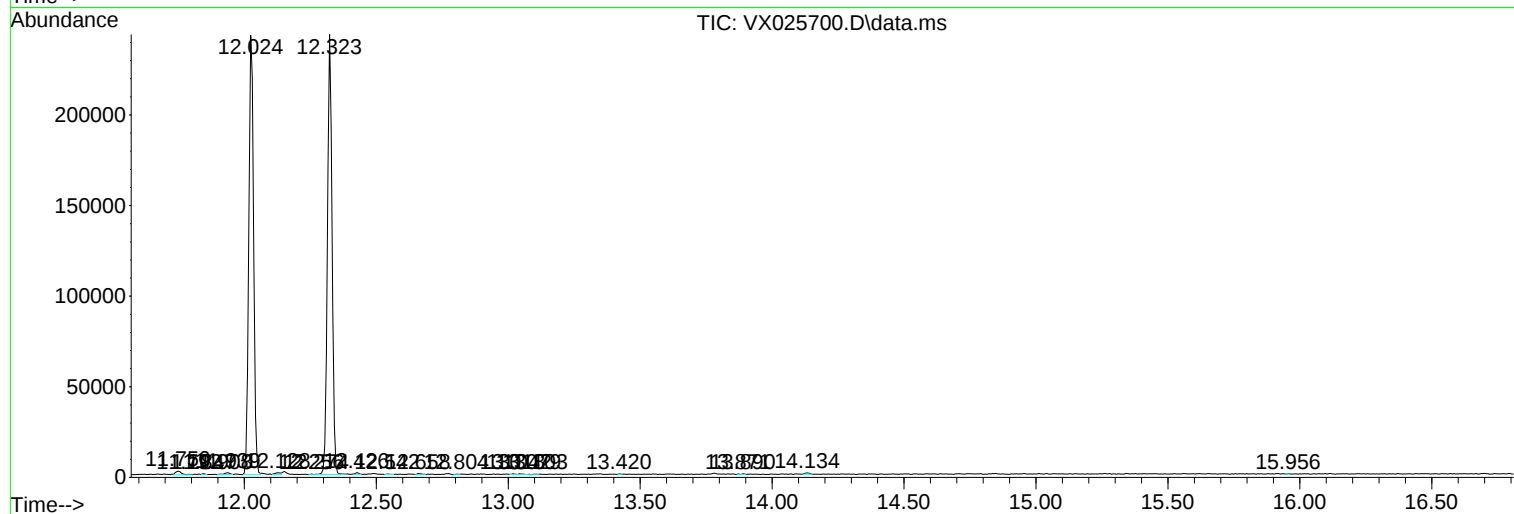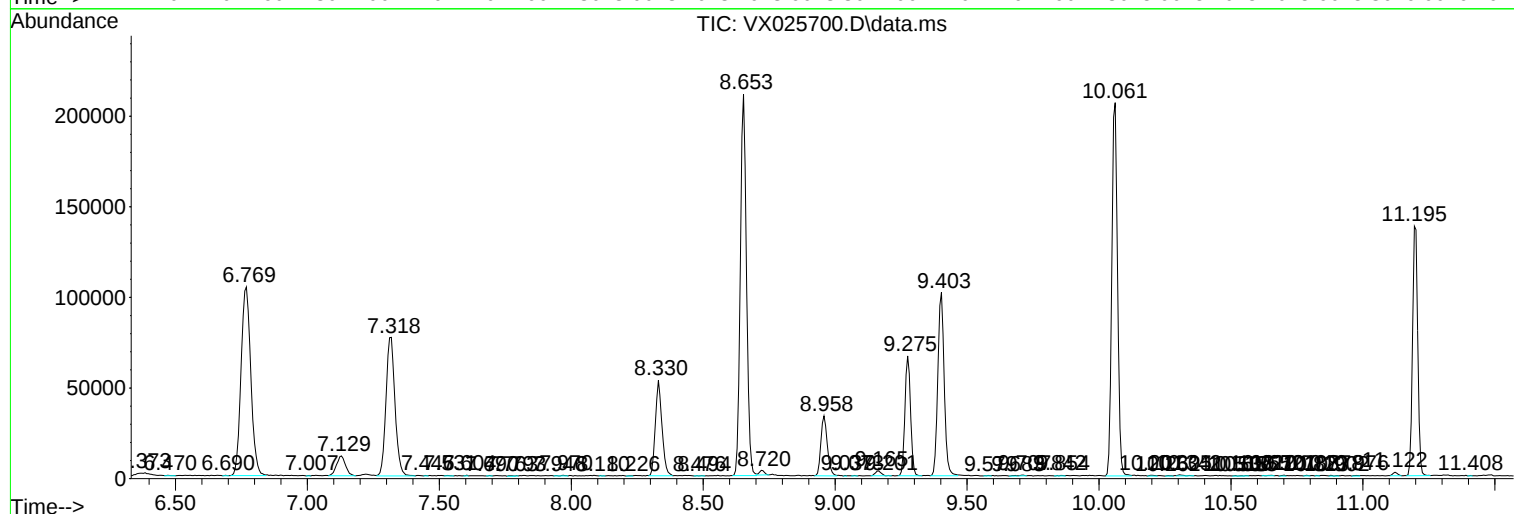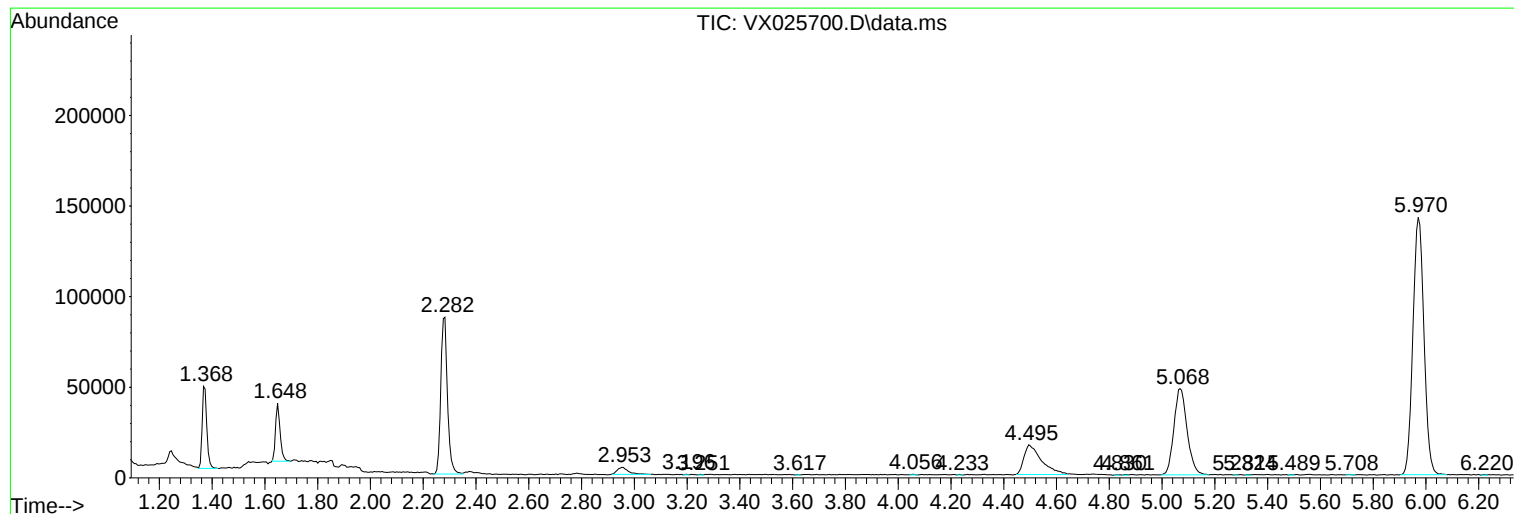

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025700.D
Acq On : 10 Dec 2021 14:41
Operator : JC/MD
Sample : M4888-02ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX8A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025700.D
Acq On : 10 Dec 2021 14:41
Operator : JC/MD
Sample : M4888-02ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX8A9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc