

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025712.D
 Acq On : 10 Dec 2021 19:34
 Operator : JC/MD
 Sample : M4981-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	50581	49017	14.09%	1.779%
2	1.666	91	95	101	rBV	36793	49009	14.08%	1.779%
3	2.306	194	200	212	rVB	76245	123919	35.61%	4.497%
4	2.806	280	282	284	rBV	292	300	0.09%	0.011%
5	2.910	297	299	301	rBV2	301	305	0.09%	0.011%
6	2.947	303	305	310	rVV2	420	660	0.19%	0.024%
7	3.093	325	329	330	rBV	333	450	0.13%	0.016%
8	3.184	342	344	347	rBV2	278	410	0.12%	0.015%
9	3.587	408	410	411	rBV	244	213	0.06%	0.008%
10	4.032	480	483	486	rBV2	368	462	0.13%	0.017%
11	4.263	519	521	522	rBV	300	262	0.08%	0.010%
12	4.459	544	553	572	rBV	28416	78930	22.68%	2.864%
13	4.965	634	636	637	rBV	236	217	0.06%	0.008%
14	5.062	641	652	668	rVV2	45517	143082	41.12%	5.193%
15	5.373	701	703	707	rBV2	262	413	0.12%	0.015%
16	5.635	745	746	749	rBV	423	279	0.08%	0.010%
17	5.970	790	801	816	rBV2	117627	347971	100.00%	12.628%
18	6.635	907	910	912	rBV2	245	334	0.10%	0.012%
19	6.690	917	919	921	rBV	330	245	0.07%	0.009%
20	6.763	922	931	943	rVV	95968	230081	66.12%	8.350%
21	6.958	960	963	966	rBV2	254	275	0.08%	0.010%
22	7.123	982	990	999	rVB7	3035	8355	2.40%	0.303%
23	7.196	999	1002	1004	rBV2	360	503	0.14%	0.018%
24	7.245	1008	1010	1013	rBV2	278	343	0.10%	0.012%
25	7.312	1013	1021	1033	rVB	72084	157568	45.28%	5.718%
26	7.391	1033	1034	1037	rBV	260	304	0.09%	0.011%
27	7.488	1047	1050	1054	rVB	314	403	0.12%	0.015%
28	7.568	1060	1063	1066	rBV2	299	427	0.12%	0.015%
29	7.799	1098	1101	1103	rBV2	227	265	0.08%	0.010%
30	7.866	1109	1112	1114	rVV	269	304	0.09%	0.011%
31	7.994	1129	1133	1135	rVB2	268	363	0.10%	0.013%
32	8.055	1140	1143	1145	rBV2	191	250	0.07%	0.009%
33	8.092	1145	1149	1150	rVB2	286	269	0.08%	0.010%
34	8.183	1163	1164	1166	rBV	292	240	0.07%	0.009%
35	8.330	1182	1188	1197	rVB	50208	83236	23.92%	3.021%
36	8.397	1197	1199	1202	rBV2	202	286	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025712.D
 Acq On : 10 Dec 2021 19:34
 Operator : JC/MD
 Sample : M4981-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.464	1209	1210	1212	rBV	285	205	0.06%	0.007%
38	8.543	1221	1223	1225	rBV2	241	267	0.08%	0.010%
39	8.568	1225	1227	1232	rBV2	149	275	0.08%	0.010%
40	8.653	1234	1241	1248	rVV	183722	287827	82.72%	10.446%
41	8.720	1249	1252	1259	rVB2	2462	3798	1.09%	0.138%
42	8.952	1284	1290	1299	rBV	37029	52298	15.03%	1.898%
43	9.128	1317	1319	1321	rBV2	304	336	0.10%	0.012%
44	9.171	1325	1326	1329	rVV2	199	225	0.06%	0.008%
45	9.275	1339	1343	1346	rBV3	1037	1258	0.36%	0.046%
46	9.384	1356	1361	1373	rBV	117409	171575	49.31%	6.227%
47	9.561	1389	1390	1393	rBV	236	225	0.06%	0.008%
48	9.836	1433	1435	1438	rVV	253	234	0.07%	0.008%
49	9.903	1442	1446	1449	rVB	281	379	0.11%	0.014%
50	9.945	1451	1453	1454	rBV	337	267	0.08%	0.010%
51	10.055	1465	1471	1481	rBV	211880	278976	80.17%	10.124%
52	10.195	1493	1494	1497	rBV	266	234	0.07%	0.008%
53	10.305	1509	1512	1516	rVV3	483	716	0.21%	0.026%
54	10.336	1516	1517	1520	rVV	317	213	0.06%	0.008%
55	10.421	1529	1531	1533	rBV2	237	207	0.06%	0.008%
56	10.573	1554	1556	1560	rBV2	257	314	0.09%	0.011%
57	10.653	1566	1569	1572	rBV2	298	312	0.09%	0.011%
58	10.683	1572	1574	1576	rBV	247	213	0.06%	0.008%
59	10.738	1580	1583	1585	rBV2	225	304	0.09%	0.011%
60	10.811	1593	1595	1597	rBV	286	253	0.07%	0.009%
61	10.957	1617	1619	1621	rBV	390	349	0.10%	0.013%
62	11.037	1630	1632	1635	rBV2	164	222	0.06%	0.008%
63	11.122	1643	1646	1652	rVV2	1015	1113	0.32%	0.040%
64	11.195	1652	1658	1666	rVB	131290	170601	49.03%	6.191%
65	11.335	1678	1681	1683	rVB	241	228	0.07%	0.008%
66	11.384	1685	1689	1691	rBV	311	327	0.09%	0.012%
67	11.488	1703	1706	1707	rBV	334	356	0.10%	0.013%
68	11.622	1725	1728	1729	rBV	213	253	0.07%	0.009%
69	11.750	1743	1749	1753	rVV3	1017	1451	0.42%	0.053%
70	11.811	1757	1759	1760	rVV	339	214	0.06%	0.008%
71	11.841	1763	1764	1767	rVV	303	242	0.07%	0.009%
72	11.878	1768	1770	1772	rVV	280	210	0.06%	0.008%
73	11.933	1776	1779	1783	rVV2	748	755	0.22%	0.027%
74	12.024	1789	1794	1806	rVB	202516	250058	71.86%	9.075%
75	12.116	1806	1809	1810	rBV2	418	417	0.12%	0.015%
76	12.152	1812	1815	1817	rVV2	907	921	0.26%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025712.D
 Acq On : 10 Dec 2021 19:34
 Operator : JC/MD
 Sample : M4981-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.250	1829	1831	1833	rVV	351	274	0.08%	0.010%
78	12.323	1837	1843	1851	rVB	186413	239379	68.79%	8.687%
79	12.433	1858	1861	1866	rVB3	496	771	0.22%	0.028%
80	12.469	1866	1867	1869	rBV2	311	286	0.08%	0.010%
81	12.518	1872	1875	1877	rVV	320	342	0.10%	0.012%
82	12.628	1890	1893	1897	rBV2	265	342	0.10%	0.012%
83	12.658	1897	1898	1901	rBV2	339	290	0.08%	0.011%
84	13.103	1969	1971	1974	rBV	329	386	0.11%	0.014%
85	13.140	1976	1977	1979	rVV2	336	238	0.07%	0.009%
86	13.536	2040	2042	2045	rBV	241	253	0.07%	0.009%
87	13.731	2073	2074	2075	rBV	427	228	0.07%	0.008%
88	13.859	2092	2095	2097	rBV2	289	336	0.10%	0.012%
89	13.975	2113	2114	2116	rBV	233	211	0.06%	0.008%
90	14.121	2136	2138	2139	rBV	364	258	0.07%	0.009%
91	14.566	2209	2211	2215	rVB2	322	345	0.10%	0.013%
92	14.914	2266	2268	2270	rVB2	365	342	0.10%	0.012%
93	15.158	2305	2308	2310	rBV	520	561	0.16%	0.020%
94	15.207	2314	2316	2317	rVB	378	217	0.06%	0.008%
95	15.341	2337	2338	2343	rVB	356	340	0.10%	0.012%
96	15.511	2363	2366	2368	rBV2	214	277	0.08%	0.010%
97	15.639	2386	2387	2390	rVB2	251	205	0.06%	0.007%
98	15.859	2422	2423	2425	rBV	353	310	0.09%	0.011%
99	16.359	2503	2505	2507	rBV	256	241	0.07%	0.009%
100	16.639	2549	2551	2555	rBV2	322	461	0.13%	0.017%

Sum of corrected areas: 2755471




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025712.D
Acq On : 10 Dec 2021 19:34
Operator : JC/MD
Sample : M4981-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CNO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

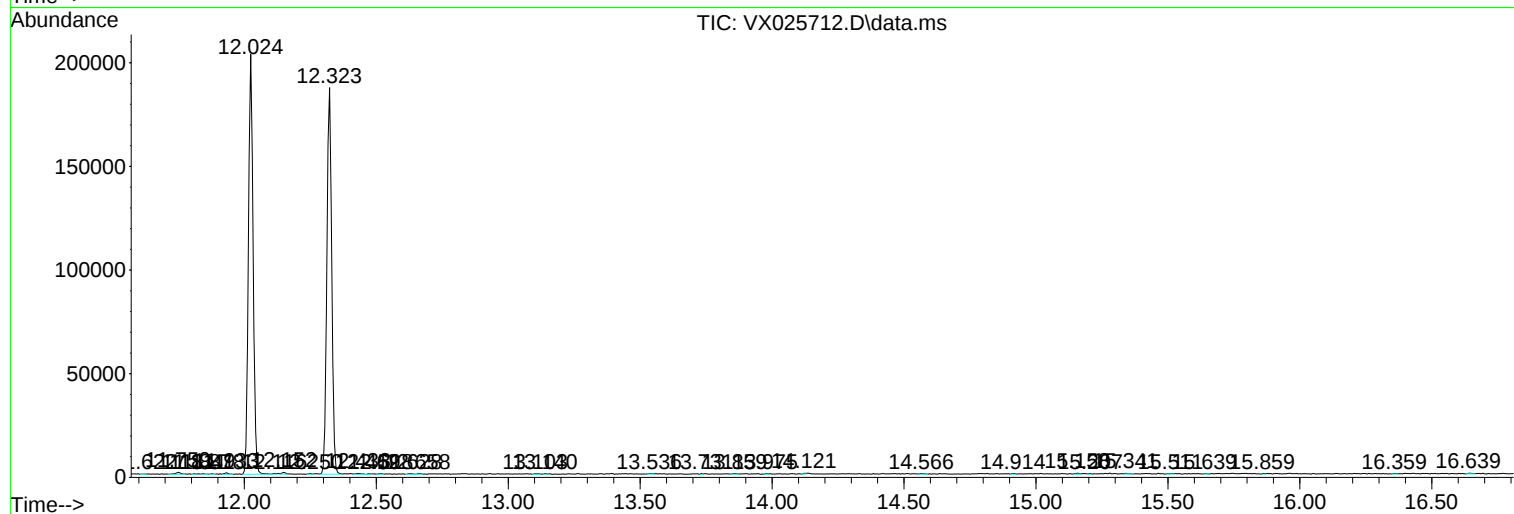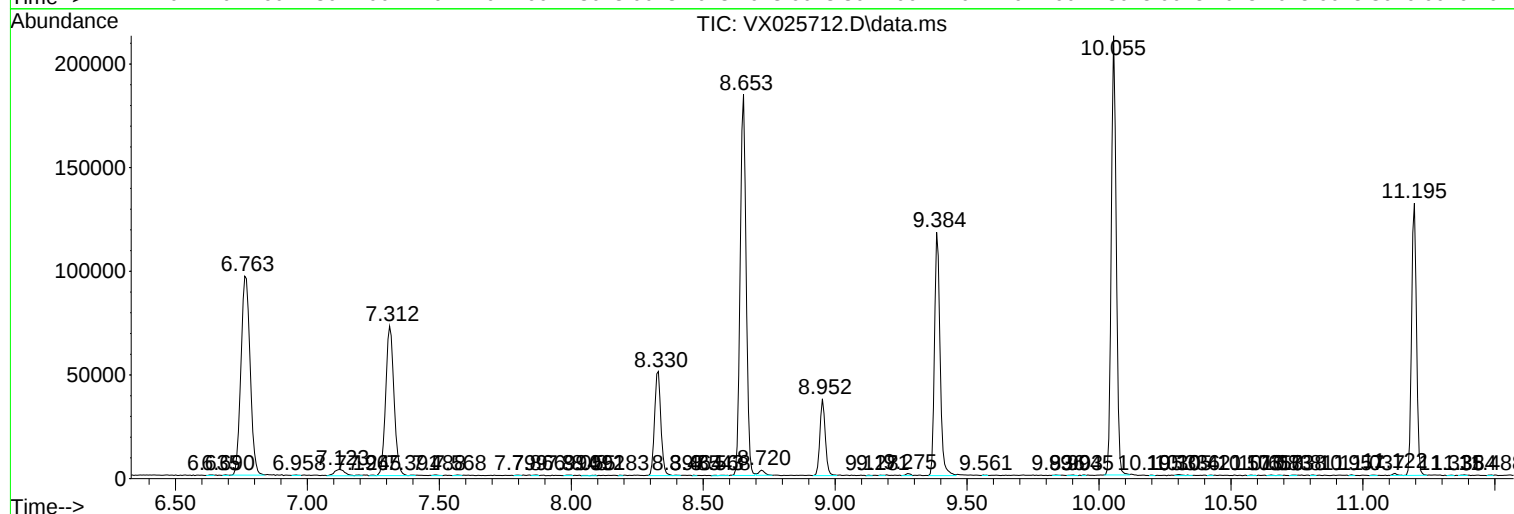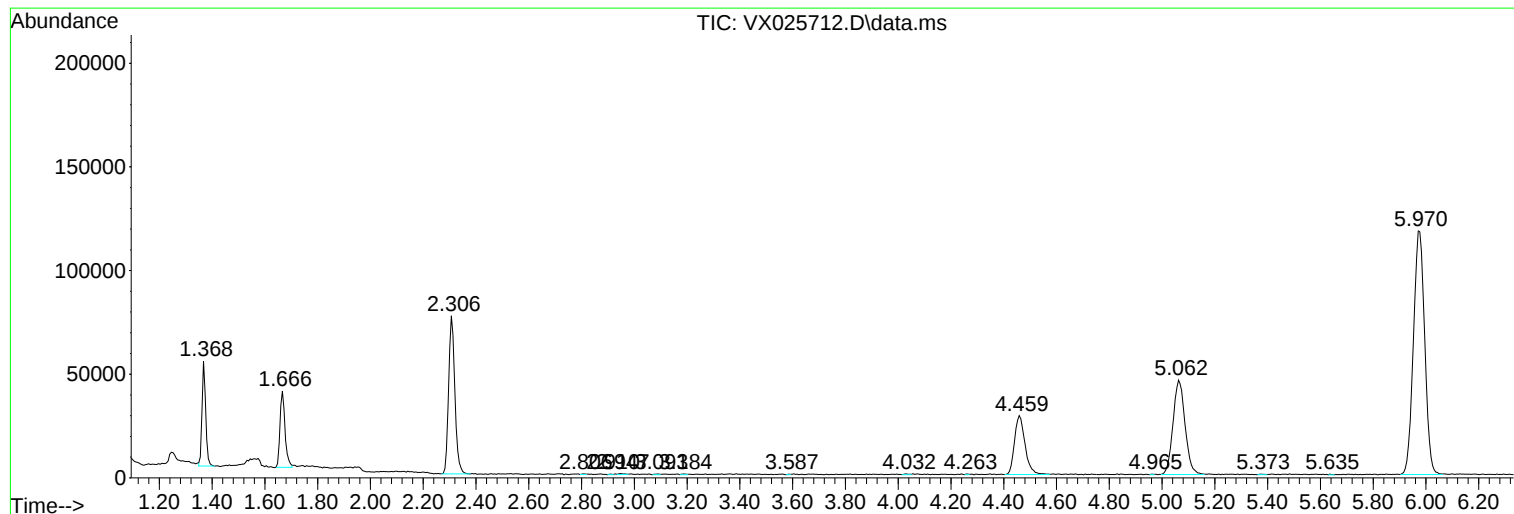

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025712.D
Acq On : 10 Dec 2021 19:34
Operator : JC/MD
Sample : M4981-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025712.D
Acq On : 10 Dec 2021 19:34
Operator : JC/MD
Sample : M4981-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
