

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025713.D
 Acq On : 10 Dec 2021 19:57
 Operator : JC/MD
 Sample : M4981-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	52	rVB	49806	47868	13.64%	1.730%
2	1.666	91	95	102	rBV	37835	48250	13.74%	1.744%
3	2.307	194	200	212	rVB	80909	125631	35.79%	4.541%
4	2.416	217	218	221	rBV	319	318	0.09%	0.011%
5	3.392	376	378	379	rBV	336	248	0.07%	0.009%
6	3.526	397	400	401	rVV2	286	264	0.08%	0.010%
7	3.575	406	408	410	rBV	264	252	0.07%	0.009%
8	3.751	436	437	440	rBV	274	266	0.08%	0.010%
9	3.806	444	446	449	rBV2	343	294	0.08%	0.011%
10	4.075	487	490	491	rBV2	334	366	0.10%	0.013%
11	4.245	515	518	521	rBV	211	313	0.09%	0.011%
12	4.300	526	527	530	rBV	288	240	0.07%	0.009%
13	4.459	544	553	565	rBV	26388	73423	20.91%	2.654%
14	4.922	627	629	634	rVB	304	411	0.12%	0.015%
15	5.062	640	652	668	rBV	46176	144138	41.06%	5.210%
16	5.294	687	690	691	rBV	341	356	0.10%	0.013%
17	5.519	725	727	730	rBV	240	321	0.09%	0.012%
18	5.842	778	780	781	rBV	274	238	0.07%	0.009%
19	5.977	790	802	818	rBV2	118538	351058	100.00%	12.689%
20	6.172	830	834	837	rBV	339	438	0.12%	0.016%
21	6.300	853	855	858	rVB	332	260	0.07%	0.009%
22	6.519	889	891	893	rBV	341	346	0.10%	0.013%
23	6.605	902	905	907	rVB	285	255	0.07%	0.009%
24	6.763	922	931	941	rVV	100188	236074	67.25%	8.533%
25	6.958	959	963	967	rBV3	286	509	0.14%	0.018%
26	7.056	978	979	982	rBV	361	263	0.07%	0.010%
27	7.111	982	988	997	rVV5	1800	4332	1.23%	0.157%
28	7.220	1004	1006	1008	rVB	286	260	0.07%	0.009%
29	7.251	1008	1011	1012	rBV2	245	275	0.08%	0.010%
30	7.312	1012	1021	1032	rVV	72590	158128	45.04%	5.716%
31	7.543	1056	1059	1062	rBV	371	515	0.15%	0.019%
32	7.757	1092	1094	1096	rVV	325	256	0.07%	0.009%
33	7.781	1096	1098	1103	rVB2	224	264	0.08%	0.010%
34	7.824	1103	1105	1109	rBV3	325	346	0.10%	0.013%
35	8.184	1162	1164	1165	rBV	361	248	0.07%	0.009%
36	8.263	1175	1177	1181	rBV2	253	322	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025713.D
 Acq On : 10 Dec 2021 19:57
 Operator : JC/MD
 Sample : M4981-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1200	rVV	51852	84395	24.04%	3.050%
38	8.531	1220	1221	1224	rBV	357	351	0.10%	0.013%
39	8.653	1234	1241	1248	rBV	185518	287358	81.85%	10.387%
40	8.775	1260	1261	1265	rBV2	266	302	0.09%	0.011%
41	8.952	1285	1290	1304	rVB	36051	52382	14.92%	1.893%
42	9.275	1341	1343	1347	rBV2	1118	1449	0.41%	0.052%
43	9.342	1350	1354	1356	rBV	316	314	0.09%	0.011%
44	9.385	1356	1361	1373	rBV	112774	164333	46.81%	5.940%
45	9.531	1384	1385	1388	rBV	213	274	0.08%	0.010%
46	9.933	1449	1451	1455	rVB2	369	301	0.09%	0.011%
47	10.055	1466	1471	1484	rVB	215840	287925	82.02%	10.407%
48	10.311	1510	1513	1514	rVB2	478	377	0.11%	0.014%
49	10.336	1514	1517	1520	rBV	308	368	0.10%	0.013%
50	10.573	1551	1556	1558	rVV2	245	348	0.10%	0.013%
51	10.787	1589	1591	1594	rVB	234	257	0.07%	0.009%
52	10.829	1594	1598	1601	rVB2	287	316	0.09%	0.011%
53	10.939	1615	1616	1620	rVB2	283	311	0.09%	0.011%
54	11.122	1643	1646	1650	rVB2	1079	1160	0.33%	0.042%
55	11.195	1652	1658	1669	rVB	134792	170849	48.67%	6.175%
56	11.274	1669	1671	1675	rVB2	289	286	0.08%	0.010%
57	11.317	1675	1678	1681	rVB3	489	588	0.17%	0.021%
58	11.354	1681	1684	1686	rBV	299	286	0.08%	0.010%
59	11.372	1686	1687	1690	rBV	302	344	0.10%	0.012%
60	11.750	1746	1749	1754	rVB3	773	1105	0.31%	0.040%
61	11.927	1776	1778	1783	rVB3	404	429	0.12%	0.016%
62	12.024	1789	1794	1807	rBV	216893	259280	73.86%	9.372%
63	12.323	1837	1843	1849	rVV	188578	240682	68.56%	8.699%
64	12.427	1857	1860	1862	rVB	580	633	0.18%	0.023%
65	12.469	1862	1867	1868	rBV2	269	427	0.12%	0.015%
66	12.555	1878	1881	1884	rBV	348	359	0.10%	0.013%
67	12.585	1884	1886	1889	rVV	219	236	0.07%	0.009%
68	12.664	1896	1899	1901	rBV2	311	335	0.10%	0.012%
69	12.744	1910	1912	1913	rBV	410	290	0.08%	0.010%
70	12.762	1913	1915	1918	rVB	285	270	0.08%	0.010%
71	12.841	1924	1928	1930	rVB	270	254	0.07%	0.009%
72	13.000	1952	1954	1956	rVB	385	272	0.08%	0.010%
73	13.030	1956	1959	1960	rBV	304	363	0.10%	0.013%
74	13.116	1970	1973	1975	rBV2	245	279	0.08%	0.010%
75	13.408	2019	2021	2024	rVB	347	266	0.08%	0.010%
76	13.536	2041	2042	2045	rVB2	266	241	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025713.D
 Acq On : 10 Dec 2021 19:57
 Operator : JC/MD
 Sample : M4981-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	13.695	2065	2068	2070	rBV	214	254	0.07%	0.009%
78	13.957	2108	2111	2113	rBV2	258	306	0.09%	0.011%
79	14.134	2137	2140	2143	rVB2	582	772	0.22%	0.028%
80	14.310	2165	2169	2171	rBV2	290	443	0.13%	0.016%
81	14.414	2185	2186	2190	rBV	236	242	0.07%	0.009%
82	14.469	2193	2195	2198	rVB2	246	264	0.08%	0.010%
83	14.493	2198	2199	2202	rBV2	279	245	0.07%	0.009%
84	14.646	2221	2224	2227	rBV	336	460	0.13%	0.017%
85	14.707	2230	2234	2237	rVV	253	418	0.12%	0.015%
86	14.768	2242	2244	2247	rVV2	236	264	0.08%	0.010%
87	14.829	2250	2254	2257	rBV	284	501	0.14%	0.018%
88	14.938	2268	2272	2275	rBV2	298	511	0.15%	0.018%
89	14.975	2275	2278	2279	rBV2	249	253	0.07%	0.009%
90	15.066	2290	2293	2295	rBV	323	343	0.10%	0.012%
91	15.170	2306	2310	2313	rBV3	367	620	0.18%	0.022%
92	15.213	2315	2317	2320	rBV3	306	446	0.13%	0.016%
93	15.322	2333	2335	2338	rVB	289	244	0.07%	0.009%
94	15.353	2338	2340	2343	rVB2	266	305	0.09%	0.011%
95	15.377	2343	2344	2346	rVB	499	340	0.10%	0.012%
96	15.408	2346	2349	2351	rBV	219	303	0.09%	0.011%
97	15.591	2378	2379	2381	rBV	335	241	0.07%	0.009%
98	15.920	2431	2433	2436	rBV2	251	294	0.08%	0.011%
99	16.255	2486	2488	2493	rVB2	244	251	0.07%	0.009%
100	16.408	2511	2513	2516	rBV2	258	364	0.10%	0.013%




Sum of corrected areas: 2766625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025713.D
Acq On : 10 Dec 2021 19:57
Operator : JC/MD
Sample : M4981-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

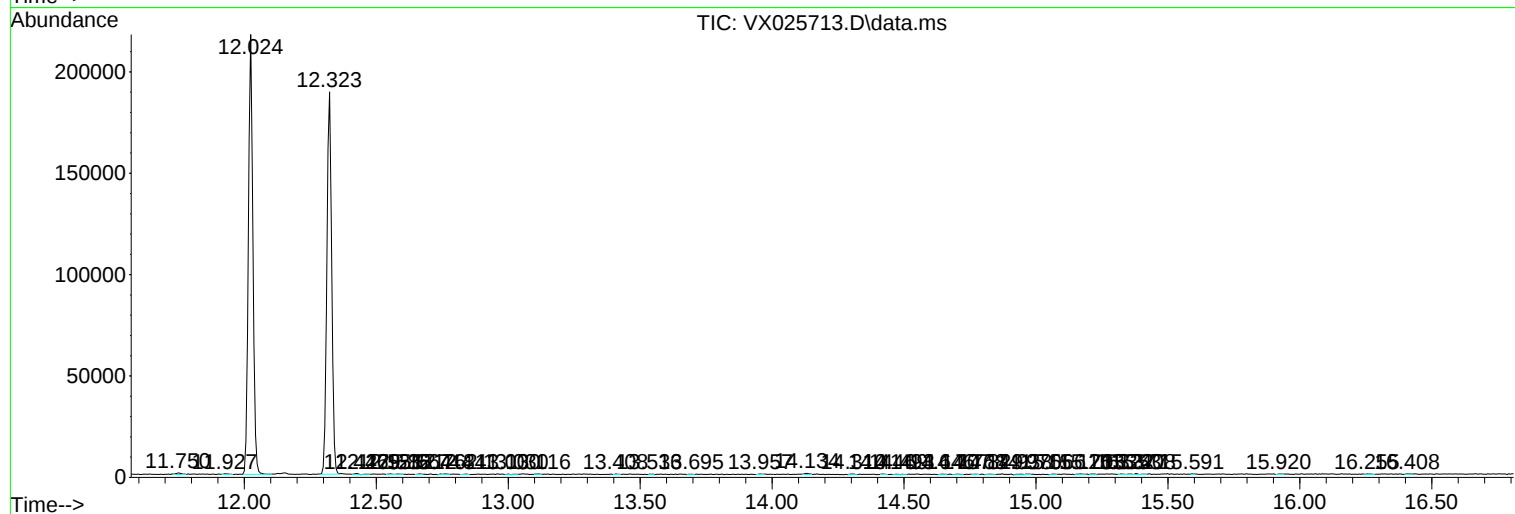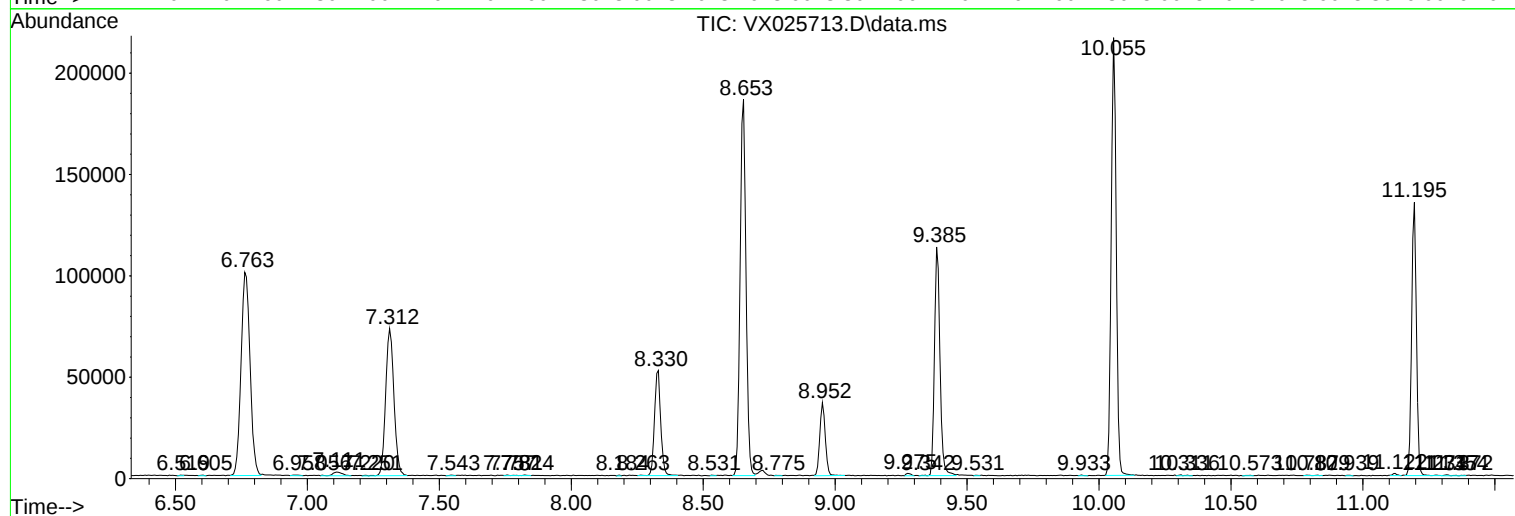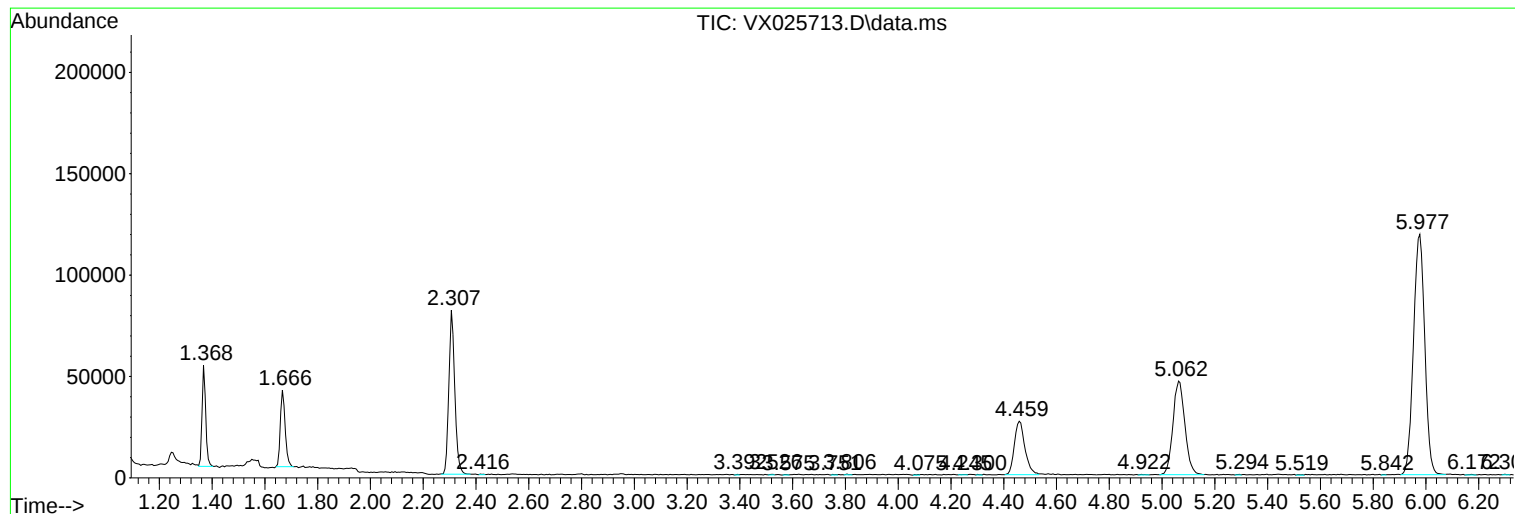

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025713.D
Acq On : 10 Dec 2021 19:57
Operator : JC/MD
Sample : M4981-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025713.D
Acq On : 10 Dec 2021 19:57
Operator : JC/MD
Sample : M4981-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc