

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025714.D
 Acq On : 10 Dec 2021 20:21
 Operator : JC/MD
 Sample : M4981-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	56	rVB	52379	49617	14.13%	1.569%
2	1.666	91	95	104	rBV	39694	50249	14.31%	1.589%
3	2.306	194	200	212	rBV2	78036	139226	39.66%	4.402%
4	2.581	243	245	247	rBV	323	316	0.09%	0.010%
5	2.751	270	273	275	rVB	363	424	0.12%	0.013%
6	2.788	275	279	280	rBV3	436	548	0.16%	0.017%
7	2.843	286	288	290	rBV2	209	222	0.06%	0.007%
8	2.953	303	306	310	rVB3	553	808	0.23%	0.026%
9	3.373	372	375	377	rBV2	166	221	0.06%	0.007%
10	3.416	380	382	383	rBV	425	355	0.10%	0.011%
11	3.611	407	414	418	rBV2	608	1062	0.30%	0.034%
12	3.830	447	450	451	rVB2	280	268	0.08%	0.008%
13	3.891	459	460	464	rVV	274	301	0.09%	0.010%
14	4.464	544	554	571	rVB2	29646	110880	31.58%	3.505%
15	4.574	571	572	574	rBV	362	256	0.07%	0.008%
16	4.599	574	576	579	rVV3	300	399	0.11%	0.013%
17	4.647	582	584	586	rBV2	283	305	0.09%	0.010%
18	4.757	600	602	605	rVB2	266	248	0.07%	0.008%
19	4.812	610	611	615	rBV2	261	395	0.11%	0.012%
20	4.946	631	633	635	rBV2	228	239	0.07%	0.008%
21	5.062	641	652	669	rBV	46633	144286	41.10%	4.562%
22	5.269	683	686	687	rVB2	262	268	0.08%	0.008%
23	5.306	690	692	695	rVB	287	313	0.09%	0.010%
24	5.336	695	697	698	rBV2	353	373	0.11%	0.012%
25	5.385	698	705	715	rVB3	4176	11890	3.39%	0.376%
26	5.580	735	737	740	rVV	259	282	0.08%	0.009%
27	5.708	756	758	759	rBV	346	287	0.08%	0.009%
28	5.794	769	772	775	rBV	302	315	0.09%	0.010%
29	5.976	790	802	817	rBV2	119112	351059	100.00%	11.099%
30	6.507	887	889	891	rVB	387	292	0.08%	0.009%
31	6.531	891	893	896	rBV	466	493	0.14%	0.016%
32	6.763	923	931	943	rVV	95902	227512	64.81%	7.193%
33	6.982	964	967	968	rBV	307	279	0.08%	0.009%
34	7.043	975	977	980	rBV	264	284	0.08%	0.009%
35	7.129	982	991	1002	rBV	160597	346540	98.71%	10.956%
36	7.312	1012	1021	1031	rBV2	71322	156302	44.52%	4.941%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025714.D
 Acq On : 10 Dec 2021 20:21
 Operator : JC/MD
 Sample : M4981-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COCN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.488	1048	1050	1052	rVB2	303	202	0.06%	0.006%
38	7.598	1067	1068	1072	rBV	403	371	0.11%	0.012%
39	8.104	1148	1151	1152	rBV2	239	210	0.06%	0.007%
40	8.330	1182	1188	1201	rVB	50974	83001	23.64%	2.624%
41	8.592	1229	1231	1234	rVB	211	221	0.06%	0.007%
42	8.653	1234	1241	1248	rBV	184060	288895	82.29%	9.133%
43	8.726	1248	1253	1258	rVB2	2484	4451	1.27%	0.141%
44	8.951	1285	1290	1297	rBV	36500	52524	14.96%	1.661%
45	9.092	1311	1313	1315	rVB	371	223	0.06%	0.007%
46	9.153	1317	1323	1325	rBV	260	418	0.12%	0.013%
47	9.226	1333	1335	1336	rBV	274	223	0.06%	0.007%
48	9.281	1340	1344	1346	rBV	963	1168	0.33%	0.037%
49	9.384	1356	1361	1375	rBV	120331	173148	49.32%	5.474%
50	9.543	1385	1387	1389	rBV2	232	241	0.07%	0.008%
51	9.951	1451	1454	1455	rBV	245	215	0.06%	0.007%
52	10.055	1466	1471	1488	rVB	207509	279427	79.60%	8.834%
53	10.171	1488	1490	1491	rBV	289	270	0.08%	0.009%
54	10.311	1510	1513	1515	rVB2	453	554	0.16%	0.018%
55	10.463	1534	1538	1540	rBV2	184	263	0.07%	0.008%
56	10.537	1548	1550	1553	rBV	255	296	0.08%	0.009%
57	10.646	1566	1568	1570	rVB	365	253	0.07%	0.008%
58	10.707	1576	1578	1581	rVB	354	267	0.08%	0.008%
59	10.732	1581	1582	1585	rBV	277	294	0.08%	0.009%
60	10.939	1614	1616	1617	rBV2	312	226	0.06%	0.007%
61	11.061	1634	1636	1638	rVB	386	257	0.07%	0.008%
62	11.122	1643	1646	1650	rVV	1098	1105	0.31%	0.035%
63	11.195	1653	1658	1666	rVV	145831	174896	49.82%	5.529%
64	11.652	1731	1733	1736	rVB	400	301	0.09%	0.010%
65	11.689	1736	1739	1740	rBV	300	342	0.10%	0.011%
66	11.744	1746	1748	1752	rBV2	923	1288	0.37%	0.041%
67	11.933	1777	1779	1784	rVB2	660	742	0.21%	0.023%
68	11.981	1784	1787	1789	rBV	224	348	0.10%	0.011%
69	12.024	1789	1794	1802	rVV	199630	248901	70.90%	7.869%
70	12.109	1806	1808	1809	rBV	327	240	0.07%	0.008%
71	12.152	1813	1815	1819	rVB2	930	1030	0.29%	0.033%
72	12.323	1837	1843	1850	rBV	192827	240222	68.43%	7.594%
73	12.670	1898	1900	1903	rBV2	331	361	0.10%	0.011%
74	12.743	1910	1912	1914	rBV	297	322	0.09%	0.010%
75	12.902	1937	1938	1941	rBV2	245	249	0.07%	0.008%
76	13.365	2012	2014	2019	rBB	206	258	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025714.D
 Acq On : 10 Dec 2021 20:21
 Operator : JC/MD
 Sample : M4981-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	13.560	2045	2046	2051	rVB	290	215	0.06%	0.007%
78	13.768	2077	2080	2083	rVB2	317	392	0.11%	0.012%
79	13.963	2110	2112	2115	rBV2	216	263	0.07%	0.008%
80	14.097	2133	2134	2137	rBV	302	321	0.09%	0.010%
81	14.133	2137	2140	2143	rVB2	498	713	0.20%	0.023%
82	14.322	2169	2171	2173	rBV	259	222	0.06%	0.007%
83	14.347	2173	2175	2177	rBV2	212	213	0.06%	0.007%
84	14.402	2182	2184	2187	rBV	255	338	0.10%	0.011%
85	14.432	2187	2189	2192	rVB	256	220	0.06%	0.007%
86	14.737	2236	2239	2240	rBV	335	332	0.09%	0.010%
87	14.859	2255	2259	2260	rBV	312	363	0.10%	0.011%
88	14.908	2266	2267	2269	rBV	264	203	0.06%	0.006%
89	14.981	2277	2279	2282	rBV2	392	407	0.12%	0.013%
90	15.060	2290	2292	2294	rVV	287	243	0.07%	0.008%
91	15.225	2317	2319	2322	rVB	307	226	0.06%	0.007%
92	15.341	2336	2338	2340	rVB3	246	215	0.06%	0.007%
93	15.365	2340	2342	2345	rBV	278	374	0.11%	0.012%
94	15.542	2369	2371	2373	rVB2	478	422	0.12%	0.013%
95	15.566	2373	2375	2376	rBV	324	240	0.07%	0.008%
96	15.694	2394	2396	2400	rBV2	288	455	0.13%	0.014%
97	16.304	2494	2496	2499	rVB3	301	278	0.08%	0.009%
98	16.383	2507	2509	2511	rBV	365	416	0.12%	0.013%
99	16.450	2518	2520	2522	rBV	318	269	0.08%	0.009%
100	16.572	2538	2540	2543	rVB2	373	432	0.12%	0.014%


Sum of corrected areas: 3163109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025714.D
Acq On : 10 Dec 2021 20:21
Operator : JC/MD
Sample : M4981-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

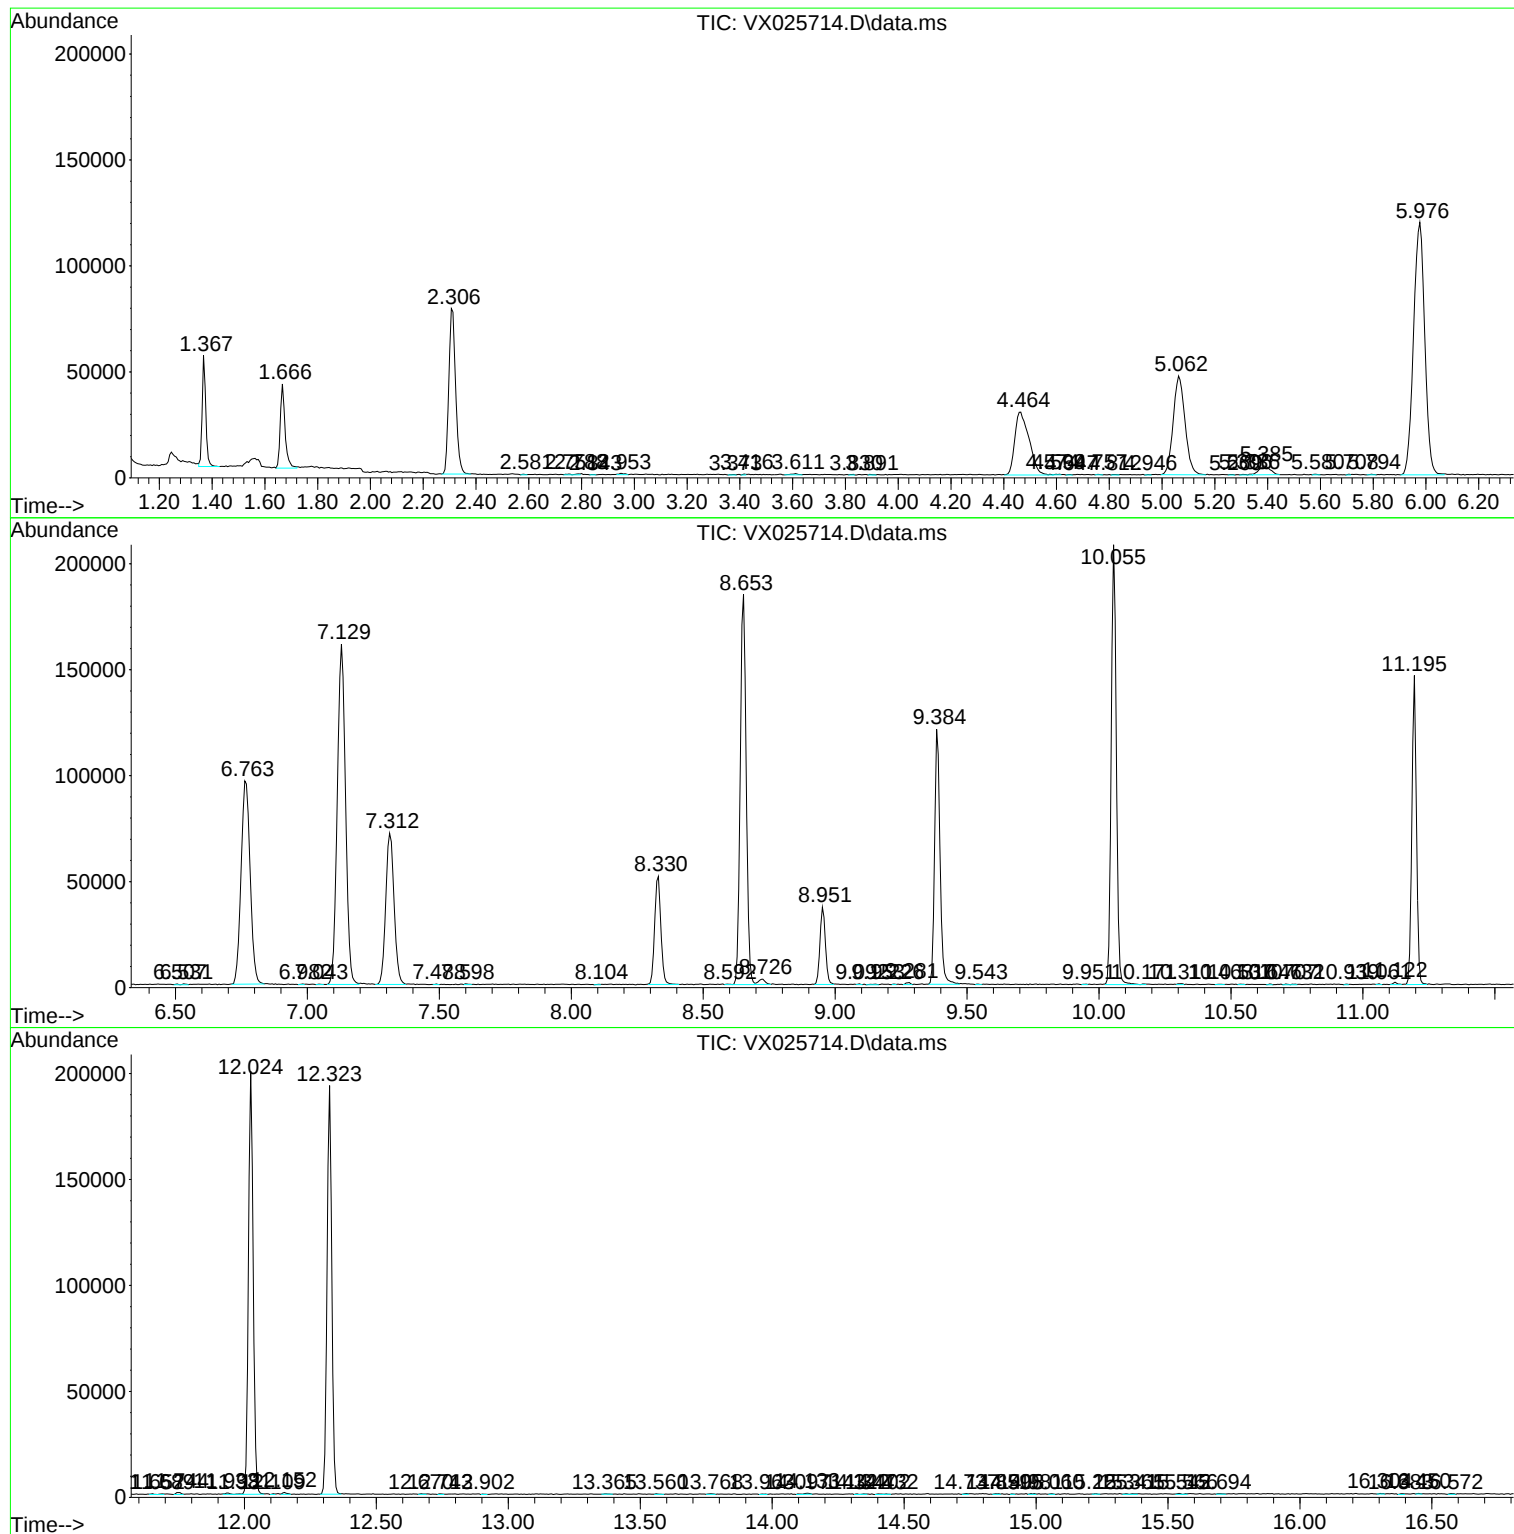

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025714.D
Acq On : 10 Dec 2021 20:21
Operator : JC/MD
Sample : M4981-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025714.D
Acq On : 10 Dec 2021 20:21
Operator : JC/MD
Sample : M4981-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc