

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025723.D
 Acq On : 10 Dec 2021 23:51
 Operator : JC/MD
 Sample : M4981-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	47844	44791	13.61%	1.720%
2	1.666	91	95	106	rVB	37161	46632	14.16%	1.791%
3	2.307	194	200	210	rVB	72701	115103	34.96%	4.420%
4	2.709	263	266	268	rVV2	380	292	0.09%	0.011%
5	2.739	268	271	274	rVB2	323	328	0.10%	0.013%
6	2.941	300	304	306	rBV2	436	494	0.15%	0.019%
7	3.136	334	336	339	rVB	271	262	0.08%	0.010%
8	3.160	339	340	343	rBV	288	235	0.07%	0.009%
9	3.629	414	417	419	rVB2	223	209	0.06%	0.008%
10	3.697	424	428	429	rBV	295	389	0.12%	0.015%
11	3.788	439	443	445	rBV2	257	259	0.08%	0.010%
12	3.989	471	476	477	rBV2	175	264	0.08%	0.010%
13	4.032	480	483	485	rBV2	252	379	0.12%	0.015%
14	4.117	495	497	500	rVB	203	215	0.07%	0.008%
15	4.154	501	503	505	rVB	294	234	0.07%	0.009%
16	4.178	505	507	508	rBV2	240	253	0.08%	0.010%
17	4.263	519	521	522	rVB	360	206	0.06%	0.008%
18	4.459	544	553	565	rBV	26437	73432	22.31%	2.820%
19	4.635	581	582	587	rVV3	222	379	0.12%	0.015%
20	4.702	591	593	595	rVV	245	274	0.08%	0.011%
21	4.922	627	629	632	rVB2	273	257	0.08%	0.010%
22	5.062	641	652	666	rVV	43929	135774	41.24%	5.214%
23	5.343	696	698	700	rBV2	337	272	0.08%	0.010%
24	5.519	723	727	728	rBV2	233	338	0.10%	0.013%
25	5.568	732	735	736	rVB	300	272	0.08%	0.010%
26	5.635	744	746	748	rVB2	350	226	0.07%	0.009%
27	5.660	748	750	752	rBV	195	233	0.07%	0.009%
28	5.897	786	789	790	rBV	301	292	0.09%	0.011%
29	5.977	790	802	816	rBV2	111462	329216	100.00%	12.643%
30	6.141	827	829	832	rVB2	287	320	0.10%	0.012%
31	6.257	847	848	851	rBV	217	215	0.07%	0.008%
32	6.483	882	885	888	rVV2	191	250	0.08%	0.010%
33	6.544	891	895	898	rBV	229	250	0.08%	0.010%
34	6.684	916	918	920	rVB	300	213	0.06%	0.008%
35	6.763	920	931	944	rBV	91808	219748	66.75%	8.439%
36	7.123	983	990	999	rVB5	6437	15016	4.56%	0.577%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025723.D
 Acq On : 10 Dec 2021 23:51
 Operator : JC/MD
 Sample : M4981-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.312	1013	1021	1032	rVB	68533	147911	44.93%	5.680%
38	7.476	1042	1048	1055	rBV2	244	725	0.22%	0.028%
39	7.549	1055	1060	1065	rVB2	333	589	0.18%	0.023%
40	7.806	1101	1102	1104	rVB	320	224	0.07%	0.009%
41	7.909	1116	1119	1120	rVB	332	273	0.08%	0.010%
42	7.921	1120	1121	1124	rBV	301	270	0.08%	0.010%
43	8.330	1181	1188	1195	rBV	46362	77649	23.59%	2.982%
44	8.470	1210	1211	1214	rBV	298	273	0.08%	0.010%
45	8.580	1227	1229	1231	rBV2	212	241	0.07%	0.009%
46	8.653	1234	1241	1248	rBV	173678	271624	82.51%	10.431%
47	8.787	1261	1263	1265	rBV2	212	234	0.07%	0.009%
48	8.952	1285	1290	1297	rBV	34475	48558	14.75%	1.865%
49	9.104	1313	1315	1319	rVB	322	311	0.09%	0.012%
50	9.275	1341	1343	1347	rVV2	539	605	0.18%	0.023%
51	9.385	1356	1361	1374	rBV	111219	163478	49.66%	6.278%
52	9.519	1381	1383	1385	rBV	259	204	0.06%	0.008%
53	9.720	1413	1416	1419	rBV	219	299	0.09%	0.011%
54	9.945	1448	1453	1457	rBV	349	539	0.16%	0.021%
55	10.055	1466	1471	1486	rVV	203735	267944	81.39%	10.290%
56	10.153	1486	1487	1490	rVB2	312	203	0.06%	0.008%
57	10.299	1505	1511	1514	rBV3	567	930	0.28%	0.036%
58	10.390	1524	1526	1528	rBV2	244	227	0.07%	0.009%
59	10.488	1540	1542	1545	rBV	264	346	0.11%	0.013%
60	10.866	1600	1604	1606	rBV2	235	356	0.11%	0.014%
61	10.939	1613	1616	1617	rBV	387	368	0.11%	0.014%
62	10.957	1617	1619	1621	rVV	268	237	0.07%	0.009%
63	11.018	1628	1629	1633	rVV	288	315	0.10%	0.012%
64	11.122	1643	1646	1650	rVV4	723	1012	0.31%	0.039%
65	11.195	1652	1658	1665	rVV	128516	161284	48.99%	6.194%
66	11.287	1670	1673	1675	rBV2	248	365	0.11%	0.014%
67	11.500	1706	1708	1710	rVV	280	279	0.08%	0.011%
68	11.561	1717	1718	1721	rBV	177	212	0.06%	0.008%
69	11.683	1736	1738	1741	rVB2	279	293	0.09%	0.011%
70	11.750	1746	1749	1752	rVB4	837	926	0.28%	0.036%
71	11.933	1777	1779	1783	rVB3	363	447	0.14%	0.017%
72	12.024	1789	1794	1805	rVB	188215	233735	71.00%	8.976%
73	12.134	1810	1812	1814	rBV	375	376	0.11%	0.014%
74	12.183	1818	1820	1823	rBV	192	250	0.08%	0.010%
75	12.238	1827	1829	1831	rBV2	214	206	0.06%	0.008%
76	12.323	1837	1843	1850	rBV	177089	225153	68.39%	8.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025723.D
 Acq On : 10 Dec 2021 23:51
 Operator : JC/MD
 Sample : M4981-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.427	1857	1860	1863	rVB	479	515	0.16%	0.020%
78	12.488	1863	1870	1871	rBV	401	598	0.18%	0.023%
79	12.530	1875	1877	1880	rBV	237	270	0.08%	0.010%
80	12.799	1919	1921	1924	rVV2	244	262	0.08%	0.010%
81	12.981	1948	1951	1953	rBV2	195	289	0.09%	0.011%
82	13.183	1983	1984	1987	rVB	304	265	0.08%	0.010%
83	13.213	1987	1989	1991	rVB	296	238	0.07%	0.009%
84	13.244	1991	1994	1995	rBV2	222	302	0.09%	0.012%
85	13.280	1999	2000	2004	rVB	307	227	0.07%	0.009%
86	13.512	2037	2038	2041	rBV2	242	296	0.09%	0.011%
87	14.030	2121	2123	2124	rBV	402	237	0.07%	0.009%
88	14.054	2126	2127	2129	rVB	356	214	0.07%	0.008%
89	14.079	2129	2131	2133	rVB	237	223	0.07%	0.009%
90	14.109	2133	2136	2137	rBV	275	271	0.08%	0.010%
91	14.134	2138	2140	2143	rVB2	457	385	0.12%	0.015%
92	14.317	2168	2170	2173	rVB	332	342	0.10%	0.013%
93	14.481	2195	2197	2198	rBV	221	204	0.06%	0.008%
94	14.579	2211	2213	2215	rBV	346	251	0.08%	0.010%
95	14.597	2215	2216	2217	rBV	389	212	0.06%	0.008%
96	14.646	2222	2224	2227	rBV2	197	213	0.06%	0.008%
97	14.914	2266	2268	2270	rBV2	192	203	0.06%	0.008%
98	14.987	2278	2280	2282	rBV	287	293	0.09%	0.011%
99	16.030	2449	2451	2454	rBV3	284	285	0.09%	0.011%
100	16.566	2537	2539	2541	rBV	403	304	0.09%	0.012%




Sum of corrected areas: 2603892

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025723.D
Acq On : 10 Dec 2021 23:51
Operator : JC/MD
Sample : M4981-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

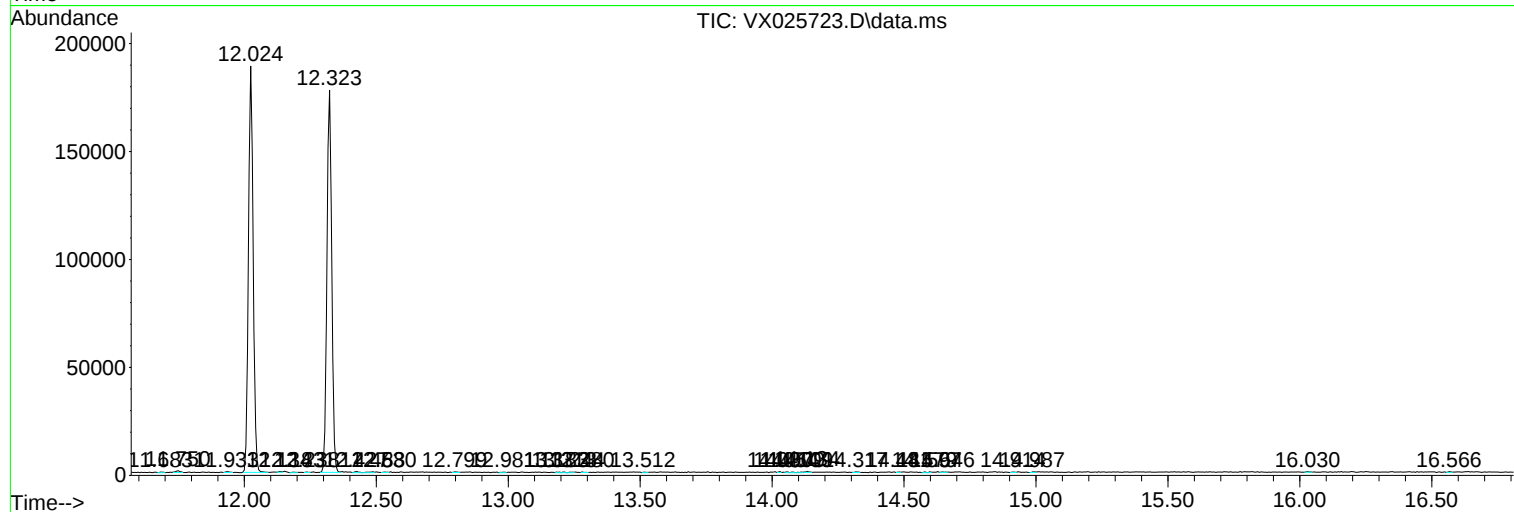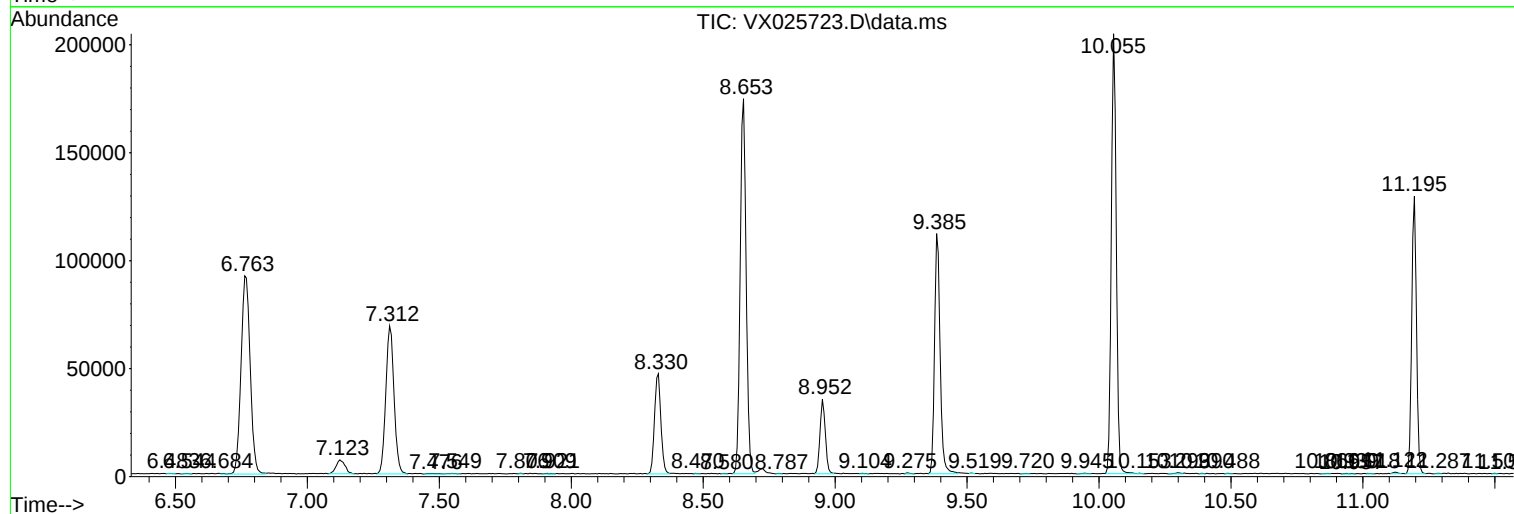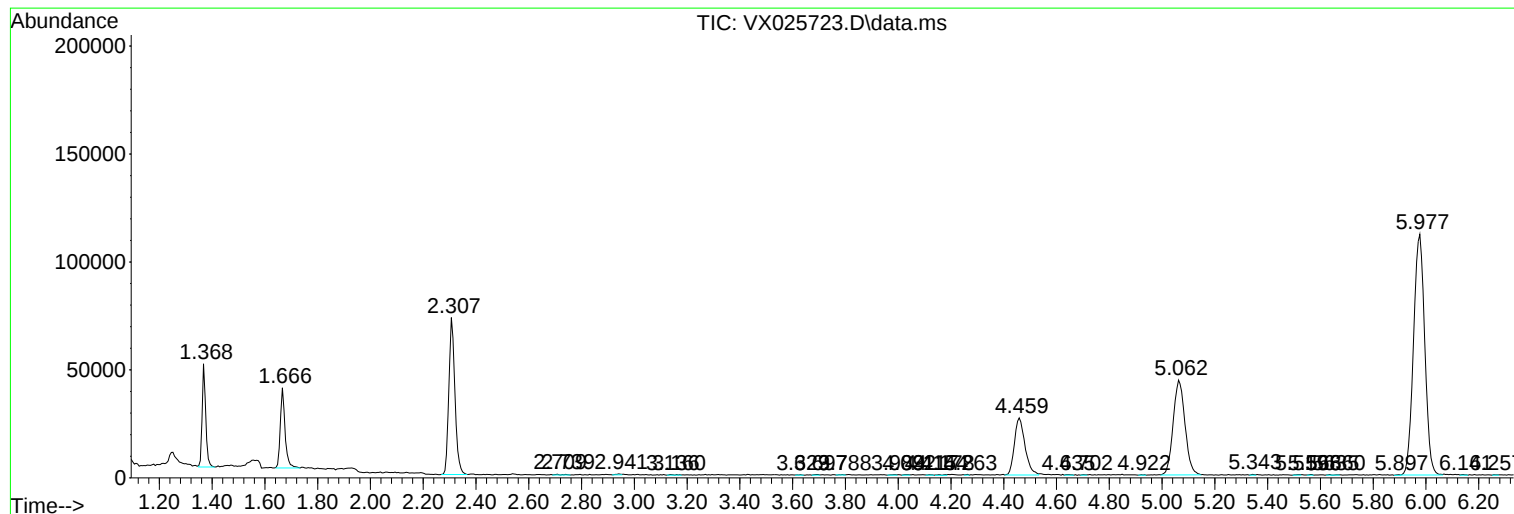

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025723.D
Acq On : 10 Dec 2021 23:51
Operator : JC/MD
Sample : M4981-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
Data File : VX025723.D
Acq On : 10 Dec 2021 23:51
Operator : JC/MD
Sample : M4981-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc