
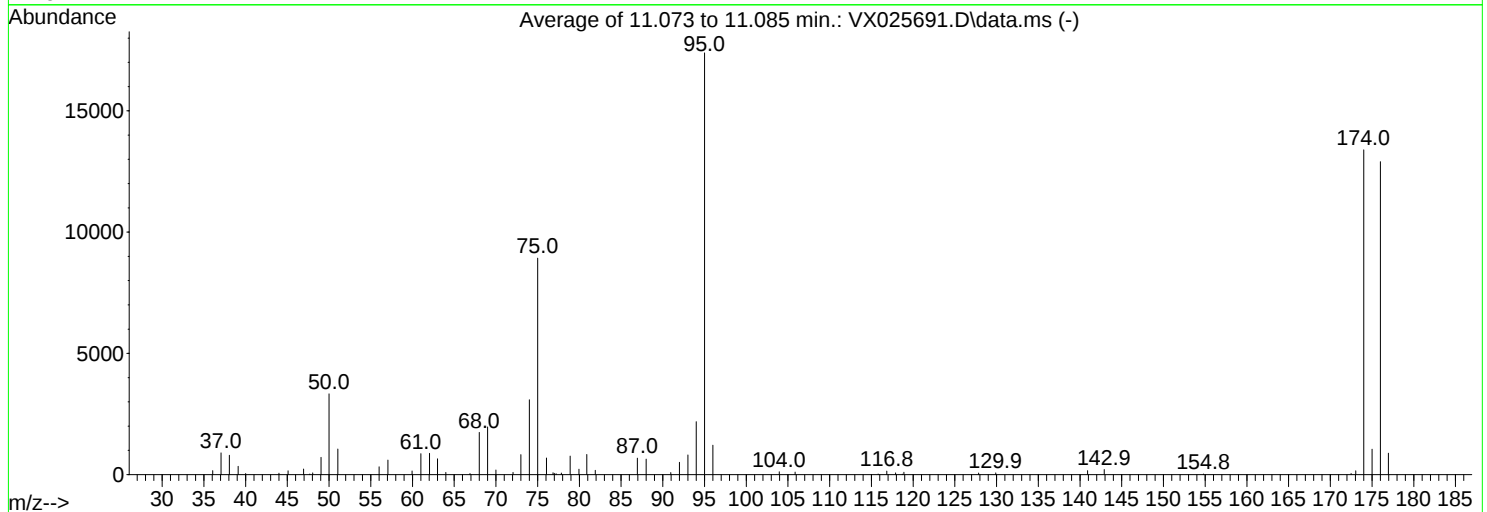


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121021\
 Data File : VX025691.D
 Acq On : 10 Dec 2021 10:01
 Operator : JC/MD
 Sample : BFB622
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB622

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Sun Dec 12 06:39:29 2021

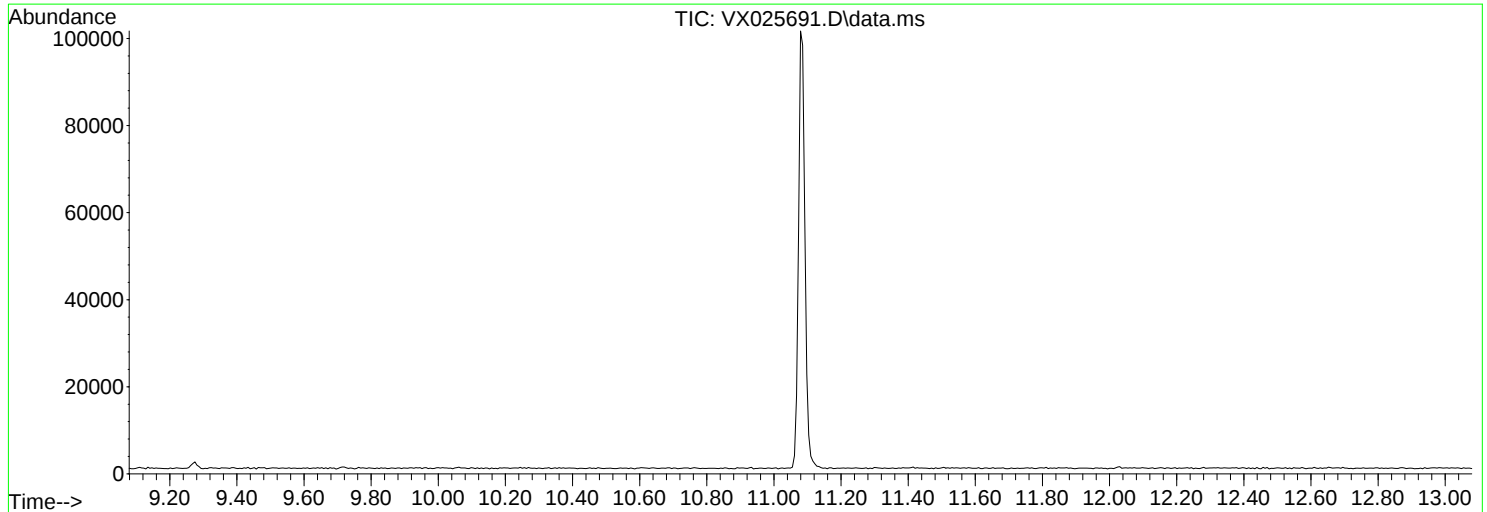

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	3334	PASS
75	95	30	80	51.3	8925	PASS
95	95	100	100	100.0	17391	PASS
96	95	5	9	7.0	1211	PASS
173	174	0.00	2	1.2	159	PASS
174	95	50	120	77.0	13390	PASS
175	174	5	9	7.8	1051	PASS
176	174	95	101	96.4	12905	PASS
177	176	5	9	6.8	882	PASS

m/z	Abundance
40.00	1156.0
43.90	89.0
44.20	99.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.10	116.0
37.10	671.0
38.10	618.0
39.00	282.0
40.00	1222.0
44.00	236.0
45.20	103.0
46.90	143.0
47.70	79.0
49.10	490.0
50.00	2653.0
51.00	840.0
56.00	215.0
57.00	428.0
59.90	117.0
61.00	723.0
62.00	602.0
63.00	541.0
64.10	72.0
68.00	1240.0
69.00	1353.0
70.00	131.0
72.10	70.0
73.00	588.0
74.00	2267.0
75.00	6330.0
76.00	552.0
76.90	114.0
77.90	72.0
78.90	520.0
79.90	145.0
80.90	536.0
82.00	132.0
86.90	436.0
88.00	395.0
91.00	69.0
92.00	355.0
93.00	583.0
94.00	1493.0
95.00	11932.0
96.00	934.0
104.00	77.0
105.80	57.0
116.80	107.0
118.70	61.0
127.80	50.0
129.90	53.0
140.90	161.0
142.90	127.0
173.10	116.0
174.00	7478.0
175.00	675.0
176.00	6979.0
177.00	529.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.00	189.0
37.00	1068.0
38.00	971.0
39.10	363.0
40.00	1227.0
44.00	232.0
45.10	203.0
47.00	299.0
48.00	113.0
49.00	899.0
50.00	3996.0
51.10	1255.0
56.00	350.0
57.00	750.0
60.00	197.0
61.00	993.0
62.00	1120.0
63.00	710.0
64.00	104.0
66.90	77.0
68.00	2175.0
69.00	2411.0
70.00	241.0
72.00	115.0
73.00	1052.0
74.00	3643.0
75.00	10798.0
76.10	826.0
76.80	117.0
77.20	122.0
77.90	70.0
78.90	985.0
80.00	288.0
80.90	946.0
81.80	179.0
87.00	826.0
88.00	771.0
90.90	118.0
91.90	613.0
93.00	985.0
94.00	2534.0
95.00	20904.0
96.00	1437.0
103.90	171.0
105.80	77.0
115.80	80.0
116.90	150.0
118.00	83.0
118.90	170.0
127.90	68.0
130.00	62.0
141.00	210.0
142.90	223.0
172.50	135.0
173.00	149.0
174.00	15419.0
175.00	1190.0
176.00	15296.0
176.90	963.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.10	191.0
37.00	947.0
38.00	799.0
39.20	384.0
40.00	1155.0
44.00	271.0
45.00	171.0
47.00	254.0
48.10	115.0
49.00	746.0
50.00	3353.0
51.00	1075.0
56.00	400.0
57.10	630.0
60.00	146.0
61.00	874.0
62.10	912.0
63.00	716.0
63.90	99.0
66.90	64.0
68.00	1802.0
69.00	2141.0
70.00	194.0
72.00	95.0
73.00	845.0
74.00	3353.0
75.00	9646.0
76.10	678.0
77.00	153.0
77.80	57.0
78.90	795.0
80.00	239.0
80.90	1005.0
81.90	232.0
87.00	775.0
88.00	754.0
91.00	75.0
92.10	553.0
93.00	863.0
94.00	2525.0
95.00	19336.0
96.00	1263.0
103.90	119.0
105.90	176.0
116.80	176.0
117.80	137.0
118.90	131.0
127.90	72.0
129.80	96.0
140.80	132.0
142.90	291.0
154.80	75.0
173.10	213.0
174.00	17272.0
175.00	1287.0
176.00	16440.0
176.90	1153.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622