

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
 Data File : VX044198.D
 Acq On : 10 Dec 2024 11:12
 Operator : JC/MD
 Sample : VX1210MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1210MBL01

Quant Time: Dec 11 01:27:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	105651	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	206502	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178441	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	71191	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	92333	50.954	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.900%
35) Dibromofluoromethane	5.379	113	67329	45.629	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.260%
50) Toluene-d8	8.647	98	249762	49.104	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.200%
62) 4-Bromofluorobenzene	11.079	95	80415	46.455	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	92.900%
Target Compounds						
					Qvalue	
5) Bromomethane	1.599	94	904	0.981	ug/l	95
6) Chloroethane	1.672	64	211	0.231	ug/l #	42
11) Tert butyl alcohol	2.941	59	1358	4.669	ug/l #	73
13) Acrolein	2.227	56	279	0.910	ug/l	89
14) Allyl chloride	2.654	41	525	0.264	ug/l #	44
15) Acrylonitrile	3.075	53	206	0.291	ug/l #	1
16) Acetone	2.386	43	1079	1.296	ug/l #	88
17) Carbon Disulfide	2.495	76	1511	0.602	ug/l	95
18) Methyl Acetate	2.703	43	509	0.263	ug/l #	69
20) Methylene Chloride	2.782	84	456	0.323	ug/l #	66
21) trans-1,2-Dichloroethene	3.087	96	460	0.366	ug/l	88
31) Cyclohexane	5.538	56	3318	1.643	ug/l #	36
36) 1,1-Dichloropropene	5.538	75	9562	5.200	ug/l #	52
38) Carbon Tetrachloride	5.538	117	12229	5.919	ug/l #	15
44) Trichloroethene	7.129	130	471	0.290	ug/l	71
49) 1,4-Dioxane	7.714	88	21	0.676	ug/l #	30
51) 4-Methyl-2-Pentanone	8.592	43	630	0.284	ug/l #	37
68) m/p-Xylenes	10.305	106	656	0.265	ug/l	90
71) Bromoform	10.811	173	79	1.289	ug/l #	29
76) 1,2,3-Trichloropropane	11.079	75	46550	29.817	ug/l #	34
77) Bromobenzene	11.201	156	265	0.203	ug/l	81
81) trans-1,4-Dichloro-2-b...	11.079	75	46550	81.363	ug/l #	7
82) 4-Chlorotoluene	11.469	91	1060	0.243	ug/l	74
87) 1,3-Dichlorobenzene	11.975	146	887	0.373	ug/l	88
88) 1,4-Dichlorobenzene	11.975	146	887	0.366	ug/l	90
89) n-Butylbenzene	12.341	91	875	0.223	ug/l #	85
91) 1,2-Dichlorobenzene	12.341	146	556	0.232	ug/l	88
93) 1,2,4-Trichlorobenzene	13.597	180	694	0.491	ug/l	96
95) Naphthalene	13.780	128	4203	0.825	ug/l #	92
96) 1,2,3-Trichlorobenzene	13.963	180	746	0.521	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044198.D
Acq On : 10 Dec 2024 11:12
Operator : JC/MD
Sample : VX1210MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01

Quant Time: Dec 11 01:27:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration




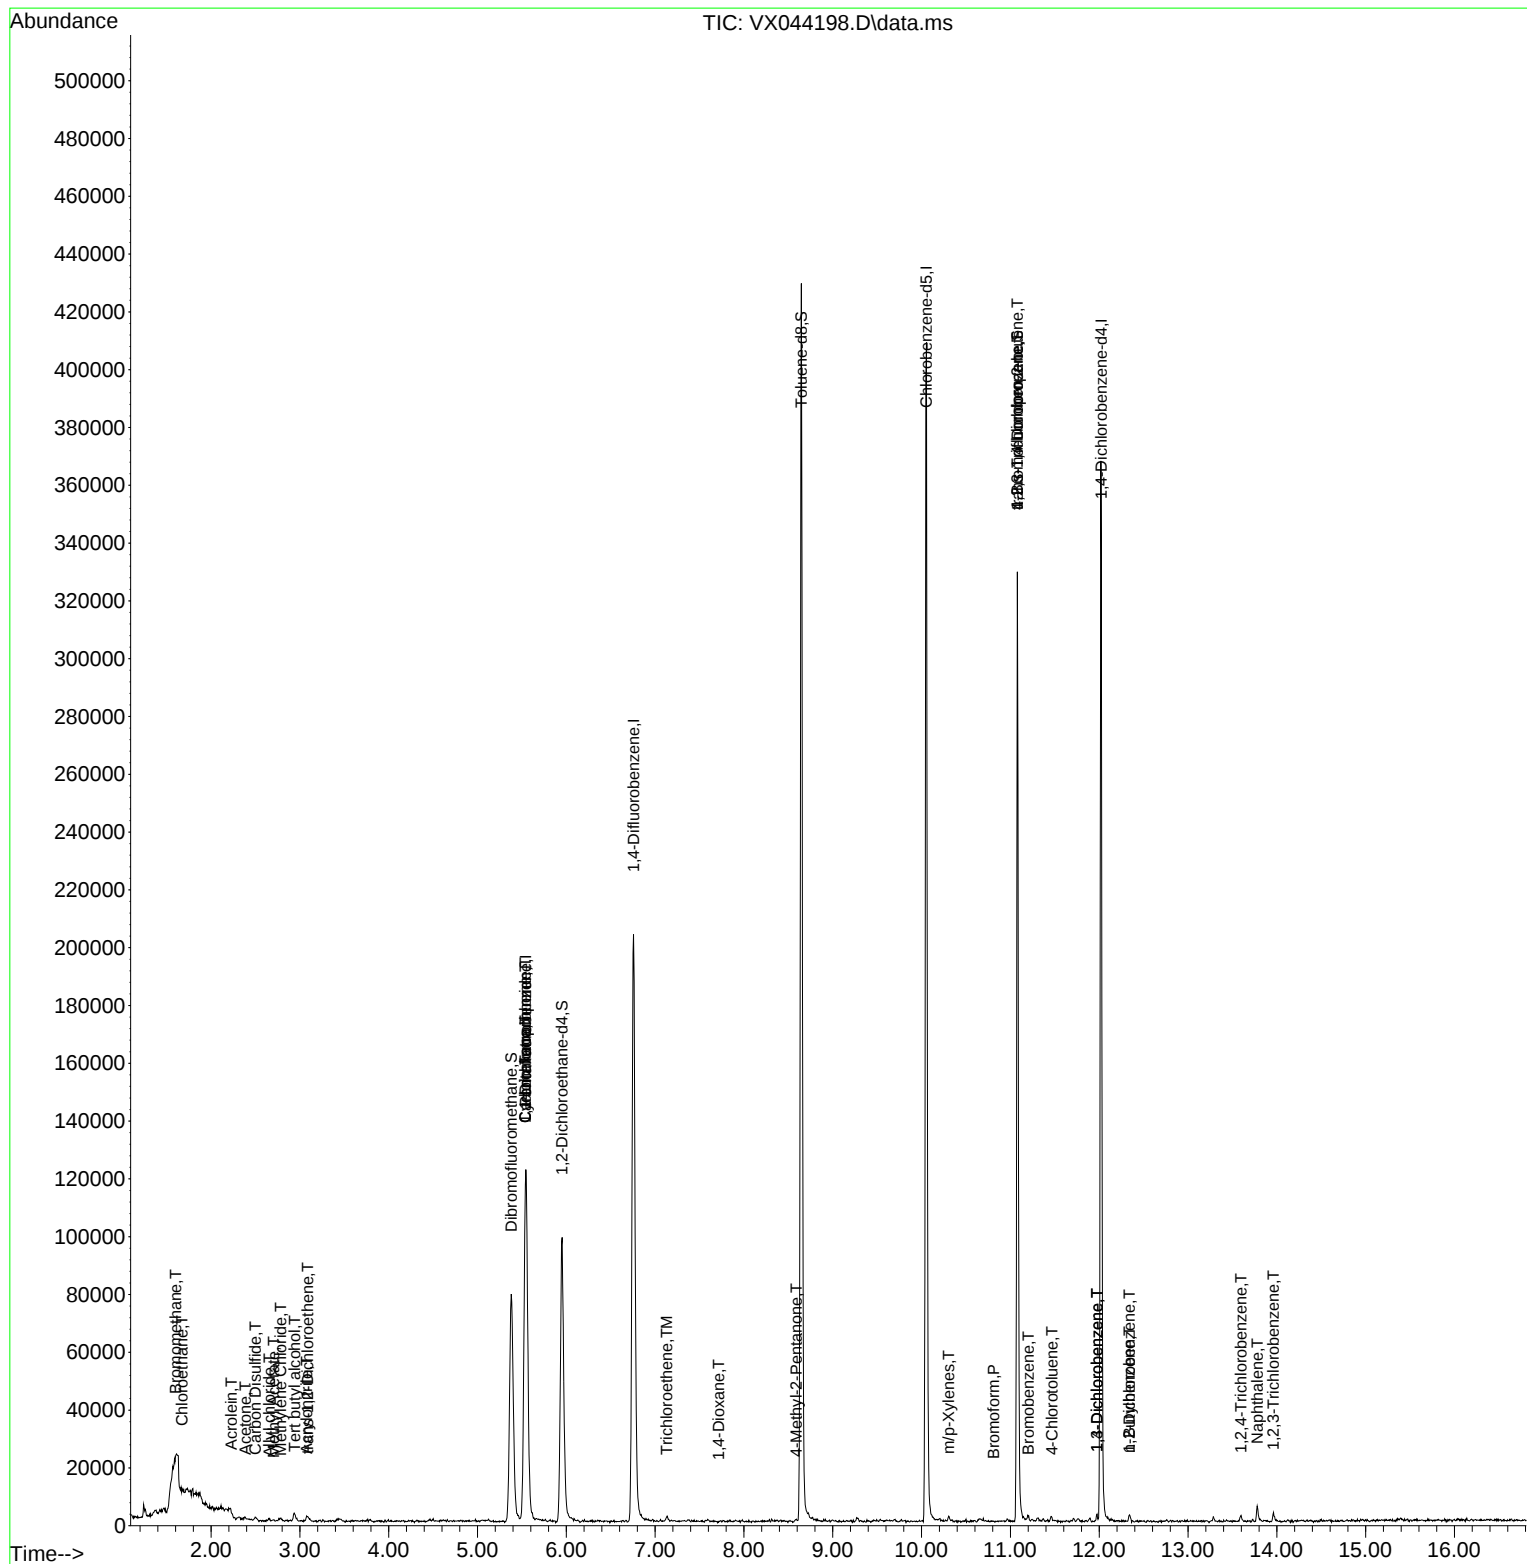




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:168 Resp: 105651
Ion Ratio Lower Upper
168 100
99 72.1 51.8 77.8

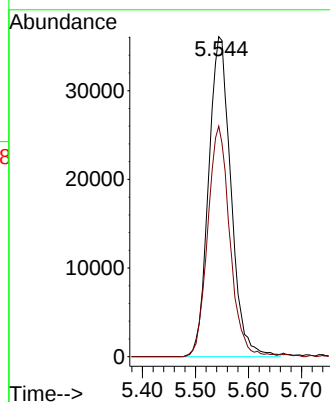

#5
Bromomethane
Concen: 0.981 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 94 Resp: 904
Ion Ratio Lower Upper
94 100
96 87.9 73.9 110.9


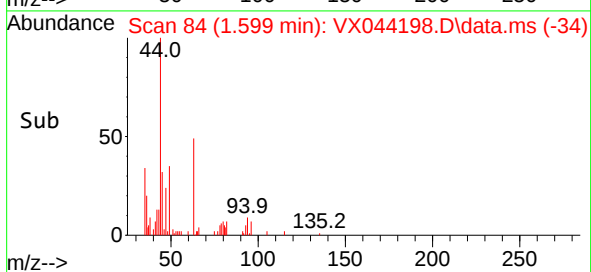
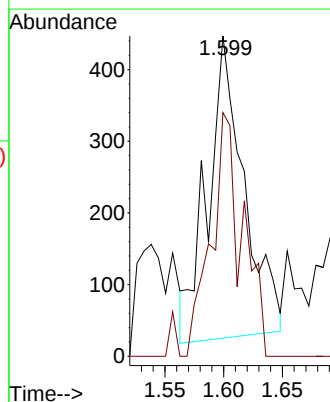
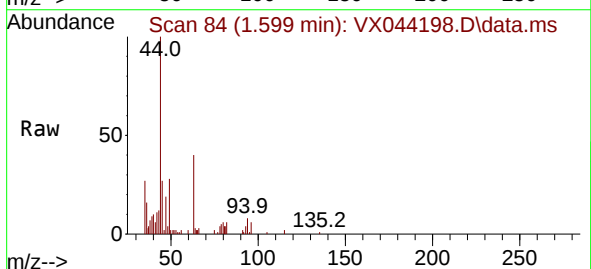


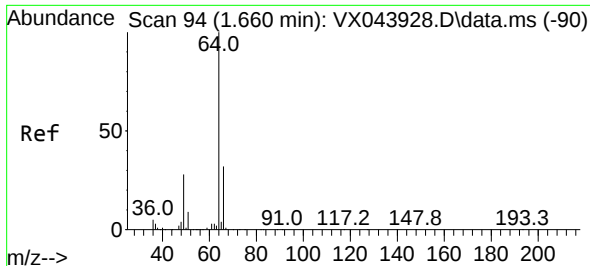

#6
Chloroethane
Concen: 0.231 ug/l
RT: 1.672 min Scan# 90
Delta R.T. 0.012 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 64 Resp: 211
Ion Ratio Lower Upper
64 100
66 0.0 25.9 38.9#

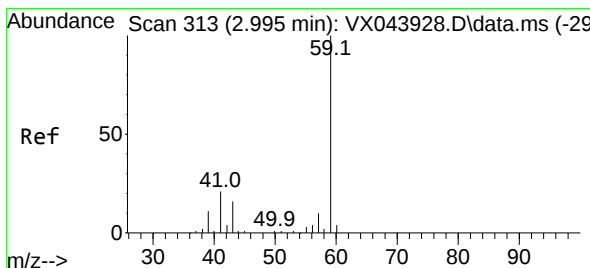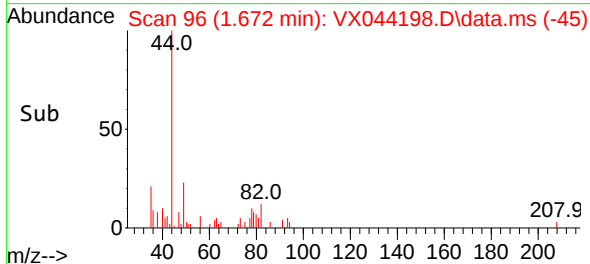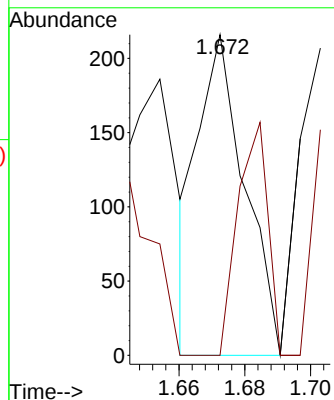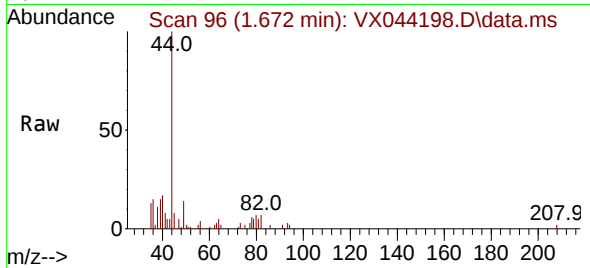

#11
Tert butyl alcohol
Concen: 4.669 ug/l
RT: 2.941 min Scan# 304
Delta R.T. -0.055 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 59 Resp: 1358
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#


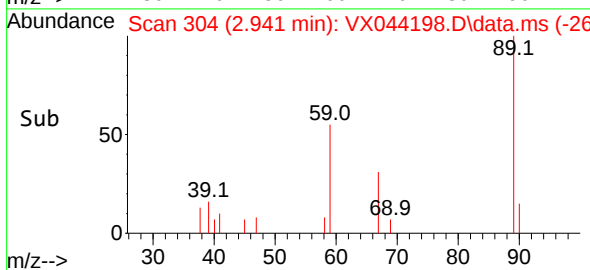
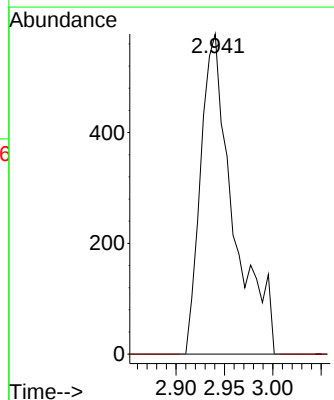
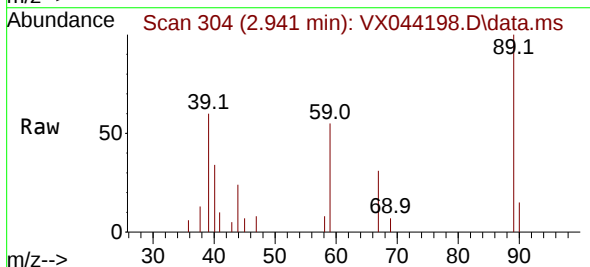




#13
Acrolein
Concen: 0.910 ug/l
RT: 2.227 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 56 Resp: 279
Ion Ratio Lower Upper
56 100
55 81.7 58.2 87.2

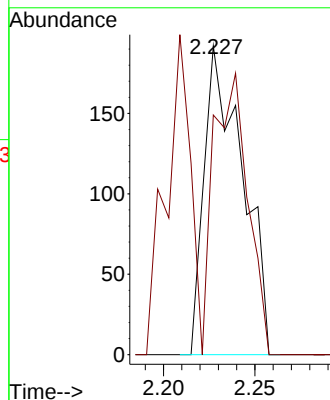

#14
Allyl chloride
Concen: 0.264 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 41 Resp: 525
Ion Ratio Lower Upper
41 100
39 22.5 59.5 89.3#
76 8.8 27.4 41.2#



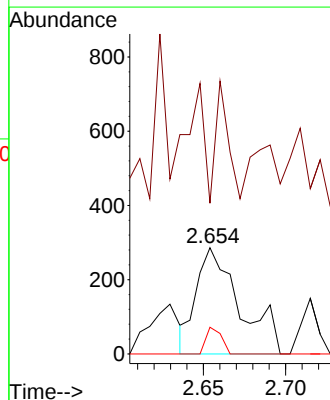





#15
Acrylonitrile
Concen: 0.291 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.012 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 53 Resp: 206
Ion Ratio Lower Upper
53 100
52 218.0 66.5 99.7#
51 85.9 30.2 45.4#

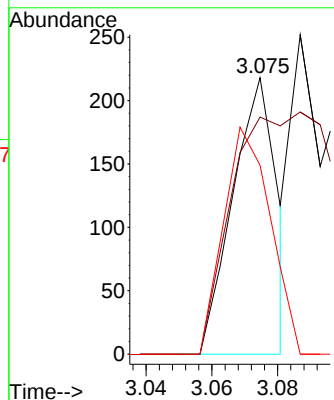

#16
Acetone
Concen: 1.296 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 43 Resp: 1079
Ion Ratio Lower Upper
43 100
58 22.2 22.7 34.1#

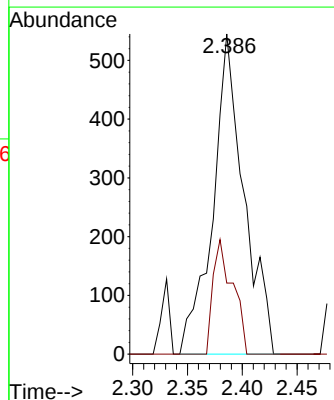

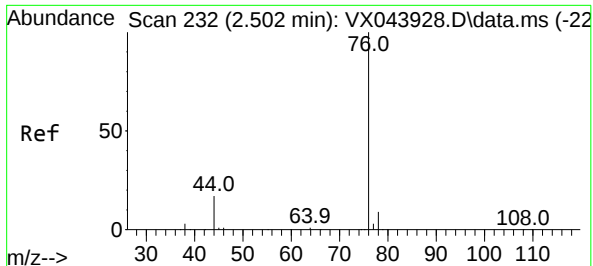

#17

Carbon Disulfide

Concen: 0.602 ug/l

RT: 2.495 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12

Instrument :

MSVOA_X

ClientSampleId :





VX1210MBL01

Tgt Ion: 76 Resp: 1511

Ion Ratio Lower Upper

76 100

78 7.2 7.0 10.6

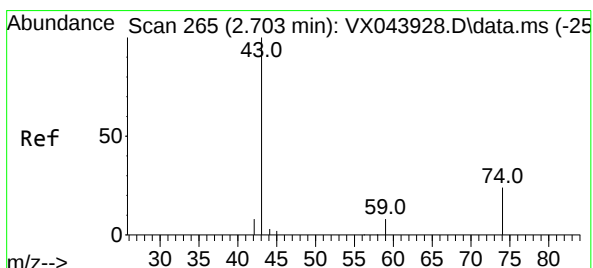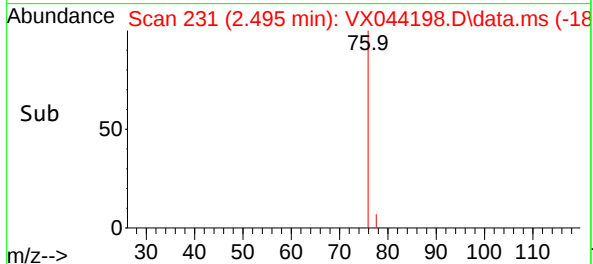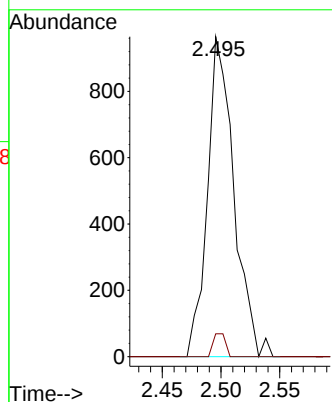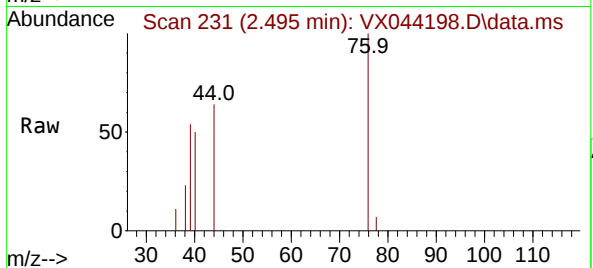

#18

Methyl Acetate

Concen: 0.263 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX044198.D




Acq: 10 Dec 2024 11:12


Tgt Ion: 43 Resp: 509

Ion Ratio Lower Upper

43 100

74 8.4 18.9 28.3#


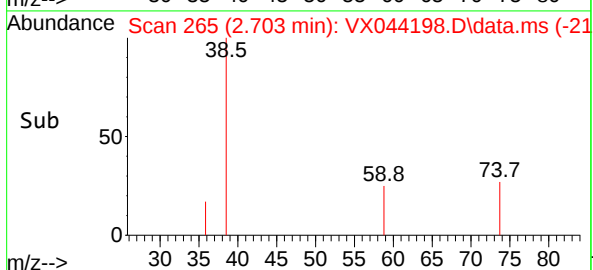

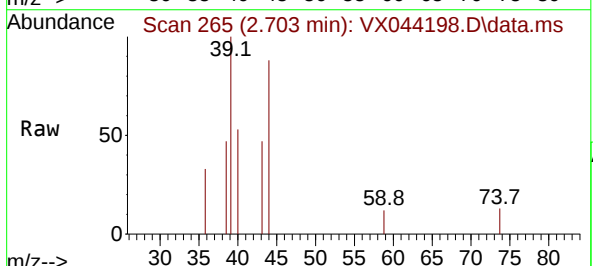




#20
Methylene Chloride
Concen: 0.323 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:	84	Resp:	456
Ion	Ratio	Lower	Upper
84	100		
49	81.7	102.7	154.1#
51	29.8	31.7	47.5#
86	41.4	53.9	80.9#



#21
trans-1,2-Dichloroethene
Concen: 0.366 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion:	96	Resp:	460
Ion	Ratio	Lower	Upper
96	100		
61	157.7	111.8	167.6
98	70.3	52.7	79.1









#31
Cyclohexane
Concen: 1.643 ug/l
RT: 5.538 min Scan# 717
Delta R.T. 0.079 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 56 Resp: 3318
Ion Ratio Lower Upper
56 100
69 136.8 24.7 37.1#
84 70.1 68.7 103.1



#33
1,2-Dichloroethane-d4
Concen: 50.954 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 65 Resp: 92333
Ion Ratio Lower Upper
65 100
67 49.6 0.0 100.8




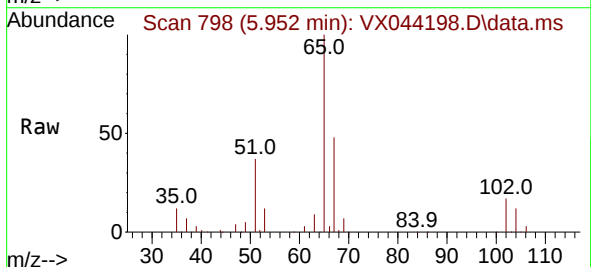




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:114 Resp: 206502
Ion Ratio Lower Upper
114 100
63 21.8 0.0 44.0
88 17.1 0.0 32.4

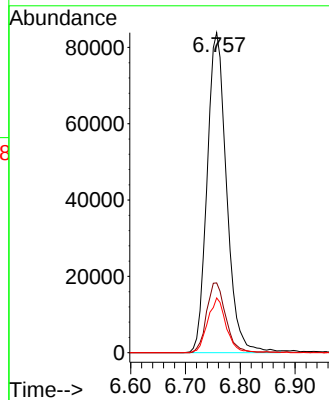

#35
Dibromofluoromethane
Concen: 45.629 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion:113 Resp: 67329
Ion Ratio Lower Upper
113 100
111 102.7 81.0 121.4
192 16.9 13.0 19.6

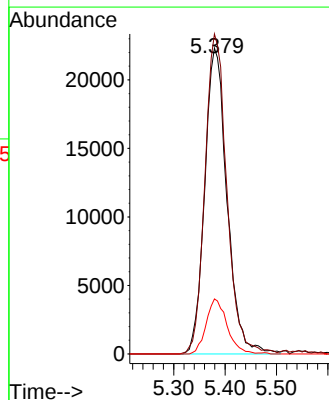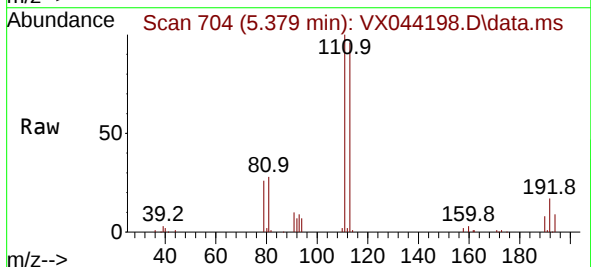



#36

1,1-Dichloropropene

Concen: 5.200 ug/l

RT: 5.538 min Scan# 710

Delta R.T. -0.140 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12

Instrument :

MSVOA_X

ClientSampleId :

VX1210MBL01





Tgt Ion: 75 Resp: 9562

Ion Ratio Lower Upper

75 100

110 12.7 17.4 52.2#

77 0.0 25.8 38.8#



#38

Carbon Tetrachloride

Concen: 5.919 ug/l

RT: 5.538 min Scan# 730

Delta R.T. -0.128 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12




Tgt Ion: 117 Resp: 12229


Ion Ratio Lower Upper

117 100

119 2.5 75.2 112.8#

121 0.0 24.5 36.7#







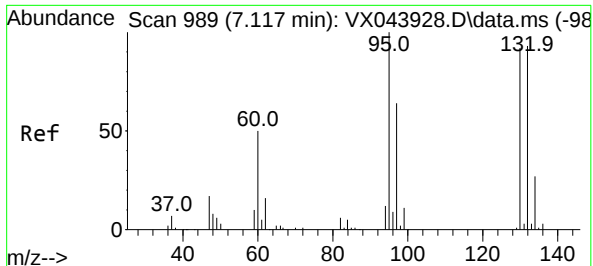

#44
Trichloroethene
Concen: 0.290 ug/l
RT: 7.129 min Scan# 91
Delta R.T. 0.012 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:130 Resp: 471
Ion Ratio Lower Upper
130 100
95 78.1 0.0 217.8

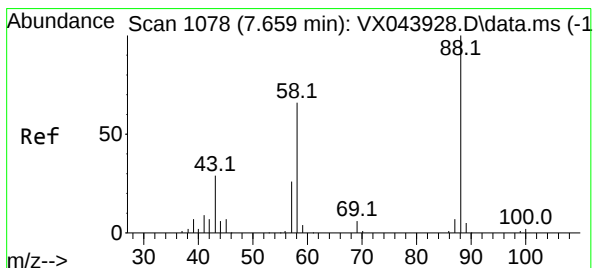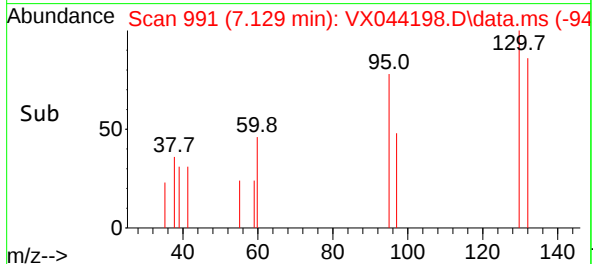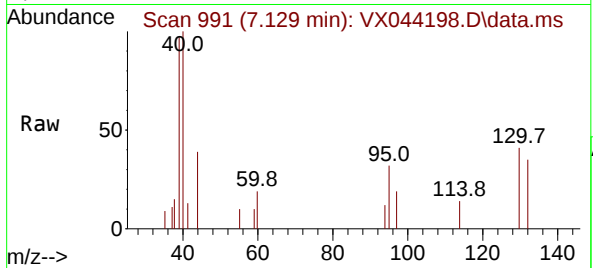

#49
1,4-Dioxane
Concen: 0.676 ug/l
RT: 7.714 min Scan# 1087
Delta R.T. 0.055 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 88 Resp: 21
Ion Ratio Lower Upper
88 100
43 0.0 26.8 40.2#
58 0.0 45.4 68.2#


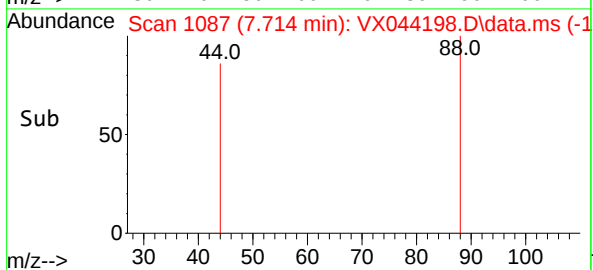

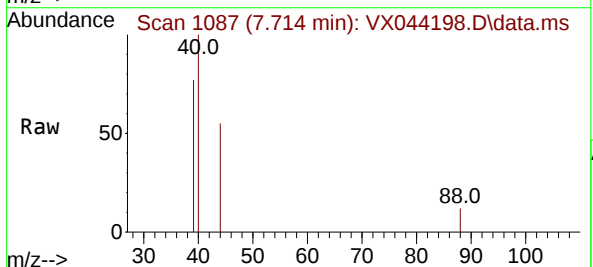


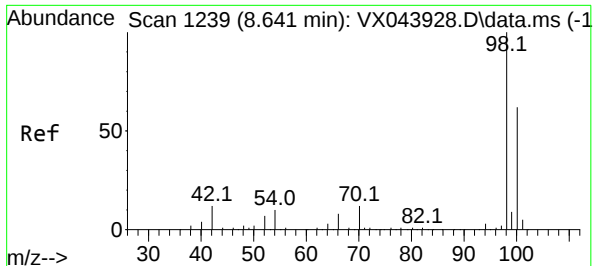

#50
Toluene-d8
Concen: 49.104 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 98 Resp: 249762
Ion Ratio Lower Upper
98 100
100 63.7 52.6 79.0

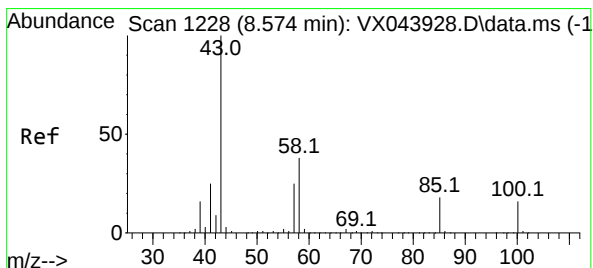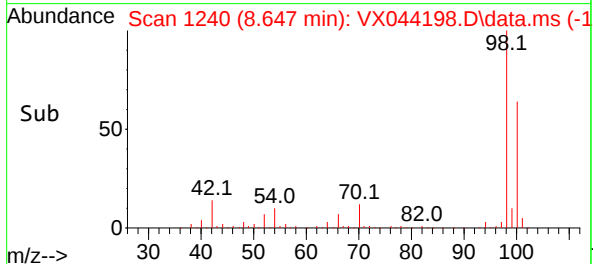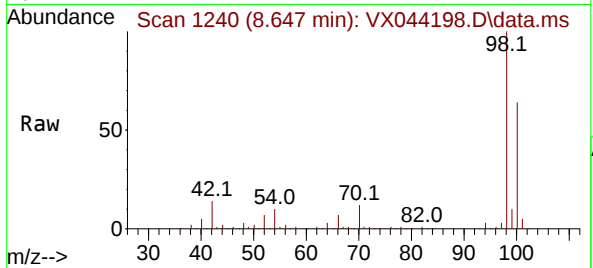

#51
4-Methyl-2-Pentanone
Concen: 0.284 ug/l
RT: 8.592 min Scan# 1231
Delta R.T. 0.018 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 43 Resp: 630
Ion Ratio Lower Upper
43 100
58 0.0 30.0 45.0#


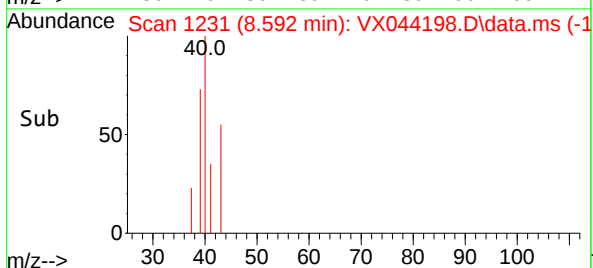

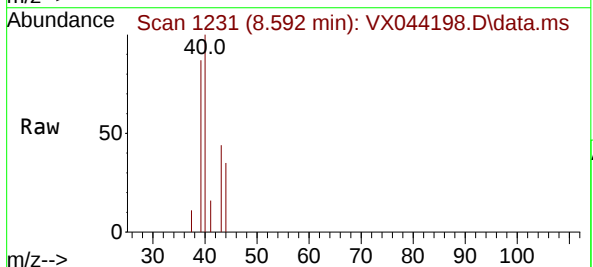




#62
4-Bromofluorobenzene
Concen: 46.455 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 95 Resp: 80415
Ion Ratio Lower Upper
95 100
174 73.6 0.0 150.4
176 71.4 0.0 146.0

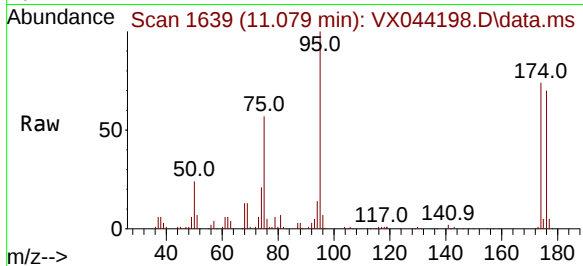

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 117 Resp: 178441
Ion Ratio Lower Upper
117 100
82 55.7 46.4 69.6
119 31.4 24.6 37.0




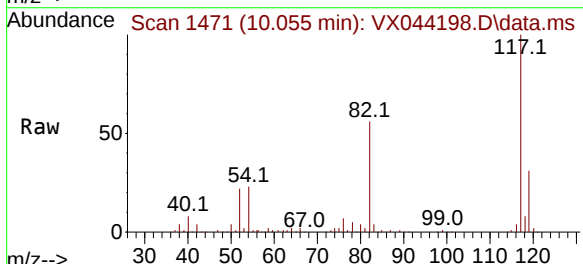




#68
m/p-Xylenes
Concen: 0.265 ug/l
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:106 Resp: 656
Ion Ratio Lower Upper
106 100
91 193.8 168.1 252.1

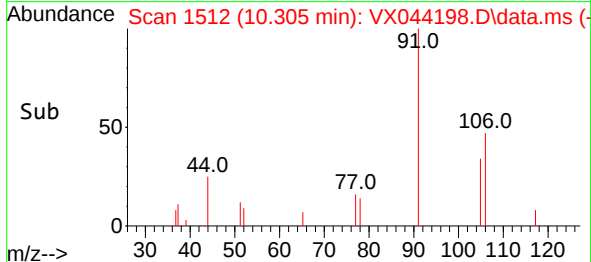

#71
Bromoform
Concen: 1.289 ug/l
RT: 10.811 min Scan# 1595
Delta R.T. 0.012 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion:173 Resp: 79
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.2#
254 0.0 0.0 0.0


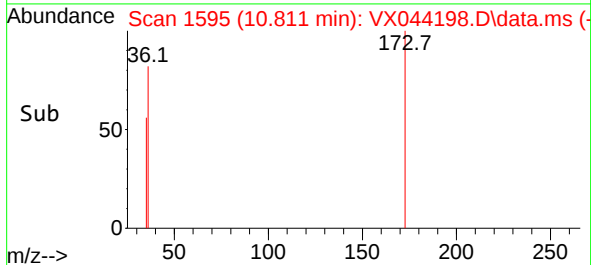

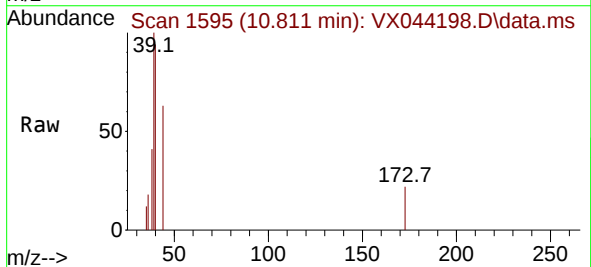




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX044198.D
 Acq: 10 Dec 2024 11:12




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1210MBL01


Tgt Ion:152 Resp: 71191
 Ion Ratio Lower Upper
 152 100
 115 64.1 45.4 136.2
 150 158.6 0.0 353.0

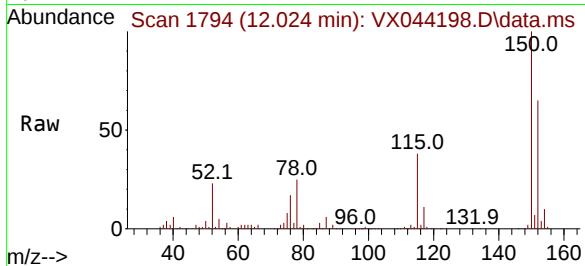

#76
 1,2,3-Trichloropropane
 Concen: 29.817 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX044198.D
 Acq: 10 Dec 2024 11:12

Tgt Ion: 75 Resp: 46550
 Ion Ratio Lower Upper
 75 100
 77 1.2 21.8 65.3#


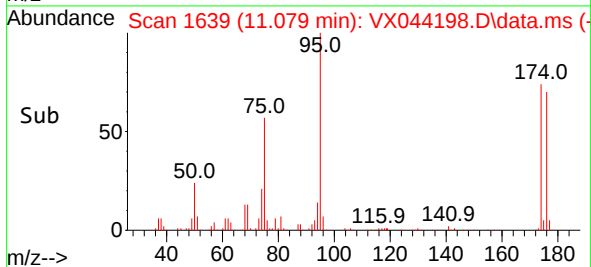

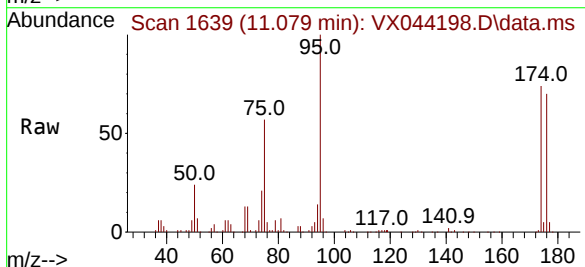




#77
Bromobenzene
Concen: 0.203 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:156 Resp: 265
Ion Ratio Lower Upper
156 100
77 205.3 83.4 250.1
158 92.5 47.6 142.8

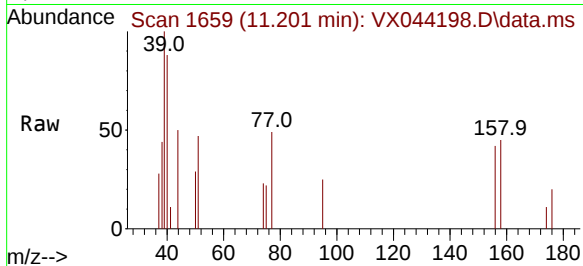

#81
trans-1,4-Dichloro-2-butene
Concen: 81.363 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion: 75 Resp: 46550
Ion Ratio Lower Upper
75 100
53 0.0 86.7 130.1#
89 0.2 38.2 57.2#




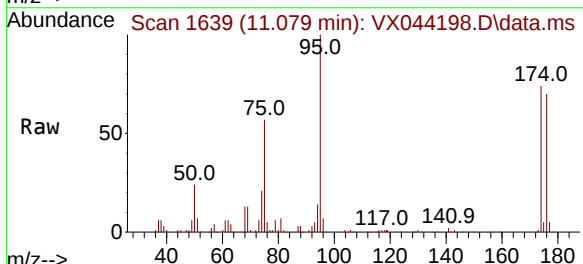


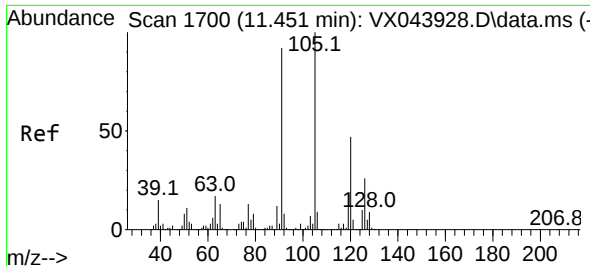

#82
4-Chlorotoluene
Concen: 0.243 ug/l
RT: 11.469 min Scan# 11
Delta R.T. 0.018 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion: 91 Resp: 1060
Ion Ratio Lower Upper
91 100
126 14.6 14.3 42.9

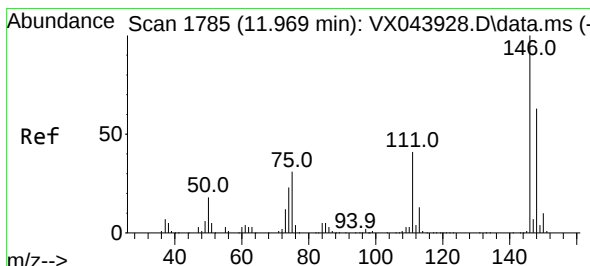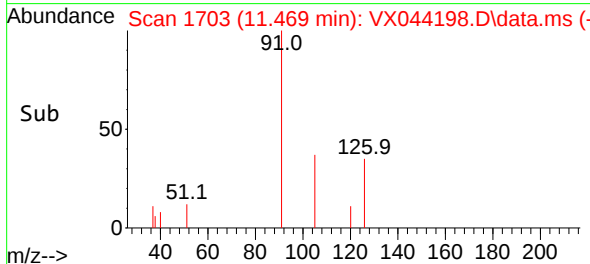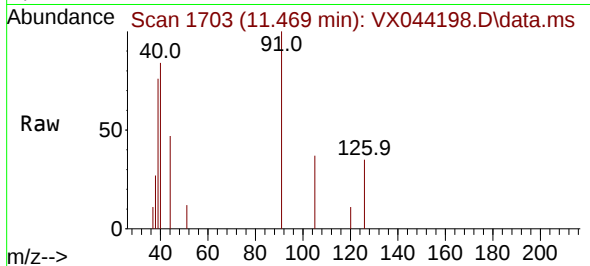

#87
1,3-Dichlorobenzene
Concen: 0.373 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion:146 Resp: 887
Ion Ratio Lower Upper
146 100
111 26.6 21.1 63.3
148 60.1 31.7 95.1

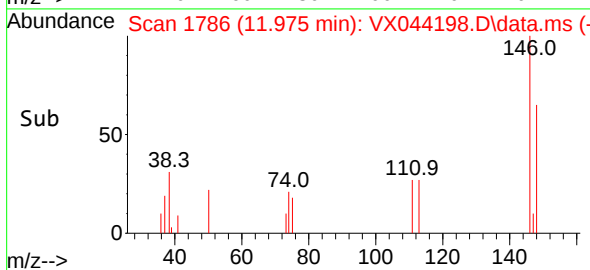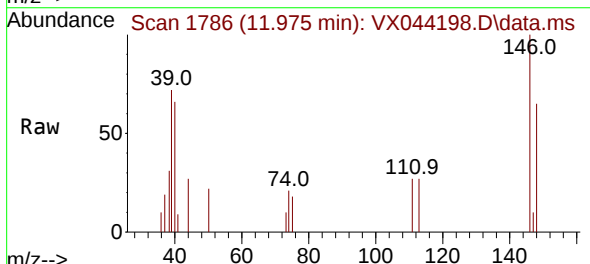



#88

1,4-Dichlorobenzene

Concen: 0.366 ug/l

RT: 11.975 min Scan# 11

Delta R.T. -0.061 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12

Instrument :

MSVOA_X

ClientSampleId :

VX1210MBL01





Tgt Ion:146 Resp: 887

Ion Ratio Lower Upper

146 100

111 26.6 20.1 60.3

148 60.1 30.9 92.8

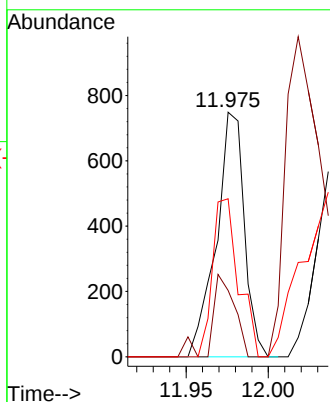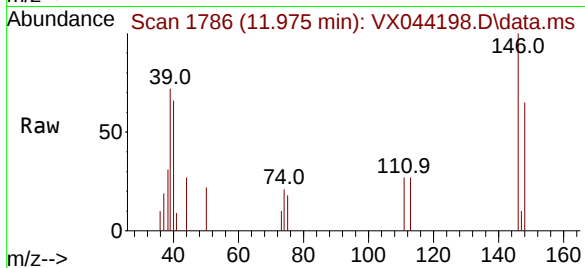

#89

n-Butylbenzene

Concen: 0.223 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.012 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12




Tgt Ion: 91 Resp: 875


Ion Ratio Lower Upper

91 100

92 50.6 26.6 79.8

134 4.9 12.4 37.2#


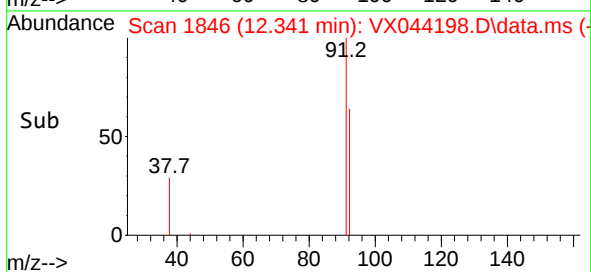
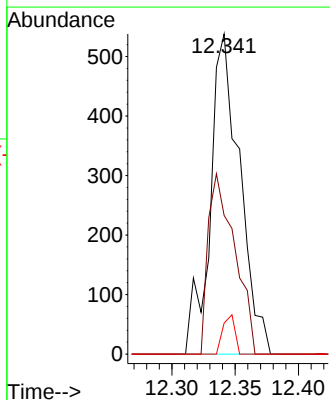
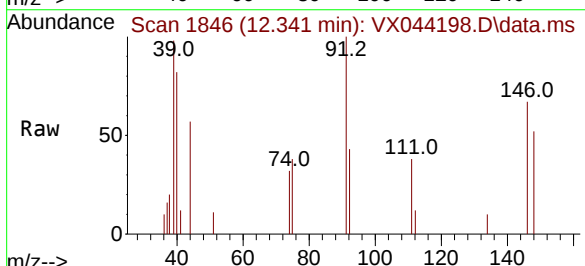




#91
1,2-Dichlorobenzene
Concen: 0.232 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12




Instrument :
MSVOA_X
ClientSampleId :
VX1210MBL01


Tgt Ion:146 Resp: 556
Ion Ratio Lower Upper
146 100
111 58.6 21.5 64.5
148 60.3 31.9 95.5



#93
1,2,4-Trichlorobenzene
Concen: 0.491 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.012 min
Lab File: VX044198.D
Acq: 10 Dec 2024 11:12

Tgt Ion:180 Resp: 694
Ion Ratio Lower Upper
180 100
182 92.4 48.0 144.2
145 31.7 16.8 50.4

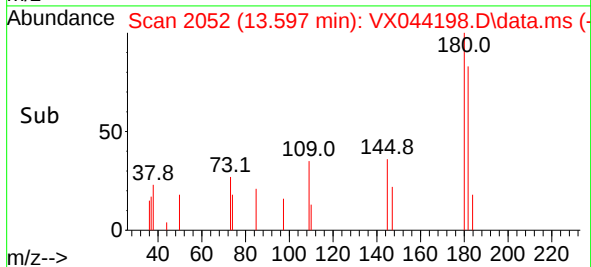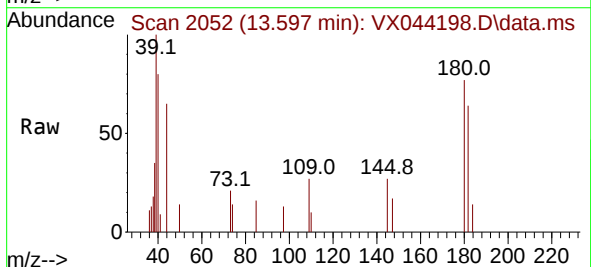



#95

Naphthalene

Concen: 0.825 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12

Instrument :

MSVOA_X

ClientSampleId :

VX1210MBL01





Tgt Ion:128 Resp: 4203

Ion Ratio Lower Upper

128 100

127 9.1 10.2 15.2#

129 8.3 8.6 12.8#

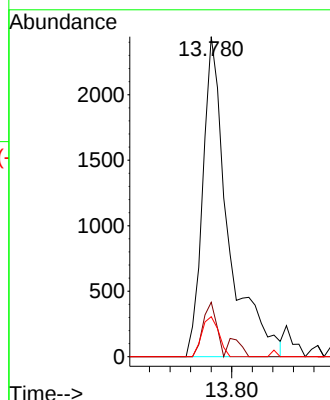

#96

1,2,3-Trichlorobenzene

Concen: 0.521 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX044198.D

Acq: 10 Dec 2024 11:12

Tgt Ion:180 Resp: 746

Ion Ratio Lower Upper

180 100

182 86.1 45.6 136.8

145 45.8 16.4 49.4

