

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
 Data File : VX044199.D
 Acq On : 10 Dec 2024 11:35
 Operator : JC/MD
 Sample : VX1210WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1210WBL01

Quant Time: Dec 11 01:27:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	110263	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	207593	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178508	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	71476	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	94012	49.710	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.420%
35) Dibromofluoromethane	5.385	113	68829	46.401	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.800%
50) Toluene-d8	8.647	98	251203	49.128	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.260%
62) 4-Bromofluorobenzene	11.079	95	82733	47.543	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	95.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044199.D
Acq On : 10 Dec 2024 11:35
Operator : JC/MD
Sample : VX1210WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1210WBL01


Quant Time: Dec 11 01:27:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

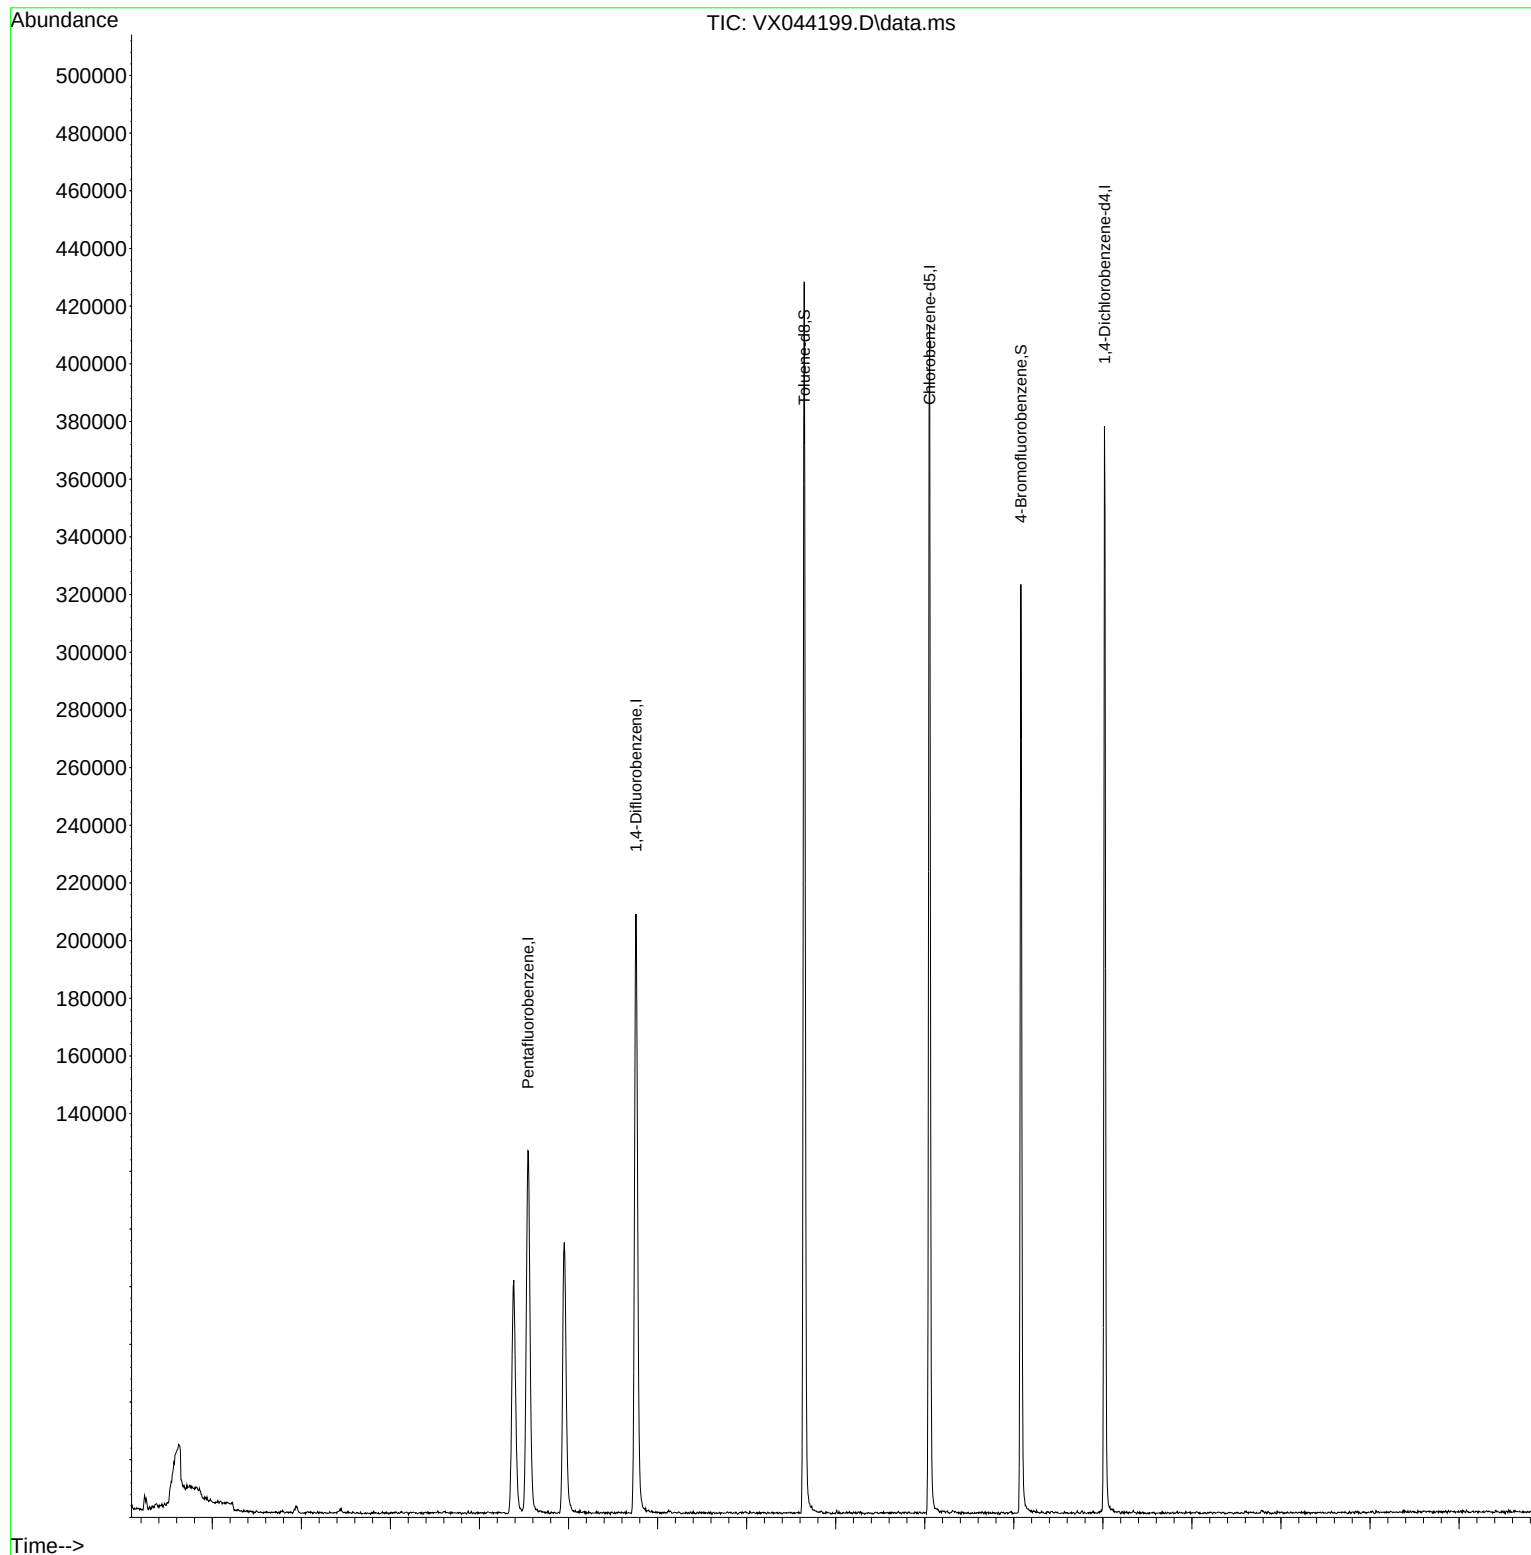



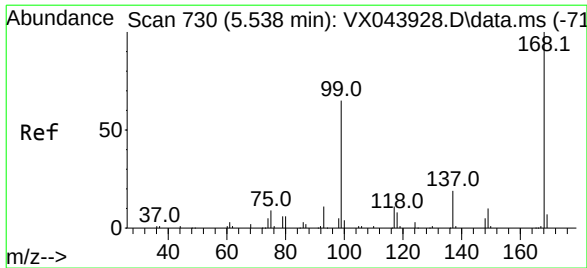


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.006 min
Lab File: VX044199.D
Acq: 10 Dec 2024 11:35

Instrument :
MSVOA_X
ClientSampleId :
VX1210WBL01



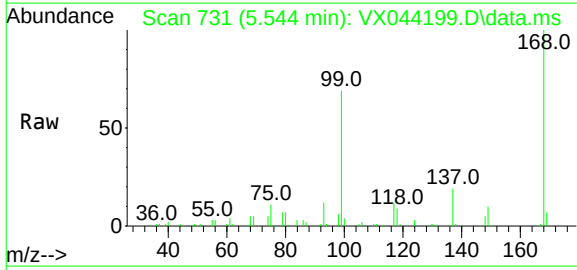



Tgt Ion:168 Resp: 110263
Ion Ratio Lower Upper
168 100
99 69.2 51.8 77.8

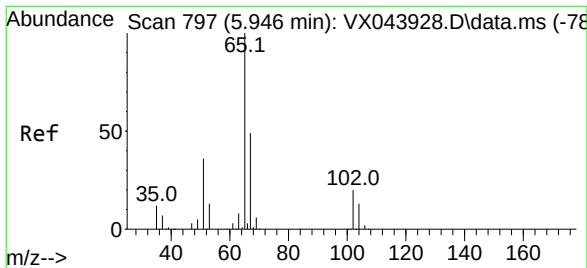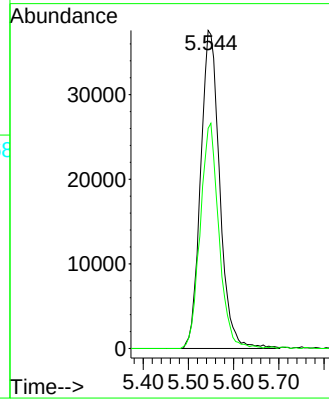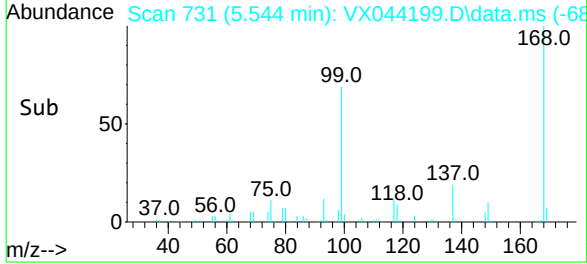

#33
1,2-Dichloroethane-d4
Concen: 49.710 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.000 min
Lab File: VX044199.D
Acq: 10 Dec 2024 11:35

Tgt Ion: 65 Resp: 94012
Ion Ratio Lower Upper
65 100
67 50.2 0.0 100.8


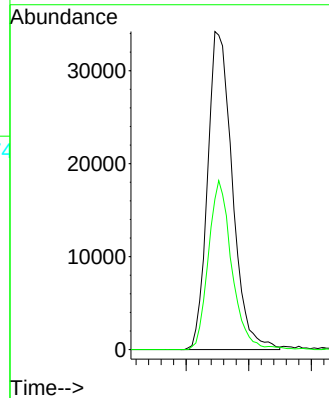
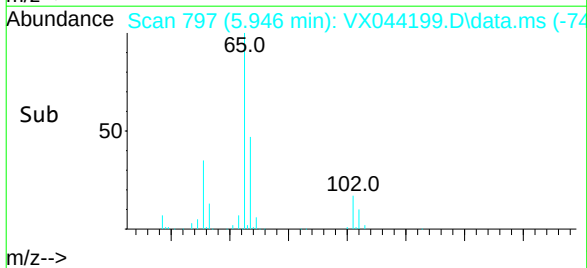
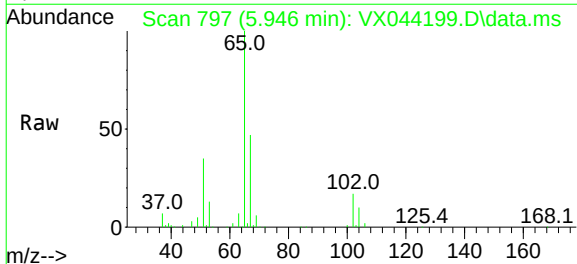


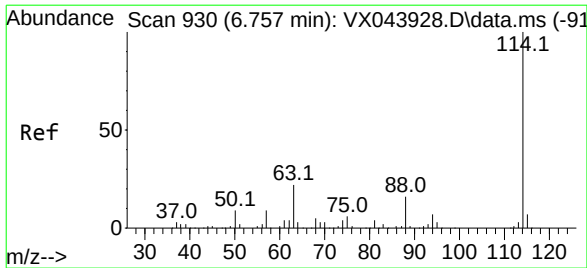

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 93
Delta R.T. -0.000 min
Lab File: VX044199.D
Acq: 10 Dec 2024 11:35




Instrument :
MSVOA_X
ClientSampleId :
VX1210WBL01


Tgt Ion:	114	Resp:	207593
Ion	Ratio	Lower	Upper
114	100		
63	21.6	0.0	44.0
88	17.2	0.0	32.4

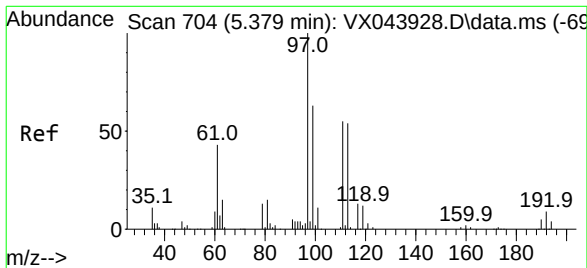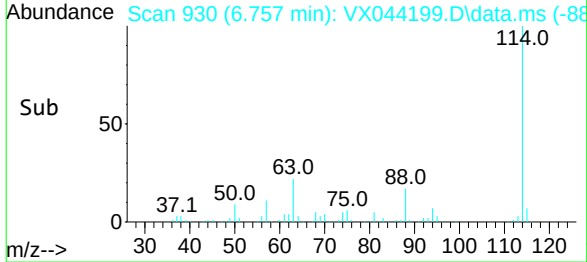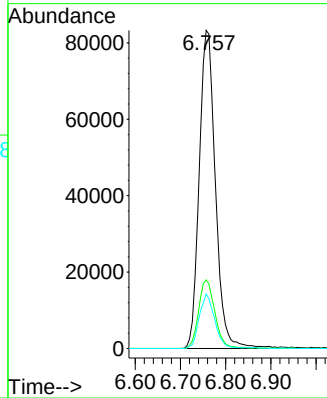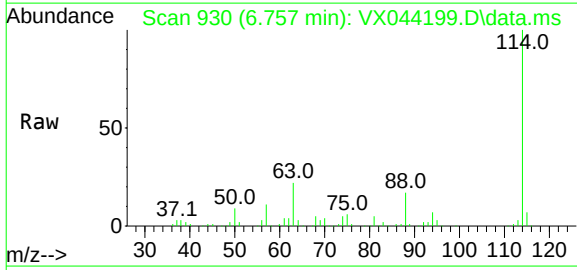

#35
Dibromofluoromethane
Concen: 46.401 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX044199.D
Acq: 10 Dec 2024 11:35

Tgt Ion:	113	Resp:	68829
Ion	Ratio	Lower	Upper
113	100		
111	103.0	81.0	121.4
192	17.3	13.0	19.6

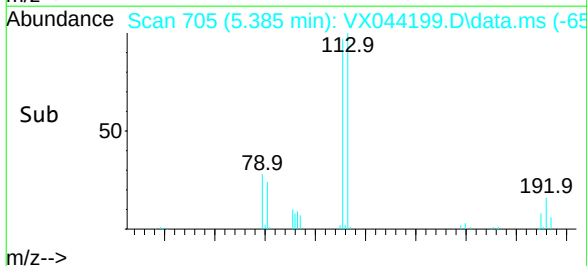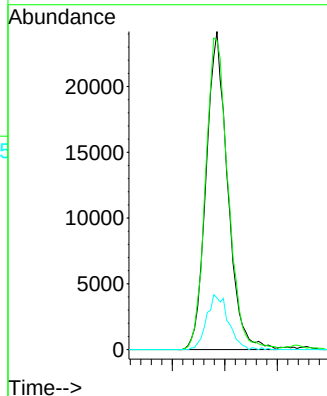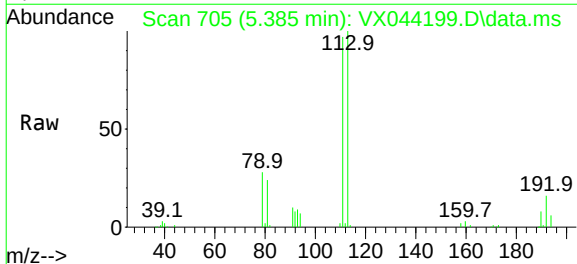

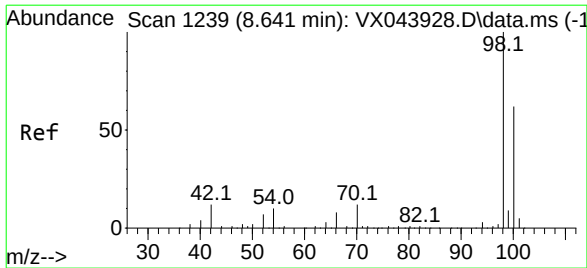

#50

Toluene-d8

Concen: 49.128 ug/l

RT: 8.647 min Scan# 12

Delta R.T. 0.006 min

Lab File: VX044199.D

Acq: 10 Dec 2024 11:35

Instrument :

MSVOA_X

ClientSampleId :





VX1210WBL01

Tgt Ion: 98 Resp: 251203

Ion Ratio Lower Upper

98 100

100 64.6 52.6 79.0

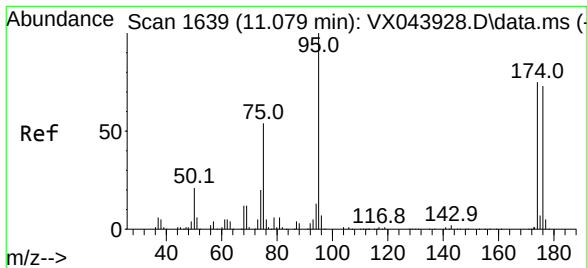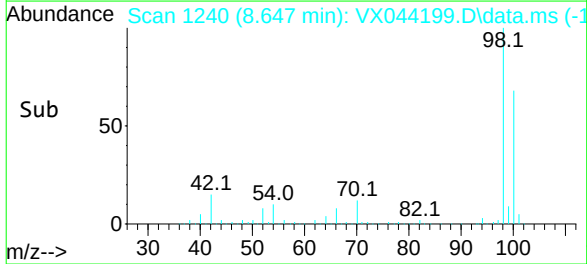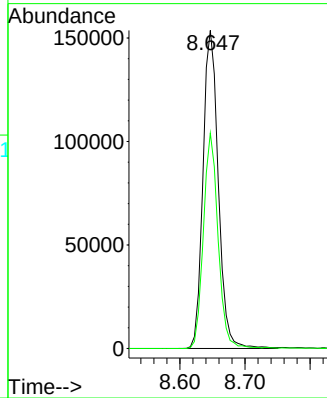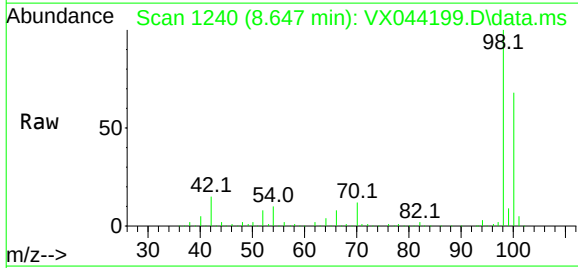

#62

4-Bromofluorobenzene

Concen: 47.543 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX044199.D

Acq: 10 Dec 2024 11:35




Tgt Ion: 95 Resp: 82733


Ion Ratio Lower Upper

95 100

174 72.6 0.0 150.4

176 70.6 0.0 146.0

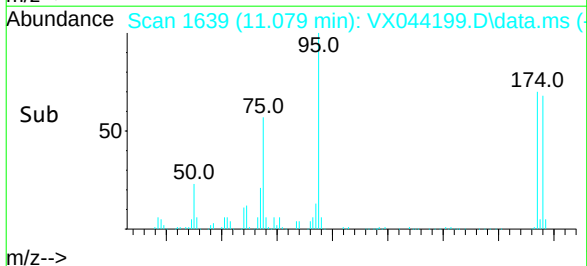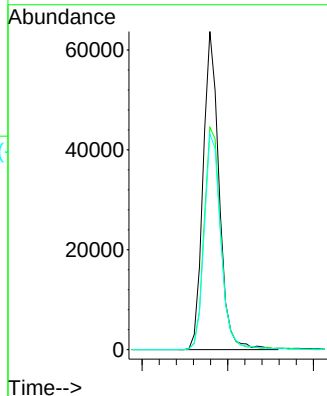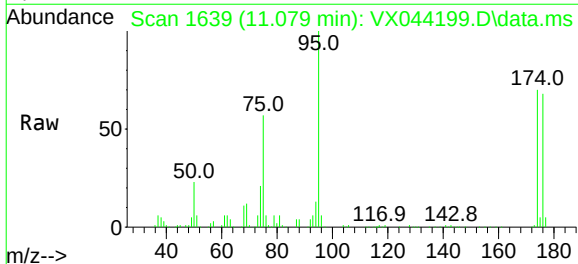

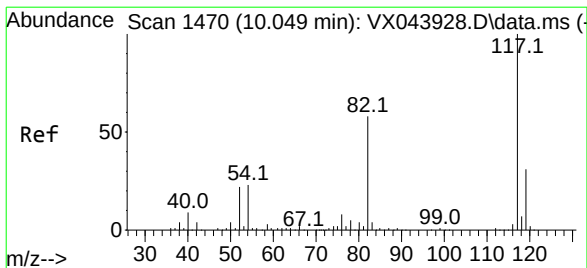

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 14

Delta R.T. 0.006 min

Lab File: VX044199.D

Acq: 10 Dec 2024 11:35

Instrument :

MSVOA_X

ClientSampleId :

VX1210WBL01





Tgt Ion:117 Resp: 178508

Ion Ratio Lower Upper

117 100

82 59.3 46.4 69.6

119 32.2 24.6 37.0

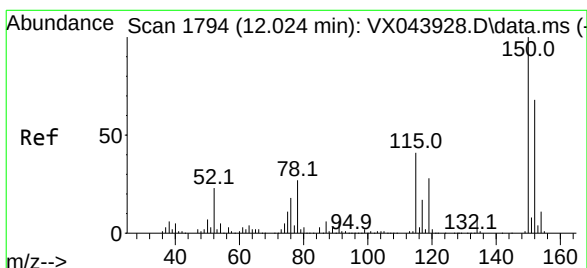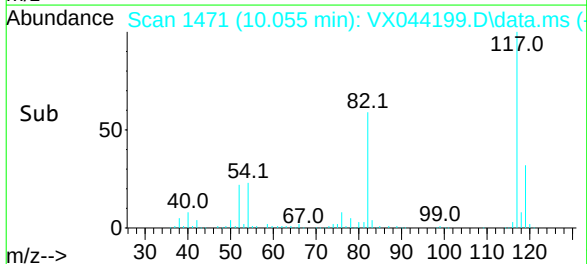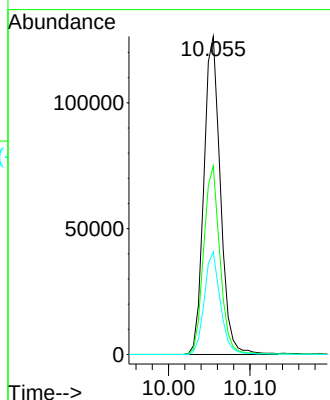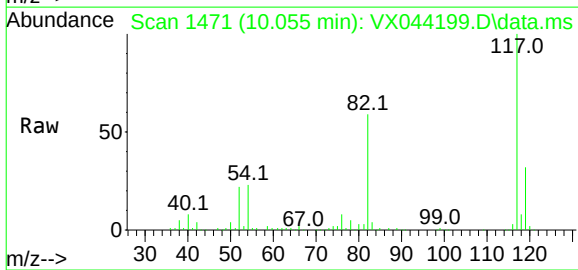

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX044199.D

Acq: 10 Dec 2024 11:35

Tgt Ion:152 Resp: 71476

Ion Ratio Lower Upper

152 100

115 62.7 45.4 136.2

150 160.5 0.0 353.0

