

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
 Data File : VX044212.D
 Acq On : 10 Dec 2024 16:47
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Title : SW846 8260

Signal : TIC: VX044212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	68	79	80	rBV6	22675	63045	8.90%	1.595%
2	2.941	297	304	311	rBV4	3321	8285	1.17%	0.210%
3	5.385	694	705	721	rBV2	82081	245456	34.66%	6.211%
4	5.544	721	731	747	rVV	129375	373329	52.71%	9.447%
5	5.952	788	798	815	rBV	98975	267032	37.70%	6.757%
6	6.757	918	930	953	rBV	214039	520646	73.51%	13.175%
7	8.647	1232	1240	1250	rBV	449367	708243	100.00%	17.922%
8	10.055	1465	1471	1482	rBV	427741	610407	86.19%	15.446%
9	11.079	1634	1639	1650	rBV	345187	454251	64.14%	11.495%
10	12.018	1788	1793	1806	rBV	404599	536600	75.76%	13.579%
11	12.219	1822	1826	1831	rBV7	3503	7530	1.06%	0.191%
12	14.036	2118	2124	2130	rBV10	4094	8007	1.13%	0.203%
13	14.323	2164	2171	2172	rBV6	4749	9241	1.30%	0.234%
14	14.756	2238	2242	2245	rBV2	9767	10739	1.52%	0.272%
15	15.115	2295	2301	2309	rBV8	12994	34098	4.81%	0.863%
16	15.487	2357	2362	2368	rBV3	19965	29985	4.23%	0.759%
17	15.615	2379	2383	2389	rVV9	6210	14259	2.01%	0.361%
18	15.664	2389	2391	2396	rVB5	5039	8179	1.15%	0.207%
19	15.883	2422	2427	2429	rBV5	3715	7166	1.01%	0.181%
20	16.377	2498	2508	2517	rBV2	16537	35315	4.99%	0.894%




Sum of corrected areas: 3951813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044212.D
Acq On : 10 Dec 2024 16:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

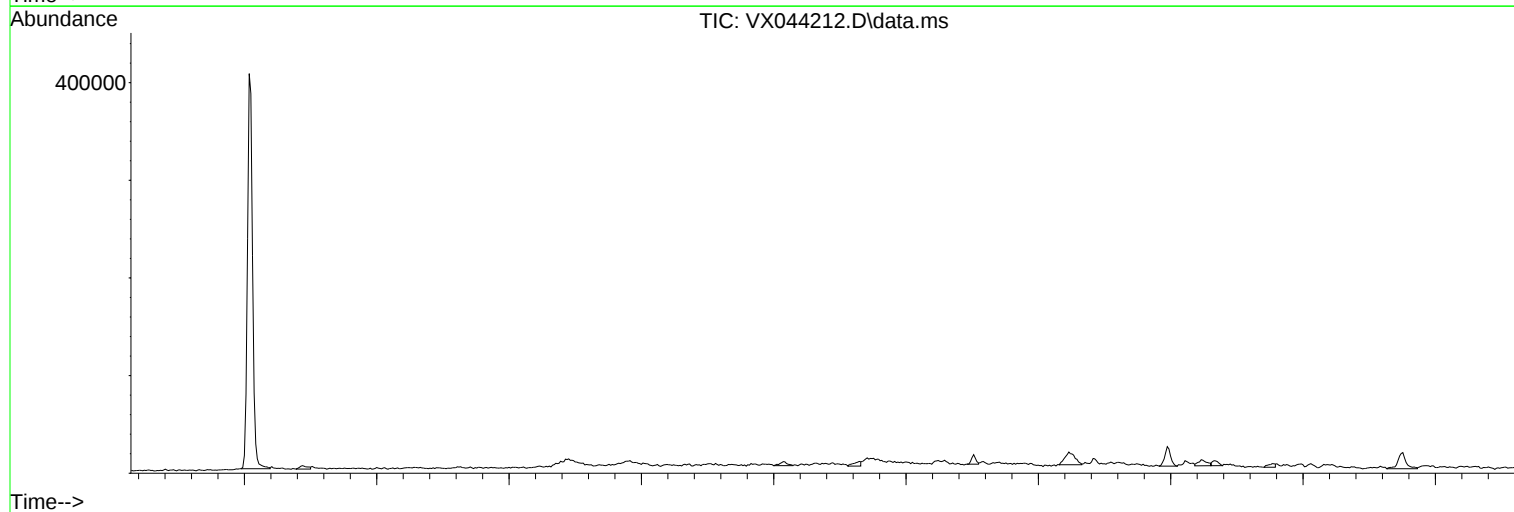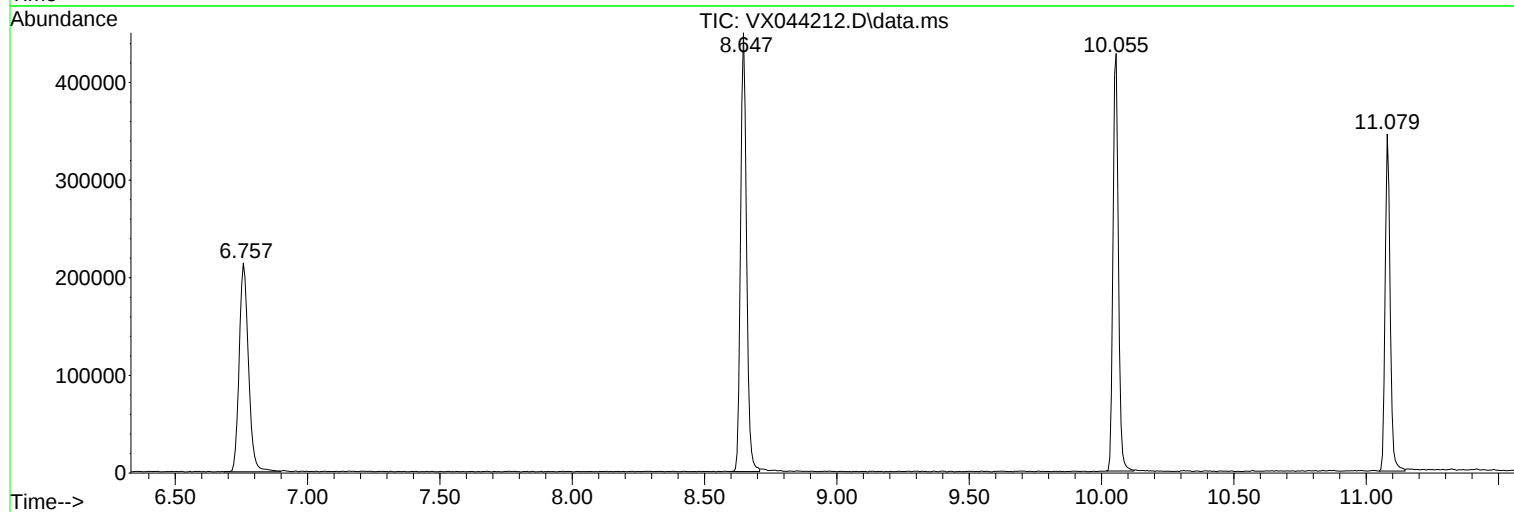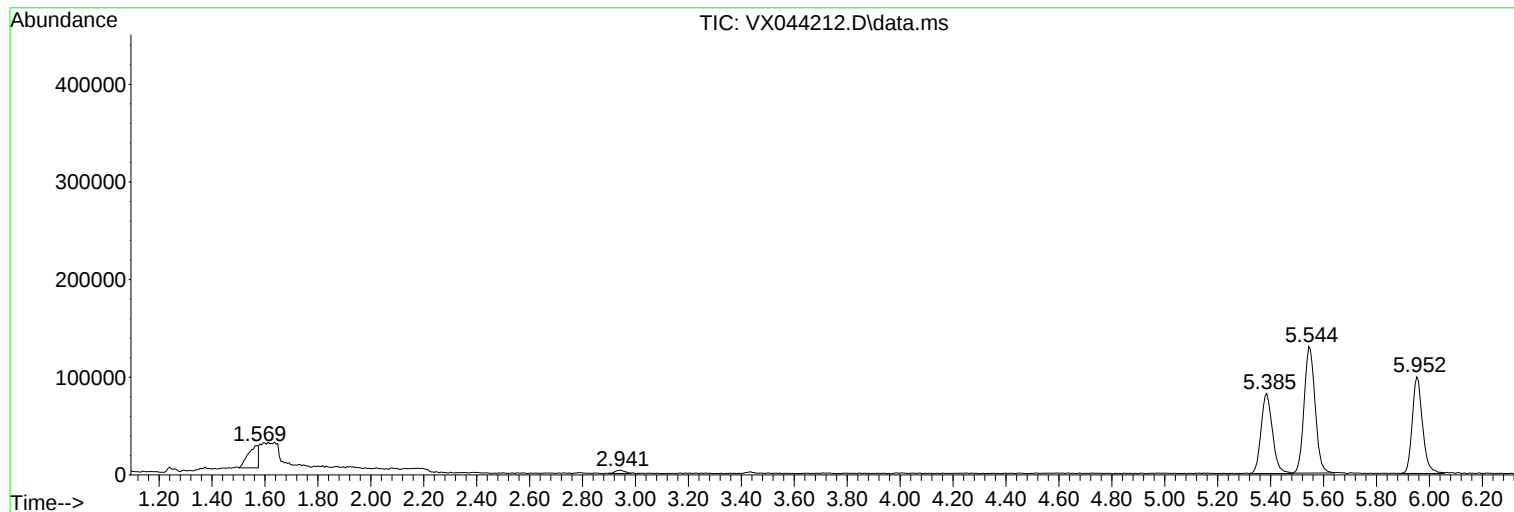

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044212.D
Acq On : 10 Dec 2024 16:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044212.D
Acq On : 10 Dec 2024 16:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------